INCH-POUND

A-A-54758
15 October 1992

COMMERCIAL ITEM DESCRIPTION

STAND, SHELF

(Corrosion Resisting Steel)

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for MIL-S-16297A which is cancelled.

This Commercial Item Description covers a shelf stand suitable for use in a surgical operating room.

Salient characteristics:

The shelf stand shall be fabricated of American Iron and Steel Institute (AISI) type 302 or 304 corrosion-resisting steel. The stand shall consist of a tubular framework for holding four equally spaced shelves, and shall conform to figure 1.


The shelf frame shall consist of 1-inch outside diameter, 0.0625 inch thick wall (No. 16 U.S. Standard Gage) tubing. The frame shall be mounted on adjustable corrosion-resisting steel, or nickel-plated steel, glides. The two rear legs forming the back supports shall be straight. The two front legs shall be curved diagonally inward, midway between the second and third shelves, to allow for the reduced width of the two upper shelves. All tubing shall be closed flush at the top by welding.

The stand shall have four shelves of 0.0625 inch thick (No. 16 U.S. Standard Gage) corrosion-resisting steel. All shelves shall be closely welded to the uprights with all joints ground smooth. Shelf corners shall be notched on a

AMSC N/A FSC 6530

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

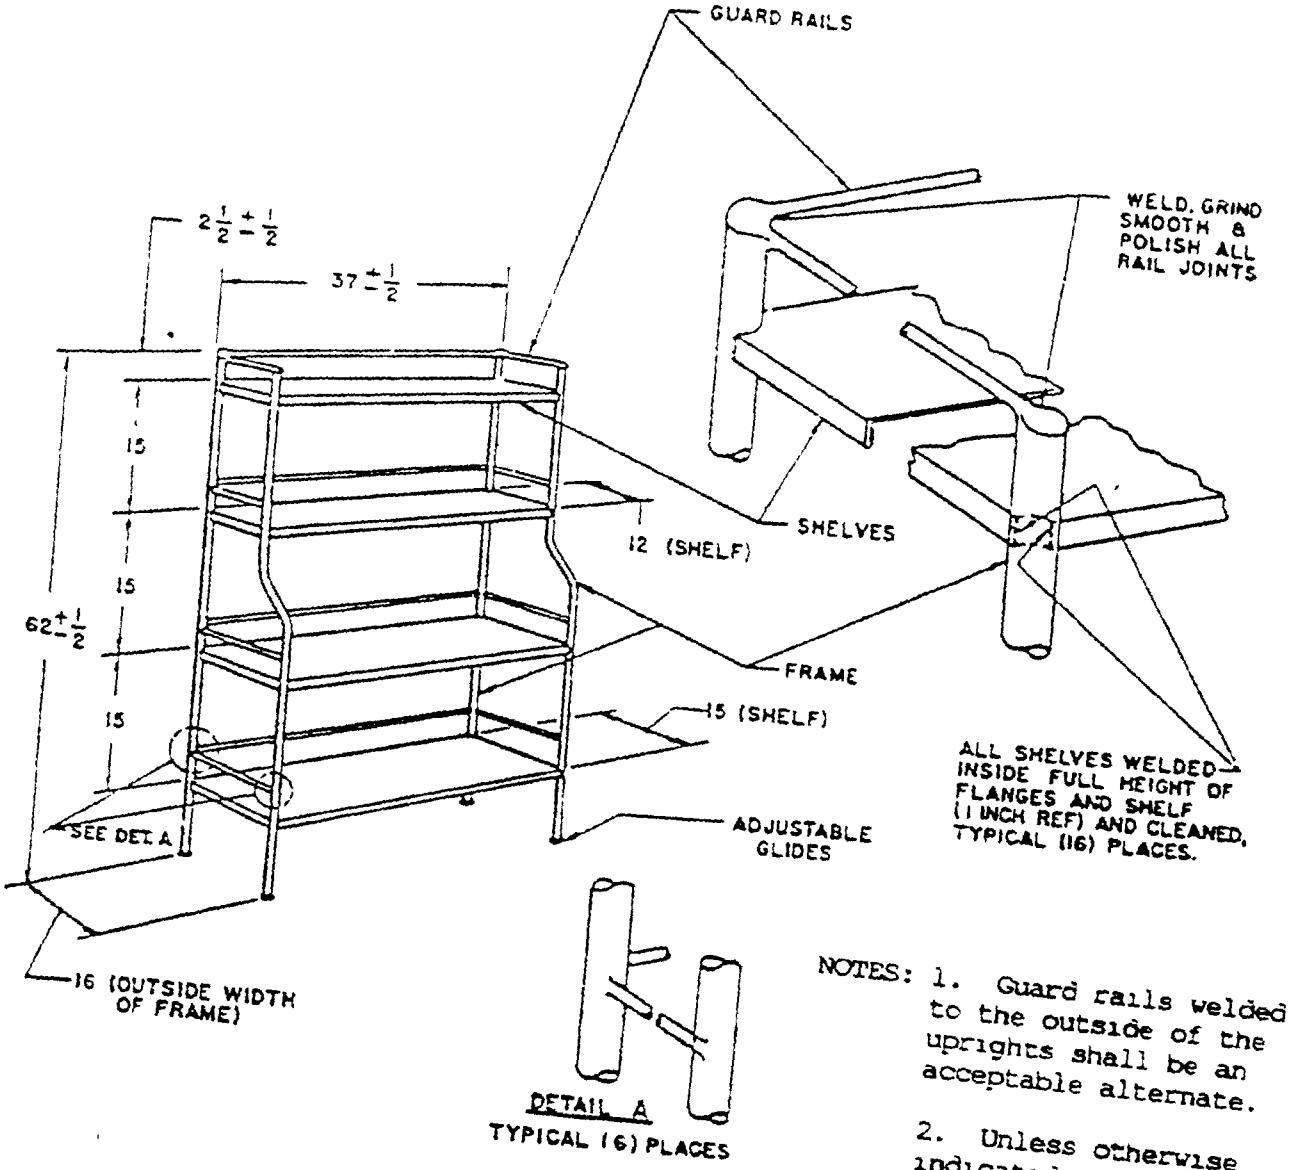

NOTES: 1. Guard rails welded to the outside of the uprights shall be an acceptable alternate.

2. Unless otherwise indicated, dimensions of less than 24 inches shall have a plus or minus 1/4 inch tolerance.

FIGURE 1. Shelf stand.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

1/2 inch radius to fit the contour of the legs, so that no opening remains. All edges of the shelves shall be flanged downward one inch, and hemmed not less than 5/8 inch.

Welding shall be as shown on figure 1. All exposed welds shall be ground and polished to blend with the adjacent areas. Welds shall be thorough, nonporous, cleaned, and ground. Welds shall be free from pit marks and imperfections.

All parts of the stand shall be free of cracks, tears, ruptures, and deformed areas. Exposed and accessible edges, and surfaces shall be free of burrs, sharpness, and sharp projections. Stand finish shall be uniform and free of course grind marks and scratched areas.

Workmanship. The shelf stand shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One stand, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 4.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one shelf stand.

Sampling for tests. Sampling for tests, including dimensional test, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-1. The unit of product for test purposes shall be one shelf stand.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document.

6530-00-708-2615

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

A-A-54758

MILITARY INTERESTS:

Custodians:

Air Force - 03
Army - MD
Navy - MS

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

FDA-MPQAS
USPHS
VA - OSS

Project Number: 6530-2379

Location: STANDC13.DOC

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER: A-A-54758	2. DOCUMENT DATE (YYMMDD): 15 October 1992

3. DOCUMENT TITLE: STAND, SHELF (Corrosion Resisting Steel)

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	e. DATE SUBMITTED (YYMMDD)

7. PREPARING ACTIVITY

a. NAME DEFENSE PERSONNEL SUPPORT CENTER ATTN: DPSC-MSE	b. TELEPHONE (Include Area Code) (1) Commercial: AC 215-737-2870 (2) AUTOVON: AV 444-2870
c. ADDRESS (Include Zip Code) 2800 SO. 20TH STREET PHILADELPHIA, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous editions are obsolete — 198/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:38Z
Check the source to verify that this is the current version before use.