MIL-T-37538A
24 September 1987
SUPERSEDING
MIL-T-37538
1 September 1976 and
MIL-W-37013
1 April 1974

MILITARY SPECIFICATION

TRIMMER, DENTAL MODEL; WHEEL, ABRASIVE, SILICON CARBIDE, DENTAL MODEL TRIMMING

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a model trimmer and replacement wheel suitable for dental laboratory use.

1.2 Classification.

1.2.1 Type I. Model Trimmer, Complete. The model trimmer shall be furnished complete with wheel and accessories.

1.2.2 Type II. Wheel, Abrasive, Silicon Carbide. Replacement wheel.

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications and standards. The following specifications and standards form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of these documents are those listed in the issue of the Department of Defense Index of Specifications and Standards (DODISS) and supplement thereto, cited in the solicitation.

AMSC N/A FSC 6520

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-RST, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.

SPECIFICATIONS

Federal

PPP-B-566 - Boxes, Folding, Paperboard.
PPP-B-601 - Boxes, Wood, Cleated-Plywood.
PPP-B-621 - Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636 - Boxes, Shipping, Fiberboard.
PPP-B-676 - Boxes, Setup.

Military

MIL-M-7298 - Manual, Technical, Commercial Equipment.
MIL-P-116 - Preservation, Methods of.
MIL-L-10547 - Liners, Case and Sheet; Overwrap; Water-Vapor-proof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.
MIL-STD-147 - Palletized Unit Loads.
MIL-STD-794 - Parts and Equipment, Procedures for Packaging of.
MIL-STD-1474- Noise Limits for Army Materiel.

(Copies of specifications, and standards required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting activity).

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of the documents which are DoD adopted are those listed in the issue of the DoDISS specified in the solicitation. Unless otherwise specified, the issue of documents not listed in the DoDISS are the issue of the nongovernment documents which are current on the date of the solicitation.

AMERICAN NATIONAL STANDARDS INSTITUTE (ANSI)

ANSI C73.11 - Electric Plugs and Receptacles - General Purpose, 125 Volts, 15 Amperes, 2 Pole, 3 Wire, Grounding Type.

(Application for copies should be addressed to the American National Standards Institute, 1430 Broadway, New York, NY 10018).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.

UNDERWRITER'S LABORATORIES, INC. (UL)

UL 1262 - Standard for Laboratory Equipment.

(Application for copies should be addressed to the Underwriter's Laboratories, Inc., 207 East Ohio Street, Chicago, IL 60611; 333 Pfingsten Road, Northbrook, IL 60062; 1285 Walt Whitman Road, Melville, L.I., NY 11746; 1655 Scott Boulevard, Santa Clara, CA 95050).

(Nongovernment standards and other publications are normally available from the organizations which prepare or which distribute the documents. These documents also may be available in or through libraries or other informational services).

2.3 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification takes precedence. Nothing in this specification, however, supersedes applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 Fire and casualty hazards.

3.1.1 Proof of compliance. The contractor shall provide proof, to the procurement contracting officer, not less than thirty days prior to delivery, that the items to be delivered under the contract conform to the applicable requirements of Underwriter's Laboratories, Inc. (UL) Standard of Safety 1262. A copy of the test report shall be made available to the Government inspection personnel for their use in determining that the units being submitted for acceptance are identical to the unit submitted for approval. Proof shall consist of one of the following:

a. UL listing and UL label affixed to the product, provided the contractor agrees to have Underwriters' Laboratories, Inc. forward a copy of the UL report directly to the contracting officer, and the Government inspection personnel, upon request.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.

b. A label or equivalent means of identification affixed to the product as evidence that the product design has been examined and tested for design safety compliance by a nationally recognized independent laboratory. If an independent laboratory is used, it must be adequately equipped and competent to determine compliance with UL standards. The Government reserves the right to require a facilities report and to conduct a facilities survey. In support of the label/product identification, the independent testing laboratory shall provide surveillance over the product manufacturing system to the degree necessary to insure that production units are manufactured in the same manner and with the same type of components as the test sample evaluated and upon which the validity of the product identification is based. The testing laboratory shall develop a detailed test report which includes a conclusion as to whether the test sample evaluated is "approved" or "not approved" as complying with all requirements of the standards of safety.

3.2 Materials. Materials shall conform to the applicable specifications, standards, and requirements specified. Materials not specifically designated shall be of high commercial quality throughout, and shall be entirely suitable for the intended purpose.

3.3 Type I, Model Trimmer, Complete. The Type I, model trimmer shall be furnished complete with accessories and one grinding wheel, as specified herein. The model trimmer shall be a heavy duty, electrically-operated model trimmer suitable for trimming stone and plaster models in the dental laboratory (see figure 1). The trimmer shall essentially consist of a motor driven grinding wheel with an aluminum back-up plate and a water spray system for wetting the grinding wheel and removing debris from the grinding wheel during operation. The trimmer shall have a grinding wheel housing with an opening suitably located for grinding operations (see 3.4.4). The trimmer shall be equipped with a slotted or perforated, removable aluminum work tray.

3.3.1 Type II, Wheel, Abrasive, Silicon Carbide. This type II wheel shall be a replacement wheel (see 3.4.6).

3.4 Construction.

3.4.1 Dimensions. The model trimmer shall have the overall dimensions: height, 14 ± 4 inches; width, 13-1/2 ± 3 inches; depth (including work tray), 16-1/2 ± 1 inches.

3.4.2 Motor. The motor shall be dynamically balanced, 1/3 horsepower, 1725 revolutions per minute, single phase, 115 volts, 60 Hertz, capacitor start or split phase. The motor shall be equipped with a heavy duty electric power cable assembly and a suitable power switch for energizing and de-energizing the motor.

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:57Z
Check the source to verify that this is the currentversion before use.

3.4.2.1 Power cable. The power cable assembly shall be a 3-conductor power cord not less than 5 feet long equipped with a 3-prong plug suitable for use with receptacles specified in ANSI Standard C73.11 for caps and receptacles, 115 volts, 15 ampere, 2 pole, 3 wire grounding type.

3.4.3 Motor support. The motor support shall be an integral part of the grinding wheel housing, or as an alternate, may be bolted to the housing. The design and construction of the motor support shall be suitable for the intended purpose. The support shall provide a firm foundation for the motor. The motor support shall be cast aluminum, cast iron or fabricated from sheet steel. The motor support shall be so constructed to provide a rearward tilt of from 0° to 6°, at the top of the grinding wheel, when mounted to the shaft of the motor.

3.4.4 Grinding wheel housing. The grinding wheel housing shall be constructed in two pieces, of cast aluminum, with the front housing hinged for easy access to the grinding wheel. As an alternate to hinges, front housing shall be removable with thumb screws. The front and rear housing shall be sufficiently sealed with a rubber gasket to provide a water tight housing when closed and ready for use. There shall be a sufficient number of screw-type fasteners, of the hand operated type, to maintain the proper gasket contact for watertightness. The front wheel housing shall have an opening with the following dimensions when the work tray is in the horizontal position: height above work tray 5 $\pm$ 1 inches, width at work tray surface 4 $\pm$ 1 inches. The opening and work tray position shall be located with respect to the grinding wheel such that the grinding force of the rotating wheel against the stone or plaster model during trimming shall be in a vertical downward direction to preclude horizontal motion of the model. The work tray shall be cast aluminum, adjustable, and have the following dimensions: 5 $\pm$ 1/2 inches wide by 4-3/4, +1/2, -1-1/2 inches deep and a minimum thickness of 5/32 inch. The work tray shall be provided with holes or slots. Beneath the work tray shall be a drip tray which empties into a waste reservoir at the bottom of the grinding wheel housing.

3.4.5 Water wheel spray system. The trimmer shall be provided with a spray system for wetting the grinding wheel and washing away grinding debris. The spray system shall be so designed that the water spreads evenly over the full radius of the grinding wheel. The grinding wheel housing shall be equipped with a water inlet fitting and a drain hose connection or drain pipe for carrying away grinding debris. The drain outlet shall have a minimum inside diameter of 3/4 inch. The trimmer shall be supplied with a full complement of accessories for connecting trimmer to water supply (see 3.4.5.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.

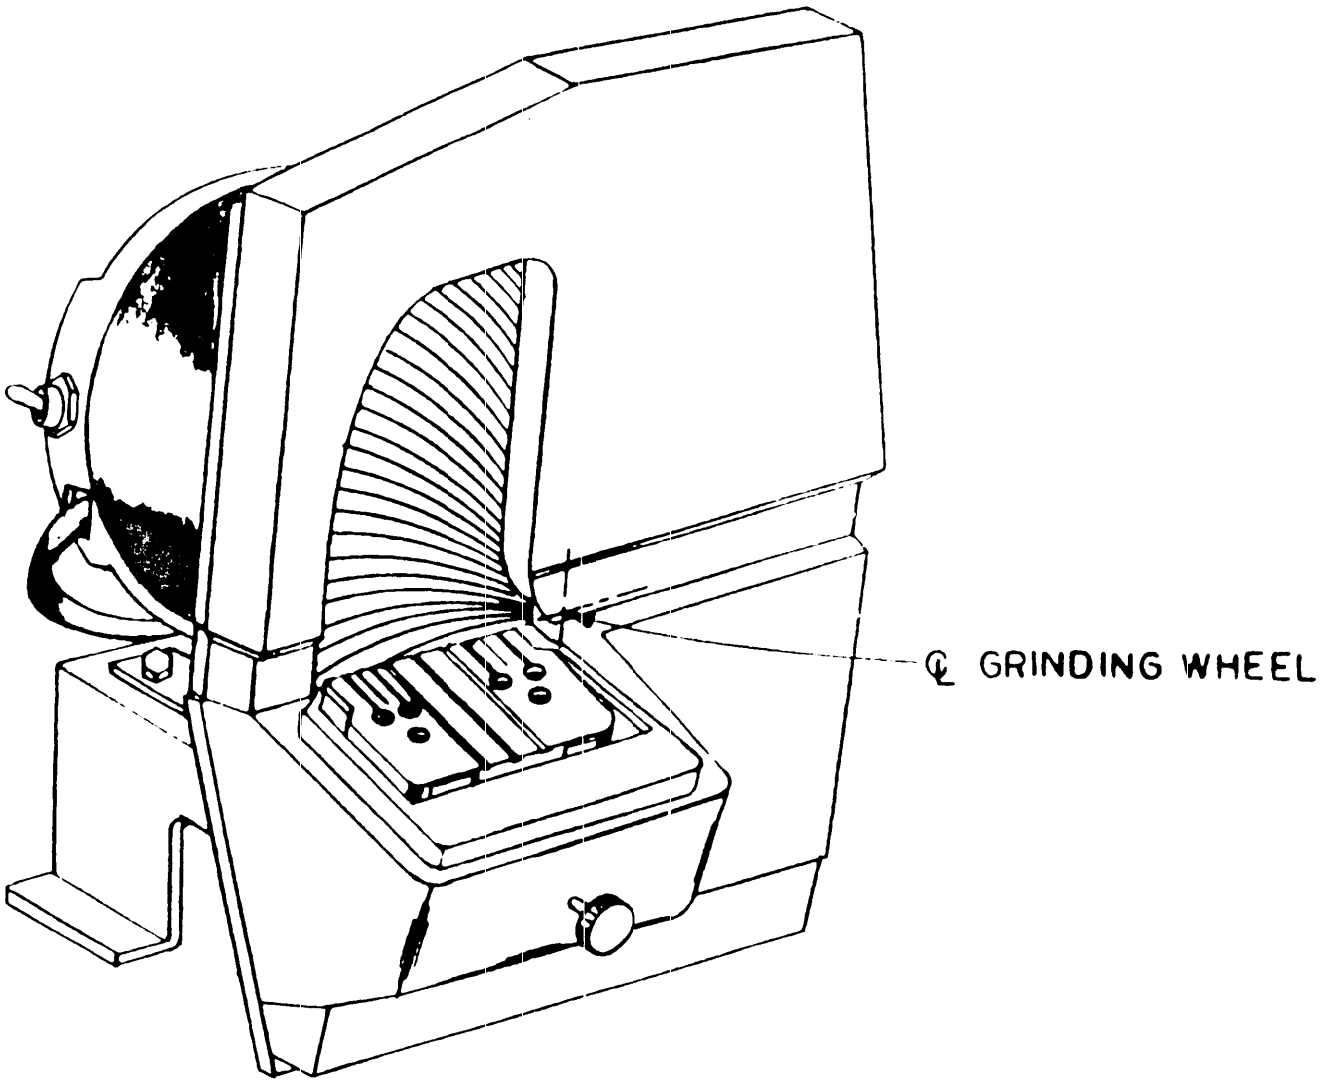


FIGURE 1. Trimmer, Dental Model.

NOTE: The trimmer shown is typical in style and design and is not intended to restrict or preclude the purchase of trimmers which are otherwise in accordance with the requirements of this document.

Source: https://assist.dla.mil -- Downloaded: 2026-02-21T10:57Z
Check the source to verify that this is the current version before use.

3.4.5.1 Accessories. The following accessories shall be supplied with the trimmer: water inlet tube having a minimum length of 4 feet, a faucet adapter for attaching water inlet tube to unthreaded faucets, a flexible rubber or vinyl translucent plastic hose having a minimum length of 2-1/2 feet suitable for attaching to the drain pipe or drain fitting, a tap-in-tap connector and shut off valve with a minimum of 4 feet of suitable copper tubing for permanent connection to water pipe. All fittings, tubes and hoses shall properly fit and function with their intended mating components. Any necessary tools required to change the grinding wheel shall be supplied.

3.4.6 Grinding wheel. The grinding wheel shall be connected directly to the shaft of the motor. The grinding wheel shall be a reversible, medium grain size, silicon carbide, resinoid bond abrasive wheel. The grinding wheel shall be 10 plus 1/8, minus 1/16 inches in diameter and 1/4 plus 1/64, minus zero thick with a 1 inch bore. The tolerance of the bore shall be plus .002 to plus .005 inch. The grinding surfaces on both sides of the wheel shall have spiral grooves to prevent excessive loading. The molded spirals shall run in a counterclockwise direction away from the center; as viewed from either side of wheel. There shall be 12 spirals to the inch at the periphery. Grit size shall be 46. Degree of hardness and abrasive grain spacing shall be such as to assure rapid, efficient trimming of dental models. An aluminum back up plate shall be provided to support the grinding wheel when in operation. Maximum runout on face and sides of wheel shall be plus or minus .010 inch. Sides shall not be concave by more than .010 inch. Each wheel shall be statically balanced to 1 gram or less. Each wheel shall be marked as specified in 3.8 herein.

3.4.7 Mounting provisions. The trimmer shall be provided with a minimum of four mounting holes. The holes shall be of sufficient size to accept a minimum bolt diameter of 1/4 inch. As an alternate the trimmer shall be provided with four rubber caster cups suitable for use under the base to prevent slipping.

3.4.8 Finish. All surfaces of the trimmer, inside and outside, with the exception of the motor, water spray system, shaft coupling and grinding wheel, shall be painted with durable enamel using the best commercial painting process. The color shall be the manufacturer's commercial color.

3.5 Acoustical Noise. The trimmer shall meet the noise limits of MIL-STD-1474, Category D (85 dBA at the operator position). Noise levels of 85 dBA or above shall constitute failure of the test.

Source: https://assist.dla.mil -- Downloaded: 20260-21T10:57Z
Check the source to verify that this is the current version before use.

3.6 Machining and welding. All bolt and rivet holes shall be accurately punched or drilled and shall have all burs and sharp edges removed. All welds shall be sound, smooth, and free from pits, undercuts, holes or fissures. All welds shall be thoroughly fused. Welded joints exposed to the outside surface shall be ground smooth.

3.7 Performance test. The model trimmer shall have efficient water distribution to wash away dust and keep the grinding wheel clean. The trimmer shall cleanly and satisfactorily trim dental models without chipping, creating dust in the atmosphere or water splashing, leakage around grinding wheel, or vibration of grindinng wheel, when tested as specified in 4.4.1.

3.8 Identification marking. Each unit shall be identified with the name or registered trademark of the manufacturer, model designation, serial number, stock number, and contract or purchase order number, horsepower, number of phases, current, voltage, speed, and cycles. Markings shall be provided on one or two readily visible nameplates, permanently affixed. The markings on the plates shall be legible and permanent and shall be accomplished by the stamping. Each wheel shall be marked in a legible manner with the manufacturer's name or trademark, diameter, thickness, bore, grain (grit) size and maximum operating speed.

3.9. Service data. The contractor shall furnish two copies of a technical manual which contains complete instructions for installation, operation, maintenance, and list of component parts. Wiring diagrams shall be included for electrical items or components. The manual shall comply with the requirements of the MIL-M-7298. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer via the cognizant Government inspector, two preliminary copies of his proposed technical manual for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract, or purchase order, In addition, the Contractor shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of contract and propose to furnish manuals identical with those previously accepted, then the requirements for the review of drafts and submission of 15 additional copies shall be at the option of the Government.

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:57Z
Check the source to verify that this is the currentversion before use.

3.10 Workmanship. The model trimmer and replacement wheel shall be free from defects which detract from their appearance or impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component/materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government, and provided also that the test methods and the results obtained comply with those described in the specification. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in table I. The unit of product for examination purposes shall be one trimmer and one wheel, as applicable.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.

TABLE I. Sampling for examination.

Type defect	Inspection level	AQL (percent defective)
Major	II	2.5
Minor	II	4.0

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table II. The unit of product for examination purposes shall be one trimmer and one wheel, as applicable.

TABLE II. Sampling for tests.

Component	Characteristic	Requirements	Test Procedure	Inspection level	AQL
Trimmer	Performance test	3.7	4.4.1	100%	1/
Trimmer	Noise test 2/	3.5	4.4.2	One trimmer	1/

1/ Acceptance number shall be zero.

2/ In lieu of testing, the contractor shall submit proof, prior to delivery, that the trimmers to be delivered under the contract meet the noise limits specified herein when tested as specified herein. Proof of compliance shall be in accordance with 3.1.1, as applicable.

4.3 Examination. The trimmer and wheel shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in table I and III.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.

TABLE III. Classification of defects.

Categories	Defects
Major	
101	Model Trimmer not furnished complete.
102	Trimmer not free of sharp edges.
103	Welds not free of cracks and porosity.
104	Screws and bolts not secured.
105	Front housing cannot be closed securely.
106	Dimensions of grinding wheel not as specified.
Minor	
201	Metal surface of trimmer not free of pits and burs.
202	Metal surface not free of dents, cracks and scratches.
203	External welds not smoothly ground.
204	Identification marking not present, complete, correct, legible, and permanent.
205	Dimensions of trimmer not as specified.

4.4 Test. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Performance test. The trimmer shall be set up on a suitable bench top location with water supply hose and drain hose connected for operation. Connect electric plug to 115 volt, 60 Hz receptacle. Turn on water faucet to a slight opening. Turn on trimmer. Using a piece of plaster of approximate size of a model to be trimmed, proceed to grind the plaster for 2 to 3 minutes. After grinding operation, allow water and motor to remain operating for 15 seconds to wash away plaster sludge. Inspect for water leakage around grinding wheel housing gasket. There shall be no leakage. Inspect for vibration. There shall be no vibration with grinding wheel in operation. Turn off water supply and electric power. Open front housing cover and inspect grinding wheel for clogging by plaster. There shall be no clogging of the grinding wheel. Excessive plaster sludge shall have been washed from the reservoir.

4.4.2 Acoustical Noise Test. The trimmer shall be tested for steady-state noise in accordance with test requirements of MIL-STD-1474

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.

4.5 Inspection of packaging. The sampling and inspection of the preservation and interior package marking shall be in accordance with groups A and B quality conformance inspection requirements of MIL-P-116. The sampling and inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

5. PACKAGING

5.1 Preservation. Preservation shall be level A or C, as specified (see 6.1).

5.1.1 Level A.

5.1.1.1 Unit package.

5.1.1.1.1 Type I, model trimmer complete. Each model trimmer along with accessories shall be clean, dry and packaged in accordance with MIL-P-116, method III.

5.1.1.1.2 Type II, abrasive wheel. Each abrasive wheel shall be clean, dry and packaged in accordance with MIL-P-116, method III.

5.1.1.2 Intermediate package.

5.1.1.2.1 Type I, model trimmer complete. An intermediate package shall not be required for complete model trimmer.

5.1.1.2.2 Type II, abrasive wheel. Twelve unit packages containing abrasive wheels shall be packaged in a box conforming to PPP-B-566, PPP-B-636, class domestic or PPP-B-676. Closure shall be as specified in the applicable box specification.

5.1.2 Level C. The level C preservation for type I model trimmer on type II abrasive wheel shall conform to the MIL-STD-794 requirements for this level.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.1).

5.2.1 Level A.

5.2.1.1 Type I, model trimmer complete. Each model trimmer packaged as specified in 5.1.1.1.1 shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, overseas type or PPP-B-621, class 2. The trimmer shall be adequately blocked, braced and cushioned within the container to prevent shifting or damage. Closure and strapping shall be as specified in the applicable box specification.

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:57Z
Check the source to verify that this is the currentversion before use.

5.2.1.2 Type II, abrasive wheel. Twenty-four intermediate packages containing abrasive wheels shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, overseas type or PPP-B-621, class 2. Closure shall be as specified in the applicable box specification.

5.2.1.2.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall be as specified in the liner specification, case liner shall not be required for fiberboard boxes.

5.2.2 Level B.

5.2.2.1 Type I, model trimmer complete. Each model trimmer packaged as specified in 5.1.1.1.1 shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, domestic type, PPP-B-621, class 1 or PPP-B-636, class domestic. The trimmer shall be adequately blocked, braced and cushioned within the container to prevent shifting or damage. Closure shall be as specified in the applicable box specification.

5.2.2.2 Type II, abrasive wheel. Twenty-four intermediate packages shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, domestic type, PPP-B-621, class 2 or PPP-B-636, class domestic. Closure shall be as specified in the applicable box specification.

5.2.3 Level C. The level C packing for type 1 model trimmers or type II abrasive wheels shall conform to the MIL-STD-794 requirements for this level.

5.2.4 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.2.5 Unitized loads. Unitized loads, commensurate with the level of packing specified in the contract or order, shall be used whenever total quantities for shipment to one destination exceed 250 pounds or 20 cubic feet. Loads shall be unitized on pallets conforming to MIL-STD-147. Quantities less than 20 cubic feet need not be unitized. Pallet loads including the pallet shall not exceed 54 inches in height, 48 inches in width, and 40 inches in length. Pallet shall conform to Type IV or Type V.

5.2.5.1 Level A and B. Type I model trimmers or Type II abrasive wheels packed as specified in 5.2.1 and 5.2.2 shall be unitized on pallets conforming to MIL-STD-147.

5.2.5.2 Level C. Type I model trimmers or Type II abrasive wheels packed as specified in 5.2.3 shall be unitized as specified in 5.2.5.

Source: https://assist.dla.mil -- Downloaded: 20260-21T10:57Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Level A, B, and C. Each unit pack, intermediate package, exterior container and unitized load shall be marked as specified in MIL-STD-129.

5.4 General.

5.4.1 Exterior container. Exterior container (see 5.2.1, 5.2.2, and 5.2.3) shall be of minimum tare and cube consistent with the protection required and shall contain equal quantities of identical stock numbered items to the greatest extent practicable.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.5.

6. NOTES

6.1 Intended use. The model trimmer covered by this specification is intended for trimming stone and plaster models in the dental laboratory.

6.2 Ordering data.

6.2.1 Acquisition requirements. Acquisition documents should specify the following:

(a) Title, number and date of this specification.
(b) Type required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(d) National Stock Number (NSN).

6.3 National Stock Number (NSN) coverage. This specification covers the following items appearing in the Federal Supply Catalog:

Stock Number	Item Identification
6520-00-564-4050	TRIMMER, DENTAL MODEL, 115V, 60 Hz
6520-00-564-4055	WHEEL, ABRASIVE, SILICON CARBIDE

6.4 Supersession data. This specification includes the requirements of MIL-T-37538 dated 1 September 1976, TRIMMER, DENTAL MODEL and MIL-W-37013 dated 1 April 1974, WHEEL, ABRASIVE, SILICON CARBIDE, DENTAL MODEL TRIMMING.

Source: https://assist.dla.mil -- Downloaded: 2026l0-21T10:57Z
Check the source to verify that this is the currentversion before use.

6.5 Subject term (key word) listing

Trimmer
Model
Wheel

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing activity:

DoD-MB

Agent

DLA-DM

Review Activities:
Army - MD
Navy - MS
Air Force - 03

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6520-1846

48201

Location: NCR, MIL-S-37538A

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-ATTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:57Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
MIL-T-37538A	TRIMMER, DENTAL MODEL, WHEEL, ABRASIVE.

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:57Z
Check the source to verify that this is the current version before use.