MILITARY SPECIFICATION

LABORATORY, PETROLEUM, SEMITRAILER MOUNTED

This military specification has been prepared by the US Army Belvoir Research, Development and Engineering Center based upon currently available technical information but it has not been approved for promulgation as a coordinated revision of MIL-L-51050. It is subject to modification. However, pending its promulgation as a coordinated military specification, it may be used in acquisition.

1. SCOPE

1.1 Scope. This specification covers a mobile petroleum laboratory, fully equipped with testing equipment, chemicals, and supplies, to test petroleum and associated products.

2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications and standards. The following specifications and standards form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of these documents shall be those listed in the issue of the Department of Defense Index of Specifications and Standards (DoDISS) and supplement thereto, cited in the solicitation.

SPECIFICATIONS

FEDERAL

TT-P-664	- Primer Coating, Synthetic, Rust-Inhibiting, Lacquer-Resisting.
PPP-T-60	- Tape: Packaging, Waterproof.

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: USA Belvoir Research, Development, and Engineering Center, ATTN: STRBE-TSE, Fort Belvoir, VA 22060-5606 by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

AMSC N/A FSC 6640
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

PPP-B-1055	- Barrier Material, Waterproof, Flexible.
PPP-C-1752	- Cushioning Material, Packaging, Unicellular Polyethylene Foam, Flexible.

MILITARY

MIL-P-116	- Preservation, Methods of.
MIL-V-173	- Varnish, Moisture- and-Fungus-Resistant (for Treatment of Communications, Electronic, and Associated Equipment).
MIL-P-514	- Plates, Identification, Instruction and Marking, Blank.
MIL-T-704	- Treatment and Painting of Materiel.
MIL-B-7883	- Brazing of Steels, Copper, Copper Alloys, Nickel Alloys, Aluminum and Aluminum Alloys.
MIL-C-46168	- Coating, Aliphatic Polyurethane, Chemical Agent Resistant.
MIL-C-53039	- Coating, Alphatic Polyurethane, Single, Component, Chemical Agent Resistant.

STANDARDS

MILITARY

MIL-STD-101	- Color Code for Pipelines and for Compressed Gas Cylinders.
MIL-STD-129	- Marking for Shipment and Storage.
MIL-STD-130	- Identification Marking of U.S. Military Property.
MIL-STD-281	- Automobiles, Trucks, Truck-Tractors, Trailers and Trailer Dollies; Preservation and Packaging of.
MIL-STD-889	- Dissimilar Metals.

FEDERAL

FED-STD-H28	- Screw-Thread Standards for Federal Services.
FED-STD-313	- Material Safety Data Sheet, Preparation and Submission of.

2.1.2 Other Government documents, drawings, and publications. The following other Government documents, drawings, and publications form a part of this specification to the extent specified herein. Unless otherwise specified, the issues shall be those in effect on the date of the solicitation.

DRAWING

ME

TA13226E6500	- Laboratory, Petroleum, Semitrailer Mounted.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

SUPPLY CATOLOG

SC 6640-97-CL-E02 - Components List, Mobile Petroleum Laboratory.

DEPARTMENT OF TRANSPORTATION (DOT)

49 CFR 171 - Hazardous Materials Regulations.
49 CFR 172 - Hazardous Materials Tables and Hazardous Materials Communication Regulations.

Motor Carrier Safety Regulations

(Application for copies should be addressed to the Superintendent of Documents, Government Printing Office, Washington, DC 20402.)

(Copies of specifications, standards, drawings, publications, and other Government documents required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting activity.)

2.2 Other publications. The following document(s) form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of the documents which are DOD adopted shall be those listed in the issue of the DoDISS specified in the solicitation. Unless otherwise specified, the issues of documents not listed in the DoDISS shall be the issue of the non-Government documents which is current on the date of the solicitation.

AMERICAN WELDING SOCIETY (AWS)

AWS D1.1 Structural Welding Code - Steel.
AWS D1.2 Structural Welding Code - Aluminum.

(Application for copies should be addressed to the American Welding Society, 55 N.W. LeJeune Rd., Miami, FL 33126.)

AMERICAN SOCIETY OF MECHANICAL ENGINEERS (ASME)

ASME Boiler and Pressure Vessel Code, section IX, Welding Qualification.

(Application for copies should be addressed to the American Society of Mechanical Engineers, 345 East 47th Street, New York, NY 10017.)

ASSOCIATION OF AMERICAN RAILROADS (AAR)

AAR Manual, Section 1 - Loading of Commodities of Open Top Cars.
AAR Rules, Section 6 - Loading of Department of Defense Material on Open Top Cars.

(Application for copies should be addressed to the Association fo American Railroads, 59 East Van Buren Street, Chicago, IL 60605.)

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

NATIONAL FIRE PROTECTION ASSOCIATION (NFPA)

National Electrical Code

(Application for copies should be addressed to the National Fire Protection Association, 60 Batterymarch Street, Boston MA 02110.)

SOCIETY OF AUTOMOTIVE ENGINEERS

SAE Handbook

(Application for copies should be addressed to the Society of Automotive Engineers, Two Pennsylvania Plaza, New York, NY 10001.)

(Non-Government standards and other publications are normally available from the organizations which prepare or which distribute the documents. These documents also may be available in or through libraries or other informational services.)

2.3 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification shall take precedence. Nothing in this specification, however, shall supersede applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 Description. The semitrailer mounted petroleum laboratory (hereinafter called "mobile laboratory") shall be in accordance with Top Assembly TA13226E6500 and as specified herein.

3.1.1 Drawings. The drawings forming a part of this specification are end product drawings. No deviation from the prescribed dimensions or tolerances is permissible without prior approval of the contracting officer. Where tolerances could cumulatively result in incorrect fits, the contractor shall provide tolerances within those prescribed on the drawings to insure correct fit, assembly, and operation of the mobile laboratory. Any data (e.g. shop drawings, layouts, flow sheets, processing procedures, etc.) prepared by the contractor or obtained from a vendor to support fabrication and manufacture of the production item shall be made available, upon request, for inspection by the contracting officer or the designated representative.

3.2 First article. Unless otherwise specified (see 6.2), a sample shall be subjected to first article inspection (see 4.3 and 6.3). Any changes or deviations of mobile laboratories from the approved first article during production will be subject to the approval of the contracting officer. Approval of the first article will not relieve the contractor of his obligation to furnish mobile laboratories conforming to this specification.

3.3 Materials. Materials shall be as specified herein and on the drawings. Materials not specified shall be selected by the contractor and shall be subject to all provisions of this specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

3.3.1 Material deterioration prevention and control. The mobile laboratory shall be fabricated from compatible materials, inherently corrosion resistant or treated to provide protection against the various forms of corrosion and deterioration that may be encountered in any of the applicable operation and storage environment to which the mobile laboratory may be exposed.

3.3.2 Dissimilar metals. Dissimilar metals shall not be used in intimate contact with each other unless protected against galvanic corrosion. Dissimilar metals and methods of protection are defined and detailed in MIL-STD-889.

3.3.3 Identification of materials and finishes. The contractor shall identify the specific material, material finish or treatment for use with component and subcomponent, and shall make information available upon request to the contracting officer or designated representative.

3.3.4 Recovered materials. For the purpose of this requirement, recovered materials are those materials which have been collected from solid waste and reprocessed to become a source of raw materials, as distinguished from virgin raw materials. The components, pieces and parts incorporated in the mobile laboratory may be newly fabricated from recovered materials to the maximum extent practicable, provided the mobile laboratory produced meets all other requirements of this specification. Used, rebuilt or remanufactured components, pieces and parts shall not be incorporated in the mobile laboratory.

3.3.5 Cushion material. Cushion material for cabinets, drawers, and shelves shall conform to PPP-C-1752, type I, class 2 and type II, class 1.

3.3.5.1 Installation. The cushion material shall be installed in all cabinets, drawers, and on all cabinet shelves with cutouts to provide protection of stored equipment from impact and vibration damage. The material used may be one layer or more of the different types and classes of cushion material specified.

3.4 Semitrailer. The semitrailer shall be a Government furnished Model XM822E1, NSN 2330-01-162-0642 (see 3.20 and 6.5).

3.5 Components. Items of equipment shall be as specified in SC 6640-97-CL-E02. When specified (see 6.2), the items of equipment shall be furnished by the contractor and shall be located in the mobile laboratory as specified herein (see appendix A) and on the applicable drawings.

3.6 Performance. The mobile laboratory shall be capable of being towed by an M-52, 5-ton, 6 by 6 tractor and sustain over-the-road, across curbing and rough terrain travel. The fully equipped laboratory shall be air transportable in the C130, C141 and C5A USAF aircraft. Removal of dolly, semitrailer underpack boxes, and placement of semitrailer landing gear in a horizontal position is permissible for air transport of the mobile laboratory in C130 and C141 aircraft. Provisions shall be provided within the mobile laboratory to secure all equipment, supplies, chemicals, books, binders, and manuals. When towed or air transported as specified herein, no damage, dislocation, deformation, breakage, cracking, or leaking shall be evident.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

3.7 Utility systems. The mobile laboratory shall contain the following utility systems as specified on the applicable drawings and shall not leak when tested as specified in 4.5.2.5.

a. Water
b. Water drainage
c. Air
d. Vacuum
e. Oxygen
f. Nitrogen

3.8 Color code marking. All utility piping and valves shall have color code marking in accordance with MIL-STD-101.

3.9 Electrically operated utility and testing equipment and systems. Electrically operated utility and testing equipment and systems shall be as specified on the applicable drawings and shall operate as intended without malfunction or without evidence of binding or overheating.

3.10 Electrical wiring. All electrical wiring shall comply with the National Electrical Code (NEC) of the National Fire Protection Association.

3.10.1 Cords. All electrical cords shall be as short as practicable while allowing sufficient slack for repair. The cords shall be installed in such a manner as to insure safe conditions for conducting test with highly volatile materials.

3.10.2 Permanent wiring. Major components of electrical equipment shall be tied into the electrical system permanently and shall be equipped with "ON" and "OFF" switches as specified on applicable drawings.

3.10.3 Protection. Grommets shall be used to prevent chafing, rubbing, and abrading where wires or harnesses pass through any structural member. Cushioned straps shall be used to support wiring and harnesses. Maximum unsupported length shall be 36 inches.

3.11 Fungus and moisture resistance. The electrical circuitry, including all components and connections, except as specified below, shall be protected from the effects of fungus growth and moisture by an overall treatment with a varnish conforming to MIL-V-173, composition as specified (see 6.2).

a. Components or circuit elements that are inherently fungus and moisture resistant, or which are hermetically sealed need not be treated.
b. Components or circuit elements whose functions will be adversely affected by the varnish coating shall not be treated.

When used, the varnish shall be applied by spray, brush, or a combination of both to give a minimum dry-film thickness of 1 mil to component or element surfaces previously cleaned and prepared so that the surfaces are free from all foreign matter which would interfere with the adherence or function of the varnish.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

3.12 Threaded parts. All screw threads shall be in accordance with FED-STD-H28 and, unless otherwise specified (see 6.2), shall be class 2 fit.

3.13 Hazardous materials. The transportation of chemicals, compressed gasses and other hazardous materials shall comply with the Department of Transportation regulation 49 CFR 171-190 (see 6.4).

3.13.1 Safety data sheet. Material safety data sheets prepared in accordance with FED-STD-313 shall be furnished for all materials, including materials listed in SC 6640-97-CL-E02, which are identified as hazardous materials (see appendix A of FED-STD-313).

3.14 Fire extinguisher. Unless otherwise specified , the Government will furnish three fire extinguishers, 4210-01-087-4989 (see 3.20, 6.2 and 6.5). The mountings shall be as specified in the applicable drawings.

3.15 Identification marking. The mobile laboratory shall be identified in accordance with MIL-STD-130. The marking shall be applied to the mobile laboratory on plates conforming to MIL-P-514, type I, style 1, composition C, of type I, grade A, class 1 material. Plates shall be attached by screws, bolts, or rivets in a conspicuous protected location.

3.16 Shipping data plate. The shipping data plate shall conform to MIL-P-514, type III, composition C, or type I, grade A, class 1 material and, in addition, shall show the silhouette of the mobile laboratory in transport position indicating the center of gravity and the location and capacity of the lifting and the tiedown attachments. The plate shall be attached by screws, bolts, or rivets in a conspicuous protected location.

3.17 Instruction plates. Each mobile laboratory shall be equipped with instruction plates or diagrams, including warnings and cautions, describing any special or important procedures to be followed in assembling, operating, or servicing the mobile laboratory. Instruction plates shall conform to MIL-P-514, type III, composition C, of type I, grade A, class 1 material. Plates shall be attached by screws, bolts, or rivets in a conspicuous protected location.

3.18 Treatment and painting. The portions of the mobile laboratory painted as specified on the applicable drawings shall be cleaned, treated, and painted in accordance with MIL-T-704, type F or G as applicable. Unless otherwise specified (see 6.2), the mobile laboratory shall then be overcoated in accordance wiht Government furnished camouflage patterns with MIL-C-46168 or MIL-C-53039 top coat of the colors specified in the camouflage patterns (see 3.20).

3.19 Instructional material. Unless otherwise specified (see 6.2), reference books and commercial catalogs as specified in SC 6640-97-CL-E02 shall be furnished by the contractor and shall be included with each mobile laboratory, together with the technical literature, data sheets and certifications (as applicable) received by the contractor from manufacturers of the component items of equipment and supply.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

3.20 Government-furnished property. When specified, the following property in the quantities indicated will be furnished by the Government (see 6.5):

Item No.	Description	Identification	Qty
1.	Semitrailer, van, XM822E1	2230-00-162-0642	1
2.	Air conditioner	4120-01-089-4053	4
3.	Fire extinguisher	4210-01-087-4989	3
4.	Binders (3) containing current specifications, inspection information, special regulations and pertinent publications		1 set
5.	Binders, empty	7510-00-188-6951	3
6.	Books, record type	7530-00-222-3525	2
7.	FED, TEST METHOD STANDARDS for TESTING Petroleum.	FED-STD-791	1
8.	Manual, Air Conditioner Parts List	TM-5-4120-356-24P	1
9.	Manual, Air Conditioner Operation and Maintenance	TM-5-4120-356-14	1
10.	Manual, Aircraft Refueling	FM 10 - 68	1
11.	Manual, Petroleum Supply Point Equipment and Operations	FM 10 - 69	1
12.	Manual, Inspecting and Testing Petroleum Products	FM 10 - 70	1
13.	Manual, Operating and Maintenance, for the Laboratory, Petroleum, Semitrailer Mounted	TM-5-6640-212-14	1
14.	Supply Catalog, Laboratory Petroleum, Semitrailer Mounted	SC 6640-97-CL-E02	1
15.	Tool Kit General Mechanics	5180-00-177-7033	1
16.	Pattern Drawings	Camouflage	as required

3.21 Vehicle weight classification. The contractor shall complete the Government-furnished vehicle weight classification forms and supply the vehicle weight classification number(s) to the mobile laboratory as specified (see 6.7).

3.22 Workmanship.

3.22.1 Metal fabrication. Metal used in fabrication shall be free from kinks and sharp bends. The straightening of material shall be done by methods that will not cause injury to the material. Corners shall be square and true. Flame cutting, using tips suitable for the thickness of the steel, may be employed for steel instead of shearing and sawing. Plasma cutting may be used only on non-heat treatable aluminum alloys. The plasma must be machined to remove the heat effected zone. All bends shall be made with controlled means to insure uniformity of size and shape. Precaution shall be taken to avoid overheating. Heated steel shall be allowed to cool slowly. External surfaces shall be free of burrs, sharp edges and corners, except when sharp edges or corners are required or where they are not detrimental to safety.

3.22.2 Welding. The surfaces of parts to be welded shall be free from rust, oxides, scale, paint, grease, mill scale that can be removed by chipping and wire brushing, and other foreign matter. Welds shall transmit stress without permanent deformation or failure when the parts connected by the welds are

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

subjected to proof and service loading. Parent materials, weld filler metals, and fabrication techniques shall be as required to enable the mobile laboratory to conform to the examination and test requirements specified in section 4. Unless otherwise specified (see 6.2), the welding process used in fabrication of the mobile laboratory shall be at the option of the contractor.

3.22.3 Welders. Before assigning any welder or welding operator work covered by this specification, the contractor shall obtain certification that the welder or welding operator has passed qualification tests as prescribed by either of the following listed codes for the type of welding operations to be performed by that welder or welding operator and that such qualification is effective as defined by the particular code:

AWS D1.1 - Structural Welding Code - Steel
AWS D1.2 - Structural Welding COde - Aluminum
ASME - Boiler and Pressure Vessel Code, Section IX, Welding Qualification

The certification shall be made available for review by the contracting officer or designated representative. Contractors who only make horizontal welds need not qualify welders for "all position welding". The Government may require the recertification of any welder or welding operator.

3.22.4 Welding practices.

a. Preheat of materials being welded and maximum interpass temperatures during welding shall be in accordance with the supplier's recommendations.
b. Tack welds shall be subject to the same quality requirements as final welds.
c. Work shall be positioned for flat welding whenever practicable.
d. Procedures and sequences shall be such that distortion and shrinkage will be held to a minimum. When straightening is required, caution shall be exercised to insure that the straightening process does not weaken the part and the mobile laboratory.

3.22.5 Welding quality.

a. The contractor shall be responsible for performing the inspections needed to insure that when the welded parts are assembled together to make the mobile laboratory, the mobile laboratory shall conform to the inspection requirements specified in section 4.
b. All weldments shall be free of slag, flux, weld spatter, and other impurities detrimental to both the appearance and strength of the weldment.
c. Undercut in weldments shall be held to a minimum but shall not be more than 1/32 inch deep or 5 percent of the thickness of the thinner material being welded, whichever is less.
d. Welds shall be free from all cracks in adjacent base metal and weld metal, and from discontinuities such as lack of fusion with base metal or between weld passes, in complete penetration or lack of prescribed fit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

e. The weld quality shall be in accordance with AWS D1.2 or AWS D1.2 as appropriate.

3.22.6 Brazing. Brazing of steels, copper alloys and nickel alloys shall conform to MIL-B-7883.

3.22.7 Bolted connections. Boltholes shall be accurately formed and shall have burrs removed. Washers or lockwashers shall be provided where necessary. Matching thread areas securing bolts conforming to SAE J429 or capscrews shall be of sufficient strength to withstand the tensile strength of the bolt. All fasteners shall be correctly torqued and shall have full thread engagement.

3.22.8 Riveted connections. Rivets shall fill the holes completely. The upset rivet heads shall be full, neatly made, concentric with the rivet holes, and in full contact with the surface of the member and shall be in accordance with SAE J492.

3.22.9 Machine work. Tolerances and gages for metal fits shall conform to the limits specified herein and on applicable drawings and to the standards of the industry.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Responsibility for compliance. All items must meet all requirements of sections 3 and 5. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in the specification shall not relieve the contractor of the responsibility of assuring that all products or supplies submitted to the Government for acceptance comply with all requirements of the contract. Sampling in quality conformance does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to acceptance of defective material.

4.2 Classification of inspection. Inspection shall be classified as follows;

a. First article inspection (see 4.3).
b. Quality conformance inspection (see 4.4).
c. Inspection of packaging (see 4.6).

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

4.3 First article inspection.

4.3.1 Examination. The first article mobile laboratory shall be examined for the defects marke "X" in columns 1 and 2 of table I. Presence of one or more defects shall be cause for rejection.

4.3.2 Tests. The first article mobile laboratory shall be tested as specified in 4.5.2.1 through 4.5.2.6. Failure of any test shall be cause for rejection.

4.4 Quality conformance inspection.

4.4.1 Examination. Each mobile laboratory shall be examined for the defects marked "X" in column 3 of table I. Presence of one or more defects shall be cause for rejection.

4.4.2 Tests. Each mobile laboratory shall be tested as specified in 4.5.2.1 through 4.5.2.3 and 4.5.2.5 through 4.5.2.6. Failure of any test shall be cause for rejection.

4.5 Inspection schedule.

4.5.1 Examination. Examination shall be in accordance with table I.

TABLE I. Examination schedule.

First article		Quality conformance	Defect
Pre-test	Post-test 1/		
1	2	3	4
X	X	X	101. Assembly incomplete for incorrect.
X	-	-	102. Design detail not as specified.
X	-	-	103. Material not as specified.
X	-	-	104. Materials not resistant to corrosion and deterioration or treated to be made resistant to corrosion and deterioration.
X	-	-	105. Dissimilar metals not in accordance with MIL-STD-889.
X	-	-	106. Material and material finish or treatment information not available.
X	-	-	107. Used, rebuilt or remanufactured components, pieces, or parts incorporated in the mobile laboratory.
X	X	X	108. Parts and components missing or not as specified.
X	-	-	109. Dimensions not as specified.
X	X	X	110. Cabinets not as specified.
X	X	X	111. Drawers not as specified.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

TABLE I. Examination schedule. (cont'd)

First article		Quality conformance	Defect	
Pre-test	Post-test[1/]			
1	2	3	4	
X	-	X	112.	Cushion material not as specified.
X	X	X	113.	Cushion material not installed as specified.
X	X	X	114.	Locking devices not as specified.
X	X	X	115.	Cabinet drawers and doors identification not as specified.
X	X	X	116.	Utility systems not as specified.
X	X	X	117.	Piping not as specified.
X	X	X	118.	Piping color code marking not as specified.
X	X	X	119.	Electrically operated utility and testing equipments not as specified.
X	-	X	120.	Shock sensitive laboratory testing equipment and vibration equipment not installed as specified.
X	X	X	121.	Electrical wiring not as specified.
X	-	X	122.	Electrical circuitry, including all components and connections, not fungus and moisture resistant as specified.
X	-	X	123.	Threaded parts not as specified.
X	-	X	124.	Explosive chemicals, compressed gasses, and other dangerous articles not installed as specified.
X	X	X	125.	Fire extinguishers missing or not mounted as specified.
X	-	X	126.	Identification marking and indentification plates not as specified.
X	-	X	127.	Shipping data plate not as specified.
X	-	X	128.	Instruction plates not as specified.
X	-	X	129.	Treatment and painting not as specified.
X	-	X	130.	Camouflage patterns not as specified.
X	X	X	131.	Technical publications and instructional material missing or not as specified.
X	-	X	132.	Vehicle weight classification missing or not as specified.
X	X	X	133.	Workmanship not as specified.
X	X	X	134.	Metal fabrication not as specified.
X	X	X	135.	Welding not as specified.
X	X	X	136.	Welders not certified as specified.
X	X	X	137.	Welding practices not as specified.
X	X	X	138.	Weld quality not as specified.
X	X	X	139.	Brazing not as specified.
X	X	X	140.	Bolted connections not as specified.
X	X	X	141.	Riveted connections not as specified.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the currentversion before use.

TABLE I. Examination schedule. (cont'd)

First article		Quality conformance	Defect
Pre-test	Post-test 1/		
1	2	3	4
X	X	X	142. Machine work not as specified.
X	X	X	143. Material Safety Data Sheet not as specified.

1/ Post test examination conducted to insure that components, parts, and assemblies were not damaged, broken or lost during testing.

4.5.2 Tests.

4.5.2.1 Test conditions. Test shall be performed with shelter and at the climatic conditions existing at the place of test. The mobile laboratory shall operate as specified herein without maintenance other than the contractor's recommended normal scheduled maintenance as established by a maintenance schedule prepared and submitted by the contractor prior to test.

4.5.2.2 Road. The mobile laboratory with all equipment, furnishing and supplies installed, shall be coupled with a government-loaned M-52 tractor truck, NSN 2320-00-835-8326, and towed over a hard surface road for a minimum of 20 miles at a speed of 50 miles per hour. A circular test track shall not be used for this test. Nonconformance to 3.6 shall constitute failure of this test.

4.5.2.3 Across curbing. The fully loaded and equipped mobile laboratory shall be towed by the M-52 tractor over a section of concrete, asphalt, or solid wood curbing at not less than 5 miles per hour. The dimensions of the curbing shall be 6 inches ±1/2 inch high by 6 inches ±1/2 inch wide. The top corners of the curbing coming into contact with the wheels of the M-52 tractor and the mobile laboratory shall be rounded to a 1 inch ± 1/8 inch radius. The curbing shall be anchored to a hard surfaced road and shall be stationary during the test. The full height of the curbing shall protrude above the surface to the road. All wheels of the M-52 tractor and mobile laboratory shall pass over the curbing at a 45 degree ±5 degree angle to the centerline of the curbing with the road side of the M-52 tractor and mobile laboratory. This test shall be repeated passing all wheels of the M-52 tractor and mobile laboratory over the curbing at a 45 degree, ±5 degree angle to the centerline of the curbing with the curb side of the M-52 tractor and mobile laboratory. Nonconformance to 3.6 shall constitute failure of this test.

4.5.2.4 Simulated aircraft loading. The simulated aircraft loading test shall be performed on the mobile laboratory with all equipment, furnishings and supplies. Nonconformance to 3.6 shall constitute failure of this test.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

4.5.2.5 Pressure testing of utility systems. The mobile laboratory systems shall be pressure tested as indicated:

System	Pressure	Medium	Duration*	Examination
Water	45 psig	Water	30	Visual
Drainage	Gravity	Water	10	Visual
Air	60 psig	Air	20	Soap solution
Vacuum	0.5 mm Hg	Negative Pressure	15	Manometer
Oxygen	Normal system pressure	Oxygen	20	Soap solution
Nitrogen	Normal system pressure	Nitrogen	20	Soap solution

*Not less than time indicated in minutes.

The above testing and examination shall be conducted for a total of two times. After first test, the pressures shall be allowed to return to ambient before pressurizing for the second time. Any evidence of leakage shall constitute failure of this test.

4.5.2.6 Functional testing of electrically operated systems and equipment. The electrically operated equipment and electrical systems shall be electrically energized and operated in accordance with the laboratory technical manual.

a. Time delay purging system.
b. Lighting blackout system.
c. Utility equipment.
d. Testing equipment.
e. 24 volt electrical system.
f. 120/208-volt electrical system.

Nonconformance to 3.9 shall constitute failure of this test.

4.6 Inspection of packaging. The packaging and marking of each mobile laboratory shall be examined for the following defects. Presence of one or more defects shall be cause for rejection. Prior to shipment any defects shall be corrected to comply with the requirements of section 5 of this specification.

144. The mobile laboratory trailer not preserved as specified for level A.
145. Equipment, supplies, accessories, overpack boxes not positioned and secured as specified for level A or C.
146. Drive belt tension not loosened as specified for level A.
147. Pulley grooves not coated with primer as specified for level A.
148. Ferrous metal surfaces requiring a preservative not coated as specified for level A.
149. Specific items not preserved as specified for level A.
150. Fluorescent lamps not secured as specified for level A or C.
151. Refrigerant charge on air conditioner not pumped down as specified for level A or C.

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

152. Air conditioner valves not closed and not tagged as specified for level A or C.
153. Exterior openings into air conditioner not closed as specified for level A.
154. Doors and weather flaps not closed and secured as specified for level A or C.
155. Marking incomplete, incorrect, or missing for level A or C.

5. PACKAGING

5.1 Preservation and packaging. Preservation of the laboratory trailer and all components of the laboratory shall be level A or C, as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Trailer.. The trailer shall be preserved in accordance with the applicable requirements of MIL-STD-281 for level A towed equipment..

5.1.1.2 Laboratory components. All equipment and accessories shall be located and secured in their designated locations as specified in table I and figures 1, 2, and 3. Overpack boxes shall be secured in their designated locations with the straps provided. Exposed, unpainted ferrous metal surfaces of mounted equipment shall be coated with appropriate preservatives in accordance with MIL-P-116. All equipment driven by belts shall have the belt tension loosened and the pulley grooves coated with primer conforming to TT-P-664. Fluorescent lamps shall be secured in position by taping over the slot of the holders with 1-inch wide tape conforming to PPP-T-60, type IV. Prior to placement in their specified locations the following components shall be preserved as specified:

a.	Manuals, books, pamphlets	IC-3
b.	Electric drill	IIC
c.	Drill set	IC-1
d.	Hot plate	IIC
e.	Rheostat	IIC
f.	Soldering gun	IIC
g.	Tool kit, machinists	IC-1

The refigirator door shall be propped and secured in open position to prevent permanent set of the door gasket.

5.1.1.2.1 Air conditioning unit. The refrigerant charge on open type systems shall be pumped down and appropriate valves closed and capped. Closed valves shall be tagged or otherwise clearly marked with instructions for restoring to service. Exterior openings into air conditioning unit not provided with covers shall be closed with waterproof barrier material conforming to PPP-B-1055, class H-5 secured in place with waterproof tape. A warning tag shall be prominently affixed to the air conditioning controls and shall caution against operating unit without opening valves and removing the waterproof paper.

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

5.1.1.2.2 Door and exterior openings. The doors and weather flaps shall be closed and secured. All inlets, outlets, joints around doors, covers, and flaps shall be sealed with minimum 2-inch wide tape conforming to PPP-T-60, type IV. Any openings to large to be sealed with tape shall be covered with waterproof barrier material secured in place with waterproof tape.

5.1.2 Level C. The trailer shall require no preservation. All equipment, supplies, accessories, and overpack boxes shall be positioned and secured as specified for level A. Specific preservation of items b through g listed in 5.1.1.2 shall not be required. The air conditioner refrigerant system shall be pumped down and tagged as specified for level A. Fluorescent lamps shall be secured in place with the tape as specified for level A. Doors and weather flaps shall be closed and secured. Additional preservation shall be applied, as deemed necessary by the supplier, to afford protection against deterioration and damage from the supplier to the initial destination.

5.2 Packing. Packing shall be level A or C, as specified (see 6.2).

5.2.1 Level A. The mobile laboratory preserved as specified in 5.1 shall not require additional packing.

5.2.2 Level C. The mobile laboratory preserved as specified in 5.1 shall not require additional packing, except doors shall be equipped with tamperproof seals to assure carrier acceptance at the lowest ratings of the carrier.

5.2.3 Rail shipment. Loading of the mobile laboratory on open top single or multi-level railcars shall be in accordance with the appliable requirements of section 1, Association of American Railroads Manual - Loading of Commodities on Open Top Cars and figure number(s) 67 and 202 of section 6 of the AAR rules, Loading of Department of Defense Material on Open Top Cars. The quantity of mobile laboratories to be loaded on each railcar, the type of railcar and the applicable transportation data shall be as specified (see 6.2).

5.2.4 Highway towaway shipment. Prior to highway shipment, no processing of the mobile laboratory's running gear shall be performed that would impair necessary operation or safety during transit. Towaway rules for shipment by drive-away shall be in accordance with the DOT Motor Carrier Safety Regulations. When vehicles are to be placed in storage or shipped overseas, processing of the trailer units running gear not accomplished prior to highway shipment shall be performed at an intermediate destination.

5.3 Marking. In addition to any caution and deprocessing marking, interior packs and units shall be marked in accordance with MIL-STD-129 and as specified herein. Special marking requirements appliacable to unpacked vehicles shall apply. Tool, spare parts and overpack boxes shall contain a list of items contained therein.

5.3.1 Humping precaution. Large signs containing the words "DO NOT HUMP" shall be secured in conspicuous places on each side of the railroad car.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Intended use. The mobile laboratory and sustaining equipment covered by this specification are to be used by Armed Forces for testing petroleum and petroleum products under tactical military operations.

6.2 Ordering data.

6.2.1 Acquisition requirements. Acquisition documents should specify the following:

a. Title, number, and date of this specification.
b. Time frame required for submission of first article (see 3.2).
c. When items of equipment shall be furnished by the contractor (see 3.5).
d. When screw threads shall be other than as specified (see 3.12).
e. Composition of varnish requested (see 3.11).
f. When the Government will not furnish the fire extinguisher (see 3.14 and 3.20).
g. When overcoat in accordance with camouflage patterns is not required (see 3.18).
h. When instructional material is not to be furnished by the contractor (see 3.19).
i. When Government-furnished property is required (see 3.20 and 6.5).
j. Weight classification numbers and instructions required (see 3.21 and 6.7).
k. When the welding process is not to be at the option of the contractor (see 3.22.2).
l. Level of preservation and packing required (see 5.1 and 5.2).
m. The number of mobile laboratories to be loaded on each railcar, the type of railcar required, and the transportation data required (see 5.2.3).

6.3 First article. When a first article inspection is required, the items should be a first produced unit. The first article should consist of one unit. The contracting officer should include specific instructions in acquisition documents regarding arrangements for examinations, tests, and approval of the first article test results and disposition of the first article.

6.4 Hazardous materials. Hazardous materials are listed in part 172 of the DOD regulation 49CFR (see 3.13).

6.4.1 Material safety data sheets. Contracting officers will identify those activities requiring copies of completed Material Safety Data Sheets prepared in accordance with FED-STD-313. The pertinent government mailing addresses for submission of data are listed in appendix B of FED-STD-313.

6.5 Government furnished property. The contracting officer should arrange to furnish the property specified in 3.20, as applicable.

6.6 Government loaned property. The contracting officer should arrange to loan the property specified in 4.5.2.2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

6.7 Vehicle weight classification. The contracting officer should arrange to furnish vehicle classification forms (see 3.21) to the contractor and request the return of the completed forms to the Government. The information obtained should be utilized to determine the weight classification number(s) for the laboratory. The contractor should then be requested by the contracting officer to apply the weight classification number(s) to the curb side of the mobile laboratory.

6.8 List of items. The contracting officer should provide a copy of the list of the items specified in SC 6640-97-CL-E02 (see 3.5).

6.9 Subject term (key word) listing.

Laboratory
Laboratory, mobile
Petroleum testing
Quality surveillance

6.10 Changes from previous issue. Asterisks (or vertical lines) are not used in this revision to identify changes with respect to the previous issue due to the extensiveness of the changes.

Custodian:
Army - ME

Preparing activity:
Army - ME

Project 6640-A083

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

APPENDIX

PACKING OF EQUIPMENT IN MOBILE LABORATORY CABINET DRAWERS AND OVERPACK BOXES

10 SCOPE

10.1 Scope. This appendix details the location of equipment packed in mobile laboratory cabinet drawers and overpack boxes. This appendix is a mandatory part of the specification. The information contained herein is intended for compliance.

20 APPLICABLE DOCUMENTS

20.1 Specifications.

Federal

PPP-C-1752 - Cushioning Material, Packaging, Unicellular Polyethylene Foam, Flexible

(Copies of specifications, standards, and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

30 REQUIREMENTS

30.1 Location of packed equipment. The mobile laboratory cabinet drawers and overpack boxes shall be packed in accordance with Table 1 and Figure 1, 2, 3, and 4.

30.2 Protection of packed equipment. Equipment packed in cabinets shall be assigned a permanent and individual storage location within each cabinet. Stored equipment shall be held in position and protected from other equipment by use of a foam liner in accordance with PPP-C-1752 Type I, Class 2 or Type II Class 1 with cutouts made in the foam liner as necessary to assure safe transport and storage of equipment. Equipment packed in overpack boxes shall be in original packing containers and shall be positioned within overpack boxes in a manner so as to assure safe transport and storage.

30.3 Identification of equipment packed within cabinets and overpack boxes. The quantity and contents of each cabinet or overpack box shall be identified with a label on the face of each cabinet door or drawer, or on the face of the overpack box as applicable.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6810-00-222-2634	ACETIC ACID, GLACIAL, ACS: Liquid; 99.7 pct min assay as acetic acid, glacial; 1 pt bottle; MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(3)-Box 6
6810-01-117-6380	ACETONE, ACS: Liquid; 1 gal. bottle; MIL-STD-1218; O-C-265		(10)-Box 6
	ADAPTER, LABORATORY GLASSWARE: Borosilicate glass;		
6640-00-494-3923	Three Way; 10/30, 24/40, 24/40 joint sizes for ASTM TEST D-322; MS36257-1	(2)-F4	
6640-00-494-3922	Glass, 24/40 external and internal joint; for ASTM TEST D-322, Lurex Glass Co., Vineland, NJ, P/N 111-2053	(2)-F4	
6640-00-852-3013	Pyrex glass; curved to 105 deg angle w/24, 40 and glass joint at one end, cut at angle other end; for ASTM TEST D-322; (80740) 1-130-01 (15747) No. 775	(2)-F4	
5935-00-081-8025	ADAPTER, CONNECTOR: 2 pole to 3 pole elect plug (22527) No. 9-525-10	(3)-W3	
6640-00-403-9344	ADAPTER, CRUCIBLE, LABORATORY: adapts crucibles to crucible holders; 12 per pack; (22527) No. 8-2395	1 pk-W1	
6810-00-543-7415	ALCOHOL, DENATURED: alcohol formula No. 3A colorless; 1 gal can; for ASTM TEST D-94 and FTMS TEST P-5415; O-E-760, grade III		(3)-Box 7
9535-00-541-2453	ALUMINUM FOIL: dry-anneal surface; 75 ft lg, 12 in. w; 10,250 sq in. per lb, 1 roll per dispensing box; for FTMS TEST F-3480; QQ-A-1876, type I, Grade A	(1)-W4	(1)-Box 3

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6810-00-753-4784	AMONIUM HYDROXIDE, ACS: 1 pt bottle; MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(3)-Box 6
8415-00-082-6108	APRON, IMPERMEABLE. cotton duck, Chloroprene rubber coated both sides; black; bib, w/tie tape back fastener; 48 in. lg, 34-5/8 in. w at waist; MIL-A-41829	(1)-L5	(1)-Box 5
6810-00-282-2910	ASCARITE: 90-95 pct sodium hydroxide, 5-10 pct asbestos; powder; particle size, 0 pct max retained on USS sieve No. 8, 0 pct max passing No. 20 sieve; 1 lb bottle; for ASTM TEST D-974; MIL-STD-1444 (ASCARITE)		(1)-Box 6
6670-00-436-9857	BALANCE, DOUBLE-BEAM, LABORATORY: Harvard, trip, w/2 removable cres pans, 6 in. dia; upper beam graduated from 0 - 100 gm in 0.1 gm div, lower beam graduated 0 - 200 gm in 10 gm div; 2000 gm cap.; sensitivity 0.1 gm. w/o wt; (22527) No. 2-052-5D (85973) No. MDL 151D	(1)-G5	
6810-00-234-8362	BARIUM HYDROXIDE, OCTAHYDRATE, ACS: crystal: 98 pct min assy as barium hydroxide, 1 lb bottle; MIL-STD-1218; for ASTM TEST D-974, O-C-265		(1)-Box 7
6640-00-966-3644	BASKET, TEST TUBE: neoprene coated steel wire; 6 x 6 x 6 in.; NNN-B-1291, type II	(1)-E5	
6640-00-359-9628	BATH, FOAMING TEST: for ASTM TEST; D-892; (23035) No. K-430		(2)-Box 1
6630-00-359-9629	BATH, CONSTANT TEMP, R. V. P.: for ASTM TEST D-323; (48619) No. 74893	(1)-T	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPA (QTY)-B
6640-00-522-1886	BATH; CORROSION, LABORATORY: for ASTM TEST D-130; (23035) No. K253-1	(1)-Y2	
6640-00-403-0420	BATH, UTILITY LABORATORY. (48619) No. 66643	(1)-U	
6640-00-403-1000	BEAD, LABORATORY: glass per DD-G-541, type I, class A; solid; 5 mm dia; 1 lb box; MS36259-2	(1)-H1	
6640-00-403-1500	BEAKER, LABORATORY. Borosilicate glass; Griffin low form; 50 ml; w/spout; NNN-B-175, type I, MS35992-4	(3)-H3	(9)-Box 2
6640-00-403-2000	Griffin low form; 100 ml; w/spout; for ASTM TEST D-381, NNN-B-175, type I; MS35992-5	(4)-K3	(8)-Box 2
6640-00-403-3500	Griffin low form; 400 ml; NNN-B-175 type I; MS35992-7	(4)-H4	(7)-Box 2
6640-00-290-6817	High form; 100 ml; 50 mm dia, 80 mm h; for ASTM TEST D-381, NNN-B-175, type III	(10)-K3	
6640-00-942-4393	Low form; 250 ml; graduated in 25 ml increments; 25-200 ml graduation range; w/spout; NNN-B-175, type I	(3)-H4	(1)-Box 2
6640-00-526-8491	500 ml; w/spout; (24546) No. 1060 (15747) No. G1716F	(2)-H5	(10)-Box 2
6640-00-942-4397	1000 ml; graduated at 50 ml intervals from 50 to 950 ml; NNN-B-175, type I	(2)-H5	(4)-Box 5
6640-00-942-4395	Glass per DD-G-541, type I, class A; 600 ml; NNN-B-175, type I	(3)-H5	(1)-Box 2
6640-00-899-2784	2000 ml; 200 to 1800 ml, 200 ml intervals graduations for ASTM TEST D-322 and D-2550; NNN-B-175, type I	(1)-H5	(3)-Box 2

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	BEAKER, STAINLESS STL 1200 ML (15741) No. G1782D	(1)-K4	
3030-00-478-8368	BELT, DRIVE: Pensky Martens; for ASTM TEST D-93, (80740) No. 95-67-905 (15747) No. G18058AP	(5)-W2	
6630-00-359-9772	BOARD, DISTILLING: 4 in. sq w/1.0 in. hole (48619) No. 76026; ASTM TEST D-86	(4)-B3	
6630-00-251-2118	BOARD, DISTILLING: 4 in. sq w/1.25 in. hole (48619) No. 76025; ASTM TEST D-86	(2)-B3	
	BOARD, DISTILLING. 4 in. sq w/2 in. hole, ASTM D-86 48619 No. 76028	(2)-B3	
6630-00-359-9655	BOMB: gum stability; for ASTM TESTS D-525 and D-873, (48619) No. 74740	(2)-J2	
6630-00-399-2964	BOMB, (R. V. P.) PETROLEUM TEST. w/air and liquid chambers, gage coupling and two O-ring gaskets; w/o gage, for ASTM TEST D-323; (48619) No. 74877	(2)-S2	
6630-00-522-1893	BOMB, CORROSION TESTING: copper strip, for ASTM TEST D-130; (22527) No 13-420-20	(2)-F3	
6640-00-131-4566	BORER SET, CORK: brass or steel, nickle plated finished, 3/16 to 5/16 in. od of borers; w/handle; set of 15; (80740) 27-084 (15747) P/N G6540H	(1)-W3	
6640-00-404-8001	BOTTLE, DROPPER: Glass, rd; w/gnd in glass pipe; for ASTM TEST D-2276, crystal clear; 60 ml, NNN-B-1194, type II, class 2, grade B, size 2	(4)-H2 (2)-X1	

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	BOTTLE, SCREW CAP: Glass; French sq; colorless; permanent lable, sample bottle, printed letters; plastic liner in plastic screw cap		
6640-00-404-0661	32 oz; 33 mm screw cap neck; (80740) No. 5-730-32 (15747) P/N G14680F	(3)-C1	(3)-Box 2
8125-00-174-0852	Polyethylene; rd; colorless 6 in. dia; 1 gal; w/plastic screw cap for std neck; MIL-B-26701	(2)-X5	(2)-Box 4
6640-00-410-4461	Polypropylene; rd, narrow mouth; colorless; for handling and storing corrosive chemicals and standards; 1 gal; w/screw cap No. 38 (15747) P/N G2231E	(2)-X5	
6640-00-404-0659	Soda Lime glass; amber; rd 32 oz; w/screw cap No. 33 (15747) P/N G2232P	(1)-C1 (1)-C3	
	BOTTLE, STOPPER: Borosilicate glass, rd; narrow mouth; mushroom glass stoppe5; NNN-B-001522 type I, class 1		
6640-00-405-1000	250 ml, size 4	(3)-B1	(1)-Box 5
6640-00-405-1500	500 ml, size 5	(2)-B1	
6640-00-405-3000	1000 ml, size 6	(1)-B1	
	Pyrex glass; red; colorless; No. 19 std neck, taper glass stopper; w/combination flat head and penny head and taper glass stopper		
8125-00-263-8241	250 ml; etched label, "ACETIC ACID" (24546) P/N 14202405	(1)-K3	
8125-00-263-8245	250 ml; etched label "HYDROCHLORIC ACID, DIL" (24546) P/N 14202090	(1)-K3	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
8125-00-263-8254	250 ml; etched label, "SULFURIC ACID DIL" (24546) P/N 14202L475	(1)-K3	
	BOTTLE STOPPER: - Continued Reagent glass; rd; colorless; narrow mouth; w/penny head and taper glass stopper;		
	250 ml; no label (24546) P/N 1500-250	(1)-K3	
8125-00-263-8262	250 ml; w/etched label, "NITRIC ACID, CON" (24546) P/N 14202L345	(1)-K3	
6640-00-069-2747	BOTTLE, WASHING: borosilicate glass; coating or cork granules on neck; w/cap assy and specially designed flask for hot or cold washings; 500 ml (22527) P/N 03-403-10	(2)-F4	
	BOTTLE, WASHING: Polyethylene graduated, 500 ml, for ASTM D 2550, (15747) P/N G2757E	(4)-X5	
4610-00-522-1882	BRACKET, WATER DEMINIERALIZER: (05852) P/N D8900	(2)-A2	
7920-00-023-1056	BRUSH, BOTTLE AND BURET: 13/16 in. lg brush part; steel or tinned twisted wire handle 9 in. lg; (22527) No. 3-608	(1)-W1	
7920-00-409-2000	Tufted tip; stiff hog bristle; 3/4 in. dia brush part; brass or galvanized steel twisted wire handle 4 in. lg; 36 in. lg; H-B-1050, style B, class 1 MDL TW	(1)-W1	(2)-Box 5
7920-00-402-2379	BRUSH, CYLINDER, LABORATORY: multifan tip; 1 in. lg bristled portion; 4 in. lg galvanized wire handle; 19 in. lg; (22527) No. 3-622	(12)-W1	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
7920-00-178-8315	BRUSH, DUSTING, BENCH: horsetail hair 14-1/2 in lg. 8 in. lg brush part, 2-3/4 in. lg clear of block; H-B-190, type I, style 2 class 2	(1)-W1	
7920-00-205-0565	BRUSH, DUSTING, LENS AND PHOTOGRAPHIC NEGATIVE: camel hair; metal ferrule; 1 in. bristles, 6 in. lg, 1 in. w; w/wood handle; H-B-1654	(1)-w1	
7920-00-409-4000	BRUSH, FLASK: Hog bristle; circular tip; 4-1/2 in lg, 2 in dia brush; 13 in lg handle; (22527) No. 3-571	(1)-W3	
7920-00-494-3688	Synthetic fil; 3 in. dia, 5-1/2 in. lg brush part; 15 in. lg; wood handle, H-B-1049, type VII	(1)-W1	(1)-Box 5
7920-00-240-6359	BRUSH, PIPET: 7 in. lg brush part, 3 in. dia tapered to 1/4 in. tip; 17 inch lg; twisted wire handle; H-B-1051, type II, style A, class 1	(2)-W1	
	BRUSH, TEST TUBE: Hog bristle, multifan tip; steel twisted wire handle;		
7920-00-282-7784	3/4 in. dia, 3 in. lg brush part; 9-1/2 in. lg; H-B-1051, type I, style A, class 1, size 3/4	(4)-W1	
7920-00-889-3381	1-1/4 in. dia. 3-1/4 in lg brush part; 10-1/4 in. lg; H-B-1051, type I, style A, class 1, size 1-1/4	(2)-W1	
7920-00-297-1510	1-1/2 in. dia, 3-1/2 in. lg brush part; 10-1/4 in. lg; H-B-1051, type I, style A, class 1, size 1-1/2	(2)-W1	
7920-00-917-5843	1-3/4 in. dia. 4 in. lg brush part; 12 in. lg; (22527) No. 3-621, size A	(6)-W3 (6)-X5	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
7920-00-917-5844	2-3/8 in. dia, 6 in. lg brush part; 20 in. lg; (22527) No. 3-621, size B	(4)-W1	(8)-Box 2
7920-00-753-5260	Single fan tip; 1-3/8 in. dia, 4 in. lg brush part; 11 in. lg; steel twisted wire handle; (35051) No. 44-34	(1)-W1	
8020-00-260-1302	BRUSH, VARNISH: flat, triple-X thk; hog bristle; 2 x 3 in.: H-B-695, class 1, grade A, size 2	(1)-W1	
6640-00-494-3726	BULB, PRESSURE AND CIRCULATING, LABORATORY: rubber, elliptical; 6 in. lg, w/pressure and suction type valves; 85 ml; for ASTM TEST D-611; MS36074-1	(2)-K2	
	BURET, STRAIGHT: Straight stopcock; calibrated for accuracy; every tenth graduation numbered:		
6640-00-409-8500	0.05 ml graduations; 10 ml; for ASTM TESTS D-94 and D-974; NNN-B-789, type I, style I, class A, grade 2, size 4; MS35971-1	(2)-F1	(6)-Box 3
6640-00-409-9000	0.1 ml graduations; 25 ml; for ASTM TEST D-94; NNN-B-789, type I, style 1, class A, grade 2, size 5; MS35971-2	(3)-F1 (1)-G1	(4)-Box 3
6640-00-410-0000	0.1 ml graduation; 50 ml; for ASTM TESTS D-94 and D-974, NNN-B-789, type I, style 1, class A, grade 2, size 6; MS35971-3	(3)-F1 (5)-K1	
6640-00-551-4082	BURNER, GAS, LABORATORY: single combustion unit; w/removable flat grid burner tip; Bunsen, Maker, high temp; designed for liquified petroleum gas; 2400-3300 Btu per cu ft; MS36275-3 (22527) 3-902P	(2)-F5	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6150-00-487-3037	CABLE ASSEMBLY, POWER, ELECTRICAL: 2 conductors; No. 16 AWG; stranded, 65 strands No. 34 AWG; rubber insulation; 300 v; 25 ft lg; J-C-1270, style 2, class 2, series 1, grade D, kind 1	(1)-L5	
	CALCIUM CHLORIDE, ANHYDROUS, ACS: granular; 1 lb bottle; MIL-STD-1218; for ASTM TEST D-93, O-C-265		(10)-Box 8
6810-00-964-3497	CALCIUM SULFATE, ANHYDROUS, TECHNICAL: powder, 1 lb bottle; for ASTM TEST D-611; (19203) No. 837020; (22527) C-140; (53078) BK-1458		(1)-Box 7
	CALCULATOR. w/3 extra rolls paper (56634) PN T15030II	(1)-M2	
6640-00-194-9728	CAP, SCREW, BOTTLE AND JAR: Plastic; w/plastic liner; 1-1/2 in. thk dia, 3/4 in. deep; cap size 33 Doz. Lot (15747), P/N G2254J	(4Dz)-Y1	
	CARBON RESIDUE APPARATUS: for ASTM TEST D-189; CSC Sci P/N 27331-000 C/O:		
	(1) Burner	(1)-B2	
	(2) Metal Funnel	(1)-B2	
	(3) Iron Crucible	(1)-B2	
	(4) Wood Block	(1)-B3	
	(5) Stand	(1)-B2	
	(6) Sand Cup	(1)-B2	
	(7) Wire Stand	(1)-B2	
	(8) Ceramic Cup COORS#07	(1)-B2	
	(9) Procelin Ring	(1)-B2	
	(10) Gas Control Valve	(1)-B2	
4610-00-222-8261	CARTRIDGE, WATER DEMINERAIZER: Organic; (05852) P/N D8904	(4)-Box 5	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	SHIELD:		
	Cone shaped tube 100 ML (48619) P/N 67359	(4)-E4	
	Pear Shaped Tube 100 ML (48619) P/N 67360	(4)-E4	
	RING, TRUNNION:		
	Cone shaped 100 ML (48619) P/N 67313	(4)-E4	
	Pear shaped 100 ML (48619) P/N 67314	(4)-E4	
	For ASTM Tests D-91, D-893, D-1796, D-2273 and FTMS Test F-5101.5		
6810-00-281-9825	CHARCOAL, ACTIVATED, TECHNICAL: granular; adaptability to impregnation in accordance w/MIL-C-13724, 3 lb can; for ASTM TEST D-974; (22527) P/N 05-685B		(1)-Box 6
	CHART:		
6640-00-248-4490	Paper; Kinematic Viscosity for ASTM TEST D-341; for constant temp bath; Type C; 25 sheet pad; 16 x 20 in.; ASTM No. 12-403-411-12	(1)-M3	
6640-00-248-4491	Type D; 25 sheet pad, 20 x 20 in.; ASTM NO. 12-403-412-12	(1)-M3	
6640-00-248-4492	Type E; 25 sheet pad; ASTM No. 12-403-417-12	(1)-M3	
6640-00-404-2749	Paper; Temperature-Viscosity Index; for comparing viscosities at various temp, incl Saybolt Universal and Furol, Rewood, Engler and the corresponding kinematic values; mtd on heavy bristol board; 16 x 22 in.; for ASTM TEST D-2270; ASTM No. 12-422-700-00	(1)-M3	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPK (QTY)-BOX
5340-00-252-5317	CLAMP (JOINT) LABORATORY, PETROLEUM TEST: cres: Polypropylene inserts; will withstand temp up to 300 deg F; 2 thd cres ring clamps and 2 slit plastic bushings; clamps and bushings slipped over the large ends of joints and screwed together; 24/40 std taper; for ASTM TEST D-322 (15747) P/N TIKS-40-WS	(4)-W2	
4730-00-908-3193	CLAMP, HOSE: cres, 2 in. id; FED-STD-66; MS35842-12	(12)-W1	
6640-00-428-2460	CLAMP, LABORATORY SUPPORT ROD: aluminum base alloy or zinc base alloy, w/nickle plated finish; 11/16 in. dia rod; double swivel jaw; NNN-C-440, type I, class 3; MS36001-3	(6)-W2	
6640-00-024-2279	CLAMP, RUBBER TUBING, REGULATING: screw compressor; 3/4 in. dia tubing; w/open side; NNN-C-435, type III, class A; MS36003-1	(6)-W2	
6640-00-418-1000	CLAMP, TEST TUBE: Stoddard; 1-1/2 in. jaw opening; MIL-C-3648; - MS36009-1	(8)-W3	
6640-00-417-6000	CLAMP, UTILITY, LABORATORY: Rd fixed jaw; 8 in. lg; 1-1/2 in. dia jaw opening; NNN-C-440, type III, class 1, size 1	(2)-W2	
6640-00-962-9820	Rd swivel jaws; 1-1/2 in. dia grip; 1/2 in. extension; (22527) 5-766	(3)-W2	
6640-00-526-7989	Three prong, fixed jaw; 10 in. lg; 3-1/2 in. dia jaw opening; w/ extension; NNN-C-440, type III, class 2, size 2; MS36012-5	(2)-W2	
6640-00-264-5024	Two prong, rd nonswivel jaws, 9 in. lg; 2-1/2 in. dia grip; w/extension arm; NNN-C-440, type III, class 1, size 2; MS36012-4	(4)-W2	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	CLEANER, INSTRUMENT, TUBING:		
6640-00-267-1784	Steel wire, w/cotton tufts; 50 ft lg; 3 mm dia (80740) 7-960-3 (15747) P/N G2925A	(1)-R4	
6640-00-267-1783	5 mm dia (80740) 7-960-5 (15747) P/N G2925B	(1)-R4	
6640-00-494-3846	8 mm dia (80740) 7-960-8 (15747) P/N G2925C	(1)-R4	
	CLIP, ELECTRICAL:		
5999-00-263-1051	Alligator style No. 1; general purpose W-C-440, type TCI, item 1	(10)-W1	
5999-00-939-7462	Battery; uninsulated; 1 screw terminal 0.750 in. jaw opening; steel, lead plated finish; 1.062 in. h, 2.875 in. lg, 0.625 in. w; 25 amp rating (64484) No. 531115	(10)-H1	
8305-00-267-3015	CLOTH, CHEESECLOTH: cotton; 1.03 oz per sq yd; white; unshrunk; 36 in. w; CCC-C-440, type II, class 2		(10 yds)-Box 5
4820-00-401-9177	COCK, PLUG: single; external thd; 3/8 in. ips; handle turns 180 deg; (80740) No. 77-960-01; (64484) No. S-76905 (15747) P/N G9847	(3)-W2	
	COLOR DISK: For ASTM TEST D-2392;		
6630-00-789-0486	(90767) No. 611-95	(1)-F3	
	COLOR DISK:		
6630-00-789-0487	(90767) No. 611-96	(1)-F3	
	COLOR DISK:		
6630-00-789-0488	(90767) No. 611-97	(1)-F3	
6630-00-713-2097	COMPARATOR, COLOR: disk, corrected for artificial light, prism viewing metal housing; w/plastic cover; for ASTM TEST D-2392 (90767) No. 611A	(1)-F5 (2)-E4-F3 (Parts)	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6640-00-081-6553	CONDENSER, LABORATORY: borosilicate glass, w/drip tip; 400 mm lg jacket; joint size, 24/40 top and 24/40 std taper bottom; for ASTM TEST D-95; (22527) 7-724-15B	(4)-G1	(1)-Box 3
	CONDENSER: Hopkins Reflex. (Replacement) Tech Glass Inc. TG 23220 u/w Tetraethyl Lead Apparatus		(2)-Box 3
6640-00-359-2218	CONE: penetrometer, for ASTM TEST D-217; (48619) No. 73526	(1)-J2	
6640-00-410-1911	CONNECTOR, LABORATORY FRAME: end to end; connects 1/2 in. dia rods; hard aluminum, 2 in. lg, 7/8 in. od; (48619) No. 69403 (15747) P/N G23174C	(2)-E2	
	CONNECTOR, ELASTIC TUBING, BRANCHED: Polypropylene; for 1/4 in. I.D. tubing; T-shaped; for ASTM TEST D-322 (22527) P/N 15-319-C	(6)-W3	
6640-00-410-4464	Polypropylene; for 1/4 in. I.D. tubing; "Y" shaped; uniform dia, serrated style connecting ends (22527) P/N 15-320-10C	(6)-W3	
6640-00-074-3339	COPPER STRIP CORROSION STANDARDS: color std for grading corrosion copper test strips; for ASTM TEST D-130; Motson Co. P/N 12-401300-00	(1)-F3	
6640-00-404-2762	CORK DRILLED: For ASTM TEST D-97; (23035) P/N K460-0-8	(12)-X3	
6640-00-404-2762	CORK, RING, TEST, LAB: For ASTM TEST D-97; (23035) P/N K460-1	(8)-W1	
6640-00-323-8689	CORROSION TEST STRIP, COPPER: 1/16 to 1/8 in. thk, 1/2 in. w, 3 in. lg; for ASTM TEST D-130; MS36252-1	(24)-F3	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6510-00-201-4000	COTTON, PURIFIED: rolled; USP: 12 in. x 10 ft lg; 1 lb pkg; for ASTM TEST D-130; JJJ-C-561, grade A, class 2 size 4	(1)-R4	
6640-00-410-1913	COVER, GRADUATED: for ASTM TEST D-86 (80740) No. 90-006-40	(2)-B3	
	CRUCIBLE, FILTERING, LABORATORY:	(3)-G3	
6640-00-419-3050	Borosilicate glass; fine porosity; 30 mm disk dia; w/beaded rim; Gooch, low form, fritted; 30 ml; MIL-C-3659	(3)-H2	
6640-00-290-6551	glass; fine porosity; w/beaded rim; Gooch, high form; 50 ml; for ASTM TEST D-873; MS36089-4	(2)-H2	
6640-00-404-0657	Porcelain; porous bottom; high form; Fine porosity; 5 micron pore radius; fired-in disk; 25 ml; for ASTM TEST D-2547 (64484) No. S-24442	(6)-G3	
6640-00-899-8976	Medium porosity; 4.4 micron pore radius; glazed; 30 ml (80740) No. 28-084-30, (15747) P/N G6703E	(4)-H2	-
	CRUCIBLE, IGNITION, LABORATORY: Porcelain; cup shaped;		
6640-00-290-6790	30 ml; glazed inside, glazed outside, except bottom; for ASTM TEST D-189; NNN-C-680, type I, size 4; MS35966-4	(4)-H2 (2)-G3	
6640-00-290-6791	50 ml; glazed inside, glazed outside except bottom, NNN-C-680, type I, size 5; MS35966-5	(2)-H2 (4)-G3	
6640-00-550-6287	100 ml; for ASTM TEST D-189; NNN-C-680, type I, size 6; MS35966-6	(2)-H4 (4)-G3	
6640-00-936-2065	CRUCIBLE, SKIDMORE, PETROLEUM TEST: for carbon residue apparatus; 70 ml; for ASTM TEST D-189; (48619) No. 68245	(1)-J2	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	CUP:		
6630-00-359-9757	Flash and fire pt; Cleveland open cup 1 for ASTM TEST D-92; (48619) No. 74604, (15747) P/N G18062B	(1)-J2	
	Flash pt:		
6630-00-359-9759	Pensky-Martens closed; for ASTM TEST D-93; (80740) No. 67-946 (15747) P/N G18058E	(1)-J2	
6630-00-359-9758	Tag closed: for ASTM TEST D-56 (80740) No. 67-885 (15747) P/N G18064	(1)-J2	
6640-00-090-4469	CUP, GLASS: u/w sediment apparatus; for ASTM TEST D-473; (20056) No. 68-825-09; (38536) No. 36320	(2)-G2	
6640-00-403-9349	CUP, GREASE DROPPING: for ASTM TEST D-566; (23035) P/N K194-018	(2)-H1	
5110-00-658-8101	CUTTING WHEEL, GLASS: GGG-C-751 Fisher #11-345 Pack/10 (15747) P/N G11041	(1 Pk)-W3	
5110-00-489-8135	CUTTER, HAWSER, HAND OPERATED: (22527) No. 11-340 (15747) P/N G11040	(1)-W3	
5180-00-596-1038	CUTTER AND FLARING TOOL KIT, TUBE, HAND: Case container, metal c/o:	(1)-R3	
	1 ea TUBE CUTTER: 1/8 to 1-1/8 in. od of tube (30327) No. 274FB 5110-00-288-6520		
	1 ea FLARING TOOL, tube hand, 1/8, 3/16, 1/4, 5/16, 3/8, 7/16, 1/2, 5/8, 3/4 (30327) No. 275FS 5120-00-251-2267		

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	CYLINDER, GRADUATED, LABORATORY: Borosilicate glass; hex base; w/ pouring spout;		
6640-00-912-8656	5 ml; 0.1 ml interval graduations (80740) No. 28-476-5 (15747) P/N G6900AA	(3)-H2	
6640-00-494-3959	25 ml; 0.2 ml interval graduations; calibrated to deliver; for ASTM TEST D-56; NNN-C-940, type I, size 4, style 1; MS35943-4	(2)-H5 (4)-H3	(2)-Box 5
6640-00-883-8516	100 ml; for ASTM TESTS D-86 and D-2550; (22527) No. 8-552E; (15747) P/N G6895D	(4)-H5 (4)-C3	(4)-Box 3
6640-00-290-6543	250 ml; 2.0 ml interval graduations; for ASTM TEST D-2276; NNN-C-940, type I, style 1, size 8	(1)-F4 (2)-G4	(1)-Box 3
6640-00-420-3000	1000 ml; 10 ml interval graduations; for ASTM TEST D-2550; NNN-C-940, type I, style 1, size 10		(2)-Box 1
6640-00-420-3500	2000 ml; 20 ml interval graduations; for ASTM D-2550; NNN-C-940, type I, style 1, size 11		(2)-Box 2
6640-00-420-6000	Circular base; mixing; 100 ml; w/std taper glass stopper; calibrated to contain; for ASTM TEST D-1094; NNN-C-940, style 2, size 6; MS35947-6	(1)-H5	(3)-Box 2
6640-00-290-6570	Hex base; 10 ml; 0.1 ml interval graduations; w/pouring spout; calibrated to contain; NNN-C-940, type I, style 1, size 2	(1)-H5 (2)-X1	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6640-00-899-6901	50 ml; 1.0 ml interval graduations w/reinforced bead around neck; calibrated to contain (22527) No. 8-549-5D (15747) P/N G6895C	(3)-H5	(2)-Box 2
6640-00-403-9339	CYLINDER, LABORATORY: borosilicate glass; for ASTM TEST D-892; (80740) No. 67-973-02, 1000 ml, graduated (Foaming Test Apparatus)		(2)-Box 3 (2)-Box 1
6640-00-244-4341	CYLINDER, UNGRADUATED, LABORATORY: borosilicate glass; hex base; w/ pouring spout; (80740) No. 28-395, 125 ML (75278) 20058-38150	(1)-F4	(2)-Box 3
6850-00-290-0042	DESICCANT, ACTIVATED: impregnated w/ moisture indicator; 5 lb can; for ASTM TEST D-892; MIL-D-3716, type IV, grade H		(2)-Box 8
6640-00-244-9478	DETECTOR KIT, WATER AUTOMOTIVE - AVIATION FUEL: Water and Solid contamination, u/w 4730-00-978-8760 Coupler, Quick Disconnect: 1/4 in. internal AVEC-4-417 (32218) GTP-323 Series 3 Syringe: GTP-165 Battery: CGTP-191	(1)-G5	
7930-00-558-1111	DETERGENT, GENERAL PURPOSE: water soluble, powder; for cleaning surgical instruments, laboratory glassware and other hospital apparatus; 5 lb; P-D-1526	(1)-C2	(1)-Box 7
	DISH, CULTURE, PETRI: Top and bottom complete;		
6640-00-422-2200	Large; NNN-D-1478, type 1, class 1, size 150 x 15 mm	(12)-X4	(12)-Box 3
6640-00-229-8689	U/w bacterial filtering disk; disposable; for ASTM TEST D-2276; MIL-D-36425; Pkg of 100	(1)-R4	
6640-00-404-2761	DISK, CORK, LAB: For ASTM TEST D-97; (23035) P/N K460-2	(12)-W1	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	DISK, FILTERING, MICROPOROUS:		
6640-00-985-2099	Aerosol and hydrosol; 25 mm dia; for ASTM TEST D-2276; (08071) HAWP-025-00; pkg of 100	(1)-F2	
6640-00-967-0501	Plain; aerosol; 47 mm dia; for ASTM TEST D-2276; (08071) AAWP-047-00; pkg of 100	(1)-F2	(2)-Box 3
6640-00-985-2096	100's; for ASTM TEST D-2276: (08071) RAWP-025-00	(2)-F2	
6640-00-688-7882	DISPENSER, FILTERING, SOLVENT: for ASTM TEST D-2276; (08071) XX66-025-00 (includes wash, bottles, milipore filter holders, plastic tubing, 90 glass stems)	(2)-F3	
7520-00-240-2411	DISPENSER, PRESSURE SENSITIVE ADHESIVE TAPE: metal; hand operated; for cellulose acetate tape; 3/4 in. w, 2-1/2 in. dia roll; 1 in. id core; GG-D-458, type V, class 5	(1)-M2	
	DISTILLING RECEIVER:		
6640-00-925-6649	Water determination, glass; 10 ml; for ASTM TEST D-95; ASTM E-123 style A	(1)-G1	
6640-00-438-6881	Oil dilution; glass; 5 ml; for ASTM TEST D-322; MS36266-1	(3)-G1	
5130-00-889-8996	DRILL, ELECTRICAL, PORTABLE: 1/4 in.; std duty; 2200 rpm, ac/dc, 115 v; straight drive; keyed jaw chuck; radio interference suppressed; fungus resistant; 3 prong plug; W-D-661, type III, class B	(1)-L4	
5133-00-278-0237	DRILL SET, TWIST: high speed steel; fractional series; 13 drill set c/o: 1 ea DRILL, TWIST: 1/16 in. dia 5133-00-227-9646	(1)-L3	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	1 ea DRILL, TWIST: 5/64 in. dia 5133-00-227-9647 1 ea DRILL, TWIST: 3/32 in. dia 5133-00-227-9648 1 ea DRILL, TWIST: 7/64 in. dia 5133-00-227-9649 1 ea DRILL, TWIST: 1/8 in. dia 5133-00-227-9650 1 ea DRILL, TWIST: 9/64 in. dia 5133-00-227-9651 1 ea DRILL, TWIST: 5/32 in. dia 5133-00-227-9652 1 ea DRILL, TWIST: 11/64 in. dia 5133-00-227-9653 1 ea DRILL, TWIST: 3/16 in. dia 5133-00-227-9654 1 ea DRILL, TWIST: 13/64 in. dia 5133-00-243-9612 1 ea DRILL, TWIST: 7/32 in. dia 5133-00-227-9656 1 ea DRILL, TWIST: 15/64 in. dia 5133-00-243-9611 1 ea DRILL, TWIST: 1/4 in. dia 5133-00-227-9658 GGG-D-751, type B, class 1, set 2C		
6635-00-359-9827	DROPPING POINT APPARATUS, PETROLEUM: Test for ASTM TEST D-566 (23035) K194A	(1)-J4	
6850-00-281-1985	DRY CLEANING, SOLVENT: Stoddard; liquid; for dry cleaning textiles; 1 gal can; for ASTM TEST D-892; P-D-680, type I		(3)-Box 7
4440-00-192-7595	DRYING APPARATUS, Air-Gas: glass, w/metal fittings; 2-1/2 in. dia 11-1/2 in. h; dries 2200 liters saturated air at 70 deg F and 740 mm pressure to a dew pt of minus 110 deg F; w/indication drierite, filter pads and metal grills; for ASTM TEST D-892; (80740) No. 31-634 (15747) P/N G7685	(1)-G4	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
7490-00-813-0152	EMBOSSING MACHINE, IDENTIFICATION TAPE: manual; 1 line, horizontal reading; 1/2 in. w strip; English characters; beveled edge impression direct reading; w/square corner tap and cut-off; 00-E-491, type III, class A, style 2	(1)-J2	
6810-00-264-8997	ETHYLENE GLYCOL MONOMETHYL ETHER, TECHNICAL: liquid; 1 pt bottle; for FTMS F-5340; O-E-780		(2)-Box 7
6640-00-450-5700	EXTRACTION ASSEMBLY: for ASTM TEST D-473; (22527) No. 09-585 Glass Parts:	(3)-W3	
	Siphon Cup w/wires (22527) P/N 09-590	(3)-L1	
	Flask (22527) P/N 09-600	(3)-K4	
4240-00-202-9473	FACE SHIELD, INDUSTRIAL: replaceable, tiltable, headgear supported visor; L-F-36, style B	(1)-A1	
5110-00-234-6550	FILE, HAND: American pattern; rd; smooth cut faces; 6 in. lg, heel to pt; Single cut; 15/64 in. dia largest sect.; GGG-F-325, type XVI, class 1, style C	(2)-L3	
5110-00-241-9160	Three sq; double cut, GGG-F-325, type XIX, style C	(2)-L3	
6640-00-404-2759	FILLER, PIPET: Caufield; w/rubber bulb and ball valve; 0.01 ml accuracy; for ASTM TEST D-611 (15747) P/N G20387	(1)-K2	
	FILLER, PIPET: rubber bulb w/plastic adapter nozzle; (Thomas Sci.) NO. 7775-A20 (15747) P/N G20424)	(3)-L1	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPAC (QTY)-BOX
	FLASK, BOILING: Rd bottom; spherical; No. 24/40 std taper mouth;		
6640-00-857-6877	Borosilicate glass; 500 ml; for ASTM TEST D-95; NNN-F-240, type I, class 2, style 3, size 3	(2)-F4	
6640-00-558-0651	1000 ml; for ASTM TESTS D-95 and D-322; NNN-F-240, type I, class 2, style 3, size 4	(2)-H4	(1)-Box 3
6640-00-899-6375	FLASK, DEWAR: borosilicate glass; cylindrical; 1900 ml; silvered; w/aluminum base; for ASTM TEST D-322 (80740) No. 35-484-1900 (15747) P/N G8815D	(1)-F5	(2)-Box 5
6640-00-423-8500	FLASK, DISTILLING borosilicate glass; side arm jointed to neck at 75 deg angle, straight side arm; cork finish mouth; 125 ml; for ASTM TEST D-86; NNN-F-240, type III, class 1, style 1, size 3; MS36058-3	(2)-K3	(4)-Box 3 (4)-Box 5
	FLASK, ERLENMEYER: Borosilicate glass; rubber stopper mouth;	(3)-G2	
6640-00-935-4286	50 ml; graduated; NNN-F-240, type IV, class 1, style 1, size 3		
6640-00-935-4269	250 ml; 50-200 ml graduation range at 25 ml intervals; for FTMS F-5415; NNN-F-240, type IV, class 1, style 1, size 5	(2)-G4	(5)-Box 4
6640-00-935-4270	500 ml; 100-500 at 50 ml intervals; graduated; (22527) No. 10-090	(3)-G4	(6)-Box 4
6640-00-935-4287	1000 ml; ungraduated; for ASTM TEST D-974, NNN-F-240, type IV, class 1, style 1, size 7; MS36062-9	(2)-K3	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	Corning brand alkali resistant, boron free, laboratory glass; 250 ml; 24/40 std taper mouth; 6 per case; for ASTM TEST D-94 (75278) P/N 26510	(2)-H5	(4)-Box 3
	FLASK, FILTERING:		
6640-00-522-1889	4000 ml; (22527) No. 10-181-5 Borosilicate glass; side tabulation; rubber stopper mouth;	(1)-E5	(3)-Box 4
6640-00-424-8000	500 ml; NNN-F-240, type V, size 4; MS36066-4	(2)-G4	(1)-E4
6640-00-522-1888	1000 ml; for ASTM TEST D-2276; NNN-F-240, type V, size 5; MS36066-5	(1)-E4	
	FLASK, LABORATORY:		
6640-00-290-6936	Iodine; borosilicate glass; w/std taper stopper and mercury steel rim; 250 ml; (22527) No. 10-094	(4)-K2	(4)-Box 2
6640-00-062-5949	500 ml; (24546) No. 5400; (75278) No. 27200	(1)-B1	(1)-Box 2
	FLASK, VOLUMETRIC:		
6640-00-425-6000	Borosolicate glass; w/glass stopper; 100 ml; NNN-F-289, type I, class A, grade 1 or 2; MS36068-4	(2)-H5 (2)-K2	
6640-00-425-8000	500 ml; NNN-F-289, type I, class A, grade 2; MS36068-6	(2)-H4	(2)-Box 5
6640-00-425-9000	1000 ml; NNN-F-289, type I, class A, grade 2; MS36068-7	(2)-H4	(2)-Box 4
5120-00-965-0603	FLINT TIP, FRICTION IGNITER: sleeve; thd, 6 - 50 NF: 6 per bx; GG-I-271, type I, style B	(1)-W3	
6680-00-762-4057	FLOWMETER KIT: calibrated; (15747) P/N G10475A (21519) P/N 36-546-001	(1)-S1	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6670-00-263-0249	FORCEPS: cres; analytical balance wt; plastic tipped; 4 in. lg (22527) No. 2-354	(1)-F2 (1)-W3	
6640-00-426-0315	FORCEPS, FLAT, BLADED: for ASTM TEST D-2276; (08071) XX62-000-06	(1)-F2	
6640-00-403-9338	FRAME ASSEMBLY, LABORATORY: Rods: (4) 1/2 D x 2" lg; (2) 18" lg; (7) 24" lg; (48619) P/N 69419; MS36014-2	(1)-E2	
6640-00-918-7719	FUNELAIRE: (22527) No. 10-331	(6)-W1	
	FUNNEL, COMMON, LABORATORY: Glass; 60 deg		
6640-00-290-6913	Ribbed; 65 mm stem lg, 45 deg tip angle; 175 mm id; 1000 ml (22527) No. 10-381D	(1)-E5	(3)-Box 4
6640-00-290-6923	Smooth; 150 mm stem lg; 50 mm id; w/small bore for analytical filteration (22527) No. 10-326A	(1)-K2 (3)-H5	
6640-00-426-8060	Smooth or fluted; short stem; 100 mm id; for ASTM TEST D-2547; MS36084-7 (22527) 10-329D	(2)-K2	
6640-00-899-8993	FUNNEL, FILTERING LABORATORY: Buchner; fitted glass; 150 ml; w/filtering disk; coarse pore; 60 mm dia; lg stem; (22527) No. 10-358M	(2)-H4	(2)-Box 5
	FUNNEL, SEPARATORY: Borosilicate glass, w/std stopper and polytetrafluoroethylene stopcock;		
6640-00-926-1313	125 ml; for ASTM TEST D-2276; NNN-F-800, type I	(1)-K3	
6640-00-926-1314	250 ml; for ASTM TESTS D-974 and D-2276; NNN-F-800, type I MS35948-4	(2)-G4 (1)-C3	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6640-00-926-1315	500 ml; for ASTM TEST D-2276; NNN-F-800, type 1	(1)-B1	(1)-Box 4
7240-00-282-3916	FUNNEL, STEEL MATERIAL, RIGID SPOUT: 1 pt capacity, 2.5 in. spout lg; for ASTM D-2550; RR-F-800, type 2, class B, style 1	(1)-R4	
6640-00-986-2721	GAGE, CORK AND RUBBER: plastic; 6 in. lg; 10 per pack; (22527) No. 11-284	(1)-W3	
	Recording Chart 100/Box Foxboro P/N 898442	200 (Bookcase)	
	Red Ink Type 1800	(2)-S2	
	Pens Foxboro P/N 12621	(2)-S2	
	Cleaning Wire Foxboro P/N 42527	(3)-S2	
	Key	(1)-S2	
	GAGE, (R.V.P.) PETROLEUM TEST:		
6685-00-194-1699	(48619) No. 74885, 0-5 psi	(1)-S2	(2)-Box 5
6685-00-194-1683	(48619) No. 74886,0-15 psi	(1)-S2	(2)-Box 5
6685-00-411-5488	GAGE (VACUUM) MERCURY MANOMETER: neg pressure readings down to 0.1 mm; adjustable scale graduated over a lg of 160 mm; mtd on wood base, w/supporting panel; for ASTM TEST D-322; (15747) P/N G10730	(1)-A1	
	GASKET:		
5330-00-401-9582	For gum stability bomb, 100 per pack; for ASTM TESTS D-525 and D-873; (48619) No. 74743	(1)-B3	
	GASKET:		
5330-00-402-2209	Composition; petroleum test; accessory to gum stability bomb; for ASTM TESTS D-525 and D-873; (48619) P/N 232240	(1)-J2	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
5330-00-350-9438	GASKET, (POLYTETRAFLUOROETHYLENE) PETROLEUM TEST: accessory to gum stability bomb; for ASTM TESTS D-525 and D-873; (23035) P/N K105-0-85	(5)-W1	
5330-00-169-0557	GASKET, (R.V.P.) PETROLEUM TEST: For ASTM TEST D-323; O-Rings (80740) No. 69-055 (48619) P/N 232068	(25)-W1	
5330-00-292-0570	Liquid chamber; 25 per pkg; O-Rings (48619) P/N 232069	(1)-W1	
	GLAND AND STIRRER: For ASTM TEST D-2386; (23035) P/N K297-0-356	(1)-H3	
8415-00-261-7015	GLOVES, CLOTH: work; men's; gauntlet cuff, knitted, napped, cotton lined; natural; large size; HH-G-450, type I, class 2, pair	(2)-L5	
	GLOVES, RUBBER: Men's; natural or synthetic rubber; acid and alkali resistant; rolled edge cuff; black; 14 in. lg; pair		
8415-00-266-8679	ZZ-G-381, type I, style 1, size 9	(1)-L5	
8145-00-266-8675	ZZ-G-381, type I, style 1, size 11	(1)-L5	
6810-00-222-2636	GLYCEROL, ACS: liquid; 1 pt bottle MIL-STD-1218; for FTMS TEST F-5340; O-C-265		(2)-Box 7
4240-00-269-7912	GOGGLES, INDUSTRIAL: W/eye cups, plastic; ventilated, clear glass lenses; 50 mm dia; rd; worn over personal spectacles; A-A-1814, class A	1 pr-A1	
5350-00-184-6255	GRAIN, ABRASIVE. silicone carbide; 140 mesh; 1 lb can; for ASTM TEST D-130; MIL-A-21380, type III	(1)-J2	(1)-Box 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
9150-00-965-2408	GREASE, GROUND GLASS JOINT: silicone, 2 oz jar; (71984) High Vacuum Grease	(1)-F2	(7)-Box 3
6635-00-359-9831	GREASE WORKING MACHINE: for ASTM TEST D-217; (48619) No. 73531	(1)-U	
6640-00-427-3960	GRID, WIRE GAUZE, LABORATORY: Carbon steel wire; clay center patch; 6 x 6 in.; NNN-G-698, type II, grade D, size 3; MS36016-2	(8)-E2	
6640-00-269-8342	Nickel chromium; 4 x 4 in. MS36015-1		(4)-E2
6640-00 269 8345	6 x 6 in. MS36015-3		(4)-E2
6640-00-840-1390	Steel; center patch; 4 x 4 in.; NNN-G-698	(8)-E2	
6640-00-980-5002	HEATER, ELECTRIC: (with (2) refractory tops and (6) rod clamps) (48619) P/N 61600	(2)-J4	
	HEATER, ELECTRIC: Kinematic Vis. Bath, ASTM Test D-445 (22527) P/N 13-580V4	(1)-R1	
	HEATER, EXTRACTION, PETROLEUM TEST: repeatable heat control; percentage timer; 1200 w, 120 V, AC/DC; 150 to 800 F temp range (Lindberg) (15747) P/N G11850D (72419) Model No. 53016	(1)-U	
	HEATER, WATER, ELECTRIC: 6 Gal (16327) P/N 3E318E 6 gal.	(1)-U1	
	HEATER, (INFRARED) LABORATORY, PETROLEUM TEST: element ptbl, for surface heating such as drying and baking; green enameled finish; reflector interior gold plated; 115 v, 60 Hz, ac; (22527) 11-504-50	(1)-G5	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6640-00-410-1915	HOLDER, CRUCIBLE: borosilicate glass; size B holds 30 and 50 ml crucible; (22527) No. 8-238B	(6)-H5	
6640-00-893-3096	HOLDER, FILTER, HYDRO: for ASTM TEST D-2276; (08071) XX20-047-20	(1)-F5	
6640-00-359-9753	HOLDER, FILTERING CRUCIBLE: 44 mm top od; u/w Gooch or Walter crucible; 6 per pack; MS36091-1	(1 pk)-H2	
6640-00-404-2756	HOLDER, POLISHING: 4 units; machined from 1/2 in. thk bakelite; for ASTM TEST D-130; (22527) No. 13-420-40; (48619) No. 75041	(1)-F3	
	HOT PLATE, LABORATORY: thermostatically controlled; 110 to 600 deg F range, polished cast aluminum, w/embedded nickel chromium heaters encased in copper tubes; 6 in. w, 10 in. deep; 3-3/8 in h; on base w support rod: (15747) P/N G11885 (Thermolyne 2300)		(1)-J2
6810-00-753-4786	HYDROCHLORIC ACID, ACS: liquid; 1 pt bottle; MIL-STD-1218; for ASTM TEST D-974; O-C-265		(12)-Box 8
	HYDROMETER, GRADUATED SCALE: w/thermometer, API gravity; 190 mm lg, 14 mm dia; 20 to 130 deg F range; 0.2 smallest increment; for ASTM TEST D-287;		
6630-00-265-7610	9 to 21 deg; MIL-H-36343, type II, class 2, style 2	(2)-V	
6630-00-265-7611	19 to 31 deg; MIL-H-36343, type II, class 2, style 3	(2)-V	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6630-00-265-7758	29 to 41 deg, MIL-H-36343, type II, class 2, style 4	(3)-V	
6630-00-265-7759	39 to 51 deg, MIL-H-36343, type II, class 2, style 5	(3)-V	
6630-00-265-7764	49 to 61 deg, MIL-H-36343, type II, class 2, style 6	(3)-V	
6630-00-265-7765	59 to 71 deg; MIL-H-36343, type II, class 2, style 7	(3)-V	
6630-00-815-2267	69 to 81 deg; MIL-H-36343, type II, class 2, style 8	(2)-V	
6630-00-404-2754	79 to 91 deg; (Daigger 15747 G13005-J)	(2)-V	
6630-00-404-2755	89 to 101 deg; (Daigger 15747 G13005-K)	(2)-V	
5120-00-965-0326	IGNITER, FRICTION: wire frame; rd file, single flint; hooded; GG-I-271, type I, style A	(2)-W3	
7510-00-267-9249	INK, RECORDING INSTRUMENT: For ASTM TESTS D-525 and D-873; Green; (22527) No. 1-175; (28480) No. 5080-3611, Bottle	(1)-F5	
7510-00-821-0258	Red; (22527) No. 1-174; (72264) No. 61100R, Bottle	(1)-F5	
6635-00-025-9152	JAR: cloud and pour, for ASTM TEST D-97; (15747) P/N G14718 (24546) P/N 6902	(6)-X3	
6640-00-403-9343	JAR, CHROMATOGRAPHY: borosilicate glass; gnd to the close tolerances needed for tight cover fit, 10-1/2 in. h; 1 gal; (22527) No. 5-719-9-1; (24546) No. 6944-1	(1)-A1	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPAC (QTY)-BOX
6640-00-359-9870	JAR, CYLINDRICAL, LABORATORY: borosilicate glass; 4-5/8 in. dia, 9 in. h; for ASTM TESTS D-86; (06542) FTMS 791 method 1001.7; (75278) P/N 32900 (15747) P/N G14712	(1)-H5	(3)-Box 4
6640-00-899-8980	JAR, DRYING, LABORATORY: borosilicate glass; 300 mm h; stopcock; for ASTM TEST D-892; (80740) No. 31-650; (75278) No. 19505 (75278) P/N 19505 (15747 P/N G7682D	(1)-F4	
6665-00-496-9623	KIT, FUEL SAMPLING: for ASTM TEST D-2276; (08071) XX64-037-30	(1)-W4	
6640-00-436-9926	KIT, LABORATORY, GLASS REPAIR: (21519) P/N 75-460-512	(1)-F5	
5110-00-223-7782	KNIFE, CRAFTSMAN'S: straight blade; sq pt; 3-1/2 in. blade lg, clear of handle; GGG-K-481, type II, class I, style 1	(1)-W3	
	LABEL: Blank; opaque;		
7530-00-526-9792	Paper; white, w/red border; single; No perforations; water activating adhesive; 1.00 in. lg, 11/16 in. w; 90 per box; UU-L-49, class A, style 2 500 Labels/Roll	(1 roll)-F2	
7530-00-663-3949	Plastic, laminated; white, w/blue border; transparent acetate film finish; acid, grease, sensitive adhesive; sealed in carbon; 0.625 in. w, 1 in. id core, 33-1/3 ft lg; A-A-204	(2 rolls)-F2 (1 roll)-H3	(2)-Box 3

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6240-00-319-4549	LAMP, FLUORESCENT: 4 w; miniature bipin base, T-5 bulb; 6 in. lg; ballast operated; emits untraviolet light; lamp No. F4T5/BLB; (32218) MDI. J-204	(1)-G5	
	LAMP, INCANDESCENT: Clear finish; white light, 1 tungsten C-2R fil;		
6240-00-155-8675	2.4 v, 0.3 amp; miniature flange base, B-2-1/2 bulb; 1-1/4 in. lg; 30 hr rated life; for ASTM TEST D-270; W-L-111, Lamp No. PR-6	(2)-H1	
6240-00-797-3750	3.7 v, 0.3 amp, miniature screw base; G-3-1/2 bulb; 15/16 in. lg; 15 hr rated life; W-L-111, Lamp No. 13	(2)-H1	
6810-00-271-1405	LEAD ACETATE, TRIHYDRATE, ACS: crystal; 1 lb bottle; MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(2)-Box 8
6810-00-236-5359	LEAD NITRATE, ACS: crystal; 1 lb bottle; MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(1)-Box 8
5210-00-619-7036	LEVEL AND PLUMB: cast iron; 9 in. lg; single face, nonadjustable; 1 ungraduated unground level vial and 1 ungraduated unground plumb vial; 1 @ 45 GGG-L-211, type II, class 1, style A	(1)-K2	
6230-00-146-8898	LIGHT, EXTENSION: 3 conductors, 18 AWG: 2 pole 3 wire plug connector; medium lamp screw base; incl wire guard, switch, reflector, hook, rubber or molded plastic handle; 50 ft lg; W-L-661, type III, class 1	(1)-L5	
6630-00-337-6890	LINER, BOMB: for ASTM TESTS D-525 and D-873; (23035) P/N K105-4; (24546) P/N 7732	(4)-K2	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the currentversion before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	LITMUS PAPER, ACS: 5 cm lg, 0.6 cm w; strip; 100 per vial; O-C-265;		
6640-00-290-0146	Blue; MS36253-2	(4)-F2	(8)-Box 2
6640-00-290-0147	Red; MS36253-1	(4)-F2	(8)-Box 2
9150-00-273-8663	LUBRICATING OIL, VACUUM PUMP: MIL-L-83767, type II		(4)-Box 2
6810-00-247-0600	MERCURIC IODIDE, RED, ACS: powder; 1/4 lb bottle; MIL-STD-1218; O-C-265		(1)-Box 8
6810-00-281-7450	MERCURY, ACS: liquid; 5 lb bottle; MIL-STD-1218; O-C-265	(2)-C2	
	METER, CONDUCTIVITY: Battery operated (23299) P/N 1152	(1)-K3	
	METER, PH: "Chemtrix", w/temp compensation, solid state electronics; interchargeable battery; w/115 v, ac conversion kit, inc; reference and buffer solution; Chemtrix Type 400	(1)-G5	
6810-00-281-2785	METHYL ETHYL KETONE, TECHNICAL: liquid; for ASTM TEST D-94; TT-M-261; gal		(2)-Box 6
6810-00-227-1259	METHYL ORANGE, ACS: powder; 1/4 lb bottle; MIL-STD-1218; for ASTM TEST D-974 and FTMS TEST F-5101.6; O-C-265		(1)-Box 8

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6625-00-691-6605	MULTIMETER, RANGE: 0 to 6000 v dc in 6 steps, 0 to 6000 ac in 6 steps, 0 to 12 amp dc in 5 steps, 0 to mego in 4 steps, minus 20 to plus 70 db in 6 steps; porm 1.5 pct accuracy on dc ranges; porm 2.5 pct accuracy on ac ranges; 50 ua sensitivity; 1.5 and 30 v dc operating power; internal battery source; 3-7/32 x 5-1/2 x 7-1/2 in.; carrying case w/Instruction Book and 2 Test Leads; (60741) Model No. 310	(1)-M2	
6810-00-227-1271	NAPTHA, ALIPHATIC: distilled from petroleum, precipitation naptha; 1 gal can; for ASTM TEST D-91		(3)-Box 6
6810-00-070-7677	P-NAPHTHOLBENZEIN: 25 gm per bottle; for ASTM TEST D-974; (22527) No. 924; (53078) EK 924		(3)-Box 6
6810-00-237-2954	NITRIC ACID, REAGENT: 5 pt bottle; MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(3)-Box 8
6810-00-234-2013	P-NITROPHENOL, REAGENT: crystal; 112 to 114 deg C mp; 100 gm per bottle; for ASTM TEST D-2547; MIL-C-51130		(1)-Box 8
9150-00-449-7819	OIL, BATH, VISCOSIMETER: 1 gal; (48619) No. 74972)		(10)-Box 8
4930-00-287-8474	OILER, HAND: 5 oz; compressible fed; steel, copper plated; 4 in. lg spout; GGG-O-591, type I, class A	(1)-R3	
6640-00-235-3820	PAD, WATER DETECTOR KIT: 100 per bx (32218) GTP-25; (Nuclepore Co.) P/N 240-610	(2)-F3	(6)-Box 2
5350-00-721-8117	PAPER, ABRASIVE: Silicon carbide; 9 x 11 in. sheets; for ASTM TEST D-130; P-P-101; Grit No. 180; closed coating; waterproof, package		(1)-Box 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
5350-00-224-7209	Grit No. 220; closed coating; waterproof, package		(1)-Box 2
5350-00-224-7207	Grit No. 240; closed coating; waterproof, package		(1)-Box 2
5350-00-224-7201	Grit No. 400; electronically applied abrasive, package		(1)-Box 2
6640-00-084-5080	PAPER (ABSORBENT) BIBULOUS: 50 sheet book, bound w/heavy paper covers; 13.5 x 10 cm sheets; (80740) No. 65-480; (53078) S-65215	(1)-F3	(5)-Box 2
	PAPER, FILTER:		
6640-00-083-5308	For ASTM TEST D-2276; (08071) HAWP-047-00, 47 mm, type HA	(100-F2	
6640-00-252-5198	Qualitative; for course and gelatinous precipitates; 12.5 cm dia; 100's NNN-P-1475, type I, class I, grade 1, style 1; MS36097-1 (Whatman 4)	(2)-F2	
	Qualitative:		
6640-00-866-1427	For fine precipitates; 12.5 cm dia, 100's NNN-P-1475, type I, class 3; MS36097-14 (Whatman 2)	(2)-F2	
6640-00-252-5202	"Whatman" No. 40, double acid washed; dense; 12,5 cm dia; for ASTM TEST, 100's, D-482; NNN-P-1475, type II, class 7	(1)-F2	
	Quantitative; double acid washed; for fine precipitates, thin; 12.5 cm dia; 100 per box;		
6640-00-291-8724	Dense NNN-P-1475, type II, class 7; MS36097-24 (Whatman 42)	(2)-F2	(2)-Box 2
6640-00-252-5205	Slow filtration; NNN-P-1475, type II, class 8; MS36097-27 (Whatman 44)	(2)-F2	(4)-Box 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6850-00-270-5526	PASTE: Gasoline Indicating (15747) P/N G18095B	(1)-F3	(4)-Box 2
6850-00-001-4194	PASTE: Water Indicating (15747) P/N G18095A (65093) P/N SAR-GEL	(1)-F3	(4)-Box 2
7510-00-174-3205	PENCIL: black; wax; extra lead; glazed surface marking; paper casing; SS-P-196		
6635-00-359-2232	PENETROMETER: 39 mm penetration; loading wt, one 100 gm, one 50 gm; w/leveling screw; rectangular base; for ASTM TEST D-217 (48619) No. 73510	(1)-K4	
6810-00-051-5872	PETROLEUM ETHER, ACS: 1 gal bottle; liquid; MIL-STD-1218; for ASTM TEST D-2276; O-C-265		(3)-Box 7
6810-00-223-7612	PHENOLPHTHALEIN, ACS: powder; 4 oz bottle; MIL-STD-1218; for ASTM TESTS D-94 and D-974; O-C-265		(1)-Box 8
6640-00-404-2758	PIPET: 10 ml; graduated; for ASTM TEST D-2276; (08071) XX10-047-09	(1)-G1	
6640-00-442-9621	PIPET, DROPPING: glass, 9/32 in. od. excl of collar; curved end; plain tip; 2 ml; rubber bulb; 1-3/16 in. lg, 1/2 in. dia; 4 in. lg; bulb forms part of bottle closure (80740) 71-570 (15747) P/N G20408B	(12)-L1	
	PIPET, VOLUMETRIC: Borosilicate glass; bulb in middle of tube; nonserialized precision; w/graduation; for ASTM TEST D-611 NNN-P-395, class A;		
6640-00-558-0575	2 ml; MS35985-2	(3)-F1 (3)-X2	
6640-00-437-8000	5 ml; MS35985-5	(4)-F1 (8)-X1	

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	Borosilicate glass; bulb in middle of tube; w/graduation; NNN-P-395, type I, class A, grade 2;		
6640-00-437-9000	10 ml; for ASTM TEST D-611 and FTMS TEST F-5101.6; MS35985-6	(3)-F1 (9)-X2	
6640-00-438-0000	25 ml; for ASTM TEST D-2547; MS35985-9	(4)-F1	(12)-Box 4
6640-00-438-0250	50 ml; MS35985-10	(2)-F2 (3)-G3	
8135-00-043-5331	PLASTIC FILM: 12 in. w; 100 ft roll; for ASTM TEST D-2276; (71983) HANDIWRAP	(2)-W4	(1)-Box 3
7930-00-266-7137	POLISH, METAL: for brass, chrome, copper and nickel; liquid; 1 pt can; flammable; P-P-556, type II, class 1	(1)-A2	(1)-Box 2
6810-00-241-1150	POTASSIUM CHLORATE, ACS: crystal; 1/4 lb bottle; MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(4)-Box 8
6810-00-222-9675	POTASSIUM DICHROMATE, ACS: crystal; 1 lb bottle; MIL-STD-1218; O-C-265		(6)-Box 7
6810-00-137-5000	POTASSIUM DIHYDROGEN PHOSPHATE, MONOBASIC, ACS: Sorensen; 100 GM bottle; MIL-STD-1218; for ASTM TEST D-1094; O-C-265		(5)-Box 8
6810-00-275-8134	POTASSIUM HYDROGEN PHTHALATE, ACIDIMETRIC STANDARD, ACS: Cook; crystal; 1/4 lb bottle; MIL-STD-1218; for ASTM TESTS D-974 and D-1287; O-C-265		(3)-Box 8
6810-00-281-9827	POTASSIUM HYDROXIDE, ACS: pellets; 1 lb bottle; MIL-STD-1218; for ASTM TESTS D-94 and D-974; O-C-265; MIL-STD-612		(2)-Box 6

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6810-00-243-4433	POTASSIUM IODIDE, ACS: crystal; 1 lb bottle; MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(5)-Box 7
6810-00-270-3255	POTASSIUM PHOSPHATE, DIBASIC, ANYHDROUS, ANALYZED REAGENT: powder; 100 gm bottle; MIL-STD-1218; for ASTM TEST D-1094; O-C-265		(2)-Box 8
6640-00-438-2150	PRESS, CORK, LABORATORY: accom 1-1/4 in. dia cork; rotary (80740) No. 27-160; (22527) No. 7-880	(1)-K4	
6230-00-411-9318	PROBE LIGHT, INSPECTION: for ASTM TEST D-270; (83303) MVXF	(1)-R3	
	PROPANE: Cylinder, Disposable odorized (small) 1 lb cyl; BB-G-110, type II		(4)-Box 5
5350-00-161-9033	PUMICE, TECHNICAL: pulverized; 1 lb can; SS-P-821, grade FFF		(1)-Box 8
6640-00-403-9341	PUMP, FILTER, LABORATORY: boro-silicate glass; evacuates 500 ml flask in 1.6 min; w/check valve as integral part of pump; for ASTM TEST D-2547; (75278) K-38004	(2)-G3	
6640-00-442-5100	RACK, TEST TUBE, LABORATORY: Cres; 34 mm od tube; 4-3/16 x 4-3/16 x 15 in.; 14 tubes; NNN-R-55, type I, size 1	(1)-F5	
6685-00-401-1422	REGULATOR, WATER LEVEL, PETROLEUM TEST: enameled brass; screws into drain hole; tubing connections for inlet and drain; for ASTM TEST D-94; (20056) No. 84-859-00; (48619) No. 66996 MDL 82	(1)-H1	
6640-00-494-3731	REMOVER, BOTTLE STOPPER, LABORATORY: hinged arm, clamp; bronze (22527) P/N 02-927	(1)-X5	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1 Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6145-00-192-1698	RESISTANCE WIRE: rd; No. 28 AWG; 80Ni-20Cr alloy conductor; 4.299 ohms per ft at 25 deg C resistivity; 1/4 lb spool; ASTM B-344	(1)-J2	
5905-00-448-5326	RHEOSTAT, (TETRAETHYL LEAD APPARATUS) PETROLEUM TEST: 25 ohms, 2 amp; for ASTM TEST D-2547; (21519) No. 69-009 (48619) No. 235032 (15747) P/N G7870	(2)-J2	
	RING, LABORATORY APPARATUS SUPPORT: Metal; closed 4-1/2 in. from ring center support rod; w/clamp		
6640-00-835-0896	2-3/8 in. id; MS35944-2	(3)-H1	
6640-00-440-1348	4-1/2 in id; NNN-R-370, type I, class A or B; MS35944-4 (22527) No. 14-050D	(3)-G2	
6640-00-290-6699	6-1/8 in. id; (80740) 74-660-7	(3)-H1	
6640-00-440-1325	RING SUPPORT: closed ring; 4 in. od; NNN-R-370, type I, class A, size 3; MS35944-3	(3)-G2	
6640-00-438-5950	ROD ASSORTMENT, STIRRING, LABORATORY: soft glass, 1 ft lg, or 4, 6, and 8 mm dia; fire-polished ends; 1 lb NNN-R-560, type I, set	(2)-Y1	
6640-00-436-9921	ROD, DROPPING POINT APPARATUS: polished metal; 1/16 in. dia, 6 in lg; u/w chromium plated grease cup; for ASTM TEST D-566; (23035) P/N K194-E6	(1)-H1	
6670-00-436-9853	ROD, SUPPORT, VIBRATION DAMPING: Anodized Alum. 18 in long Eberbach P/N 9725 (15747) P/N G1387PT	(1)-K4	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6630-00-151-5310	SAMPLE AND GAGING KIT, PETROLEUM: ptbl; for ASTM Tests D-270, D-287, D-1085, D-1086, D-1250 and D-1298; MIL-S-51028; (84583) P/N 5310	(1)-D1	
6695-00-946-3602	SAMPLER LIQUID: 16 oz for ASTM TEST D-270; (20222) No. 33531-03 (23035) P/N K277A	(1)-J2	
	SAND, SEA, 5 lb pg (64484) 5-73845A for ASTM TEST D-189		(1)-Box 4
6670-00-436-9860	SCOOP, BALANCE, LABORATORY: Analytical balance; (53088) No. 726002	(1)-G5	
6640-00-063-5240	SCRAPER, LABORATORY, RUBBER: Diagonal; Pure gum rubber; 1-3/8 in. lg, 7/16 in. w/scraper; 1/8 in. dia rod (80740) No. 74-810-1-8 (22527) P/N 14-105A	(12)-W3	
6640-00-410-4463	25 mm lg, 3.15 mm dia scraper; 152.4 mm lg glass rod (80740) No. 74-800 (21519) P/N 74-800	(6)-Y1	
5120-00-421-0000	SCRIBER, DIAMOND POINT: MIL-S-15825 (15747) P/N G18018	(1)-L3	
2330-01-136-7663	SEMITRAILER, VAN: 10 ton, 4 wheel, series XM971E1; MIL-S-46756 w/exception letter TASCOM 9 Jul 82		
6680-00-496-9612	SHAFT (EXTENSION) TACHOMETER: petroleum test; 12 in. lg; (57733) No. 412850	(1)-F3	
6640-00-403-9348	SHAFT, STIRRER, FLEXIBLE: 11-1/2 in. lg, w/1/4 in. chuck at one end; 1/4 in. dia 6-3/4 in. lg support rod; for ASTM TEST D-93; (23035) P/N K160-9	(1)-J4	(3)-Box 2

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
5110-00-263-0248	SHARPENER, CORK BORED: 22 mm cutting edges dia of cork bore; (80740) No. 27-170 (15747) P/N G6560	(1)-W3	
5110-00-223-6371	SHEARS, STRAIGHT TRIMMERS: steel blades; w/1 sharp pointed blade end and one beveled blade end; 8 in. lg; w/steel handle; GGG-S-278, type I, class 1, design 2, style A	(1)-H1	
6640-00-359-9641	SHIELD, HEAT, DISTILLING FLASK: Porcelain; 4-3/4 in. lg, 4-3/4 in. w, 3/4 in. thk, 1.0 in. dia center hole; w/bevel recess; (48619) No. 61832 MS36345-4	(2)-X3	(2)-Box 2
6640-00-359-9646	Porcelain; 1-1/2 in. center hole dia, 4-3/4 in. lg, 4-3/4 in. w, 7/8 in. thk; for ASTM TEST D-86; (48619) No. 61825, MS36345-2	(1)-X4 (1)-X3	
6640-00-359-9642	Vermiculite-cement; for ASTM TEST D-86; 4-3/4 in. lg, 4-3/4 in. w, 3/4 in. thk, 2 in. dia center hole; w/bevel recess; (48619) No. 61834, MS36345-5	(2)-X4	
6810-00-233-0126	SILVER NITRATE, ACS: crystal; 1/4 lb bottle; MIL-STD-1218; for ASTM TEST D-94; O-C-265		(1)-Box 8
6810-00-241-1143	SODIUM BICARBONATE, ACS: crystal; 1 lb bottle; MIL-STD-1218; O-C-265		(10)-Box 8
6810-00-264-6593	SODIUM CARBONATE, ANHYDROUS, ACS: granular; 1 lb bottle; MIL-STD-1218; O-C-265		(1)-Box 7
6810-00-264-6592	SODIUM CHLORIDE, ACS: crystal, 1 lb bottle; MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(1)-Box 7
6810-00-262-8582	SODIUM DICHROMATE, DIHYDRATE, ANALYZED REAGENT: crystal; 1 lb bottle; (22527) No. S-235		(2)-Box 7

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6810-00-174-6585	SODIUM HYDROXIDE, ACS: pellet; 1 lb bottle; MIL-STD-1218; O-C-265		(2)-Box 6
6810-00-234-8377	SODIUM SULFATE, ANHYDROUS, ACS: for ASTM TESTS D-86 and D-611; O-C-265		(2)-Box 7
6810-00-237-2908	SODIUM SULFIDE, NONHYDRATE, ACS: crystal; 100 GM bottle; MIL-STD-1218; for ASTM TEST D-2547, O-C-265		(1)-Box 8
6810-00-234-8380	SODIUM THIOSULFATE, PENTAHYDRATE, ACS: crystal; 1 lb bottle; MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(2)-Box 8
3439-00-269-9610	SOLDER, TIN ALLOY: 1 lb spool; QQ-S-571, type SN 60 wrap 3	(1)-L4	
3439-00-618-6623	SOLDERING GUN: ac, 115 v, 60 Hz. single phase, 3 wire plug; 3 in. w, 7 in. h, 12 in. lg; w/pistol grip handle and spotlight; W-S-564, type I, cord assey B, class 1	(1)-L4	
	SPATULA, LABORATORY:		
6640-00-171-5198	Cres blade; wood handle; 3/4 in. w, 4 in. blade lg, 7-3/8 in. lg; NNN-S-1356, class II, size 2	(2)-W3	
6640-00-439-7375	1/1/4 in. w, 8 in. blade lg, 12-5/8 in. lg; NNN-S-1356, class II, size 4; MS36208-4	(2)-W3	
6640-00-975-0453	3 in. blade lg, 7 in. lg; weighting, thin flexible blade, (22527) No. 14-371A	(2)-W3	
7920-00-240-2559	SPONGE, CELLULOSE: rectangular; 5-3/4 in. lg, 3-5/8 in. w, 1-3/4 in. thk; L-S-626, type II, class 2, porosity A	(2)-L2	

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	STAND, FREEZING POINT APPARATUS: u/w Tubes 6640-00-436-9939 for ASTM Test D-2386 (23035) K297	(2)-H3	
6640-00-290-6717	STAND, LABORATORY APPARATUS SUPPORT: Metal base, 5 x 8 in.; 20 in. lg rod; NNN-S-750, type I, grade A, size 2; MS36019-1	(2)-J3	
6400-00-440-1300	Porcelain base, 7 x 13 in.; 23 in. lg rod; for ASTM TEST D-94; NNN-S-750, tyep I, grade B, size 2; MS36020-1 (22527) No. 14-667	(2)-J3	
	STANDARDS: Millipore - (08071) P/N XX64-037-85	(1)-F5	
6810-00-275-8126	STARCH, SOLUBLE, ACS: powder 1 lb bottle, MIL-STD-1218; for ASTM TEST D-2547; O-C-265		(2)-Box 7
5350-00-240-2920	STEEL WOOL: 1 lb roll; FF-W-1825, type I, class 00 fine	(1)-L2	
6640-00-488-5221	STIRRER, AGITATOR LABORATORY: cres; 3 bladed, 2 in. dia; propeller; 1/4 in. dia rod; 10 in. lg; (22527) #14-518-75	(2)-F2	
6640-00-531-5022	STIRRER, ELECTRIC LABORATORY: 110 v, 50/60 Hz, ac; 80-115 rpm; on-off toggle switch; universal clamp mtg; for ASTM TEST D-93; (48619) No. 75765	(1)-J4	
6640-00-482-7235	STIRRER-HOT PLATE, MAGNETIC, LABORATORY: 775 w; variable stirring speed; w/one 1/2 in. one 1-1/2 in. and one 3 in. stirring bar; 110 v, ac, 60 Hz; for ASTM TEST D-322; (53078) S40990	(1)-G5	
6640-00-310-8550	STONE: foam test apparatus; for ASTM TEST D-892; (80740) No. 68-758-01; (23035) P/N ME46239B	(2)-K2	(2)-Box 1

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6645-00-126-0286	STOPWATCH: laboratory; 1/5 to 5 sec dial graduations; 30 min register; 2 sweep hands; 7 jewels, stem wound; nonmagnetic; shockproof; open face, pocket; white numerals and graduations, black background; GG-S-764, type I, class 3	(4)-F3	
	STOPCOCK, LABORATORY APPARATUS: Glass; straight; for ASTM TEST D-2276;	(2)-G2	
6640-00-440-7000	2 mm; DD-S-720, type I, grade A; MS35988-4 (with plugs)		
6640-00-852-3452	4 mm; std taper; DD-S-720, type I, composition I, grade A; MS35988-5 (with plugs)	(2)-G2	
6640-00-410-1917	STOPCOCK, PLASTIC: tapered ends; 3/8 to 1/4 in.; (80740) No. F3089 (15747) P/N G23025A	(6)-W1	
	STOPPER, BOTTLE: Cork, w/std taper; regular; 100's;	(1)-Y1	
6640-00-116-2823	No. 4 stopper; 0.63 top dia, 0.47 in. bottom dia; (80740) No. 26-970-4 (15747) P/N G6500G		
6640-00-232-5991	No. 5 stopper; 0.69 in. top dia, 0.53 in. bottom dia, (80740) No. 26-970-5 (100's) (15747) P/N G6500H	(1)-Y1	
6640-00-232-6014	No. 6 stopper; 0.75 in. top dia, 0.58 bottom dia; (80740) No. 26-970-6 (100's) (15747) P/N G6500I	(1)-Y1	
6640-00-232-5992	No. 7 stopper; 0.81 in. top dia, 0.63 in. bottom dia; (80740) No. 26-970-7 (100's) (15747) P/N G6500K	(1)-Y1	

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
8125-00-281-4107	Nonblooming red rubber, w/low sulfur content; 0.413 top dia, 0.118 bottom dia (22527) No. 21-381 (15747) P/N G21635	(12)-W3	
6640-00-232-6007	Rubber; No. 7 stopper; 1.457 in. top dia, 1.181 bottom dia; (80740) No. 74-930-7; (22527) No. 14-141-7 (15747) P/N G21600L	(12)-Y1	
	Synthetic rubber;		
6640-00-232-6012	No. 2 stopper; 0.78740 in. top dia, 0.62992 in. bottom dia; MS36369-4	(5)-Y1	
6640-00-232-6011	No. 3 stopper; 0.94488 in. top dia, 0.70866 in. bottom dia; MS36444-1	(12)-Y1	
6640-00-232-6010	No. 4 stopper; 1.0236 in. top dia, 0.78740 in. bottom dia; MS36444-2	(12)-Y1	
6640-00-232-6009	No. 5 stopper; 1.0630 in. top dia, 0.9055 in. bottom dia; MS36444-3	(12)-Y1	
6640-00-935-1105	No. 6 stopper; 1.2598 in. top dia, 1.0244 in. bottom dia; (80740) No. 74-930-6	(12)-Y1	
6640-00-232-6006	No. 8 stopper; 1.6142 in. top dia, 1.2992 in. bottom dia; MS36444-6	(12)-Y1	
6640-00-232-6005	No. 9 stopper; 1.771 in. top dia, 1.456 in. bottom dia; (80740) No. 74-930-9 (15747) P/N G21600N	(12)-Y1	
6640-00-232-6004	No. 11 stopper; 2.205 in. top dia, 1.890 in. bottom dia; (80740) No. 74-930-11 (15747) P;N G21600R	(5)-Y1	
6640-00-103-1845	No. 12 stopper; 2.524 in. top dia, 2.126 in. bottom dia; (80740) No. 74-930-12 (15747) P/N G21600T	(5)-Y1	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6640-00-179-2558	STOPPER, CORK QUALITY: (80740) No. 27-000 (15747) P/N G6501A	(100)-X5	
6640-00-410-4466	STOPPER, SPLIT CORK: for ASTM TEST D-566; (23035) P/N K194A-09	(6)-H1	
	STRAINER: for ASTM TEST D-974; (1) 100 Mesh (23035) P/N K220-6 (1) 100 Mesh Replaceable Cloth (23035) P/N K2206A (1) 200 Mesh (23035) P/N K220-6B	(1 ea)-J3	
6640-00-055-0071	STRETCHER, RUBBER TUBING: (22527) No. 14-196	(1)-F2	
6810-00-146-7520	SULFURIC ACID, ACS: 5 pt per 9 lb bottle; MIL-STD-1218; for ASTM TEST D-1094; O-C-265		(5)-Box 7
	SUPPORT ROD: 1/2 dia x Alum 6061-T6	24.00 Lg	(4)-E4
6640-00-359-9985	SUPPORT: sediment apparatus; for ASTM TEST D-473; (23035) P/N K485	(2)-K2	
6640-00-392-8643	SUPPORT ARM, FUNNEL, LABORATORY: w/4 conical shaped holes, 1/2 in. w slots; cast iron clamp; 11/16 in. dia hardwood rod, 12-1/2 in. lg, 2-1/2 in. w; MS36021-1 (22527) No. 14-740 (15747) P/N G23396	(2)-J3	
6640-00-410-1919	SUPPORT RACK, PIPET: (20056) No. 71-720 (15747) P/N G23400	(1)-A1	
6640-00-359-9995	SWAB: for ASTM TEST D-86; (26340) No. 90-006-37; (48619) No. 76018	(2)-H1	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6515-00-068-5022	SYRINGE: luer; general purpose; glass; 100 cc; 10 cc graduations; needle lock, concentric; plunger, dark precision line around base; w/button thumb rest; for ASTM TEST D-322 (08474) No. 80-2317	(1)-K2	
6680-00-526-6889	TACHOMETER, MECHANICAL LABORATORY, PETROLEUM TEST: (57733) No. 757W	(1)-F5	
8030-00-889-3535	TAPE, ANTISEIZING: polytetrafluoro-ethylene; used as an antiseize and sealant of pipe thd on liquid and gaseous oxygen systems of 2,000 lb psi and less; w/dispenser; 1/2 in. w, 260 in. lg; MIL-T-27730, size II	(2)-F2 (8)-R1	
5210-00-287-3335	TAPE, MEASURING: steel; general purpose; 1/2 in. w, graduated in 1/32, 1/16 and 1 in.; lh and rh reading; 72 in. lg; w/case, butt end, pull-push rewind; GGG-T-106, type V, class A, style 2	(1)-F3	
7510-00-082-2520	TAPE, PRESSURE SENSITIVE: 300 in. lg 3.4 in. w; A-A-113, TY II, CL A	(1 roll)-L3	
6630-00-359-9730	TEST BATH, CLOUD AND POUR POINT: copper and steel reservoir, 8-1/2 x 10 in.; w/cover, for ASTM TEST D-97; c/o. 4 ea CORK, TEST JARS: 4 ea JACKET: copper and cork disks and ring 4 ea JAR, TEST GLASS: 5 ea THERMOMETER: 4 ea TEST JAR CAP: (06542) FTMS 791 (23035) P/N K460	(1)-Y2 Y2 Y2 Y2-V	 Y2
6640-00-861-6215	TEST PAPER, LEAD ACETATE: type "B" strips; 100 strips per vial; for ASTM TEST D-2547; (22527) No. 14-862; (53078) No. S-65255 (15741) P/N G12500B	12-E3 Vials	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6630-00-442-9005	TEST PAPER AND COLOR CHART, HYDROGEN ION: color chart visible both sizes;		(1)-F2
	1 to 11 and 2 to 10 pH ranges; two 15 ft rolls in double refillable dispenser; w/:	(2)-L1	
	5 roll/pack TEST PAPER REFILL: 1 ro 11 pH range 6630-00-442-9015	1 pk-F2 2 pk-L1	
	5 roll/pack TEST PAPER REFILL: 2 to 10 pH range 6630-00-442-9025 NNN-T-001529, wide range, pH range 1 and 2, class A, style 1	1 pk-F2 2 pk-L1	
	TEST TUBE:		
6640-00-404-2757	Borosilicate glass; flat; 250 mm lg, 17 mm w, 9 mm thk; for copper strip test; for ASTM TEST D-130 (22527) No. 13-420-45	(6)-H2	(12)-Box 2
	Glass; NNN-T-189, type I, style I, size 9;		
6640-00-061-8967 (17)-Box 5	150 mm lg, 25 mm od		(5)-H2
6640-00-061-8966 (17)-Box 5	175 mm lg, 22 mm od		(5)-H2
6640-00-298-7258	Highly resistant to heat, chemically stable; 150 mm lg, 18 mm od, 1.75 mm wall thk; NNN-T-189, type I, style 2; MS36183-3	(5)-H2	(5)-Box 5
6630-00-244-9415	TESTER, FLASH POINT:		(1)-K4
	Electric heated; closed type, 110 v, 50/60 Hz, ac; two 20 to 230 deg F range thermometers; one brass sample cup; for ASTM TEST D-56; (23035) P/N K146	(1)-J2	
	Electrically heated;		(1)-A2
6630-00-530-0987	Closed type, 110 v, 60 Hz, ac; two thermometers; one 20 to 230 deg F range and one 200 to 700 deg F range; flexible metal shaft; for ASTM TEST D-93; MIL-T-36385 (48619) No. 74537		

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPAC (QTY)-BOX
6630-00-359-9787	Open type, 110 v, 60 Hz, ac; one thermometer, 20 to 760 deg F range; for ASTM TEST D-92; w/: 1 ea BOARD, REFRACTORY: 1 ea BURNER, GAS, TEST FLAME: 1 ea CLAMP, THERMOMETER: 1 ea CUP, PLATFORM: 1 ea DISK, REFRACTORY: 1 ea HEATER, AUTOMATIC: w/built-in autotransformer 1 ea HOOK, THERMOMETER: 1 ea PLATE, CAST IRON: (22527) No. 13-528	(1)-D (under centrifuge)	
	TOTE PAN, ICE: 18 x 12 x 6 35 Gal Polyethylene (13147) P/N 3509		
6630-00-404-2750	TETRAETHYL LEAD APPARATUS, PETROLEUM: TEST: for ASTM TEST D-2547; (80740) No. 69-007 (3 glass parts) Lurex Glass Co. Vineland, NJ, P/N 151-9151	(1 Prt) -G2 (1 Prt) -G4 (1 Prt) -K3	(1 ea, 3 Prts-Box 4
	THERMOMETER, SELF-INDICATING, BIMETALLIC:		
6685-00-975-0041	0 to 200 deg F range; dial; w/adapter; for ASTM TEST D-217 (48619) No. 73503	(1)-K2	
	THERMOMETER, SELF-INDICATING, LIQUID IN GLASS: Mercury; etched stem scale; Minus 20 to plus 50 deg C range; 1 deg accuracy rating; 0.5 deg smallest graduation; 57 mm immersion; w/expansion chamber and ring; 282 to 292 mm lg; for ASTM TEST D-56; ASTM E1 No. 57C (22527) No. 13-510-105	(2)-V	
	Minus 20 to plus 102 deg C range; 0.1 deg accuracy rating; 0.2 deg smallest graduation; 415 to 425 mm lg; w/expansion chamber and ring; for ASTM TEST E1 No. 12C	(4)-V	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	Minus 34 to plus 49 deg C range; 0.5 deg smallest graduation; total immersion; w/expansion chamber and ring; 300 to 305 mm lg; for ASTM TEST D-323; ASTM E1 No. 58C	(3)-V	
	Minus 38 to plus 50 deg C range; 0.5 deg accuracy rating; 2 deg smallest graduation; 108 mm immersion; 226 to 236 mm lg for ASTM TEST D-97; ASTM E1 No. 5C	(4)-V	
	Minus 38 to plus 42 deg F range; 0.5 deg smallest graduation; 51 mm immersion; w/expansion chamber and ring; 414 to 424 mm lg; for ASTM TEST D-611; ASTM E1 No. 33C	(1)-V	
	Minus 7 to plus 110 deg C range; 0.5 deg C accuracy rating; 0.5 deg smallest graduation; 57 mm immersion; 282 to 295 lg; for ASTM TEST D-93, ASTM E1 No. 9C	(4)-V	
	Minus 5 to plus 300 deg C range; 1 deg smallest graduation; 76 mm immersion; w/ring; 385 to 395 mm lg; ASTM E1 No. 2C	(2)-V	
	Minus 5 to plus 400 deg C range; 1 deg smallest graduation; 76 mm immersion; w/ring and carrying case; 408 to 418 mm lg; for ASTM TEST D-381; ASTM E1 No. 3C	(3)-V	
	Minus 6 to plus 400 deg C ranges; 1.0 deg accuracy rating; 5 deg smallest graduation; 25 mm immersion; w/ring; 303 to 315 mm lg; for ASTM TEST D-92; ASTM E1 No. 11C	(3)-V	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	Minus 2 to plus 300 deg C range; 0.5 deg accuracy rating; 1 deg smallest graduation; total immersion; w/ ring; 381 to 391 mm lg; for ASTM TEST D-86; ASTM E1 No. 7C	(5)-V	
	Minus 2 to plus 400 deg C range; 1 deg accuracy rating; 2 deg smallest graduation; total immersion, w/expansion chamber and rings; 381 to 391 mm lg; for ASTM TEST D-86; ASTM E1 No. 8C	(5)-V	
	Plus 25 to 105 deg C range; 0.2 deg C smallest graduation; 51 mm immersion; w/expansion chamber and ring; 414 to 424 mm; for ASTM TESTS D-611; ASTM E1 No. 34C	(3)-V	
	Plus 34 to plus 42 deg C range; .006 deg accuracy rating, 0.2 deg smallest graduation; total immersion; w/expansion chamber and ring; 280 to 290 mm lg; w/carrying case; for ASTM TEST D-323; ASTM E1 No. 18C	(3)-V	
6685-00-247-3765 (No "C" Scale Equiv.)	Plus 97.5 to plus 102.5 deg F range; 0.2 deg accuracy rating; 0.1 smallest graduation; total immersion; w/expansion chamber and ring; 300 to 310 mm lg; for ASTM TEST D-445; ASTM E1 No. 28F	(2)-V	
6685-00-247-3764 (No "C" Scale Equiv.)	Plus 127.5 to plus 132.5 deg F range; 0.2 deg accuracy rating; 0.1 deg smallest graduation, total immersion; w/expansion chamber and ring; 300 to 310 mm lg; for ASTM TEST D-445; ASTM E1 No. 29F	(2)-V	
	Plus 90 to plus 170 deg C range; 0.2 deg smallest graduation; 51 mm immersion, w/expansion chamber and ring; 414 to 424 mm lg; for ASTM TEST D-611; ASTM E1 No. 35C	(2)-V	

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	Plus 90 to plus 370 deg C range; 1.0 deg F accuracy rating; 2 deg smallest graduation; 57 mm immersion; w/expansion chamber and ring; 282 to 295 mm lg; w/carrying case; for ASTM TEST D-93; ASTM E1 No. 10C	(2)-V	
	Plus 95 to plus 103 deg C range; 0.1 deg accuracy rating; 0.1 smallest graduation; total immersion; w/expansion chamber and ring; 280 to 290 mm lg; w/carrying case; for ASTM TESTS D-525, D-873 and D-942; ASTM E1 No. 22C	(2)-V	
6685-00-242-3763 (No "C" Scale Equiv.)	Plus 207.5 to plus 215.5 deg F range; 0.2 accuracy rating; 0.1 smallest graduation; total immersion; w/expansion chamber and ring; 300 to 310 mm lg; for ASTM TEST D-445; ASTM E1 No. 30F	(2)-V	
	Minus 18 to plus 82 deg C range; 0.25 deg accuracy rating; 0.5 deg smallest graduation; total immersion; w/expansion chamber and ring; 300 to 305 mm lg; ASTM E1 No. 59C	(2)-V	
	Minus 20 to plus 150 deg C range; 0.5 deg accuracy rating; 1 deg smallest graduation; 76 mm immersion; w/ring; 317 to 327 mm lg; ASTM E1 No. 1C	(2)-V	
	Toluol, etched stem scale; minus 80 to plus 20 deg C range; 2 deg accuracy rating; 1 smallest graduation; 76 mm immersion; w/expansion chamber, 227 to 237 mm lg; for ASTM TEST D-97; ASTM E1 No. 6C	(4)-V	
	Minus 80 to plus 20 deg C range; 0.5 deg C, smallest graduated div, total immersion; 300 mm lg; ASTM E1 No. 114C	(2)-V	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
	THERMOMETER SET: minus 36 to plus 761 deg F, minus 38 to plus 405 deg C, calibrated; etched stem scale; set of 9; ASTM E1 No. 62C through 70C; (80740) No. 80-211-22 (15741) P/N G23792	(2)-F5	
	THERMOREGULATOR, MICRO-SET: regulating; 50 to 220 deg F range; provides accurate and rapid temp control; sealed glass unit; twin capillaries in stem that terminate in enlarged bulb; contacts sealed w/inert gas under pressure; 2-1/8 in. bulb, 14-1/2 in. lg; Thomas-Scientific, P/N 9366-H50	(5)-V (5 Bulb Sockets with wires)-X3	
6640-00-360-0011	THIMBLE, EXTRACTION: Alundum, dense; 70 x 25.4 mm od; for ASTM TEST D-473; (80740) No. 33-500-70 (22527) P/N 09-660B	(2)-K2	
6645-00-235-4685	TIMER, SWITCH, CLOCK, ELECTRICAL, PETROLEUM TEST: Self-sorting; 115 v, ac, 60 Hz, 10 Amp, 1000 W with cord and plug (22527) No. 6-657	(1)-G5	
6810-00-281-2002	TOLUENE, TECHNICAL: liquid; 1 gal can; for ASTM TESTS D-1796 and D-2550 TT-T-548		(2)-Box 6
	TONGS, LABORATORY:		
6640-00-360-0013	Beaker; cres; smooth jaws, covered w/mittens; 13 in. lg; for ASTM TESTS D-525 and D-873 (22527) No. 2-620	(2)-W3	
	Crucible;		
6640-00-444-8000	Cres; riveted joint; 9 in. lg; NNN-T-580; type III, composition A, size 1; MS36023-2	(2)-W3	

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6640-00-494-3779	Nickel chromium alloy; nickel plated finish; 9 in. lg; serated jaws; (22527) No. 15-190	(4)-W3	
6640-00-063-3420	Steel; double bent; 9 in. lg; smooth jaws; (22527) No. 15-186	(2)-W3	
5180-00-177-7033	TOOL KIT, GENERAL MECHANIC'S: Automotive SC 5180-90-CL-N26	(1)-W4	
7920-00-965-1709	TOWEL, PAPER: single fold; 15 in. w; 72 per self-dispensing box; UU-T-598	(1)-R4	(2)-Box 4
6640-00-436-9941	TRAY, LABORATORY: 12 x 7-5/8 x 2 in.; (80740) No. 82-005 (15747) P/N G22150K	(1)-A1	
	TRIANGLE, WIRE, LABORATORY: nickel chromium alloy wire, covered w/ glazed silica tubes; 2 in. inside lg of side (80740) 82-060 (15747) P/N G25402B	(3)-H1	
	TUBE, CENTRIFUGE:		(2)-F2
6640-00-477-3274	Borosilicate glass; 100 ml 24/40 std taper external joint; for ASTM TESTS D-322, D-1796 and D-2273; (75278) P/N 45241		
6640-00-445-6625	Graduated; conical bottom, 199 mm lg, 37 mm od, 17 mm id mouth; for ASTM TESTS D-91, D-1796 and FTMS TEST F-5101.5; NNN-T-780, type I, MS36165-1	(10)-E1	
6640-00-403-9342	TUBE, CENTRIFUGE, PETROLEUM TEST: borosilicate glass; 0.005 ml smallest graduations; for ASTM TEST D-2273; (80740) No. 69-030	(4)-E1	

Source: https://assist.dla.mil -- Downloaded: 202640-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6640-00-445-5000	TUBE, DRYING, LABORATORY: 150 mm; NNN-T-792, type I, size 2; MS36181-2	(4)-G3	
6640-00-436-9939	TUBE, FREEZING POINT APPARATUS: u/w Stand, Freezing Pt. Apparatus, 6640-00-377-9383; for ASTM TEST D-2386; (23035) P/N K297	(1 large)-H4 (2 small)-H3	(1 large)-Box 5
6640-00-360-0046	TUBE, MELTING POINT DETERMINATION: borosilicate glass; w/test tube, grease cup and rod; for ASTM TEST D-566; (23035) P/N K194-A0B	(2)-H2	
4720-00-360-0047	TUBING: for a 2 pen recorder for ASTM TESTS D-525 and D-873; (80740) No. 68-459-01; (48619) No. 74739	(1)-R	
	TUBING, PLASTIC: Flexible; for ASTM TEST D-2276;		
4720-00-410-9506	3/8 in. id; (80740) No. 74-995	25 ft-Box 3	
4720-00-411-5451	1/2 in. id; (80740) No. 74-995	25 ft-Box 3	
	Tygon, medical grade polyvinhl-chloride;		
4720-00-456-1036	1/4 in. bore size 10 Ft lg at ASTM TEST D-2276	(3)-10 ft roll-B3	(3)-10 ft roll-Box 4
4720-00-410-9505	3/8 in. bore size; 50 ft/lg (08071) R4000		(2)-Box 5
4720-00-411-5450	1/2 in. bore size; (80471) R4000		(30 ft)-Box 3
	TUBING: Natural;		
4720-00-640-0329	Translucent, heavy wall; .375 in. .125 in. wall thk, 3000 psi ts; 4 ft lg; for ASTM TEST D-2276; ZZ-T-831, type V, class 2; total 24 ft	(1)-F2	(5)-Box 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
4720-00-277-5388	3/16 in. id, 7/64 in. wall thk; 3000 psi; 10 ft lg; ZZ-T-831, type V, class 2	(1)-B3	
4720-00-260-6877	.188 in. bore, .188 in. wall thk; petroleum resistant; red; (81346) No. S73590C		(100 ft)-Box 5
4720-00-429-6874	.250 in. bore, .125 in. wall thk; 7 ft 6 in. lg; (81346) No. S73645	(4)-B3	
4720-00-729-6406	Neoprene; 50 ft lg; .188 in. bore, .063 in. wall thk; black; (22527) No. 14-171A	(1)-B3	
4720-00-273-1032	.250 in. bore, .094 in. wall thk; 2500 psi ts; petroleum resistant; (22527) No. 14-171B		(50 ft)-Box 5
	VISCOMETER, CAPILLIARY TYPE: Calibrated for opeque liquids; Cannon-Fenske reverse flow; for ASTM TEST D-445;		
6630-00-359-9888	Size 100; ASTM D-446	(2)-K1	(2)-Box 4
6630-00-359-9889	Size 200; ASTM D-446	(2)-K1	(2)-Box 3
6630-00-359-9890	Size 300; ASTM D-446	(2)-K1	(2)-Box 3
6640-00-359-9891	Size 400; ASTM D-446	(2)-K1	(2)-Box 4
6630-00-450-3479	Size 500; ASTM D-446	(2)-K1	(1)-Box 3
6630-00-450-5699	Size 600; (22527) No. 13-615-5J7-2	(2)-K1	
	Calibrated for transparent liquids; Cannon-Fenske routine; for ASTM TEST D-445;		
6630-00-359-9886	Size 25; ASTM D-446	(1)-J1	(2)-Box 4
6630-00-397-9293	Size 50; ASTM D-446	(2)-J1	(2)-Box 4

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6630-00-359-9903	Size 100; ASTM D-446	(2)-J1	(2)-Box 4
6630-00-359-9904	Size 200; ASTM D-446	(2)-J1	(2)-Box 4
6630-00-359-9905	Size 300; ASTM D-446	(2)-J1	(2)-Box 4
6630-00-397-9309	Size 400; ASTM D-446	(2)-J1	(1)-Box 4
6630-00-397-9311	Size 450; ASTM D-446	(1)-J1	(1)-Box 4
6630-00-359-9892	Size 500; ASTM D-446	(1)-J1	(1)-Box 4
6630-00-359-9893	Size 600; (22527) No. 13-617	(2)-J1	(1)-Box 3
6640-00-314-2097	WASH BOTTLE, LABORATORY: polyethelene; 500 ml; (22527) No. 3-409-10; (53078) S-9486C	(2)-P2	
	WATCH GLASS, LABORATORY: Circular;		
6640-00-290-6808	65 mm dia; DD-W-131 Class A MS36000-1 (15747) P/N G28705C	(6)-X4	
6640-00-290-6789	100 mm dia; DD-W-131, class A; MS36000-3 (15747) P/N G28705F	(8)-X4	
6640-00-848-8209	150 mm dia; borosilicate glass; heavy wall; chemical durability; fire polished edge; DD-W-131, class A; MS36000-5 (15747) P/N G28705H	(8)-X4	
6640-00-282-5708	3 1/2" (90 mm) dia; borosilicate glass ribbed on convex side; (15747) P/N G1860B	(1)-X4	
6640-00-282-5717	4" (100 mm) dia; borosilicate glass; ribbed on convex side; (15747) P/N G1860C	(1)-X4	

Source: https://assist.dla.mil -- Downloaded: 202610-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
6670-00-351-2356	WEIGHT SET, BALANCE: Co-bs, class S; w/forceps, in filled box; 1 ea Weight, BALANCE: cres, cadmium plated; 1 gm 2 ea Weight, BALANCE: cres, cadmium plated; 2 gm 1 ea Weight, BALANCE: cres, cadmium plated; 5 gm 1 ea Weight, BALANCE: cres, cadmium plated; 10 gm 2 ea Weight, BALANCE: cres, cadmium plated; 20 gm 1 ea Weight, BALANCE: cres, cadmium plated; 50 gm 1 ea Weight, BALANCE: tantalum; fractional; 500 mg 2 ea Weight, BALANCE: tantalum; fractional; 200 mg 1 ea Weight BALANCE; tantalum; fractional; 100 mg 1 ea Weight BALANCE: tantalum; fractional; 50 mg 2 ea Weight BALANCE: tantalum; fractional; 20 mg 1 ea Weight BALANCE: tantalum; fractional; 10 mg (22527) No. 2-214A	(1)-F4	(1)-Box 3
6670-00-803-9680	Brass; 1 to 1000 gm; tall form; NBS, class C tolerance; w/vinyl plastic block; 12 wt; AAA-W-200, set	(1)-F4	
	WING TOP LABORATORY GAS BURNER: brass; 1/2 in od burner tube; friction fit mtg, (15747) No. G39028	(1)-F5	
6640-00-360-0067	WRENCH: for gum stability bomb for ASTM TESTS D-525 and D-873 (80740) No. 68-456, (48619) No. 74741	(1)-H1	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Table 1. Packing of equipment in mobile laboratory cabinets and overpack boxes

NATIONAL STOCK NUMBER	DESCRIPTION	QUANTITY/LOCATION LAB (QTY)-DRAWER SEE FIG 1, 2, 3	QUANTITY/LOCATION OVERPACK (QTY)-BOX
5120-00-244-4389	WRENCH, BUNG: multiple size; non-sparking, nonmagnetic; 20 different bungs accom; for ASTM TEST D-270; GGG-W-642	(1)-K4	(1)-Box 5
6810-00-815-6105	XYLENE, ACS: 350 ml; for ASTM TESTS D-56 and D-95; O-C-265		(2)-Box 6
6810-00-241-1157	ZINC OXIDE, ACS: powder; 1 lb per bottle; MIL-STD-1218; O-C-265		(1)-Box 7

*U.S. GOVERNMENT PRINTING OFFICE 1987-704-036/70132

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

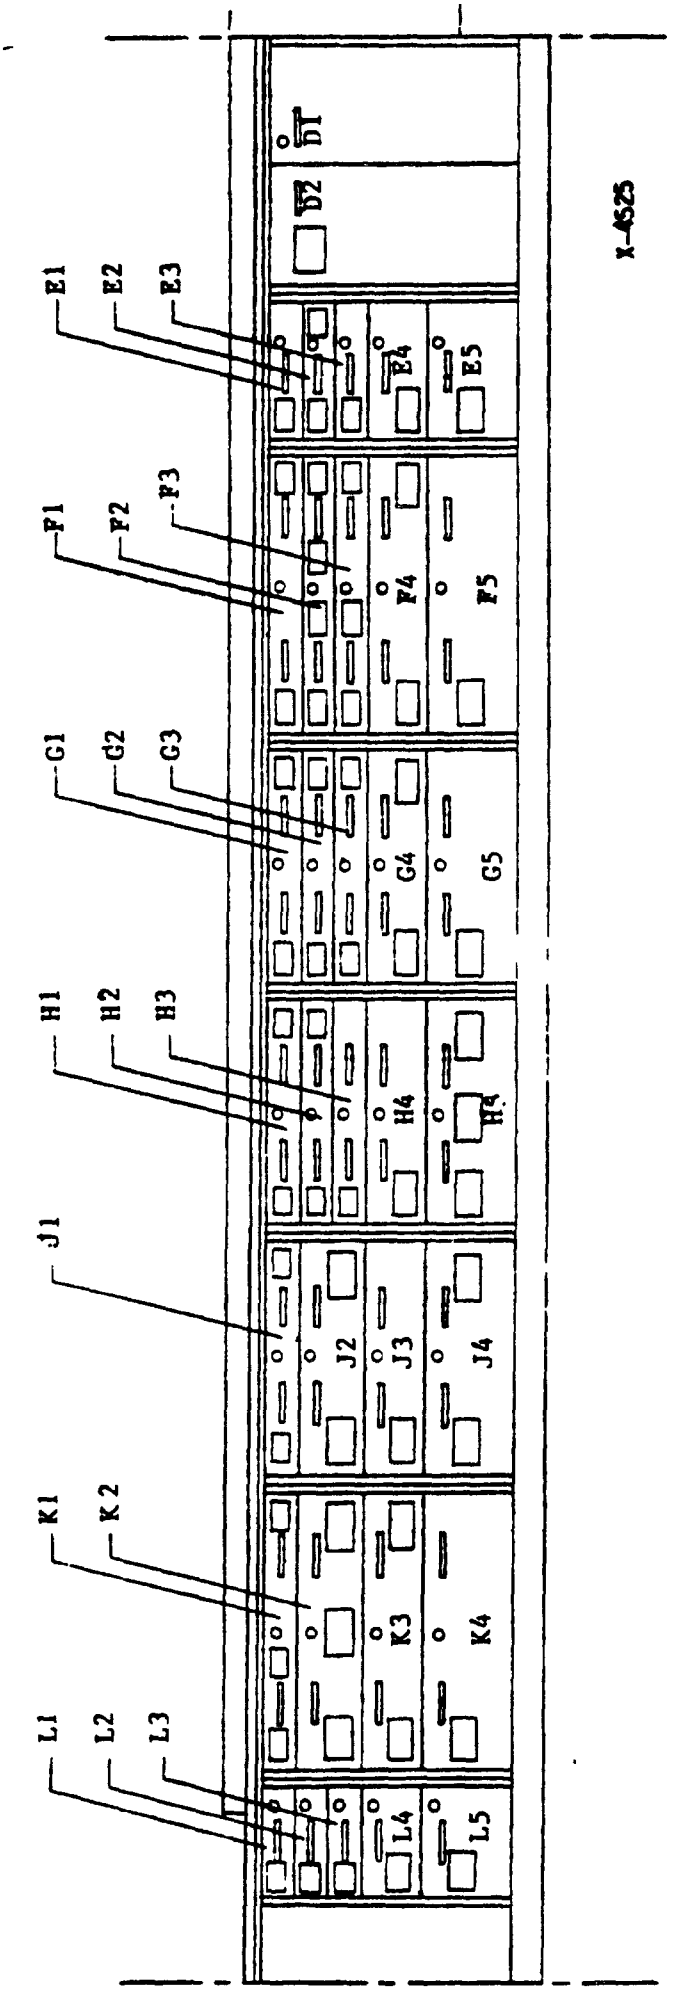


FIGURE 1. Roadside cabinet installation

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

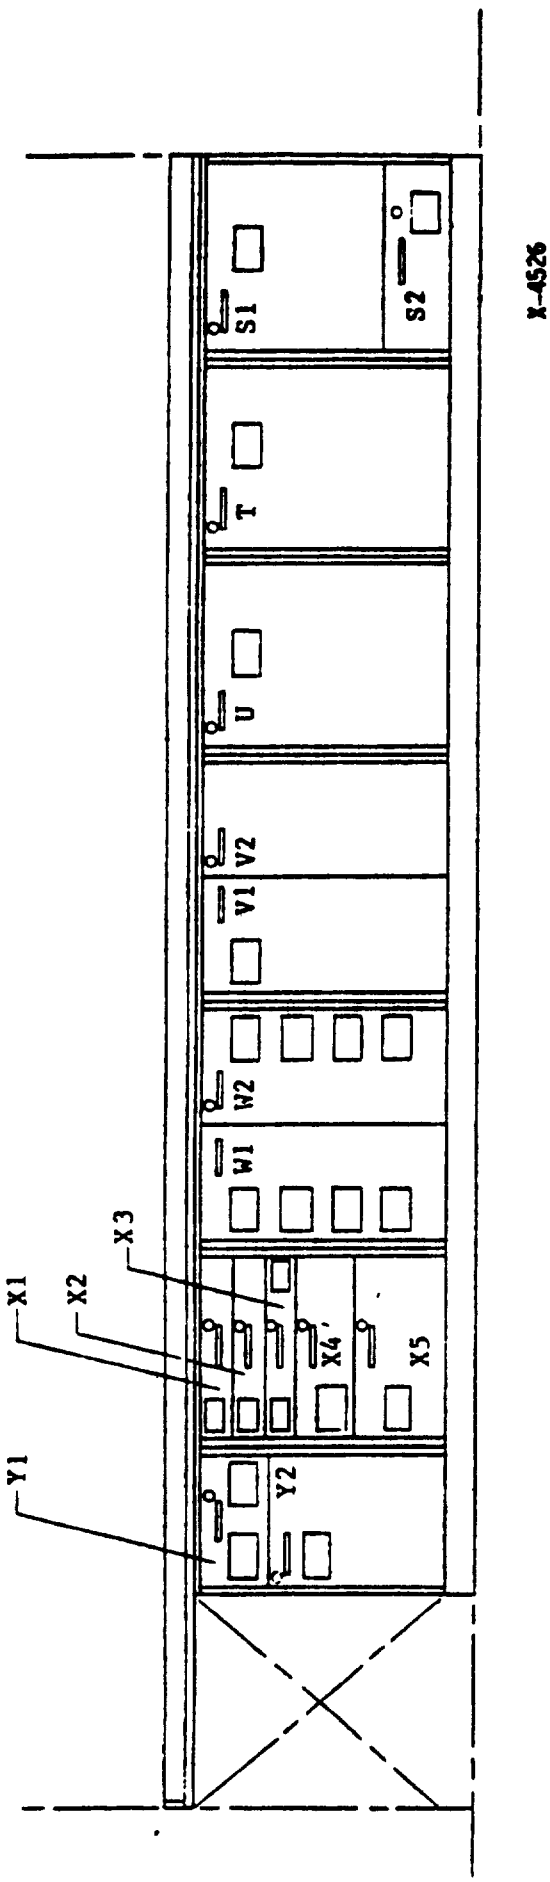


FIGURE 2. Curbside cabinet installation

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

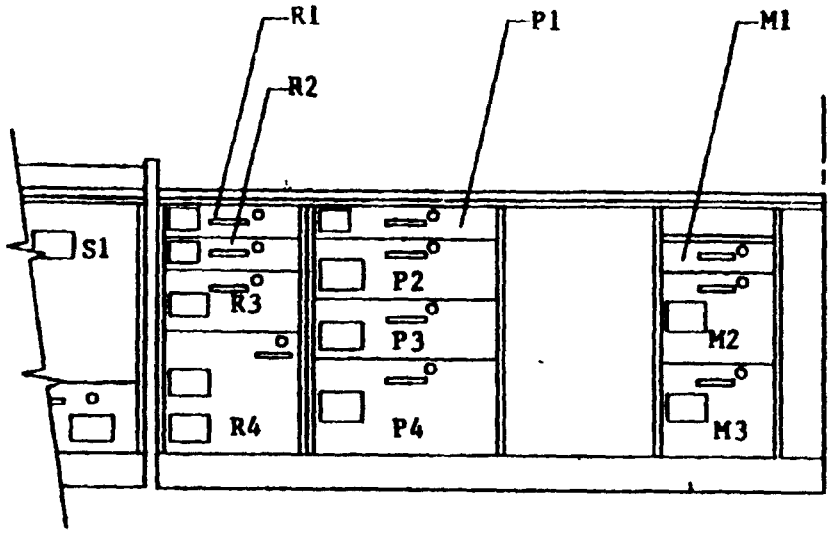


FIGURE 2. Curbside cabinet installation - continued

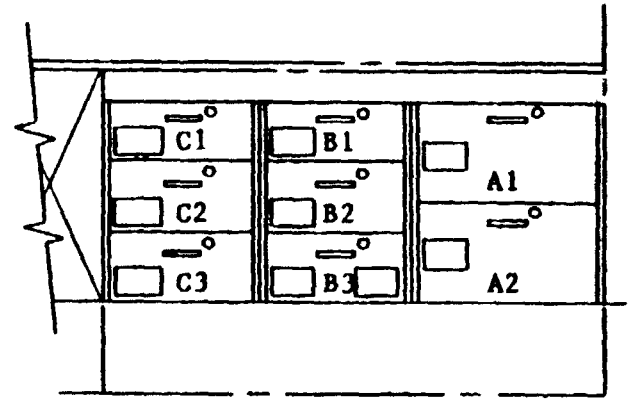


FIGURE 3. Fume hood & gum bath cabinets

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEPARTMENT OF THE ARMY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 12062 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEPARTMENT OF THE ARMY

Commander
US Army Belvoir RDE Center
ATTN: STRBE-TSE
Ft. Belvoir, VA 22060-5606

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
MIL-L-0051050C(ME)	Laboratory, Petroleum, Semitrailer Mounted

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR ☐ USER ☐ MANUFACTURER ☐ OTHER *(Specify)*: _____
b. ADDRESS *(Street, City, State, ZIP Code)*	

5. PROBLEM AREAS

a. Paragraph Number and Wording.

b. Recommended Wording

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T04:04Z
Check the source to verify that this is the current version before use.