MIL-C-42028 (DM)
6 October 1986

MILITARY SPECIFICATION

# COMPRESSOR-DEHYDRATOR, DENTAL EQUIPMENT, PORTABLE, 115 Volts, 60 Hz, AC

This specification is approved for use within DLA, Defense Personnel Support Center (DM), and is available for use by all Departments and Agencies of the Department of Defense.

## 1. SCOPE

1.1 Scope. This specification covers a portable air compressor-dehydrator suitable for use with NSN 6520-00-140-7663, DENTAL OPERATING AND TREATMENT UNIT, FIELD.

## 2. APPLICABLE DOCUMENTS

2.1 Government documents.

2.1.1 Specifications and standards. The following specifications and standards form a part of this specification to the extent specified herein. Unless otherwise specified, the issues of these documents shall be those listed in the issue of the Department of Defense Index of Specifications and Standards (DODISS) and supplement thereto, cited in the solicitation.

SPECIFICATIONS

FEDERAL

| | |
|---|---|
| L-P-390 | - Plastic, Molding and Extrusion Material, Polyethylene, and Copolymers (Low, Medium, and High Density). |
| PPP-B-601 | - Boxes, Wood, Cleated-Plywood. |

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-RST, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

MILITARY

| | |
|---|---|
| MIL-M-7298 | - Manual, Technical, Commercial Equipment. |
| MIL-L-10547 | - Liners, Case and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible. |
| MIL-V-27166 | - Valve, Pressure Equalizing, Gaseous Products. |
| MIL-C-46168 | - Coating, Aliphatic Polyurethane, Chemical Agent Resistant. |

STANDARDS

FEDERAL

| | |
|---|---|
| FED-STD-101 | - Test Procedures for Packaging Materials. |

MILITARY

| | |
|---|---|
| MIL-STD-105 | - Sampling Procedures and Tables for Inspection by Attributes. |
| MIL-STD-129 | - Marking for Shipment and Storage. |
| MIL-STD-147 | - Palletized Unit Loads. |
| MIL-STD-794 | - Parts and Equipment, Procedures for Packaging of. |
| MIL-STD-1472 | - Human Engineering Design Criteria for Military Systems, Equipment and Facilities. |

(Copies of specifications and standards required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting activity).

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise specified, the issue of the documents which are DoD adopted shall be those listed in the issue of the DoDISS specified in the solicitation. Unless otherwise specified, the issues of documents not listed in the DoDISS shall be the issue of the non-government document which is current on the date of the solicitation.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

UNDERWRITERS' LABORATORY, INC. (UL)

UL 544 Standard for Safety Medical and Dental Equipment

(Application for copies should be addressed to the Underwriters' Laboratories, Inc., 207 East Ohio Street, Chicago, IL 60611, 333 Pfingsten Road, Northbrook, IL 60062, 1285 Walt Whitman Road, Melville, LI, NY 11746, and 1655 Scott Blvd., Santa Clara, CA 95050).

2.3 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification shall take precedence. Nothing in this specification, however, shall supersede applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

3.1 Materials. Materials shall be as specified herein. When materials are not specifically designated, those used shall be new, of the same or better quality as used in commercial practice, and entirely suitable for the purpose intended. When dissimilar metals are used in contact with each other, suitable protection against galvanic corrosion shall be applied to material.

3.2 First article. The contractor shall furnish one or more compressors as specified for examination and testing within the time frame specified by contracting officer to prove prior to starting production that his production methods will produce compressors that comply with the requirements of this specification. Examination and tests shall be as specified herein. All examinations and tests shall be conducted by the contractor subject to surveillance and approval by the Government.

3.3 Description. The air compressor and dehydrator shall be a portable, compact, integral unit using a nominal 1.5 horsepower (hp) motor coupled directly to compressor. The unit shall be equipped with a storage tank and an air dryer, all stored within a reinforced carrying case. The system shall be reliable under harsh field conditions at temperatures from 40 to 120 degrees Fahrenheit ($^{o}$F).

3.4 Design, construction and performance.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

3.4.1 Compressor. The compressor shall be of the oil-less type, producing 100 percent (%) oil-free air without the use of coalescent or other types of filters. The compressor cylinders and cylinder heads shall be finned for maximum heat dissipation. A spring-jacket, lap-joint type teflon compression ring and teflon guide sleeve shall be used on each piston. All cylinders shall have brass sleeve liners. Rotating components shall be dynamically balanced. Valves shall be of leaf-type construction. The compressor crankcase shall be ventilated with built-in cooling fan.

The compressor shall be capable of producing an air flow of no less than 5.4 standard cubic feet per minute (scfm) at 60 pounds per square inch gauge (psig) and a dew point of no greater than 0°F at 80 psig. Compressor noise level shall be no greater than 77 decibel scale A (dBa) with the case cover placed above compressor on support arms and measured in accordance with tests specified in 4.4.3.1 and 4.4.3.2. The compressor shall meet the aging test specified in 4.4.3.6.

3.4.2 Dryer. The air dryer shall be of the single-tower, desiccant type. Dryer regeneration shall be automatic each cycle. Dryer shall employ a totally pneumatic mechanism such that only dry air is stored and no condensate shall form in the storage tank at temperatures above 0°F. Dew point measurement shall be made at 80 psig and after operation at a 40 percent duty cycle, averaged over a 15 minute period in accordance with test specified in 4.4.3.3. The drying chamber shall be field replaceable.

3.4.3 Motor. The compressor shall be capacitor start and capacitor run with a heavy-duty centrifugal switch. Shall be of the totally enclosed, fan cooled type with cast end bells and stator housing to minimize noise. A high-efficiency fan shall cool the motor and also cool the compressed air before it is introduced into the desiccant chamber. The compressor shall be directly coupled to the motor without the use of gear boxes or belts. The front motor bearing shall be oversized and shall be both press-fitted and "lok-tited" in place to prevent outer race rotation. Motor bearings shall be ball bearing type, permanently lubricated, with high temperature grease. The motor shall be nominally 1800 RPM (revolutions per minute) and rated at 1.5 hp, with a maximum operating current rating not exceeding 20 amperes. The motor shall operate on 115 volts, 60 hertz, alternating current power. The motor maximum winding temperature shall not exceed 130°F (above ambient). A line circuit breaker shall provide a power control to the unit and electrical overload protection to the motor.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

3.4.4 Cord. An electric cord, at least 10 feet in length with "hospital grade" plug shall be provided to permit connection of air compressor to electrical system. The air compressor shall withstand the dielectric strength test specified in 4.4.3.8.

3.4.5 Storage tank. The storage tank shall be at least 3.0 gallons and tested to meet the requirements of A.S.M.E Boiler and Pressure Vessel code or be National Board Approved (stamped UM, inspected by tank manufacturer). Tank shall be constructed for internal pressure of at least 375 psig at 650°F. The inside of the tank shall be treated or coated for protection against and the prevention of corrosion and rust. The storage tank shall be provided with a pressure gauge reading in pounds per square inch, a pressure relief valve and a visual moisture monitor to indicate that the stored air is dry. A manual drain valve for contingency use shall be provided.

3.4.6 Pressure gauge. An air pressure gauge shall be mounted on storage tank. The gauge shall be graduated from 0 to 100 psig.

3.4.7 Pressure relief valve. The pressure relief valve shall be mechanically operated requiring no electrical power, wiring or switches. The valve shall operate automatically, sensing pressure in the storage tank and activating to prevent pressure build-up greater than 125 psig in storage tank.

3.4.8 Pressure switch. Shall be an Underwriters' Laboratories (UL) recognized, heavy duty double-pole, snap-action switch, actuated by pressure in the tank to start and stop compressor to maintain a pressure differential of 20 psi, starting with the compressor at 60 psig and stopping the compressor at 80 psig.

3.4.9 Hoses and fittings. The compressor shall be provided with two (2) high pressure air delivery hoses each 10 feet in length and fitted with a No. 294-PB, 3/8 inch O.D. female Kwik-Connect Coupler body, or equal, on one end, and a No. 294-PM, 3/8 inch O.D. male Kwik-Connect Coupler, or equal, on the other end.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

3.4.10 Case. The compressor shall be furnished completely assembled in a olive drab, rotationally molded, corrosion resistant, dust-proof, moisture vapor proof and rigid polyethylene reuseable carrying storage case. The storage case shell material shall meet the requirements of Federal Specification L-P-390 for type I, class M, grade 2, polyethylene or equal. The case shall be lined with a sound absorbing material. Provisions shall be made to permit compressor operation with the cover portion of the carrying case elevated at least four inches above the lower portion, by means of rotatable support arms so as to achieve maximum sound reduction. The case shall be equipped with a cushioning and support system sufficient to protect the contents from damage in transit and storage due to vibration, shock, or compression. Materials used in case design and construction shall be compatible with chemical agent decontamination or painted with a chemical agent resistant aliphatic polyurethane coating in accordance with MIL-C-46168.

The case shall provide the compressor storage and transport protection in environments where temperatures range from 40° to 60°C (storage) and minus 30° to 50°C (transport) and relative humidity range from 0 to 95% (non-condensing).

An automatic/manual pressure/vacuum relief valve in accordance with MIL-V-27166 (set at ± 0.5 psig) shall be installed within a recessed area of the case wall (see 4.4.3.7). Seal shall be verified by pneumatic pressure technique of Federal Standard Test Method 101, method 5009. The case outer surfaces shall be self draining when stored in the normal upright shipping attitude.

The case shall have corrosion resistant steel, spring loaded, fullgrip 90° stop handles, capable of being used by personnel wearing gloves or mittens. Inside dimension of the bail shall be 4 inches by 1.5 inches minimum. Quantity and placement of handles shall be in accordance with MIL-STD-1472. The mounting of compressor and case design shall meet the vibration and shock tests specified in 4.4.3.4 and 4.4.3.5, respectively. The case, with compressor packed inside shall not exceed 10,000 cubic inches or 160 pounds in total weight.

3.5 Finish. The compressor shall be fabricated from materials which are inherently resistant to corrosion or which are treated to render them corrosion-resistant. Where painting or plating is used, appropriate cleaning and priming shall be performed prior to finishing. Unless otherwise specified, finish shall be equivalent or superior to that of comparable commercial equipment, and shall be free of gaps, scratches, chips and other imperfections.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

3.6 Workmanship.

3.6.1 Castings. All castings shall be free of extraneous material such as sand, dirt, pits, sprues, scale, and flux. Fins resulting from line-of-parting of sand molds shall be ground or machined flush with adjacent material. Imperfections in castings may be corrected by welding provided it will cause no degradation in strength or performance.

3.6.2 Welding. The surfaces of parts to be welded shall be free from rust, scale, burn spots, paint, grease, and other foreign matter. Welds shall transmit stress without permanent deformation or failure when the parts connected by the welds are subjected to proof and service loading. Complete and uniform penetration and fusion of the metal shall be obtained.

3.6.3 Metal fabrication. Metal sheet and plate used in the fabrication of the compressor shall be free from kinks and sharp bends. The straightening of material shall be done by methods that will not cause cracking or permanent deformation. Shearing and clipping shall be done neatly and accurately. Corners shall be square and true. Flame cutting may be employed. All bends of a major character shall be made with metal dies or fixtures in order to insure uniformity of size and shape. All burrs and rough edges shall be removed.

3.6.4 Bolted connections. Bolt holes shall be punched or drilled and shall have the burrs removed. All bolts, nuts and screws shall be tightened so that they will not work loose under vibration.

3.7 Identification marking. Each unit shall be marked with the following information:

COMPRESSOR - DEHYDRATOR, DENTAL EQUIPMENT,
PORTABLE, 115 Volts, 60 Hz, AC
NSN 6520-00-139-1246

Name or registered trademark of
the manufacturer

Contract or purchase order number

Serial number

3.8 Tolerances. Where tolerances are not specified, standard commercial tolerances shall be permissible. Tolerances shall be held to a minimum where accuracy is of paramount importance for proper operation and interchangeability of component parts. Assemblies shall be precision-fitted for durable, smooth, and consistent functioning.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

3.9 Interchangeability. All parts having the same manufacturer's part number shall be functionally and dimensionally interchangeable.

3.10 Service data. The contractor shall furnish, with each compressor two copies each of the technical manual which contains complete instructions for installation, operation, maintenance, and list of component parts. The manual shall comply with the requirements of MIL-M-7298.

As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer, via the cognizant Government inspector, two preliminary copies of his proposed technical manual, for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract or purchase order. In addition, the Contractor shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of the contract and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies may be waived upon request to the Contracting Officer. Waiver of submission of 15 additional copies shall be at the option of the Government.

## 4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements. Certificates of quality may be furnished for the following: material composition, hardness, tempers, torque requirements on springs, machining and casting requirements (such as flatness, concentricity, and finish), and plating or coating.

4.2 Classification of inspection. The inspection requirements specified herein are classified as follows:

1. First article inspection (see 4.3).

2. Quality conformance inspection (see 4.4).

4.3 First article inspection. When a first article is specified in the contract, the first article inspection shall consist of all examinations specified herein, and all testing specified herein and shall apply to the first article sample only (see 6.2). The failure of compliance with any examination or test shall be cause for rejection of the first article.

4.4 Quality conformance inspection. Except as otherwise specified herein, sampling for inspection shall be performed in accordance with the provisions set forth in MIL-STD-105.

4.4.1 End item examination.

4.4.1.1 Visual examination. End item examination shall be conducted in accordance with the following classification of defects. Examination shall include, but shall not be limited to, the defects listed in table I. The inspection level shall be II with an acceptable quality level (AQL) of 1.0 for major defects and an AQL of 10 for minor defects. The unit of product shall be the component of an end item or an end item, as applicable.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

TABLE I. End Item Classification of Defects.

| | Major | Minor |
|---|---|---|
| **Design and Construction:** | | |
| Design and construction of unit not as specified. | X | |
| **Hardware:** | | |
| Components, such as pins, screws, and fasteners missing, broken, stripped, cracked or deformed. | X | |
| Fasteners loose. | | X |
| **Finish:** | | |
| Finish not as specified. | X | |
| Surfaces not clean, not free of foreign matter, flux, spatters, or other defects. | | X |
| Damage or defects on exterior or interior surfaces, such as burrs, slivers, cracks, or sharp edges which effect function or serviceability. | X | |
| Damage or defects on exterior or interior surfaces, such as burrs, slivers, cracks, or sharp edges which do not effect function or serviceability. | | X |
| Plating missing (affecting function). | X | |
| Plating missing (not affecting function). | | X |
| Plating not uniform in appearance. | | X |
| Plating not free from blisters, peeling, visible porosity, or other defects. | X | |
| **Workmanship:** | | |
| Any component fractured, broken, punctured, torn, burned, bowed, deteriorated, corroded, or malformed. | X | |
| Any component dented or creased. | | X |
| Any component misplaced or not in proper alignment. | X | |
| Any component not connected or not joined properly. | | X |
| Fastening device requiring loosening or removal is swaged, peened, staked, or otherwise permanently fastened. | X | |
| Components missing. | X | |
| Components do not fit or mate properly. | X | |
| Interface fits between components not proper (too loose, too tight/binding). | X | |
| Components not free from defects which may impair their serviceability. | X | |



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

| | Major | Minor |
|---|---|---|
| Workmanship (cont'd): | | |
| Components not free from defects which do not impair their serviceability. | | X |
| Removable components cannot be removed and replaced without difficulty. | X | |
| Components not properly assembled or aligned. | X | |
| Machine work: | | |
| Coarse machine, tool, or die marks which affect function or serviceability. | X | |
| | X | |
| Coarse machine, tool, or die marks which do not affect function or serviceability. | | X |
| Identification Marking: | | |
| Identification marking missing, incomplete, not legible. | | X |
| Identification marking incorrect or not permanent. | | X |
| Marking not properly located. | | X |
| Service Data: | | |
| Service data not included. | X | |

4.4.2 Dimensional examination. Dimensional examination shall be conducted for compliance with dimensions specified. Any dimension not within specification tolerance shall be a defect. The inspection level shall be S-3 with an AQL of 1.0. Unit of product shall be the component of an end item or an end item, as applicable.

4.4.3 End item testing. End item testing shall be conducted in accordance with MIL-STD-105 and as indicated in table II, except that the acceptance number shall be zero for all sample sizes. Unit of product shall be compressor - dehydrator.

TABLE II. Sampling for tests.

| Component | Requirement | Test Procedure | Inspection level |
|---|---|---|---|
| Air delivery | 3.4.1 | 4.4.3.1 | S-2 |
| Noise level | 3.4.1 | 4.4.3.2 | S-2 |
| Moisture Removal | 3.4.2 | 4.4.3.3 | S-2 |
| Vibration Test | 3.4.10 | 4.4.3.4 | S-2 |
| Shock Test | 3.4.10 | 4.4.3.5 | S-2 |
| Case seal pressure | 3.4.10 | 4.4.3.7 | S-2 |
| Dielectric strength | 3.4.4 | 4.4.3.8 | S-2 |



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

4.4.3.1 Air delivery. The compressor output shall be measured with an air flow meter when storage tank pressure is 60 psig. Airflow shall be at least 5.4 scfm (324 scfh).

4.4.3.2 Noise level. The compressor noise level shall be measured with a sound measuring device capable of measuring sound level on an "A WEIGHTED SCALE". Set up the compressor with its cover mounted over the unit on the four (4) rotatable support arms provided. Operate the unit. Sound measurements shall be made in a plane 36 inches above the floor, at a distance of 24 inches from the unit.

4.4.3.3 Moisture removal. The compressor shall be operated at a 40 percent duty cycle averaged over a 15 minute period. Connect air line from storage tank outlet to a Dew-point Apparatus (Lectrodryer or equal) and fill apparatus inner cup with acetone. Insert thermometer capable of measuring -100°F to + 100°F into inner cup.

Slowly add dry ice to lower its temperature. When moisture is observed to form on reflecting surface of Dew-point Apparatus, record the temperature. This temperature is the dew-point of the compressed air at 14.7 pounds per square inch absolute (psia). Using the conversion chart in Figure 1, convert this dew point to dew point at 80 psig. Maximum dew-point shall be 0°F at 80 psig.

4.4.3.4 Vibration test. Each of the six faces of the unit in its transit case shall be placed, in turn, on a vibration platform. Operate the platform at 140 cycles per minute with 1 inch displacement. Vibrate each face for 10 minutes. Observe for damage and repeat air delivery test above (see 4.4.3.1).

4.4.3.5 Shock test. Drop each face of compressor in its case onto a piece of two-inch (2") thick plywood covering a concrete or steel surface, from a height of 36 inches.

4.4.3.6 Aging test. Place compressor in an environmental chamber capable of maintaining a temperature as low as -65°F and as high as 160°F.

a) Raise temperature to +160°F and maintain for 48 hours.
b) Decrease temperature to +100°F and check compressor for proper operation.
c) Increase temperature to +160°F and maintain for 4 hours.
d) Decrease temperature to +100°F and check compressor for proper operation.

Perform steps (a) through (d) a total of three (3) times.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

e) Reduce temperature to -65°F and maintain for 72 hours.
f) Increase temperature to +72°F and check compressor for proper operation.

Perform steps (e) and (f) once.

4.4.3.7 Case seal pressure. The case seal shall be verified by pneumatic pressure technique of Federal Standard Test Method 101, method 5009.

4.4.3.8 Dielectric strength. A dielectric test in accordance with UL requirements shall be performed after compressor has been warmed by operation. The compressor shall be operated to determine proper functioning. The compressor shall not be defective.

4.5 Inspection of packaging. The sampling and inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

5. PACKAGING.

5.1 Preservation. Preservation shall be level A or C, as specified (see 6.2).

5.1.1 Level A. Each compressor-dehydrator, along with accessories, shall be positioned within the carrying case specified in 3.4.10.

5.1.2 Level C. Each compressor-dehydrator, along with accessories, shall be preserved as specified in 5.1.1.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

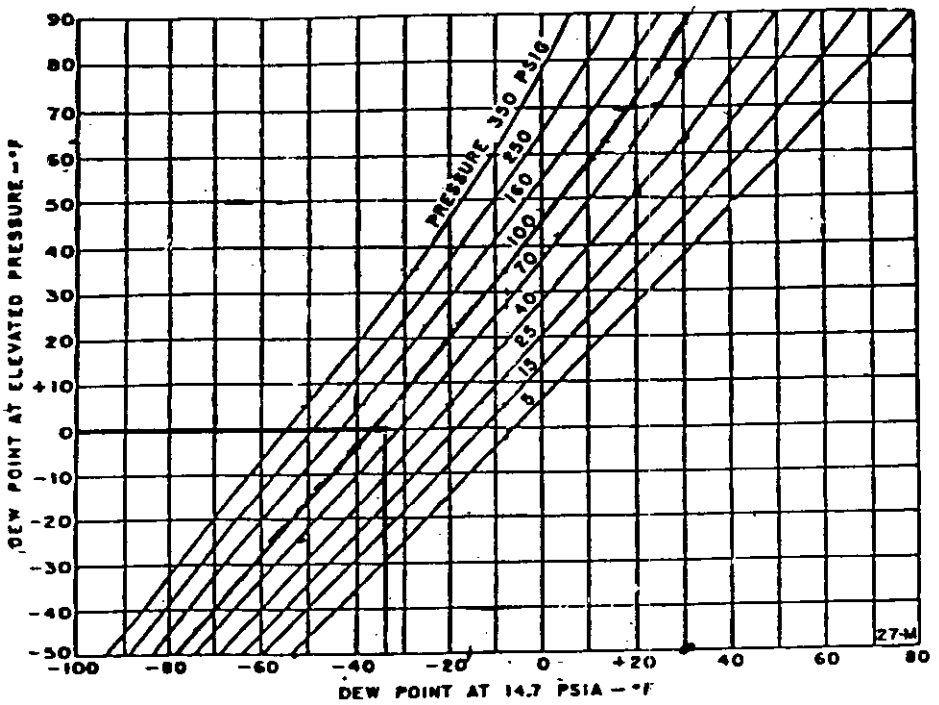



Figure 1. Dew Point Conversion Chart



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

5.2 Packing. Packing shall be level A or C, as specified (see 6.2).

5.2.1 Level A. Each unit positioned within the carrying case as specified in 5.1.1 shall be further packed in an exterior container conforming to PPP-B-601, overseas type. The container shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing of the liner shall be as specified in the liner specification. The carrying case shall be cushioned within the box by use of fiberboard pads or other suitable material to prevent the case from rupturing the liner. Closure and strapping shall be as specified in the box specification.

5.2.2 Level C. Each unit positioned within the carrying case as specified in 5.1.2 shall be packed as specified in MIL-STD-794 for level C.

5.2.5 Unitized loads. Unitized loads, commensurate with the level of packing specified in the contract or order, shall be used whenever total quantities for shipment to one destination equal 40 cubic feet or more. Loads shall be unitized on pallets conforming to MIL-STD-147. Quantities less than 40 cubic feet need not be unitized. Pallet loads including the pallet shall not exceed 43 inches in height, 48 inches in width, and 40 inches in length. Pallet shall conform to Type IV or Type V.

5.2.5.1 Level A. Compressor-dehydrators packed as specified in 5.2.1 shall be unitized on pallets as specified in 5.2.5.

5.2.5.2 Level C. Compressor-dehydrators packed as specified in 5.2.2 shall be unitized as specified in MIL-STD-794.

5.3 Marking.

5.3.1 Levels A and C. Each carrying case, exterior container and unitized load shall be marked as specified in MIL-STD-129.

5.4 General.

5.4.1 Exterior container. Exterior container (see 5.2.1 and 5.2.2) shall be of minimum tare and cube consistent with the protection required.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.5.



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

6. NOTES.

6.1 Intended use. The compressor-dehydrator is intended to be used as a dry air source for NSN 6520-00-140-7663 DENTAL OPERATING AND TREATMENT UNIT, FIELD.

6.2 Ordering data.

6.2.1 Acquisition requirements. Acquisition documents should specify the following:

a. Title, number and date of this specification.
b. First article, when required (see 3.2).
c. Selection of applicable levels of preservation and packing (see 5.1 and 5.2).

6.3 National Stock Number (NSN) coverage. This specification covers the following item listed in the Federal Supply Catalog.

| NSN | ITEM IDENTIFICATION |
|---|---|
| 6520-00-139-1246 | COMPRESSOR-DEHYDRATOR, DENTAL EQUIPMENT, Portable, 115 volt, 60 Hz, AC |

6.4 Subject term (key word) listing.

Compressor-Dehydrator
Dental Equipment
Portable

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DOD-MB

Agent:

DLA-DM

Project No. 6520-1976
Location: NCR DISK-7



Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.

# STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

*(See Instructions – Reverse Side)*

| 1. DOCUMENT NUMBER | 2. DOCUMENT TITLE |
|---|---|
| MIL-C-42028 (DM) | COMPRESSOR-DEHYDRATOR, DENTAL EQUIPMENT, PORTABLE, 115V, 60H,AC |

| 3a. NAME OF SUBMITTING ORGANIZATION | 4. TYPE OF ORGANIZATION *(Mark one)* |
|---|---|
| | ☐ VENDOR<br>☐ USER<br>☐ MANUFACTURER<br>☐ OTHER *(Specify)*: _____ |
| b. ADDRESS *(Street, City, State, ZIP Code)* | |

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

| 7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional | b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional |
|---|---|
| c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional | 8. DATE OF SUBMISSION *(YYMMDD)* |

*(TO DETACH THIS FORM, CUT ALONG THIS LINE.)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T20:15Z
Check the source to verify that this is the current version before use.