AA-S-00651a (DSA-DM)

30 August 1966

Interim Revision of
Fed. Spec. AA-S-651
1 June 1951

INTERIM FEDERAL SPECIFICATION

CABINET, MEDICINE, COMBINATION

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification AA-S-651 dated 1 June 1951.

1. SCOPE

1.1 This specification covers a combination medicine cabinet with open upper section for storing large clinical utensils and bulky dressings for which an entirely closed cabinet is not adequate.

2. APPLICABLE SPECIFICATIONS, STANDARDS, DRAWINGS AND OTHER PUBLICATIONS

2.1 Specifications and standards. The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

FF-C-77	Casters, Institutional Duty.
UU-P-271	Paper, Wrapping, Waterproofed Kraft.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

Military

MIL-L-10547 Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

STANDARDS

Federal

FED-STD-NO. 66 Steel, Chemical Composition and Hardenability.

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which included cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C., 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 First Article. Unless otherwise specified, prior to the start of production of the contract quantity, one sample of the medicine cabinet shall be assembled, completely finished, and tested by the contractor. The sample shall be submitted, together with the contractor's inspection and test reports, to the procuring contracting officer for examination and testing to determine compliance with the requirements of this specification. Written approval of the materials, construction, and performance of the sample shall be obtained from the procuring contracting officer, or his authorized representative, prior to the manufacture and assembly of the remaining quantity to be manufactured. Pending approval of the first article, acquisition of materials, components, or commencement of production is at the sole risk of the contractor. Accepted sample shall become the property of the procuring activity and shall be included in the quantity called for in the contract or order. In the event that the sample is not approved, the contractor shall submit a new sample for approval, or modify the existent sample so as to remove the deficiencies cited.

3.2 Material. All materials used in fabrication of the medicine cabinet shall be as specified herein. Commercial tolerances on gage sizes shall apply.

3.2.1 Steel. Steel shall conform to the requirements of FED-STD-66 for class 302 or 304.

3.2.2 Tubing. Tubing shall be seamless or welded construction corrosion-resisting steel of a chemical composition similar to the sheet steel.

3.3 Construction. The combination medicine cabinet shall consist of a cabinet mounted in a tubular frame, two shelves located above the cabinet, and guard rails. Construction and dimensions shall be as shown in Figure 1.

3.3.1 Frame. Frame shall consist of 1-inch outside diameter tubing with 0.062 inch wall thickness, No. 16, United States Standard (U.S.S.) gage, mounted on casters. The two rear legs forming the back supports shall be straight. The two front legs shall be curved diagonally in midway to allow for the reduced width of the shelves. Uprights or legs shall be closed flush at top by welding.

Source: https://assist.dla.mil -- Downloaded: 20261O-26T11:40Z
Check the source to verify that this is the current version before use.

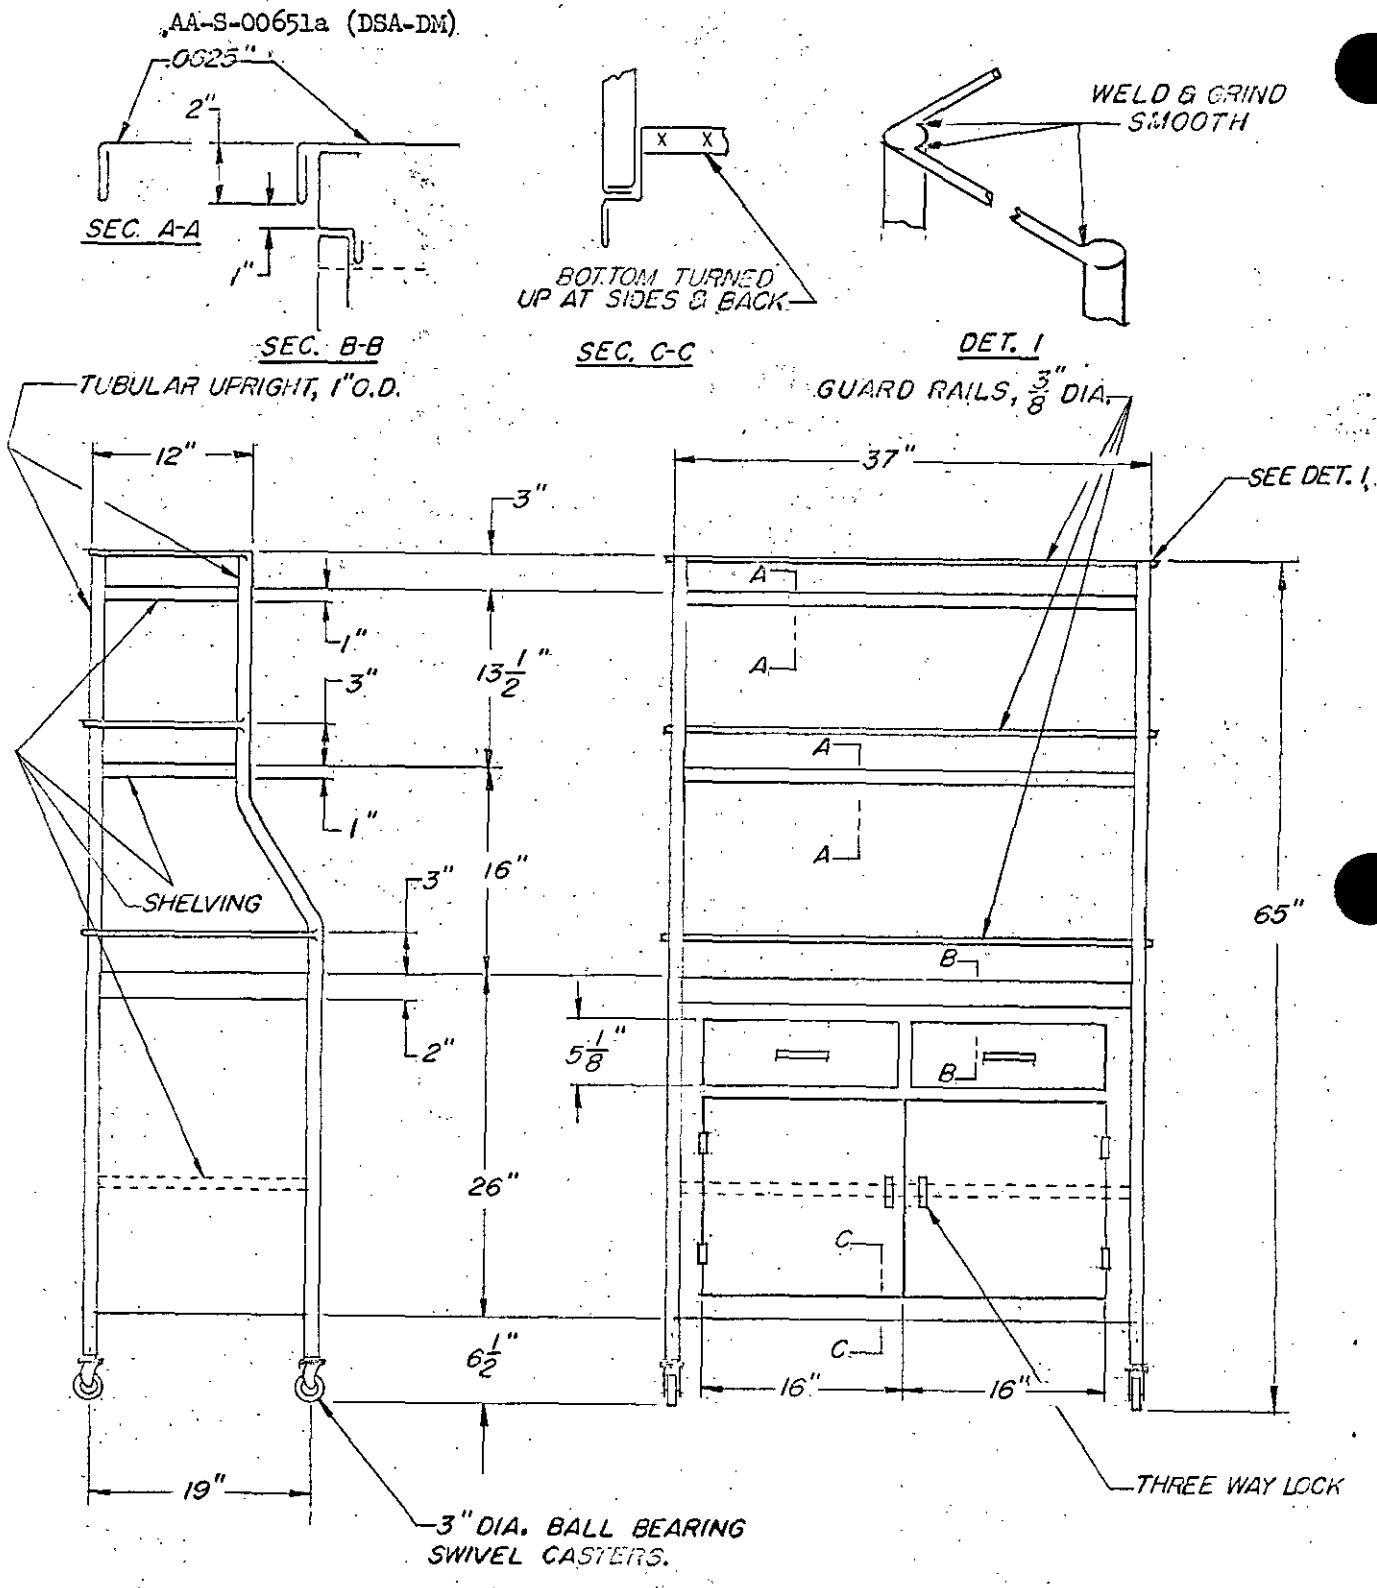


FIGURE 1
Combination Medicine Cabinet (CRS)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

3.3.1.1 Casters. The casters shall conform to FF-C-77 for type II, class F, size 3, wheel style 4, mounting A.

3.3.2 Cabinet. Cabinet shall be constructed of 0.050 inch thick, No. 18, U.S.S. gage, corrosion-resisting steel, 36 inches long and 18 inches wide. The lower portion of the cabinet shall be fitted with two doors with a drawer above each door and an inner shelf. Cabinet shall be neatly welded to legs at a height 6 1/2 inches above floor level including casters. The cabinet body and shelf shall be notched out to the radius of the tubing and shall be perpendicular to the tubing. Body shall be welded to tubing on the inside. Shelf shall be continuously welded to the tubing along the notches on the underside. The front face of the cabinet shall be welded to give a seamless appearance without joints or crevices. All inner edges of cabinet facia shall be flanged inward for a distance of 15/16-inch and then formed at a 90° angle and hemmed to form a rabbet for the doors and drawers. Side and back panels shall each be one piece. The bottom shall be constructed of 0.050 inch thick sheet No. 18, U.S.S. gage, with the front edge suitably formed to provide a rabbeted recess for recessing the door in flush position. The recess shall flange downward from the bottom for easy cleaning. Back and sides of bottom shall be flanged-up and spot-welded to body.

3.3.2.1 Doors. Doors shall be of 0.037 inch thick, No. 20, U.S.S. gage, double-walled construction with reinforcing channel the full height of door. Both inner and outer panels shall be pan-shaped, with the inner panel fitting tightly inside the outer and welded together. Suitable fire-resistant, sound-deadening material shall be placed in door and drawer fronts. Doors shall be dust-proof, the outer surface being flush with front face of cabinet. Door faces shall be seamless.

3.3.2.1.1 Lock. Right-hand door shall be equipped with a triplex key-in-handle chromium-plated latch and the left-hand door fitted with a dummy handle of similar design. Active leaf shall close against a strike welded to the back of the inactive leaf, which shall have a catch to prevent its swinging open. Both doors shall close against rubber bumpers.

3.3.2.1.2 Hinges. Doors shall be hung on semi-concealed, fast-pin, five-knuckle, cabinet butt hinges of corrosion-resisting steel. Cabinet frames and door frames shall be notched out to receive these hinges so that only the butts are visible on the outside.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:40Z
Check the source to verify that this is the current version before use.

3.3.2.2 Drawers. Bodies of drawers shall be 0.037 inch thick, No. 20, U.S.S. gage, welded to box-type double-walled fronts of same thickness, and fitted with chromium-plated cast brass or cast aluminum handles. Sound-deadening material shall be enclosed in double-walled drawer fronts. Drawers shall travel on 0.078 inch thick, No. 14, U.S.S. gage, slides 2 1/4 inches high at front welded to drawer housing. Front of slide shall have a roller bearing with face not less than 5/16-inch. Behind the roller bearing the slide shall be formed to provide a track 3/8-inch wide by 3/8-inch high under which another roller bearing shall ride. This bearing shall be fastened to the back of a companion glide of Z-shaped section welded to each side of drawer body. Drawer head shall close against rubber bumpers and be flush with the front of the casing, resting in an intergral rabbeted frame.

3.3.2.3 Inner shelf. Midway between bottom of cabinet and top of cupboard shall be welded the inner shelf with a 1 inch flange. The front edge of the shelf shall be fully hemmed.

3.3.3 Exterior shelves. Exterior shelves shall be constructed of 0.062 inch thick, No. 16, U.S.S. gage, corrosion-resisting steel. Shelves shall be closely welded to uprights with all joints ground smooth. All edges of shelves shall be flanged downward 1 inch and fully hemmed. Shelves shall be 12 inches wide and 36 inches long.

3.3.4 Guard rails. Continuous guard rails of 3/8-inch rod shall be fully welded between the ends of frame, 2 1/2 inches above upper shelves and cabinet top. Welds shall be ground smooth and shall blend with adjacent surfaces.

3.4 Finish. All exposed surfaces of corrosion-resisting steel shall have a No. 4 commercial finish.

3.5 Identification marking. Each medicine cabinet shall be permanently marked with the following:

Manufacturers name or registered trademark

Contract or purchase order number

Federal stock number

Letters U.S.

Markings secured by adhesives shall not be used.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:40Z
Check the source to verify that this is the current version before use.

3.6 Workmanship. Workmanship shall be first class throughout. Units shall be free from defects which detract from their appearance or which may impair their serviceability. Forming shall be neatly done without scratches or tears.

3.6.1 Welding. The welding shall be electric-arc or oxyacetylene welding using welding rod of composition similar to parent metal. Welds shall be thorough, nonporous, cleaned, ground, and finished smooth to match adjoining surfaces. Welds shall be free from pit marks and other imperfections. All surfaces shall be free from sharp edges.

4. SAMPLING, INSPECTION AND TEST PROCEDURES

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties)of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105.

For visual examination	Inspection level	AQL (defects per hundeed units)
Major defects	II	1.0
Total (major and minor combined) defects	II	4.0
For dimensional examination	S1	2.5

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:40Z
Check the source to verify that this is the current version before use.

4.3 Examination. The cabinets shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Categories and defects*

Major

101 Any component missing.
102 Any component fractured, split, cracked, punctured, cut, dented, sprung, malformed, creased, or otherwise impaired, affecting serviceability (check flanges and hems).
103 Any part misplaced, loose, or not in proper alignment, affecting serviceability.
104 Any sharp edge, burr, or sliver.
105 Any operation omitted or not properly performed.
106 Any functioning component, inoperative or will not operate as intended.
107 Any screw stripped, missing, or loose.
108 Any weld missing or not complete.
109 Any weld burned through, cracked, or undercut.

Minor

201 Finish not as specified; not free of scratches, rough grind marks, and other defects.
202 Unit not clean; not free of dirt, oil, and grease.
203 Any weld not free of flash, splatter, flux, and burns.
204 Any weld not ground and polished to blend with adjacent surfaces; not free of pit marks and seams.
205 Identification marking missing, incomplete, impermanent, or illegible.
206 Rubber bumper missing.
207 Sound-deadening material missing.

*Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The cabinets shall be examined for defects in dimensions. Any dimension not within the tolerance specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One cabinet, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Unit preparation. Casters shall be removed, adequately protected, and packaged within the cabinet or drawer in such a manner as to prevent damage during shipment or storage. Exterior finished surfaces of the cabinet shall be protected by wrapping with kraft paper or by a kraft paper shroud, and by cushioning at points of contact of interior braces or interior faces of container with excelsior pads or flexible corrugated fiberboard. Wrapping and cushioning material shall be secured in position. Work shall be accomplished in such a manner as to insure against marring, scratching, or damage to the unit.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Each unit, prepared as specified in 5.1.2.1, shall be packed in an exterior container designed for type 3 load, and constructed in accordance with PPP-B-601, table II, using type III, class 1 plywood; or PPP-B-621, table IV. The unit shall be adequately secured within the exterior container by means of bolts, wood braces, or other interior fittings, to insure against shifting, breakage, or marring or denting of surfaces. All box panels, except base, shall be lined with waterproof barrier material conforming to requirements of UU-P-271, class L-2 in such a manner as to prevent direct entry of water. The exterior container design shall include three skids of not less than 1-1/2 inches in thickness applied crosswise of base, so positioned as to facilitate handling with a fork lift truck and to maintain unit in an upright position. Closure shall comply with appendix of applicable box specification. Strapping will not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

5.2.2 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Exterior containers. Exterior container shall be marked in accordance with MIL-STD-129.

In addition, arrows shall be applied in accordance with paragraph 5.6.7.3 of MIL-STD-129. Instructions for opening the container shall be stencilled on the front panel.

Example: Instructions for UNPACKING

1. LAY FLAT.

2. Remove this panel.

3. Remove interior braces.

4. STAND container in upright position.

5. REMOVE CABINET."

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packing (see 5.1 and 5.2).
(c) When first article is not required (see 3.1).
(d) Where first article shall be sent (see 3.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

6.2 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity *(as indicated on reverse hereof)*.

SPECIFICATION

AA-S-00651a (DSA-DM)

ORGANIZATION *(Of submitter)*

CITY AND STATE

CONTRACT NO.

QUANTITY OF ITEMS PROCURED

DOLLAR AMOUNT

$

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES.

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO IF "YES", IN WHAT WAY?

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity)*

DATE

DD FORM 1426

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.