FEDERAL SPECIFICATION

STAND AND CABINET COMBINATION, DRESSING ROOM

This specification was approved on the above date by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal Agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers a combination dressing room stand and cabinet constructed of corrosion-resisting steel.

1.2 Classification.—This specification covers one type, grade, and size of combination dressing room stand and cabinet.

2. APPLICABLE SPECIFICATIONS

2.1. The following Federal Specifications, of the issues in effect on the date of invitation for bids, form a part of this specification:

FF–C–86–Casters; Truck.

QQ–S–766 — Steel, Corrosion-Resisting, Plates, Sheets, Strips, and Structural Shapes.

(Copies of Federal Specifications and the Federal Specifications Index may be obtained upon application, accompanied by money order, coupon, or cash, to the Superintendent of Documents, Government Printing Office, Washington 25, D. C. Prices may be obtained from the Superintendent of Documents.)

2.2. Specifications applicable only to individual departments are listed in section 7.

3. REQUIREMENTS

3.1 Material.—Material shall conform in all respects to the applicable specifications and as hereinafter specified.

3.1.1 *Steel.*—Steel shall conform to the requirements of Specification QQ–S–766 for class 1 or class 2 and shall be subject to tolerances stated therein.

3.1.2 *Tubing.*—Tubing shall be seamless or welded construction corrosion-resisting steel of a chemical composition similar to the sheet steel.

3.2 Construction and dimensions.—Unit shall consist of a cabinet mounted in a tubular frame with two shelves located above the cabinet. Construction and dimensions shall be as shown in figure 1.

3.2.1 *Frame.*—Framework shall consist of 1-inch outside diameter, 0.0625-inch wall thickness tubing mounted on casters. The two rear legs forming the back supports shall be straight. The two front legs shall be curved diagonally in midway to allow for the reduced width of the shelves. Uprights or legs shall be closed flush at top by welding.

3.2.1.1 *Casters.*—The casters shall be 3-inch diameter rubber-tired, ball bearing swivel conforming to the requirements of Federal Specification FF–C–86, type II, class B.

3.2.2 *Cabinet.*—Cabinet shall be constructed of 0.050-inch-thick corrosion-resisting steel approximately 36 inches long and approximately 18 inches wide. Cabinet shall be neatly welded to legs at a height approximately 6½ inches above floor level including casters. The lower portion of the cabinet shall be fitted with two doors with a drawer above each door. The front face of the cabinet shall be welded to give a seamless appearance without joints or crevices. All inner edges of cabinet facia shall be flanged inward for a distance of $^{15}/_{16}$ inch and then formed at 90° and hemmed to form a rabbet for the doors and drawers. Side and back panels shall each be one piece. The bottom shall be constructed of 0.050-inch-thick sheet with the front edge suitably formed to provide a rabbeted recess for recessing the door in flush position. The recess shall flange downward from the bottom for easy cleaning. Back and sides of bottom shall be flanged-up and spot-welded to body.

3.2.3 *Doors.*—Doors shall be of 0.0375-inch-thick double-walled construction with reinforcing channel the full height of door. Both inner and outer panels shall be pan-shaped, with the inner panel fitting tightly inside the outer and welded together. Suitable fire-resistant,

901680—51—No. 265

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

sound-deadening material shall be placed in door and drawer fronts. Doors shall be dustproof, the outer surface being flush with front face of cabinet. Door faces shall be seamless.

3.2.4 *Lock.*—Right-hand door shall be equipped with a triplex key-in-handle chromium-plated latch and the left-hand door fitted with a dummy handle of similar design. Active leaf shall close against a strike welded to the back of the inactive leaf, which shall have a catch to prevent its swinging open. Both doors shall close against rubber bumpers.

3.2.5 *Hinges.*—Doors shall be hung on semi-concealed, fast-pin, five-knuckle, cabinet butt hinges of chromium-plated brass or bronze. Cabinet frames and door frames shall be notched out to receive these hinges so that only the butts are visible on the outside.

3.2.6 *Drawers.*—Bodies of drawers shall be 0.0375 inch thick, welded to box-type double-walled fronts of same thickness, and fitted with chromium-plated cast brass or cast aluminum handles. Sound-deadening material shall be enclosed in double-walled drawer fronts. Drawers shall travel on 0.078-inch thick slides 2¼ inches high at front welded to drawer housing. Front of slide shall have a roller bearing with face not less than 5/16 inch. Behind the roller bearing the slide shall be formed to provide a track ⅜ inch wide by ⅜ inch high under which another roller bearing shall ride. This bearing shall be fastened to the back of a companion glide of Z-shaped section welded to each side of drawer body. Drawer head shall close against rubber bumpers and be flush with the front of the casing, resting in an integral rabbeted frame.

3.2.7 *Inner shelf.*—Midway between bottom of cabinet and top of cupboard shall be welded a permanent shelf with a 1-inch flange. The front edge of the shelf shall be fully hemmed.

3.2.8 *Exterior shelves.*—Exterior shelves shall be constructed of 0.0625-inch-thick corrosion-resisting steel. Shelves shall be closely welded to uprights with all joints ground smooth. All edges of shelves shall be flanged downward 1 inch and fully hemmed. Shelves shall be 12 inches wide and 36 inches long.

3.2.9 *Guard rails.*—Continuous guard rails of ⅜-inch rod shall be fully welded around back and ends of frame approximately 2½ inches above upper shelves and cabinet top. Welds shall be ground smooth and shall blend with adjacent surfaces.

3.2.10 *Welding.*—The welding shall be electric-arc or oxyacetylene welding, continuous on all contact surfaces, using welding rod of composition similar to parent metal. Welds shall be thorough, nonporous, cleaned, ground, and finished smooth to match adjoining surfaces. Welds shall be free from pit marks and other imperfections. All surfaces shall be free from sharp edges.

3.3 Finish.—All exposed surfaces of corrosion-resisting steel shall be finished in a No. 4 commercial finish.

3.4 Workmanship.—Workmanship shall be first class throughout. Units shall be free from defects which detract from their appearance or which may impair their serviceability. Forming shall be neatly done without scratches or tears.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *Cabinets.*—Unless otherwise specified, each unit delivered shall be inspected and tested.

4.2 Inspection.—Each unit shall be inspected for material, design, dimensions, construction, accessories, finish, workmanship, packaging, packing, and marking.

4.3 Tests.

4.3.1 *Performance.*—Each unit shall be tested for operational performance.

5. PREPARATION FOR DELIVERY

5.1 Packaging.—Unless otherwise specified, each stand and cabinet shall be packaged in accordance with accepted commercial practice.

5.2 Packing.—The subject commodity shall be prepared for shipment to permit acceptance by carrier for transportation at the lowest applicable rate and to afford maximum protection from normal hazards of transportation.

5.3 Marking.

5.3.1 *Shipping containers.*—Unless otherwise specified, each shipping container shall be marked with the name of the commodity as defined by the contract or order under which the shipment is made, the quantity contained

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

therein, the name of the contractor, the number of the contract or order, the name and address of the consignee, and the gross weight.

6. NOTES

6.1 Ordering data.—Purchasers should exercise any desired options offered herein. (See 4.1.1, 5.1, 5.3.1, 6.3, and 7.2.6.)

6.2 This specification covers the following item listed in the Armed Services Catalog of Medical Matériel:

7–082–715—Stand and Cabinet Combination, Dressing Room, CRM.

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.4 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification or which are commercially available but is intended to cover the type, size, etc., which is normally procured to meet Federal Government requirements.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

7. DEPARTMENTAL REQUIREMENTS

7.1 The following specifications, of the issues in effect on date of invitation for bids, and special requirements form a part of this specification for purchases made under this specification by the respective departments.

7.2 Army, Navy, and Air Force.

7.2.1 *Applicable specifications.*

Federal Specifications:

NN–B–601 — Boxes; Wood-Cleated-Plywood, for Domestic Shipment.

NN–B–621—Boxes; Wood, Nailed and Lock-Corner.

Military Specifications:

JAN–P–105—Packaging and Packing for Overseas Shipment — Boxes, Wood, Cleated, Plywood.

JAN–P–106—Packaging and Packing for Overseas Shipment — Boxes, Wood, Nailed.

JAN–P–125—Packaging and Packing for Overseas Shipment—Barrier-Materials, Waterproof, Flexible.

JAN–P–140—Packaging and Packing for Overseas Shipment—Adhesives, Water-Resistant, Case Liner.

MIL–M–3157—Marking of Domestic Shipments by Contractors for Supplies and Equipment Consigned to the Medical Departments of the Armed Services.

U. S. Army Specification:

100–73—Crates, Wood, Nailed, Domestic Shipment, 1,000 Pounds Maximum Net Load.

Navy Department Specification:

General Specifications for Inspection of Material.[1]

(Copies of specifications required for Army and Air Force purchases may be obtained upon application to the procuring agency. Both the title and identifying symbol or number should be stipulated when requesting copies.)

(Copies of Federal and Military specifications required for Navy purchases and Navy Department specifications may be obtained without cost upon application to the Bureau of Supplies and Accounts, Department of the Navy, Washington 25, D. C., except that Naval activities should make application to the Commanding Officer, Naval Supply Depot, Scotia 2, New York. Both the title and identifying symbol or number should be stipulated when requesting copies of specifications.)

7.2.2 *Inspection procedures (Navy only).*—The general inspection procedures shall be in accordance with General Specifications for Inspection of Material.

[1] Applicable for Navy purchases only.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

7.2.3 *Packaging.*—Each unit shall be protected by wrapping with kraft paper and cushioning with excelsior pads or flexible corrugated fiberboard or other suitable materials. All wrapping and cushioning material shall be secured by tying with twine or sealing with kraft gummed paper tape.

7.2.4 *Packing.*

7.2.4.1 *Domestic.*—Each unit shall be packed in a shipping container conforming to the requirements of Federal Specification NN-B-601 or NN-B-621. As an alternate to the above, each unit shall be packed in a three-way-corner crate conforming to the requirements of U. S. Army Specification 100-73. In addition to the regular specification requirements, the shipping container design shall include skids of appropriate size to facilitate handling and to maintain unit in an upright position. The unit shall be adequately secured within the shipping container by means of bolts, wood braces, blocks, or other suitable devices to insure against shifting and breakage or marring of surfaces. The work shall be accomplished in such a manner that the weight of the unit will not be carried directly by its legs or casters.

7.2.4.2 *Overseas.*—Each unit shall be packed in a shipping container designed for type 3 load and conforming to the requirements of Military Specification JAN-P-105 or JAN-P-106. Closure and strapping shall conform to the requirements of the appendix to the applicable box specification. Each shipping container shall be lined with a sealed waterproof bag, or its equivalent, made from material conforming to the requirements of Military Specification JAN-P-125, for case liners; seams and closures shall be completely sealed with a continuous seam at least ¾ inch wide of water-resistant adhesive conforming to the requirements of Military Specification JAN-P-140. In addition to the regular specification requirements, the shipping container design shall include skids of appropriate size to facilitate handling and to maintain unit in an upright position. The unit shall be adequately secured within the shipping container by means of bolts, wood braces, blocks, or other suitable devices to insure against shifting and breakage or marring of surfaces. The work shall be accomplished in such a manner that the weight of the unit will not be carried directly by its legs or casters.

7.2.5 *Marking.*

7.2.5.1 *Shipping containers.*

7.2.5.1.1 *For domestic shipment.*—Each shipping container shall be marked in accordance with Military Specification MIL-M-3157.

7.2.5.1.2 *For overseas shipment.*—Each shipping container shall be marked as specified by the procuring agency.

7.2.6 *Ordering data.*—Procurement documents should specify whether the subject commodity is to be packed and shipping containers marked for domestic or overseas shipment. (See 7.2.4 and 7.2.5.)

Navy Interest: Md

(See following figure 1.)

This specification is a part of Section IV, Part 5, of the Federal Standard Stock Catalog

For sale by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C. Price 5 cents.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

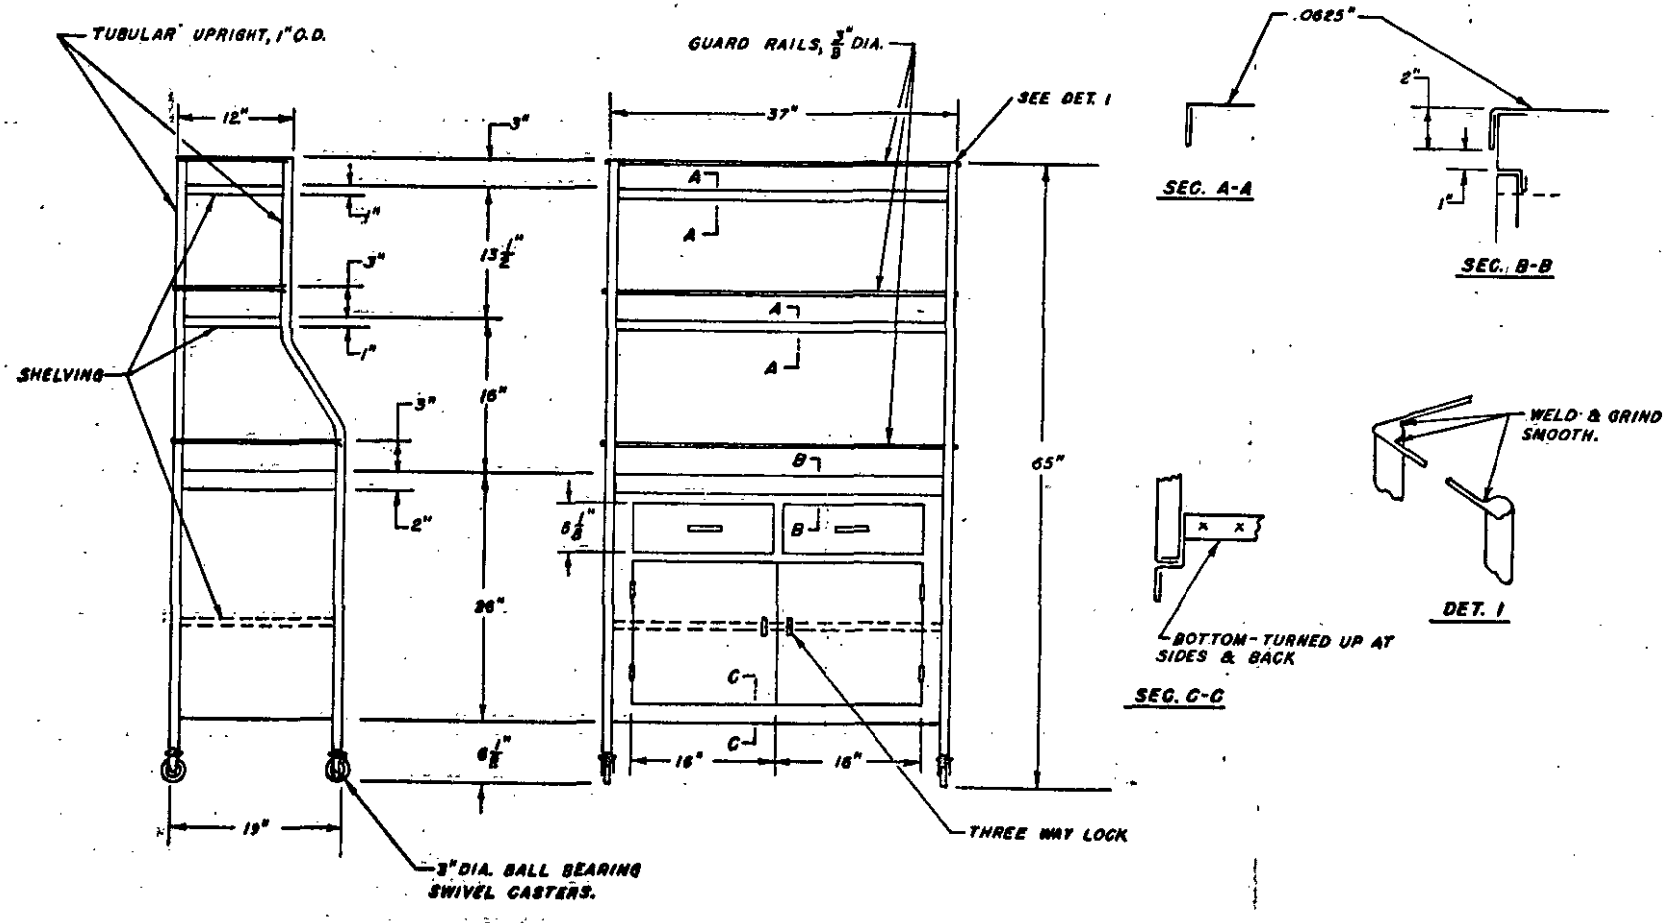


FIGURE 1.—*Stand and cabinet combination, dressing room (ORM).*

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 119-R004

INSTRUCTIONS

This sheet is to be filled out by personnel either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity *(as indicated on reverse hereof)*.

SPECIFICATION

ORGANIZATION *(Of submitter)*

CITY AND STATE

CONTRACT NO.

QUANTITY OF ITEMS PROCURED

DOLLAR AMOUNT
$

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES.

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO IF "YES", IN WHAT WAY?

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity)*

DATE

DD FORM 1 APR 63 1426 REPLACES NAVSHIPS FORM 4863, WHICH IS OBSOLETE C-0270

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:40Z
Check the source to verify that this is the current version before use.