AA-S-696B
October 1, 1976
SUPERSEDING
Fed. Spec. AA-S-696A
March 26, 1962

FEDERAL SPECIFICATION

STOOL, REVOLVING, SURGEON'S

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 Scope. This specification covers one type of surgeon's adjustable revolving stool.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

Federal Specifications:

PPP-B-636 - Boxes, Shipping, Fiberboard.

Federal Standards:

Fed. Std. No. 66 - Steel, Chemical Composition and Hardenability.
Fed. Std. No. 123 - Marking for Shipment (Civil Agencies).
Fed. Test Method Std. No. 151 - Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, US Government Printing Office, Washington, DC 20402.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers at the General Services Administration Regional Office in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

American Iron and Steel Institute (AISI)

AISI Steel Products Manual - "Stainless and Heat Resistant Steels".

(Applications for copies should be addressed to the American Iron and Steel Institute, 1000 16th St., N.W., Washington, DC 20036.)

National Bureau of Standards (NBS)

Handbook H 28 - Screw-Thread Standards for Federal Services. Part III - 1957

(Applications for copies should be addressed to the Superintendent of Documents, Government Printing Office, Washington, DC 20402.)

National Fire Protection Association (NFPA)

NFPA 56A - Standard for the Use of Inhalation Anesthetics

(Application for copies should be addressed to the National Fire Protection Association, 470 Atlantic Avenue, Boston, MA 02210).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 First article. When specified in the procurement document, the contractor shall furnish sample unit(s) for first article inspection and approval (see 4.1.2.1 and 6.2).

3.2 Material.

3.2.1 Corrosion-resisting steel. With the exception of the seat screw and adapter flange, all parts of the stool shall be made from corrosion-resisting steel conforming with the AISI type 300 series as indicated in the AISI Steel Products Manual. Gages and diameters specified herein are minimum. Commercial tolerances shall apply.

3.2.2 Carbon steel. The seat screw and adapter flange shall be AISI B 1113 leaded carbon steel conforming to Fed. Std. No. 66.

3.2.3 Screw Socket. The screw socket shall be corrosion-resisting steel (see 3.2.1). As an alternate, the screw socket may be carbon steel (see 3.2.2) with a corrosion-resisting steel housing.

3.3 Style, design, and construction. The stools shall be of the conventional four-legged design, with revolving adjustable seat, in accordance with style A or B as shown in figures 1 and 2. The stools shall be of welded construction throughout.


3.3.1 Seat. The seat shall be of corrosion-resisting steel with a well-rounded apron. The upper surface of the seat shall be slightly concave (see detail B, figure 2).

3.3.2 Adapter flange. The adapter flange shall be designed in accordance with detail A, figure 2. The flange shall be securely and permanently attached on the center of the undersurface of the seat (see detail A, figure 2). The flange shall be formed to receive and hold the screw securely. The screw shall be continuously welded to the adapter flange on the underside.

3.3.3 Screw. The threaded portion of the screw shall have acme machined threads which meet the requirements of section XII of Screw Thread Standards for Federal Services, National Bureau of Standards, Handbook H 28 and detail A, figure 2.

3.3.4 Screw socket. The screw socket shall be provided with acme machined threads which meet the requirements of section XII of Screw Thread Standards for Federal Services, National Bureau of Standards, Handbook H28. The screw socket threads shall fit the threaded screw mounted on the seat. The screw and socket threads shall permit easy height adjustment of seat without noise, chatter or play.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

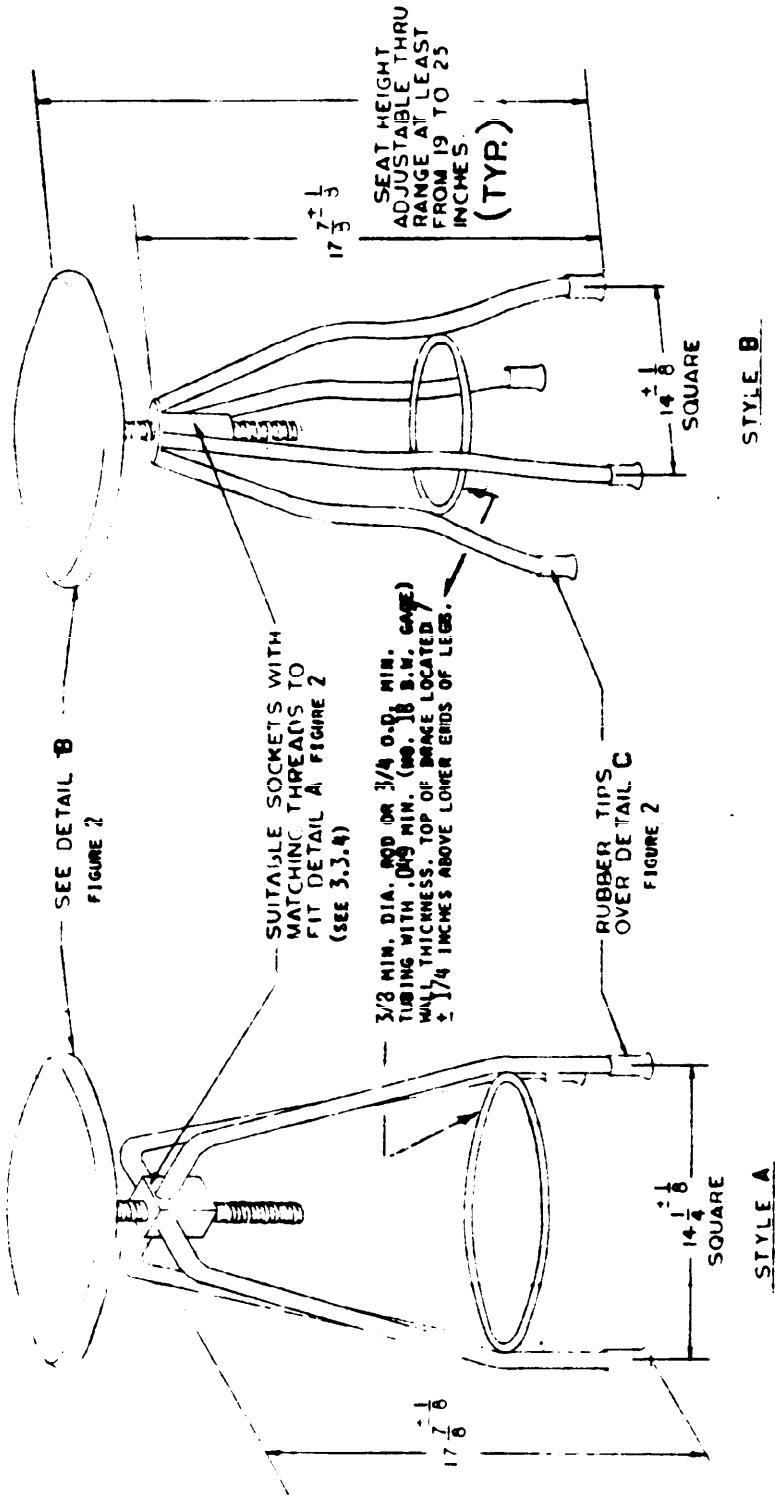


GENERAL NOTES


1. REMOVE BURRS AND BREAK ALL SHARP EDGES.
2. DIMENSIONS ARE IN INCHES

Figure 1. Stool, revolving, surgeon's


Source: https://assist.dla.mil -- Downloaded: 202610-26T11:41Z
Check the source to verify that this is the current version before use.

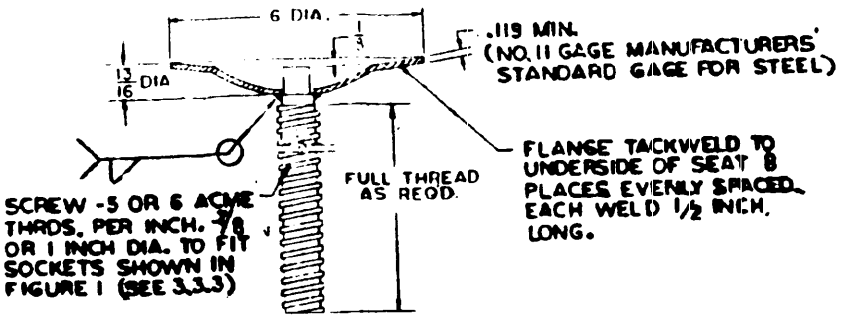


DETAIL A
FLANGE AND SCREW

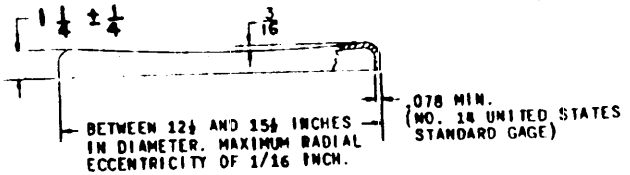

DETAIL B
SEAT

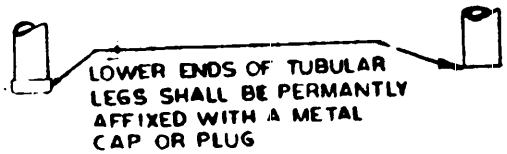

DETAIL C
LEG

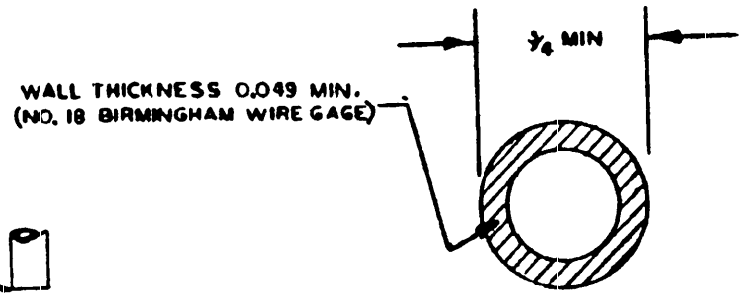

DETAIL D
LEG

GENERAL NOTES

1. REMOVE BURRS AND BREAK ALL SHARP EDGES.
2. DIMENSIONS ARE IN INCHES
3. UNLESS OTHERWISE SPECIFIED, TOLERANCES ON FRACTIONS — ± 1/16

Figure 2. Stool, revolving, surgeon's (detail)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

3.3.5 Legs. The legs shall be made of tubing (see detail D, figure 2). The legs shall be shaped and spaced apart as shown in figure 1. The end of each leg shall be closed off flush with a metal plug or cap, and shall be equipped with a snug-fitting rubber tip.

3.3.6 Plugs or caps. The metal plugs or caps used to close off the end of each leg shall be secured firmly and permanently in place.

3.3.7 Brace. The plane of the brace shall be perpendicular to the vertical axis of the stool (see figure 1). Tubing shall be in contact with the inner surface of each leg and shall be welded all around the contact points of the leg and brace. Rod shall be fitted into notches in each leg and welded all around the contact points of the leg and brace. Alternately, when rod of 1/2 inch diameter or larger is used, the rod, instead of the leg tubing, may be notched; welding shall be as specified above.

3.3.8 Rubber tips. The rubber tips shall conform to the conductivity requirements for Reduction of Electrostatic Hazard-Furniture as specified in NFPA 56A, when tested as specified in 4.4.2.

3.4 Finish. All exposed surfaces of the stool shall be given a No. 4 commercial finish or better. The underside of the steel seat adapter flange shall be painted with aluminum bronze paint (cured according to paint manufacturer's specifications), smooth and free from blisters.

3.5 Workmanship. The stools shall be smoothly and properly finished, and shall be free from defects which affect their appearance or which may impair their serviceability.

3.5.1 Welding. Welding shall be durable, sound in every detail and in accordance with the latest practices recommended by the American Welding Society. All welds shall be produced by qualified welding operators with satisfactory welding equipment using satisfactory filler metal or electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreign matter. Any cleaning method which will remove these substances and leave the surface clean is satisfactory. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Beads shall be smooth and free of slag, excessive undercut, or excessive splatter. Sufficient metal shall be added to provide a suitable fillet or reinforcement unless otherwise specified. Welds shall not be oxidized. All welds shall be continuous with no visible voids, pin holes, or cracks.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2.1 Classification of inspection. The inspection requirements specified herein are classified as follows:

a. First article inspection.
b. Quality conformance inspection.

4.1.2.1.1 First article inspection. First article inspection shall be performed on the stool when a first article sample is required (see 3.1). This inspection shall include examination of 4.3 and test(s) of 4.4.

4.1.2.1.2 Quality conformance inspection. Quality conformance inspection shall include the examination of 4.3 and test(s) of 4.4.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the material or components may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and table I.

TABLE I. Sampling for examination

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	S-4	1.0
Total defects (Major and Minor combined)	S-4	4.0
For dimensional examination	S-1	2.5

4.2.2 For tests.

4.2.2.1 Chemical composition. Four ounces from each lot of metal used in the stool, shall be selected for chemical analysis as specified in 4.4.1.

4.2.2.2 Electrical conductivity. Sampling for electrical conductivity testing shall be 100%. Acceptance number shall be zero.

4.3 Examination. The stool shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in table II. Examination shall not be restricted to the classified possible defects listed below.

TABLE II. Classification of defects

Categories	Defects
Major:	
101	Stool not free of sharp edges.
102	Stool not free of rocking when the four legs are placed on a smooth flat surface.
103	Seat does not maintain height either free standing or under normal load.
104	Vertical position of the seat cannot be changed; seat cannot be revolved without binding.
105	Steel caps or plugs not present on floor end of legs.
106	Steel caps or plugs not permanently and firmly secured.
107	Rubber crutch tips not present.
108	Rubber crutch tips do not fit snugly.
109	Type, number, and length of welds not as specified.
110	Welds not free of cracks.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

TABLE II. Classification of defects (continued)

Catagories	Defects
Minor:	
201	Stool not free of grind marks, trim marks, bulges, and scratches.
202	Upper surface of seat not concave.
203	Unexposed welds not properly cleaned before painting.
204	Undersurface of seat not painted.
205	Painted surface not free of blisters.
206	Rubber crutch tips not free of tears.
207	Unpainted welds not ground and polished smooth.

4.3.2 Dimensional examination. The stools shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.3.3 Examination of preparation for delivery. An examination shall be made to determine compliance with the packaging, packing and marking requirements of section 5. Defects shall be scored as specified in table III. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with AQL of 4.0 expressed in terms of percent defective.

TABLE III. Examination of preparation for delivery

Examine	Defect
Container	Not as specified.
Marking	Omitted; incorrect; illegible; improper size, location, sequence or method of application.
Material	Component missing or damaged.
Workmanship	Bulging or distoration of containers.

4.3.3.1 Examination of closure, waterproofing and banding of container. When the shipping container is required to comply with PPP-B-636, the examination for defects in closure, waterproofing or banding shall be in accordance with the appendix of the box specification.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111 or 112 of Fed. Test Method Std. No. 151.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

4.4.2 Electrical conductivity. The stool with rubber tips in place shall be tested in accordance with NFPA 56A.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C, as specified (see 6.2).

5.1.1 Level A. Each stool shall be protected by being wrapped with kraft paper or other suitable material.

5.1.2 Level C. Stools shall be individually packaged in a manner that will afford adequate protection against corrosion or physical damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.2).

5.2.1 Level A. Each stool shall be packed in an exterior container designed for a type 3 load and conforming to PPP-B-636, class weather-resistant. The stool shall be secured within the box by use of fiberboard inserts or other suitable material. Closure, strapping, and waterproofing shall be as specified in the appendix of the box specification.

5.2.2 Level B. Each stool shall be packed as specified in 5.2.1 except that the exterior shall conform to PPP-B-636, class domestic and waterproofing and strapping shall not be required.

5.2.3 Level C. The packaged stools shall be packed in shipping containers that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier rules and regulations.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with Fed. Std. No. 123.

5.3.2 Military activities. Exterior containers shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. This stool shall be suitable for use in the surgical service of hospitals.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

6.2 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents.

a. Title, number and date of this specification.
b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
c. When a first article is required (see 3.1, 4.1.2.1 and 6.3).

6.3 First article. When a first article is required, it shall be tested and approved under the appropriate provisions of 7-104.55 of the Armed Services Procurement Regulation. The contract or purchase order specifies the quantity, procedure for delivery and other specific instructions for inspection and approval of the first article.

6.4 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number (NSN)	Item
6530-00-708-8000	Stool, Revolving, Surgeon's Corrosion-Resisting Metal

MILITARY CUSTODIANS:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
DSA-DM

Civil Agency Coordinating Activities:
GSA-FSS
VA-DMS

Project No. 6530-1397

U. S. GOVERNMENT PRINTING OFFICE : 1976 - 241-233/1016

Orders for this publication are to be placed with General Services Administration, acting as agent for the Superintendent of Documents. See section 2 of this specification to obtain copies of documents referenced herein. Price 35 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON D. C.
POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-LS
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.