AA-S-698B
July 17, 1975
SUPERSEDING
Int. Fed. Spec. AA-S-00698A
March 24, 1965 and
Fed. Spec. AA-S-698
February 25, 1955

FEDERAL SPECIFICATION

STOOL, STRAIGHT

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 This specification covers one type of rectangular, nonadjustable footstool, suitable for use in hospital operating rooms.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issues in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

Federal Specifications:

ZZ-T-351 - Tip, Cane and Crutch, Rubber.
PPP-B-585 - Boxes, Wood, Wirebound.
PPP-B-601 - Boxes, Wood, Cleated-Plywood.
PPP-B-621 - Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636 - Boxes, Shipping, Fiberboard.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

Federal Standards:

Fed. Std. No. 66 - Steel: Chemical Composition and Hardenability.
Fed. Std. No. 123 - Marking for Shipment (Civil Agencies).
Fed. Test Method Std. No. 151 - Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specifications:

MIL-L-10547 - Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

Military Standards:

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

2.2 Other publication. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

NATIONAL FIRE PROTECTION ASSOCIATION

NFPA No. 56A Flammable Anesthetics Code Standards by the National Fire Protection Association.

(Application for copies should be addressed to the National Fire Protection Association, 60 Batterymarch St., Boston, MA 02110)

3. REQUIREMENTS

3.1 Material.


3.1.1 Corrosion-resisting steel. Corrosion-resisting steel strip, sheet, and tubing used in the construction of the stool shall conform to AISI 302 or 304 of FED-STD-66, and shall pass the test for chemical composition specified in 4.4.1.


3.1.2 Rubber tips. The rubber tips shall conform to size 20 of ZZ-T-351, except that the height overall shall be 1-9/16 inches minimum. The tips shall meet the requirements for Reduction of Electrostatic Hazard-Furniture as specified in NFPA No. 56A, when tested as specified in 4.4.2.

3.2 Design and construction. The footstool fabricated of corrosion-resisting steel shall be designed and constructed so that when placed on a flat or plane surface it will safely support a 300 pound weight without wobble or distortion. The design and construction shall be in strict accordance with figure 1. Gages specified herein are minimum. Commercial tolerances shall apply.


3.2.1 Top. The top shall be formed from a single piece of 0.125 inch (No. 11, United States Standard gage) corrosion-resisting steel. All sides shall be flanged downward to provide an apron. When not formed seamlessly, all corners shall be welded and ground to present a seamless appearance with rounded corners. The top surface shall have a well-raised diamond lug tread pattern. The raised pattern shall be as indicated, subject to normal manufacturing tolerances. As an alternate the 1-1/2 and 1/2 inch dimensions shown in detail B of the figure shall be 1-3/8 and 1/4 inch, respectively.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

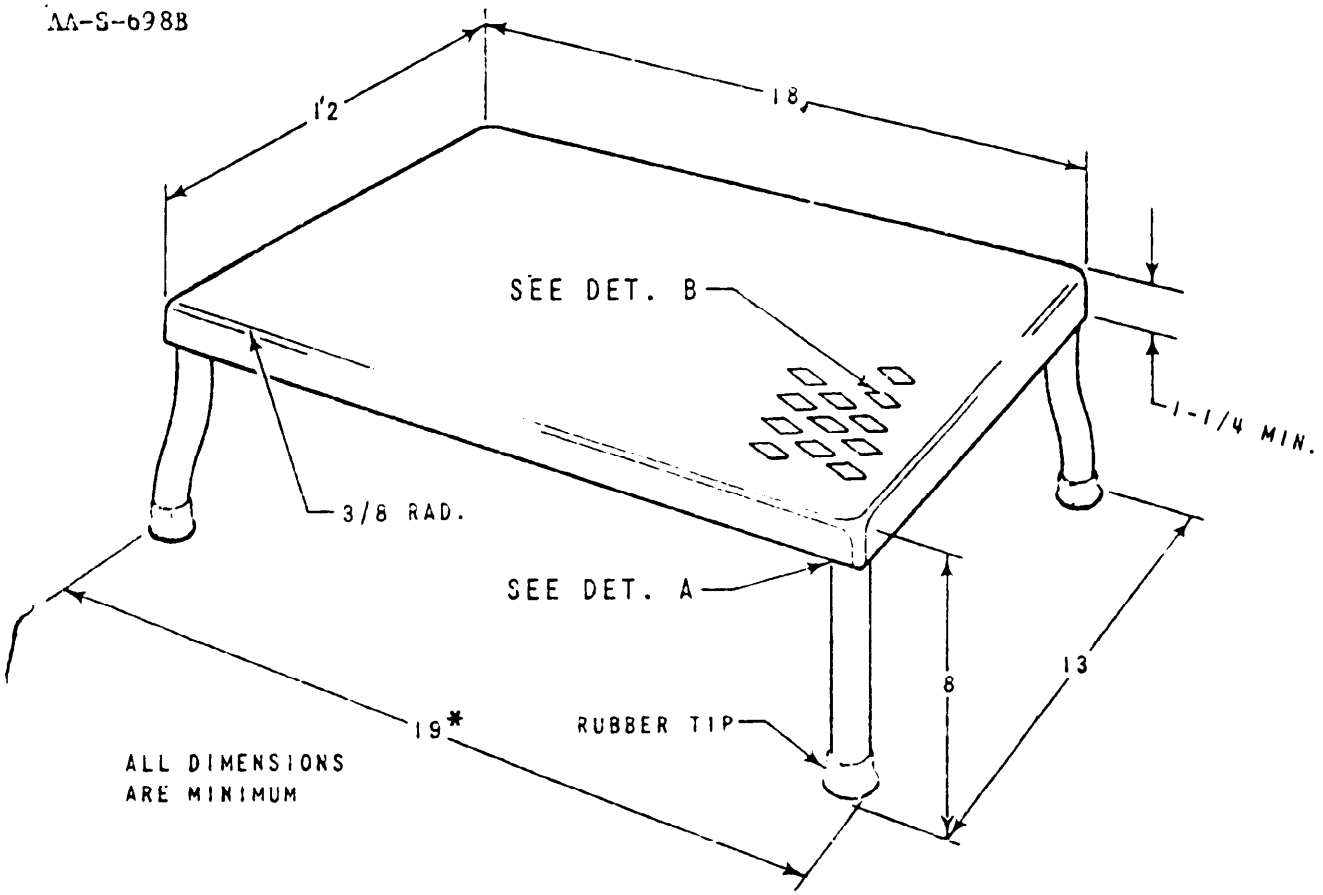

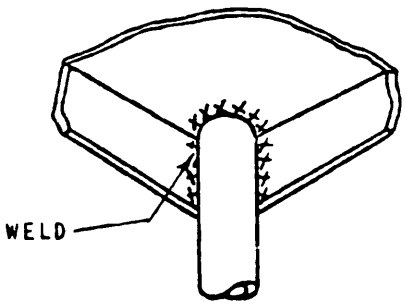

DET. A

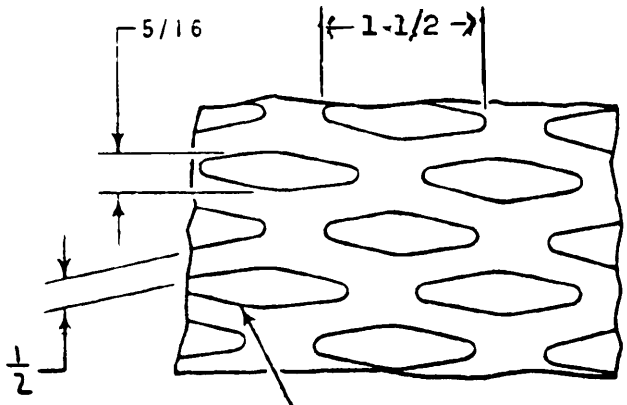

DET. B

TYPICAL TREAD DESIGN

Figure 1

*Measured without tips

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

3.2.2 Legs. The legs shall be made of corrosion-resisting steel tubing not less than 1 inch in outside diameter, having a wall thickness of not less than .078 inch (No. 14 USS gage), or may be made of corrosion-resisting steel rod not less than 1 inch outside in diameter. One end of the legs shall be welded to the inside corners of the top, and the opposite end of the legs shall be equipped with snug-fitting rubber tips. The legs shall be offset as shown on figure 1. The bottom end of the legs made of tubing shall be deburred to prevent damage to the rubber tips.

3.3 Finish. The top and turned-down flanges shall be sandblasted to provide a rough finish. The legs shall be given a No. 4 standard commercial finish.

3.4 Identification marking. Stools shall be permanently, clearly, and legibly marked on the underside with the manufacturer's name or registered trademark, national stock number, contract or purchase order number, and the letters U. S. Marking secured by adhesives shall not be employed.

3.5 Workmanship. Workmanship shall be first class throughout. Stools shall be free from defects which detract from their appearance or may impair their serviceability.

3.5.1 Welding. Welding shall be continuous on all contact surfaces. Welding on exposed surfaces shall not show pits or extrusions, and when the surface of metal is thus defaced in fabrication, it shall be filled or ground smooth to prevent unsightly blemishes on the finished surface. Welds shall be thorough, nonporous, and free of pits, cracks, and other imperfections. The welds shall be of the same color as, and shall blend with the adjoining surfaces.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the component or material may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and Table I.

Table I. Sampling for Examination

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Total (major and minor combined) defects	II	2.5
For dimensional examination	S-3	2.5
For electrical conductivity test	S-4	*

*Acceptance number shall be zero. Not less than three samples shall be taken, regardless of lot size.

4.2.2 Raw materials. Four ounces of each lot of each metal used in the construction of the stools shall be selected for chemical analysis.

4.3 Examination. The stools shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects listed in Table II.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

Table II. Classification of Defects

Categories and defects*	
Major	
101	Unit not free of cracks, tears, ruptures, and deformed surfaces.
102	Stool not stable on a flat surface (rocks).
103	Exposed or accessible edges (notably flanged edges), corners, and surfaces not free of burrs, sharpness, and sharp projections.
104	Welds attaching legs to top not sound, not free of cracks, or not free of porosity.
105	Top surfaces and turned-down flanges not sandblasted.
106	Corners not formed as specified.
107	Top not formed from a single piece of corrosion-resisting steel.
Minor	
201	Rubber tips not snug fitting.
202	End of each leg not finished to preclude damage to rubber tips.
203	Welds not smooth, not clean, or not free of slag and spatter.
204	Finish not free of coarse grind marks, chips, and scratched areas.
205	Identification marking not present, complete, legible, correct, or permanent.
206	Finish not as specified.

*Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The stools shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111 or 112 of FED-STD-151.

4.4.2 Electrical conductivity. The stool, complete with rubber tips, shall be tested using the equipment described in 4628 (c) NFPA No. 56A.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

4.5 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of Section 5. Defects shall be scored as specified in Table III. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

Table III. Examination for Preparation for Delivery

Examination	Defect
Containers	Not as specified
Quantity	Quantity in interior packages and shipping containers not as specified.
Packaging and Packing Materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be Level A or C as specified (see 6.1).

5.1.1 Unit of issue. One stool, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Unit package. Each unit shall be packaged in a box of appropriate size constructed in accordance with PPP-B-636, type CF, class domestic. Box shall be designed with interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to the contents. Closure shall be adequate to prevent accidental opening.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

5.2.1 Level A.

5.2.1.1 Exterior container. Four (4) units shall be packed in a box designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof as specified in the appendix of PPP-B-636.

5.2.2 Level B.

5.2.2.1 Exterior container. Four (4) units shall be packed in a box designed for type 2 load, and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Packing variation (applicable to Levels A and B). If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.2.4 Level C. Units shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with FED-STD-123.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

5.3.2 Military activities.

5.3.2.1 Unit package. Each unit package shall be marked in accordance with MIL-STD-129. Marking shall include the contract or purchase order number and name of contractor.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Purchasers should select the preferred options permitted herein, and include the following information in procurement documents:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification covers the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6530-00-708-6975	Stool, Straight, Corrosion-Resisting Steel, 8 inches high

6.3 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

MILITARY CUSTODIANS:

Army - MD
Navy - MS
Air Force - 03

Civil Agency Coordinating Activities:

GSA - FSS

Preparing Activity:

DSA - DM
Project No. 6530-1325

U. S. GOVERNMENT PRINTING OFFICE : 1975 - 210-814/969

Orders for this publication are to be placed with General Services Administration, acting as an agent for the Superintendent of Documents. See section 2 of this specification to obtain extra copies and other documents referenced herein. Price 35 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

AA-S-698B STOOL, STRAIGHT

NAME OF ORGANIZATION AND ADDRESS	CONTRACT NUMBER
	MATERIAL PROCURED UNDER A ☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*	TELEPHONE NO.
	DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:41Z
Check the source to verify that this is the current version before use.