MIL-H-36730
11 December 1970

MILITARY SPECIFICATION

HANDPIECE, DENTAL, STRAIGHT, ROUND NOSE, BELT DRIVEN

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a belt driven straight handpiece with a round nose suitable for driving rotary instruments and short contra-angle and prophylaxis handpieces in dental restorative procedures.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following specifications and standards of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

MMM-A-250	Adhesive, Water-resistant, (For Sealing Fiberboard Boxes).
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-Plywood.
PPP-B-621	Box, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-T-76	Tape, Pressure-sensitive Adhesive Paper, Water-Resistant, (for Carton Sealing).

Military

MIL-P-116	Preservation, Methods of.
MIL-M-7298	Manual, Technical Commercial Equipment.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:13Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-STD-66	Steel, Chemical Composition and Hardenability.
FED-STD-151	Metal, Test Methods.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

ASTM E 18 - Rockwell Hardness and Rockwell Superficial Hardness of Metallic Materials, Tests for.

ASTM E 92 - Vickers Hardness of Metallic Materials, Tests for.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, Pa. 19103).

3. REQUIREMENTS

3.1 Materials. Materials shall be new and shall conform to the requirements specified herein. Materials not specifically designated in table I shall be of high commercial quality throughout and shall be suitable for the intended purpose.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:13Z
Check the source to verify that this is the current version before use.

Table I. Materials

Part No.	Part Name	No. req'd	Material*	Hardness
1	Spindle	1	AISI 304	Nitride case hardened to depth of 0.002".
	Bearing and collar	1	AISI 303	Nitride case hardened Knoop 950 min.
2	Chuck rod (complete)	1	AISI 416	-
3	Plunger	1	AISI 440C	Rockwell C58 min.
4	Sheath	1	AISI 302 or 304	-
	Nosepiece	1	AISI 303	Nitride case hardened Knoop 950 min.
5	Chuck	1	AISI 440C	Rockwell C58 min.
6	Spindle pulley	1	AISI 416	-
7	Wrist joint frame	1	Corrosion-resistant steel	-
	Shaft	1	AISI 303	Nitride case hardened Knoop 950 min.
8	Wrist joint swivel spindle	1	AISI 416	-
9	Wrist joint swivel spindle bushing	2	AISI 416	-
10	Wrist joint swivel spindle dog	1	AISI 420	-
11	Wrist joint hinge	1	AISI 303 or 430	-
12	Union nut	1	AISI 416	-
13	Wrist joint hinge screw	2	AISI 416	-
14	Wrist joint swivel spindle screw	1	AISI 416	-
15	Wrist joint pulley	2	AISI 303	Nitride case hardened Knoop 950 min.
16	Wrist joint pulley guard	2	AISI 302	-
17	Wrist joint pulley guard screw	2	AISI 416	-
18	Slip joint collect	1	AISI 416	-
19	Wrist joint latch screw	1	AISI 416	-
20	Wrench	1	AISI C1010 nickel plated	-
21	Wrist joint latch	1	AISI 302 (spring tempered)	Rockwell C38 to C40
22	Wrist joint latch pin	1	AISI 416	-

* Composition shall conform to requirements of FED-STD-66.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:13Z
Check the source to verify that this is the current version before use.


3.2 Design and construction. The handpiece shall be a round nose straight handpiece, equipped with a standard wrist-joint for attachment to the conventional type belt arm of the dental engine. The handpiece shall be suitable for use in the treatment of dental patients during operative, surgical and prophylactic procedures. The handpiece shall consist essentially of a sheath and nosepiece, spindle, chuck and wrist joint. The handpiece design and dimensions shall be as indicated in figures 1 and 2; part numbers shall be as indicated in table I and figure 1; part names, number of parts required, material and hardness shall be as indicated in table I. The handpiece shall be precision made and shall operate satisfactorily at speeds up to 13,500 revolutions per minute (r.p.m.). The handpiece shall accommodate round sleeve prophylaxis angle handpiece, Federal Stock Number (FSN) 6520-935-7141 and round sleeve angle handpiece, FSN 6520-935-7142. Numbered parts shown in figure 1 shall be replaceable and interchangeable. All bearing points shall be properly case hardened. Sufficient oil holes shall be provided for the proper lubrication of all bearing surfaces.

3.2.1 Sheath and nosepiece. The end shake adjustment shall be factory set and fixed to prevent misadjustment which can be detrimental to the handpiece. Thrust bearings shall be nitrided to prevent wear. The nosepiece shall be locked into the sheath forming one integral combination without soldering. For sterilization and cleaning the sheath shall be easily removable from spindle upon releasing the knurled union nut. Sheath shall resist turning with the handpiece spindle when running at 13,500 r.p.m. with no load. When a standard round sleeve angle handpiece (FSN 6520-935-7141 or FSN 6520-935-7142) is attached, no erractic turning, appreciable vibration, or frictional heat shall develop.

3.2.2 Spindle. The spindle shall be of one-piece construction. End play of the spindle in relation to the nosepiece shall be no less than 0.0025 inch nor more than 0.0085 inch when tested as specified in 4.4.3. Side play of spindle at nosepiece end shall not exceed 0.002 inch total indicator reading measured 1/2 inch from the spindle end when teated as specified in 4.4.3. Spindle pulley shall be a two step "V" type pulley for two speed selections at the handpiece. A nickel-plated carbon steel wrench tool shall be provided for disassembly of the rear bearing.

3.2.3 Chuck. The chuck shall have four jaws and shall accept standard straight handpiece burs and mandrel shanks of 0.0919 to 0.0929 inch diameter. The chuck shall receive burs and mandrel shanks readily without resistance to the shank, shall hold then securely, and upon releasing chuck tension, the shank must be free in the chuck. Chuck runout, measured 1/2 inch from the spindle end with test pin in place, shall be less than 0.003 inch total indicator reading at assembly, when tested as specified in 4.4.4.


Source: https://assist.dla.mil -- Downloaded: 202610-21T09:13Z
Check the source to verify that this is the currentversion before use.

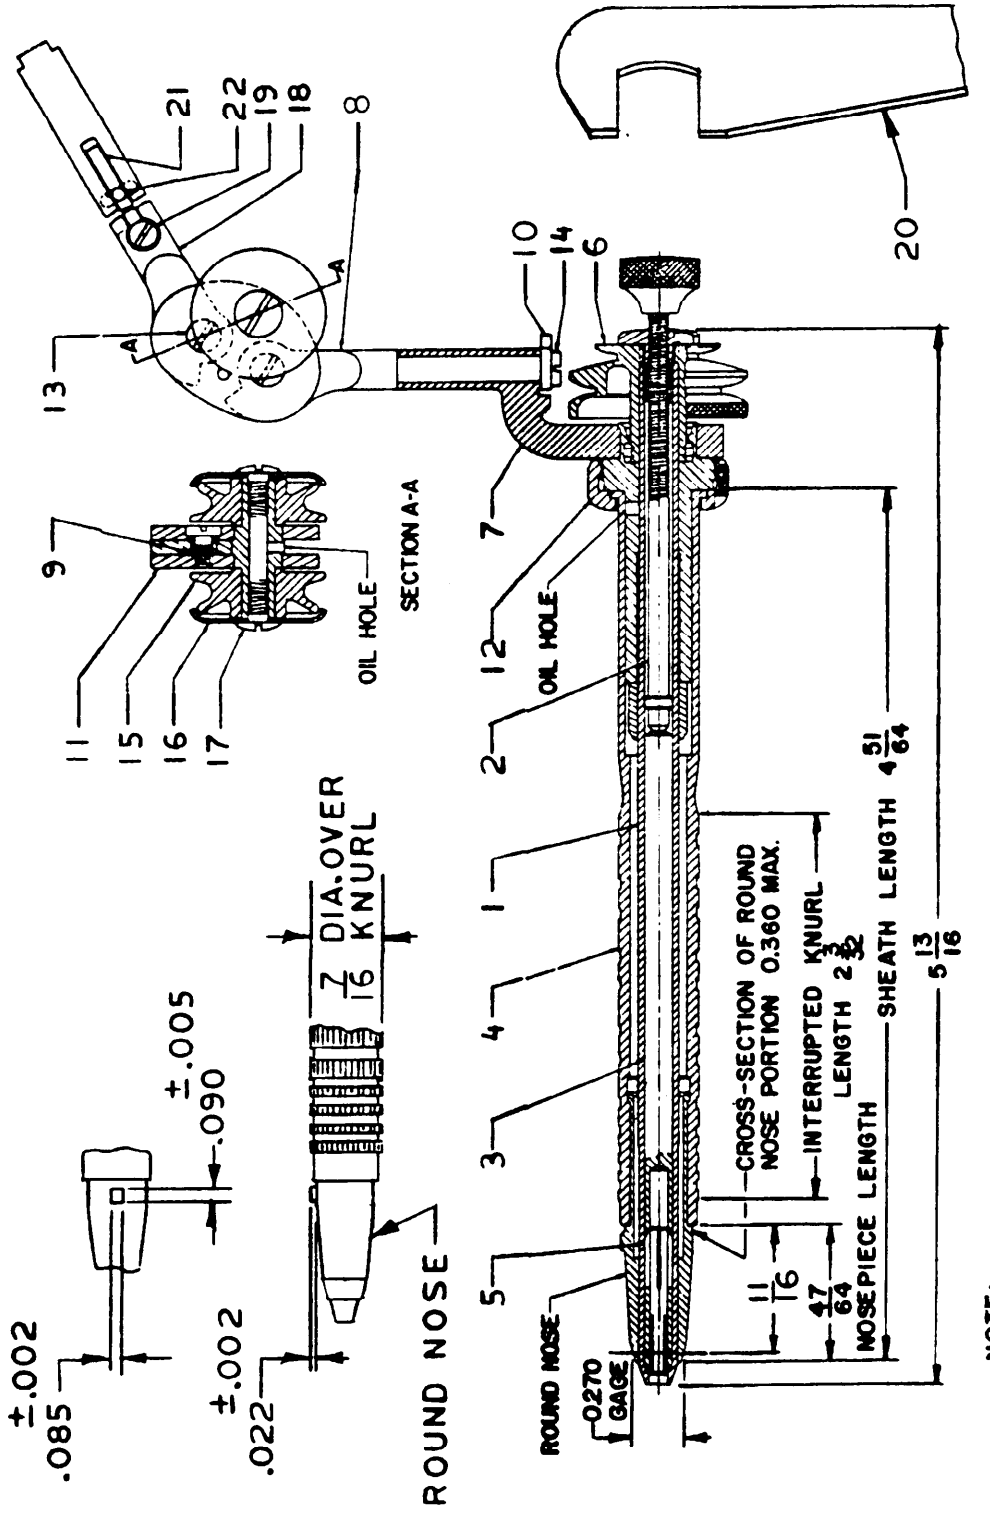

NOTE:
1. FOR ABOVE PART NO. IDENTIFICATION SEE TABLE I.
2. ALL DIMENSIONS ARE IN INCHES. TOLERANCE ± 1/32

FIGURE-1- HANDPIECE

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:13Z
Check the source to verify that this is the current version before use.

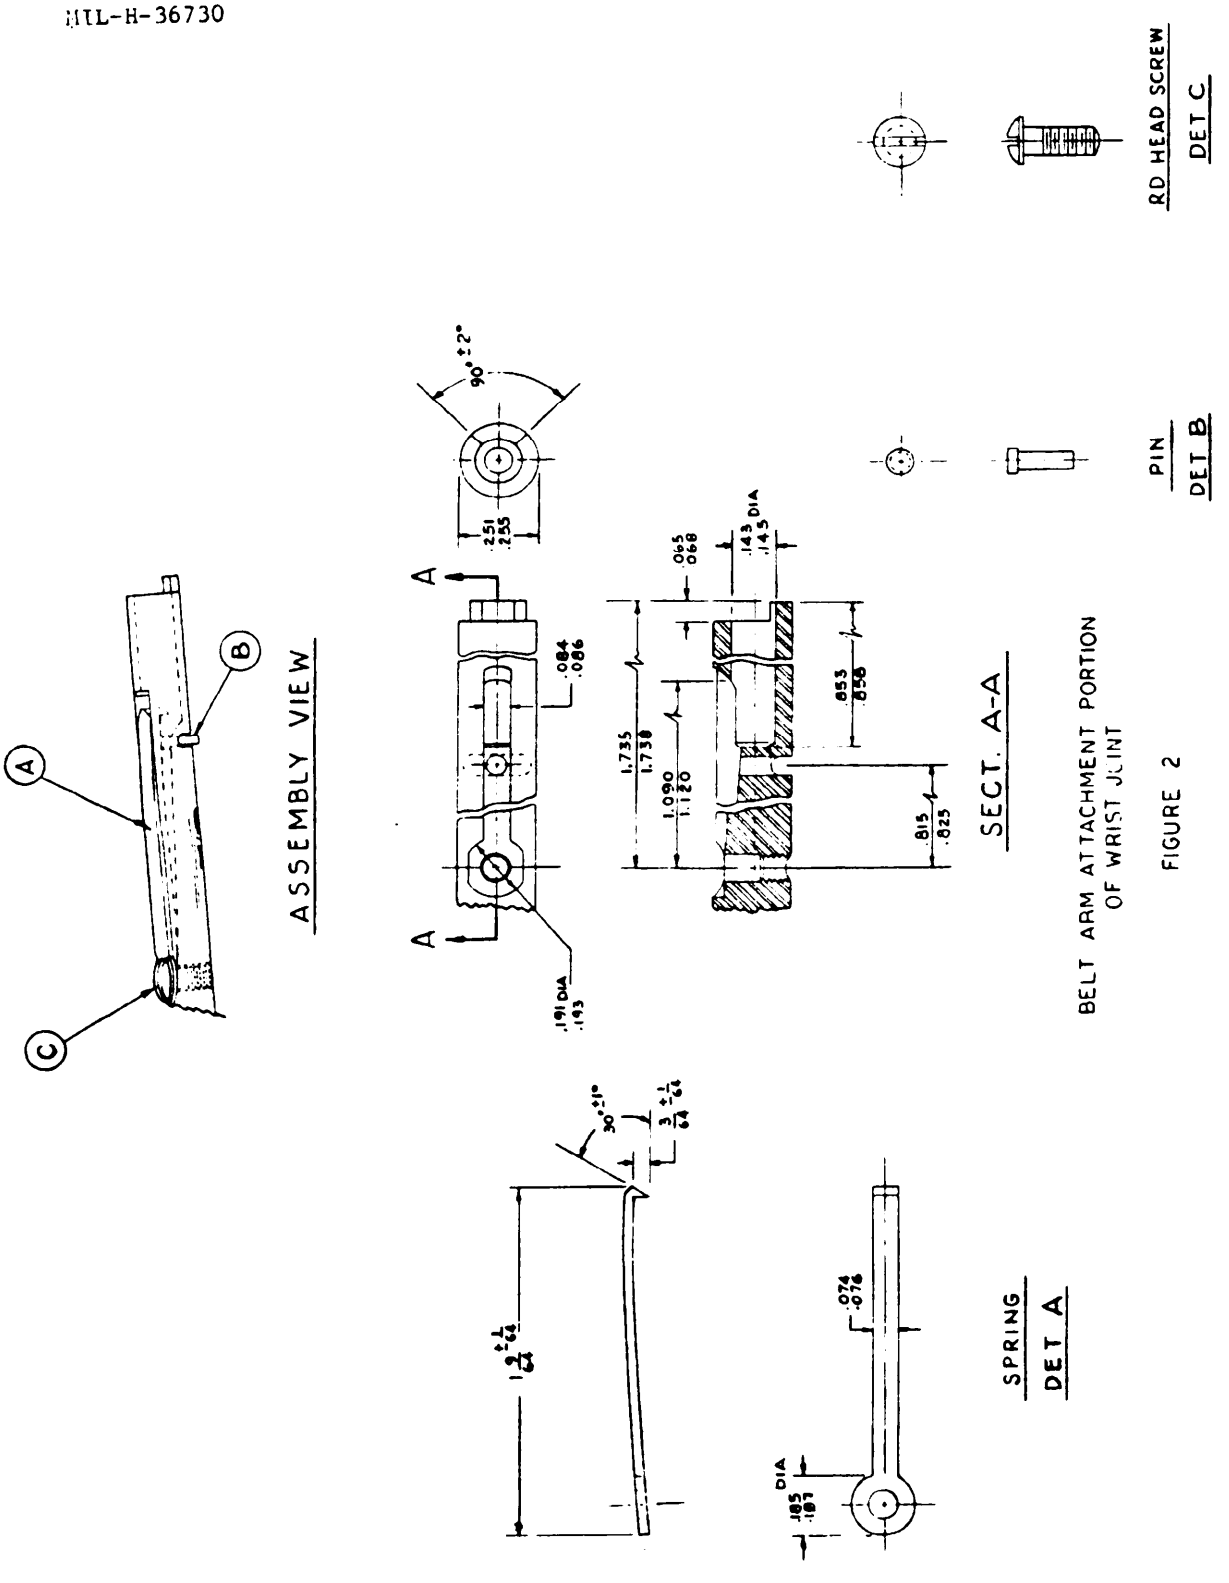

BELT ARM ATTACHMENT PORTION
OF WRIST JOINT

FIGURE 2

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:13Z
Check the source to verify that this is the current version before use.

3.2.4 Wrist joint. The belt arm attachment portion shall conform to figure 2 in design and dimensions. The wrist joint shall be attached to wrist joint frame at one end by means of a moving joint, and the opposing end shall be designed for the attachment to a standard dental engine lower belt arm. Wrist joint shall be provided with two "V" type pulleys mounted on the hardened shaft. The periphery of pulleys shall not extend beyond hinge of joint.

3.3 Vibration and heat rise. The handpieces shall pass the test for vibration and heat rise specified in 4.4.5.

3.4 Endurance test. The handpieces shall withstand one hour of operation without showing vibration, excessive wear of bearing surfaces, and excessive generation of heat, when tested as specified in 4.4.6.

3.5 Corrosion test. The handpieces shall show less than 2 percent corrosion, when tested as specified in 4.4.7.

3.6 Finish. Exposed surfaces shall have a mirror or satin finish except for knurled portions and black oxide finished pulleys.

3.7 Identification marking. Each handpiece shall be permanently and legibly marked with either the name or registered trademark of the manufacturer.

3.8 Service data. The contractor shall furnish, with each unit, two copies each of a technical manual which contains complete instructions for installation, operation, and maintenance and lists of component parts. The manual shall comply with the requirements of MIL-M-7298. As soon as practicable after award of the contract or purchase order, the contractor shall furnish to the Contracting Officer, via the cognizant Government inspector, two preliminary copies of his proposed technical manual, for review and comment by the Directorate of Medical Materiel, Defense Personnel Support Center. The preliminary manuals shall be submitted sufficiently early to permit adequate review by the Directorate of Medical Materiel, Defense Personnel Support Center (based on a maximum period of 30 days for such review) and to allow incorporation by the contractor of any required revisions and corrections in the final manual without delaying delivery under the contract or purchase order. In addition, the Contractor shall furnish 15 copies of the approved technical manual to the Contracting Officer for distribution. Should the supplier have furnished acceptable manuals for the identical item within two years preceding the date of contract and propose to furnish manuals identical with those previously accepted, then the requirements for review of drafts and submission of 15 additional copies may be waived upon request to the Contracting Officer. Waiver of submission of 15 additional copies shall be at the option of the Government.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:13Z
Check the source to verify that this is the current version before use.

3.9 Workmanship. Workmanship shall be first class throughout. Handpieces shall be free from defects which detract from their appearance or which may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials used in the handpieces, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the name of the material, the lot number, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered are classified as specified in Table II and IV (see 4.2.1 and 4.3) and Table III (see 4.2.2).

4.2.1 Sampling for examination. Sampling for examination for the handpiece shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in Table II. The unit of product for examination purposes shall be one handpiece.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:13Z
Check the source to verify that this is the currentversion before use.

Table II. Inspection and Acceptable Quality Levels

Type defect	Inspection level	AQL (percent defective)
Major A	II	1.0
Major B	S-1	2.5
Minor A	II	2.5
Minor B	S-1	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and Table III for the handpiece. The acceptance number shall be zero for all sample sizes. The unit of product for test purposes shall be one handpiece. Where feasible, the same sample unit may be used for the determination of two or more test characteristics.

Table III. Sampling criteria for Testing

Component	Characteristic	Requirement	Test procedure	Inspection level
All parts in table I	Chemical Analysis	3.1	4.4.1	*
Parts indicated in table I	Hardness	3.1	4.4.2	S-1
Assembled handpiece	End play and side play	3.2.2	4.4.3	100%
Assembled handpiece	Runout	3.2.3	4.4.4	100%
Assembled handpiece	Vibration and heat rise	3.3	4.4.5	100%
Assembled handpiece	Endurance	3.4	4.4.6	5 units per lot
Assembled handpiece	Corrosion	3.5	4.4.7	S-1

* A sufficient amount from each lot of raw materials used in the construction of the item shall be selected for chemical analysis.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:13Z
Check the source to verify that this is the current version before use.

4.3 Examination. The handpiece shall be examined to determine compliance with requirements contained in this specification. Examination shall be conducted in accordance with the following classification of defects. Examination shall include, but shall not be limited to, the defects listed in table IV.

Table IV. Classification of Defects

Categories	Defects
Critical	None defined
Major A	
101	Nosepiece will not accept and lock-in FSN's 6520-935-7141 and 6520-935-7142, Handpieces, (see 6.2).
102	Belt arm attachment portion of wrist joint will not accept and lock-in to a standard dental engine lower belt arm.
103	All parts listed in table I not interchangeable.
104	Finish not as specified.
105	Slivers and burs present.
Major B	
151	Dimensions affecting fit of nosepiece to FSN's 6520-935-7141 and 6520-935-7142, Handpieces, not as specified.
152	Dimensions affecting fit of belt arm attachment portion of wrist joint to standard dental engine lower belt arm not as specified.
Minor A	
201	Service data technical manuals missing.
202	Identification marking missing.
203	Identification marking not permanently applied and not as specified.
204	Pits, nicks and discoloration present on outer surfaces.
Minor B	
251	Dimensions (other than 151 and 152) not as specified.

4.4 Tests.

4.4.1 Chemical analysis. Metal analysis shall be conducted in accordance with method 111 or 112 of FED-STD-151.

4.4.2 Hardness test.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:13Z
Check the source to verify that this is the current version before use.

4.4.2.1 Knoop hardness test. The Knoop hardness number shall be determined on a Tukon tester under a 100 gram load, using a rhombus-shaped diamond indenting tool with a longitudinal angle of 172.5 degrees and a transverse angle of 130 degrees.

4.4.2.2 Rockwell hardness test. Hardness shall be determined in accordance with ASTM Designation E 18 (Rockwell) or E 92 (Vickers or Diamond Pyramid).

4.4.3 End play and side play. A true running test shank gage shall be screwed into socket of assembled handpiece. A dial indicator sensitive to 0.0002 inch, equipped with a knife edge foot or other suitable equipment of equal accuracy, shall be employed. The indicator shall be placed in a position perpendicular to the axis of the spindle. The test shank gage shall be pushed toward and away from the nosepiece, in a plane horizontal to the spindle, and the end play measured. The difference between the maximum and minimum readings of the indicator shall be reported as end play. The test shank gage shall be pushed toward and away from the nosepiece, in a plane perpendicular to the spindle, and the side play measured. The difference between the maximum and minimum readings of the indicator shall be reported as side play.

4.4.4 Runout. A true running test shank gage shall be screwed into socket of assembled handpiece and rotated slowly. A dial indicator sensitive to 0.0002 inch equipped with a knife edge foot or other suitable equipment of equal accuracy shall be employed. The difference between the maximum and minimum readings for one full rotation of the gage shall be reported as the runout.

4.4.5 Vibration and heat rise. The assembled and lubricated handpiece shall be tested by running the handpiece under no load for 3 minutes at 13,500 r.p.m. The handpiece shall be tested for excessive vibration when hand held; and excessive heat rise (greater than 50 degrees Fahrenheit) when tested with a pyrometer held against the bearing areas.

4.4.6 Endurance test. The lubricated handpiece shall be tested by running the handpiece, containing a No. 557 steel straight handpiece bur at 8,000 r.p.m. for 15 cycles of 3 minutes each "on", with 15 intermittent cycles of 1 minute each "off". Test shall be made under a 1 pound load against a plate glass slab at least 1/8 inch thick. After the 15 cycles of operation, the handpiece shall be retested for excessive vibration and heat rise as in 4.4.5. The handpiece shall then be disassembled and examined under the microscope at 15 power (15X) magnification for excessive wear of components, such as bearing surfaces.

Source: https://assist.dla.mil -- Downloaded: 202640-21T09:13Z
Check the source to verify that this is the current version before use.

4.4.7 Boil test. The handpiece shall be scrubbed with soap and water and rinsed thoroughly in distilled water. After cleaning, the handpiece shall be suspended in a glass container filled with distilled water. The water shall be boiled for 30 minutes and the submerged handpiece shall remain in the water for 24 hours. The handpiece shall then be removed from the water and examined for corrosion.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One handpiece, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table V shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table V. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	6 units	72 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive materials.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method IA-15.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:13Z
Check the source to verify that this is the current version before use.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2 inch wide tape conforming to PPP-T-76. Closing of bottom flaps with adhesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure of wood boxes shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:13Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 Standard samples. For access to standard samples, address the procuring activity issuing the solicitation (see 3.2, 3.2.1. 3.2.4 and 4.3).

6.3 Limitations. This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet Military requirements.

6.4 Federal Stock Number (FSN) coverage. This specification covers the following item appearing in the Federal Supply Catalog:

Stock Number	Item Identification
6520-584-3463	Handpiece, Dental, Straight, Round Nose, Belt Driven.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6520-1277

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 202610-21T09:13Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements .

SPECIFICATION
MIL-H-36730 FSN:

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A
☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)* | DATE

DD FORM 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:13Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:13Z
Check the source to verify that this is the current version before use.