
FED. SUP CLASS
6640

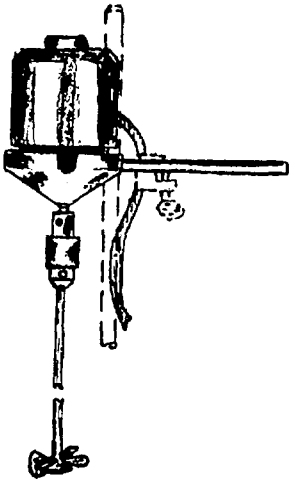

MATERIAL: The material used in the fabrication of electric laboratory stirrers shall be durable and equal in quality normally used by the manufacturer in his standard commercial items. The electrical wiring shall conform to all the requirements of the Underwriters Laboratory, Code Number UL73.

DESIGN: A laboratory stand mounted stirrer shall consist of a heavy-duty constant torque induction, spark proof motor of up to 1600 rpm, 115V/ 60Hz. The chuck adapter assembly shall fit a 7.9 mm (5/16") motor drive shaft and any impeller shaft up to 9.5 mm (3/8") diameter. The impellers shall be fabricated of stainless steel and to the dimension as specified in the table.

TABLE I. IMPELLERS

PART NO.	LENGTH ± .2 cm	SHAFT DIA. ± 1 mm	IMPELLER DIA. ± .2 cm
MS36509-2	31 (12")	6.4 (1/4")	4.4 (1-3/4")
MS36509-3	41 (16")	7.9 (5/16")	6.4 (2-1/2")
MS36509-4	46 (18")	9.5 (3/8")	8.9 (3-1/2")

MS36509-1 shall be the complete assembly less the impeller.

INTENDED USE: For mixing tars, petroleum products, plastics, paints, and other laboratory uses including flammable materials.

NOTES:
1. Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements specified herein.

APPROVED 30 APR 1982 REVISED

USER ACTIVITIES: ARMY - MD, DM
NAVY - MS

REVIEWER ACTIVITIES: ARMY - ME
NAVY - OS
AIR FORCE - 03

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A.	EA	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust	MS 99		STIRRER, ELECTRIC, LABORATORY	MS36509
Procurement Specifications: NONE		SUPERSEDES:		SHEET 1 OF 1

DD FORM 1 MAY 73 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE PROJECT NUMBER 6640-0715 STANDARD DATE

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:42Z
Check the source to verify that this is the current version before use.