MILITARY SPECIFICATION

FORCEPS, TISSUE, ADSON

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers one size of tweezer tissue forceps, Adson type, suitable for delicate tissue manipulation during general surgical procedures.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal form a part of this specification to the extent specified herein:

SPECIFICATIONS

FEDERAL

GG-I-526	- Instruments, Dental and Surgical; General Specifications.
PPP-B-566	- Boxes, Folding, Paperboard.
PPP-B-585	- Boxes, Wood, Wirebound.
PPP-B-601	- Boxes, Wood, Cleated-Plywood.
PPP-B-621	- Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	- Boxes, Fiberboard.
PPP-B-676	- Boxes, Set-Up.

MILITARY

MIL-P-116	- Preservation, Methods of.
MIL-L-10547	- Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:22Z
Check the source to verify that this is the current version before use.

STANDARDS

FEDERAL

FED-STD-151 - Metal, Test Methods.

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.

(Copies of specifications, standards, and publications required by contractors in connection with specific procurement functions should be obtained from procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

American Society for Testing and Materials (ASTM) Standards

E-18 Rockwell Hardness and Rockwell Superficial Hardness of Metallic Materials

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103.)

(Technical society and technical association specifications and standards are generally available for reference from libraries. They are also distributed among technical groups and using Federal agencies.)

3. REQUIREMENTS

3.1 General requirements. The individual part requirements shall be as specified herein and in accordance with the applicable requirements of GG-I-526. In the event of any conflict between the requirements of GG-I-526 and those of this specifications, the latter shall govern.

Source: https://assist.dla.mil -- Downloaded: 202640-21T10:22Z
Check the source to verify that this is the current version before use.

3.2 Materials. The tissue forceps shall be fabricated from Class 4, Type 420 stainless steel as specified in GG-I-526, except that the minimum carbon content may be 0.14 percent.

3.3 Design and construction. The instrument shall be a tissue forceps, Adson type, approximately 4.5 inches in length with one by two teeth.

3.3.1 Teeth. The teeth shall mesh and shall be sharp, fitting closely without play. The single tooth shall extend beyond the shank at least 0.017 inch and extend fully into the double teeth but not beyond.

3.3.2 Physical dimensions. The physical dimensions of the instrument shall be in accordance with Figure 1.

3.3.3 Hardness. When tested as specified in 4.5.1 the finished instrument shall have a Rockwell hardness of C40 to C45, after proper stress relieving.


3.3.4 Corrosion resistance. The instrument shall be corrosion resistant conforming with the requirements of GG-I-526 when tested as specified in 4.5.2.1 and 4.5.2.2.

3.4 Finish. The finished instrument shall have a mirror finish.

3.4.1 Passivation. As a final finish operation the complete instrument shall be passivated.

3.5 Identification marking. Identification marking of finished instruments shall be in accordance with GG-I-526. In addition to the requirements specified, instruments of foreign manufacture shall also be marked "stainless".

Source: https://assist.dla.mil -- Downloaded: 20261O-21T10:22Z
Check the source to verify that this is the current version before use.

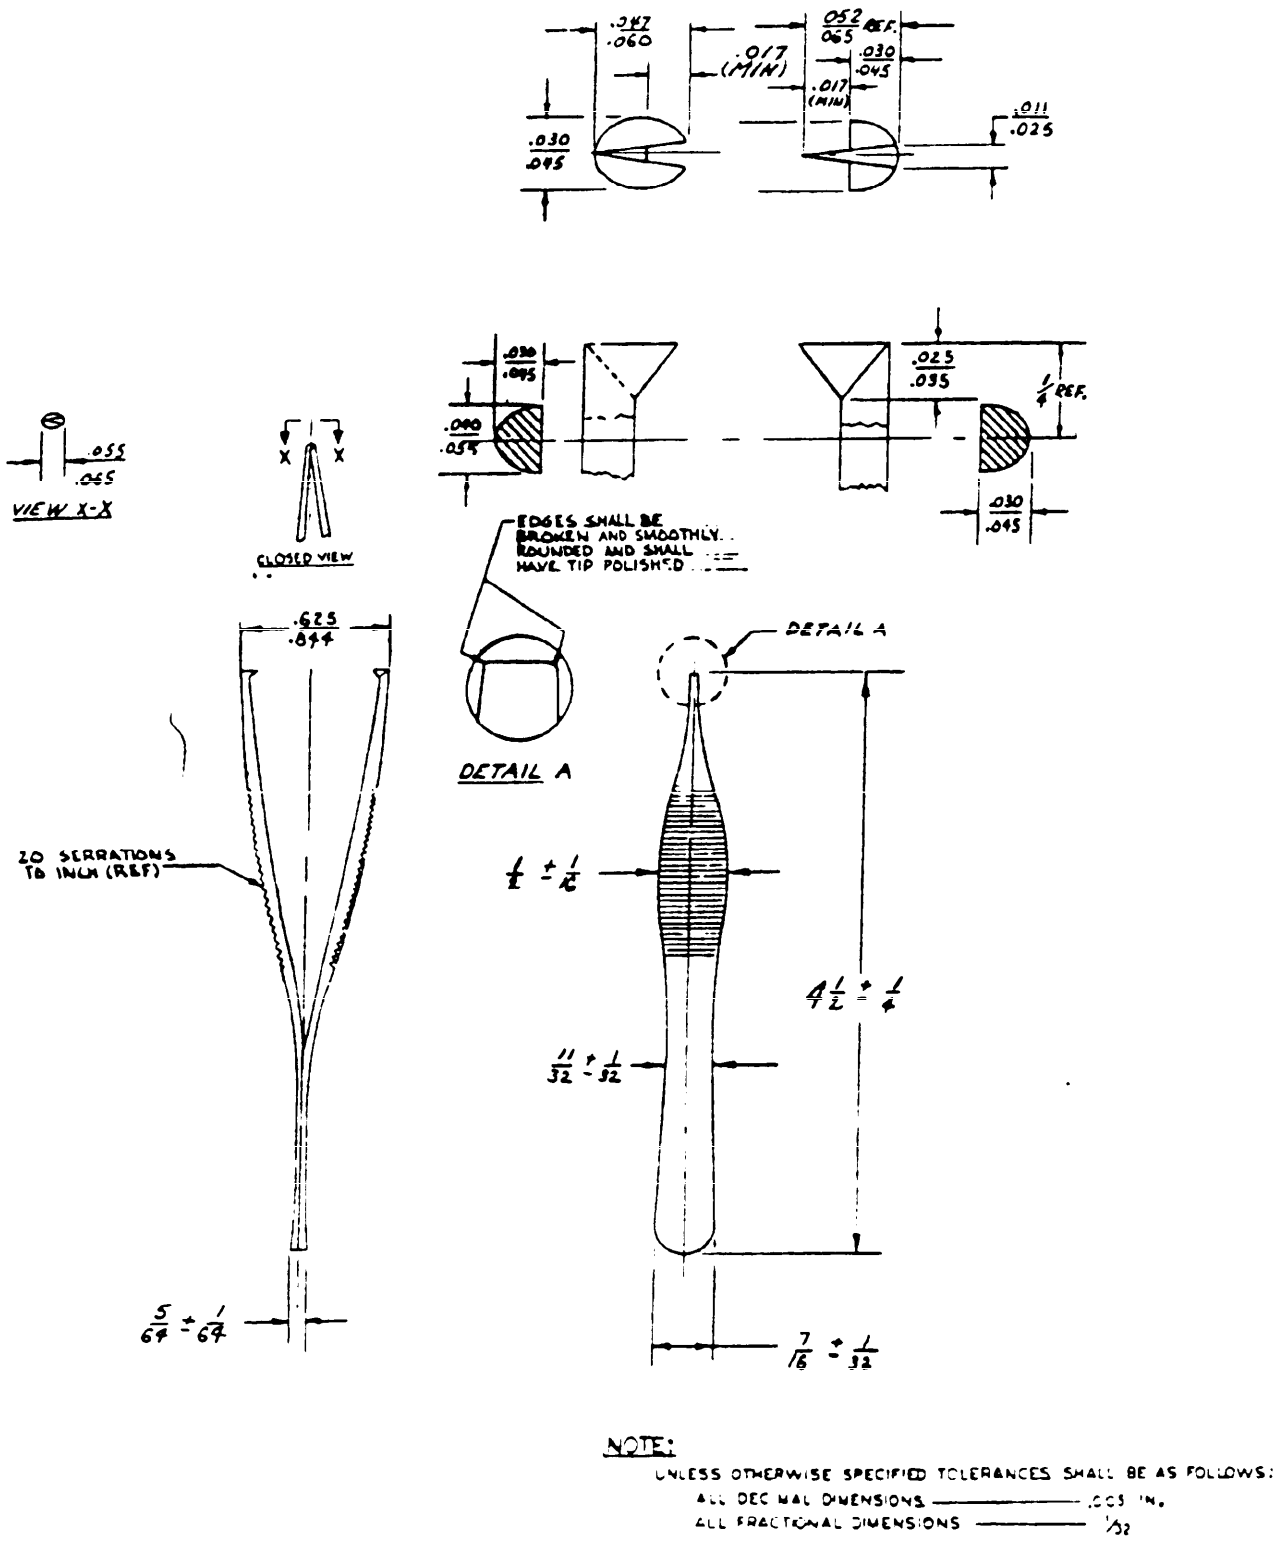

NOTE:

UNLESS OTHERWISE SPECIFIED TOLERANCES SHALL BE AS FOLLOWS:

ALL DECIMAL DIMENSIONS ——— .005 IN.

ALL FRACTIONAL DIMENSIONS ——— 1/32

FIGURE 1. Forceps, tissue, tweezer type, Adson

Source: https://assist.dla.mil -- Downloaded: 202640-21T10:22Z
Check the source to verify that this is the current version before use.

3.6 Workmanship. Workmanship shall be first class throughout. The instrument shall be processed in such a manner as to be uniform in quality and shall be free from surface roughness, burrs, pits, scale, corrosion, or any other defect that will affect life, serviceability or appearance.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the corrosion resistant metals may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number, (NSN) the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:22Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 Inspection lot. The inspection lot shall be determined in accordance with MIL-STD-105.

4.2.2 Preparation for delivery. The inspection lot size shall be expressed in units of one fully prepared shipping container, containing complete instruments fully prepared for delivery and made from essentially the same materials and components. The sample unit shall be one fully prepared shipping container, containing instruments fully prepared for delivery, with the exception that it need not be sealed. The inspection shall be Inspection Level S-2 and the Acceptable Quality Level shall be 4.0 percent defective.

4.2.3 Sampling for visual and dimensional examination. A random sample of instruments shall be selected from each lot offered to the Government in accordance with MIL-STD-105. The Acceptable Quality Levels (AQL) shall be as indicated in table I. The unit of product shall be one forceps.

TABLE I. Sampling for examination

Type of defect	Inspection level	AQL (percent defective)
Major A	II	1.0
Major B	S-4	1.0
Minor A	II	4.0
Minor B	S-2	4.0

4.2.4 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in table II. Where feasible, the same sample shall be used for the determination of two or more test characteristics. Unless otherwise specified, the unit of product for tests shall be one forceps.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:22Z
Check the source to verify that this is the current version before use.

TABLE II. Sampling for tests

Component	Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Forceps	Rockwell hardness	3.3.3	4.5.1	S-1	1.0
	Corrosion	3.3.4	4.5.2.1 & 4.5.2.2	S-2	1.0

4.2.5 Raw materials. A sufficient amount from each lot of each metal used in the construction of the instrument shall be selected for chemical analysis.

4.3 Examination for visual and dimensional defects. The instrument shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in tables I and III. Examination however, shall not be restricted to defects listed in table III. Any instrument in the sample containing one or more defects shall be rejected and if the number of defective instruments in any sample exceeds the acceptance number for that sample, the lot represented by that sample shall be rejected.

TABLE III. Classification of defects

Categories	Defects
Critical	None defined.
Major A	
101	Style and design not as specified.
102	Instrument not constructed as specified.
103	Instrument not free from sharp edges, rough areas, burrs, cracks, grind marks or overlaps.
104	Serrations not free of foreign matter.
Major B	
151	Teeth profile dimensions not as specified.
152	Teeth don't meet requirement specified in 3.3.1.
Minor A	
201	Finish not as specified.
202	Instrument not permanently and legibly marked with either the name or trademark of the contractor.
Minor B	
251	Physical dimensions other than teeth not as specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:22Z
Check the source to verify that this is the current version before use.

4.4 Examination of preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of Section 5. Defects shall be scored as specified in table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

TABLE IV. Examination of preparation for delivery

Examination	Defects
Containers	Not as specified.
Quantity	Quantity in interior package and shipping containers not as specified.
Packaging and packing materials.	Any component missing or damaged.
Workmanship	Inadequate application of components such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

4.5 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.5.1 Hardness. Rockwell hardness shall be determined in accordance with ASTM test method E18. A minimum of 5 hardness readings shall be made on test specimens representative of the material used in the fabrication of the instrument or on the finished instrument.

4.5.2 Corrosion tests.

4.5.2.1 Boil test. The instrument shall be subjected to the boil test as specified in GG-I-526.

4.5.2.2 Copper Sulfate Test. The instrument shall be subjected to the copper sulfate test as specified in GG-I-526.

Source: https://assist.dla.mil -- Downloaded: 20260-21T10:22Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be Level A or C as specified (see 6.1).

5.1.1 Level A.

5.1.1.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.1.2 Preservative. No preservative shall be applied.

5.1.1.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.1.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method 1C1.

5.1.1.5 Intermediate package. Twelve (12) units shall be packaged in a box of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676, or PPP-B-636 type CF, class domestic, except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree or protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Thirty (30) intermediate packages shall be packaged in a box designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements as specified in table II of PPP-B-636 shall apply for fiberboard boxes.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:22Z
Check the source to verify that this is the current version before use.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraph of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

5.2.2 Level B.

5.2.2.1 Exterior container. Thirty (30) intermediate packages shall be packaged in a box designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II as specified in PPP-B-636. In addition, fiberboard boxes shall conform to the special requirements as specified in table I of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(c) National Stock Number.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:22Z
Check the source to verify that this is the current version before use.

6.2 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6515-00-337-7800	FORCEPS, TISSUE, Adson, 4-1/2"

6.3 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1974

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:22Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:22Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:22Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-F-37291 FORCEPS, TISSUE, Adson

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:22Z
Check the source to verify that this is the current version before use.