FEDERAL SPECIFICATION

JAR, STERILIZING, SCALPEL BLADES

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE

1.1 This specification covers a glass sterilizing jar with cover and rack, suitable for holding 100 scalpel blades during sterilization at ordinary room temperature.

2. APPLICABLE SPECIFICATIONS, STANDARDS, AND DRAWINGS

2.1 The following specifications, standards, and drawings of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

QQ–S–766 — Steel, Corrosion-Resisting, Plates, Sheets, Strips, and Structural Shapes.

PPP–B–621 — Boxes; Wood, Nailed and Lock-Corner.

PPP–B–636—Boxes; Fiber.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging and Packing Levels.

Fed. Test Method Std. No. 151—Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specifications:

MIL–L–10547 — Liners, Case, Waterproof.

Military Standards:

MIL–STD–105 — Sampling Procedures and Tables for Inspection by Attributes.

MIL–STD–129 — Marking for Shipment and Storage.

Drawing:

Military Medical Supply Agency:

MS 16686—Medical Services Symbol

(Copies of Military Specifications, Standards, and Drawings required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 **Material.** — Components of the sterilizer shall be made of the materials hereinafter specified.

3.1.1 *Jar.*—The jar, including its cover, shall be formed of clear lime glass, fully annealed, smooth, and free from any significant

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.

quantities of seams, bubbles, stones, pits, and striae.

3.1.1.1 *Seal.*—The cover seal ring shall be made of suitably soft neoprene rubber.

3.1.2 *Rack.*—The insert rack shall be fabricated of corrosion-resisting steel conforming to Federal Specification QQ–S–766, for class 4, condition c, and shall meet the chemical requirements specified therein when tested as specified in 4.3.2.

3.2 **Design and construction.**—Design shall be in accordance with figure 1. The sterilizing jar shall be suitably designed to hold the scalpel blades submerged within the sterilizing liquid. It shall consist of a flat-bottom cylindrical jar, with cover and seal, and a removable rack.

3.2.1 *Jar.*—The jar shall be formed with a uniform thickness of ¼-inch, with an outside radius at the bottom of ½-inch and an outside flange at the top, approximately ⅛-inch wide and ¼-inch deep, with edges appropriately rounded. The horizontal top face shall be finished ground to provide a proper surface for the cover seal.

3.2.2 *Cover.*—The jar cover shall be formed with a horizontal thickness of $\frac{7}{32}$-inch, and with the general contour indicated on figure 1. The annular seating face of the cover shall be finished ground to provide a proper surface for the cover seal.

3.2.3 *Seal.*—The cover seal shall fit around the top of the insert flange, and shall be ¼-inch wide and $\frac{1}{16}$-inch thick. The characteristics of the seal shall be such that it will cushion the weight of the cover and effect a suitable plane seat contact with the ground surfaces of the jar and cover. The seal shall be cemented with waterproof adhesive to the seating face of the cover.

3.2.4 *Rack.*—The scalpel blade support rack shall fit neatly within the jar. The rack shall accommodate 100 scalpel blades, grouped so that 25 blades may be suspended on each beam. The rack shall be so assembled as to stand rigidly erect centrally within the jar. The rack arms and legs shall be formed from 0.037-inch (No. 20, U.S. Standard gage) corrosion-resisting steel sheet. The center post shall be formed from ¼-inch-diameter corrosion-resisting steel rod.

3.3 **Finish.**—The exposed surfaces of the rack shall be polished to a mirror finish, and all sharp edges shall be appropriately rounded. All discoloration due to welds shall be removed. The finished rack shall pass the boil test specified in 4.3.1. The total surface area showing corrosion after testing shall not exceed 2 percent.

3.4 **Identification marking.**—Each jar shall be legibly and permanently marked on the outside bottom with the name or registered trade-mark of the manufacturer. Marking shall be waterproof and black in color. Decalcomanias shall not be employed.

3.4.1 *Marking for Military Medical Supply Agency procurement.*—In addition to the manufacturer's name or registered trademark required in 3.4, the side of the jar shall be permanently marked via the silk screen or other suitable process with the medical services symbol. The letters "U" and "S" shall be ½ inch high and the caduceus of appropriate size as shown on Military Standard MS 16686 for type I.

3.5 **Workmanship.**—Workmanship shall be first class in every respect, and the sterilizer shall be free from any defects which may detract from its appearance or may impair its serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *For visual examination.*—Sampling procedures for visual examination shall be conducted in accordance with the procedures set forth in Military Standard MIL–STD–105.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.

4.1.2 *For tests.* — Sample sizes for tests shall be as indicated for inspection level L–2 in Appendix to Military Standard MIL–STD–105, except that the acceptance number shall be zero (0) for all sample sizes, and a minimum of three (3) samples shall be taken.

4.2 **Inspection.**—The inspector shall ascertain that jars have been examined and tested in accordance with specification requirements.

4.2.1 *Classification of defects.*—Inspection shall be conducted in accordance with the following classification of defects:

Categories and defects

Major *AQL 1.0 percent defective*

101. Jar assembly not furnished complete with all specified components.
102. Mating surfaces of cover and jar not properly ground to provide suitable flat surfaces for seal.
103. Component parts not free of burs, flash chips, or sharp edges.
104. Glass and metal components not free of cracks.
105. Spotwelding of rack not free of burns or other welding defects.
106. Rack fails to fit into, and stand rigidly erect in, jar.
107. Rack fails to properly accommodate 100 scalpel blades.

Minor *AQL 2.5 percent defective*

201. Glass components not substantially free of seams, bubbles, stones, pits, and striae.
202. Rack finish not mirror and substantially free of scratches or mar marks.
203. Dimensions not within specified tolerances.
204. Identification and medical services symbol marking omitted in whole or in part, or not as specified.
205. Jar components not free of chips, dirt, or foreign material.

*Special requirements**

501. Material for component parts shall be as specified.
502. Style, design, and construction shall conform to the requirements of specification and figure 1.
503. Packaging, packing, and marking shall be as specified.

*Noncompliance with any one of the special requirements is cause for rejection.

Note.—Any defect not specifically covered above, but which adversely affects the appearance or serviceability of the jar, shall be added to the above defects in the proper classification as determined by the inspector.

4.3 **Tests.**

4.3.1 *Boil test.*—Racks shall be scrubbed with soap and water, rinsed thoroughly in distilled water, and placed in a glass container of boiling distilled water. The rack shall be boiled for 30 minutes and shall be allowed to remain submerged for 24 hours.

4.3.2 *Chemical composition.* — Tests for chemical analysis shall be conducted in accordance with method 111 or 112 of Federal Test Method Standard 151. In lieu of the above, a certificate of quality, showing results of tests performed to indicate that material is as specified in 3.1.2, may be furnished.

4.4 **Supplier responsibilities for inspection.** —The supplier shall perform the examinations and tests set forth in this specification to substantiate conformance of supplies to specification requirements. The examinations and tests shall be at the expense of the supplier. Suppliers shall have adequate test facilities or shall arrange for the utilization of test facilities acceptable to the Government to be used for executing specific prescribed tests. Records of examinations and tests performed by the supplier shall be maintained by the supplier and made available to the Government upon the Government's request, at any time, or from time to time, for a period of 2 years after the delivery of the supplies to which these records relate. The supplier shall be responsible for compliance with all requirements of this specification, and all other technical requirements of the contract.

5. PREPARATION FOR DELIVERY

The levels of preservation, packaging and packing protection used are defined in Fed. Std. No. 102 (for civil agencies only).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.

TABLE I.—*Packaging quantities*

Federal stock number	Unit package	Intermediate package	Shipping container
6530–299–8602 or 6530–782–7800	1 unit	Not required	24 units

5.1 Packaging.

5.1.1 *Unit of issue.*—One jar, as specified, constitutes one unit.

5.1.2 *Packaging quantities.*—The number of units of issue indicated in table I shall be packaged in each unit and exterior container, as applicable, for the required level of protection specified in the procurement document.

5.1.2.1 *Packing variation permitted.* — If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container, of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Unit package.*—Each unit shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP–B–636, type I, class 1 or type II, class 1. Carton shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to, the contents. Closure shall be adequate to insure against spillage of contents under normal handling.

5.1.4 *Level C.*—Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—Exterior container shall be constructed in accordance with Federal Specification PPP–B–621, table IV.

5.2.1.2 *Case liner.*—Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.* — Strapping, when required, shall be in accordance with applicable box specification.

Note.—Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.*—Exterior container shall be constructed in accordance with Federal Specification PPP–B–621, table II.

5.2.3 *Level C.* — The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 *Unit package.* — Each unit package

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.

shall be marked in accordance with section 5 of Military Standard MIL–STD–129.

5.3.2 *Shipping container.*—Shipping container shall be marked in accordance with Military Standard MIL–STD–129. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

6. NOTES

6.1 Ordering data.—Purchasers should exercise any desired options offered herein and procurement documents should specify the following:

(*a*) Title, number and date of this specification.

(*b*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification covers the following items appearing in the Armed Services Medical Stock List:

6530–299–8602 JAR, STERILIZING, Glass.

6530–782–7800 JAR, STERILIZING, Scalpel Blades, Glass.

6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.4 Transportation description.—Transportation description applicable to this item is:

Sterilizers, not otherwise indexed by name, other than cabinet.

Carload minimum weight 24,000 pounds, subject to Rule 34, Uniform Freight Classification.


Motor volume minimum weight 24,000 pounds, subject to Rule 34, National Motor Freight Classification.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:

Army—M
Navy—Md
Air Force.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.

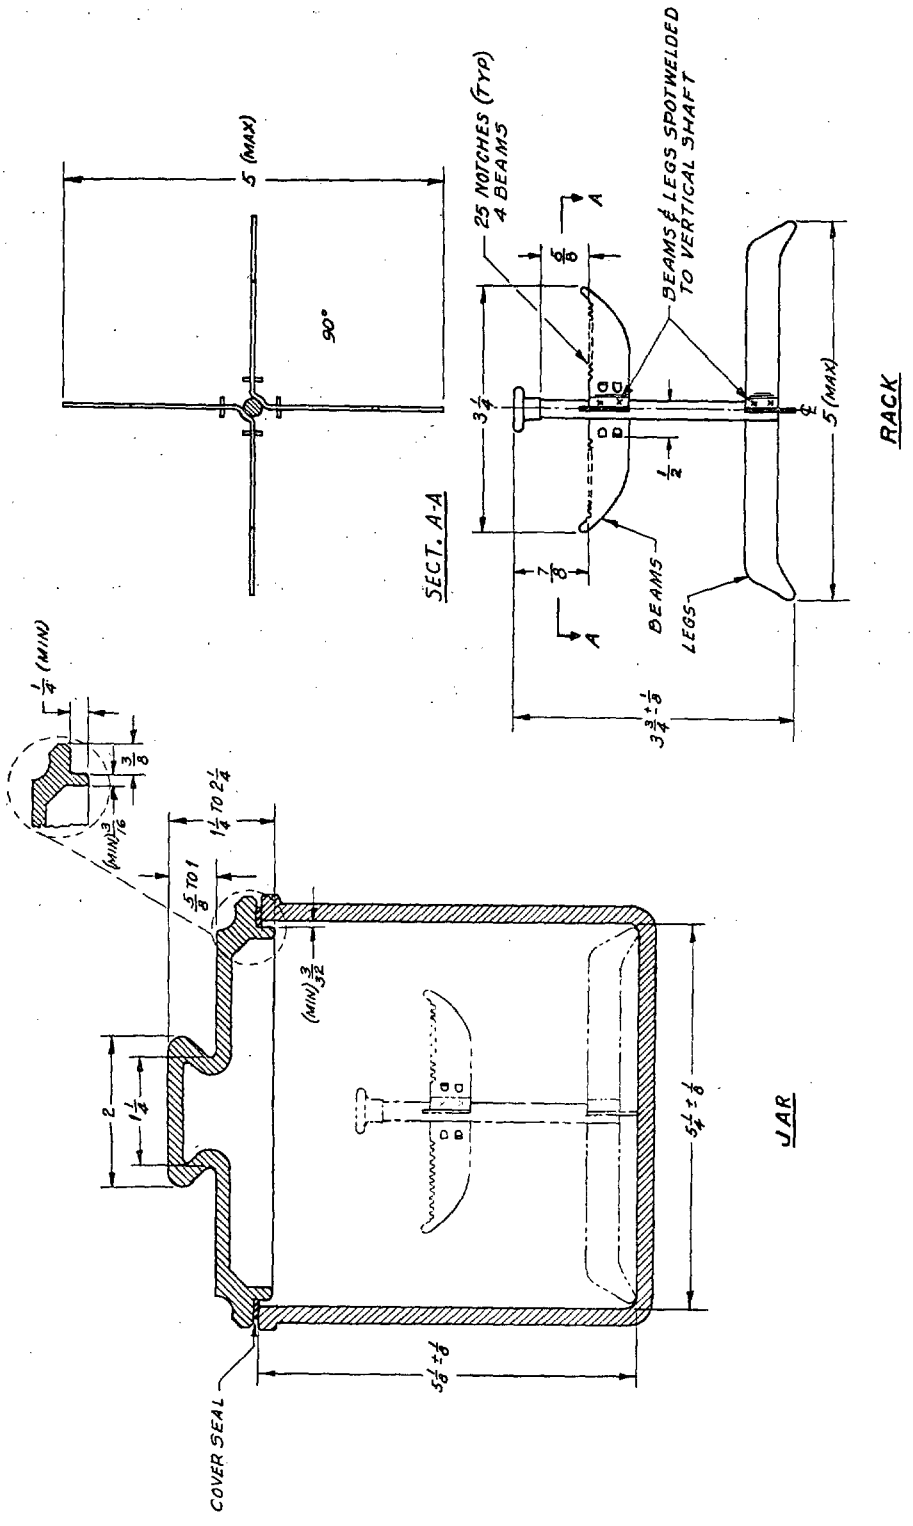

UNLESS OTHERWISE SPECIFIED TOLERANCES ARE AS FOLLOWS:
± 1/16
± 3°

FIGURE 1.

Copies of this specification may be purchased for 5 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.