DD-M-00440a(DSA-DM)
July 2, 1971
Interim Revision of
Fed. Spec. DD-M-440
September 24, 1956

INTERIM FEDERAL SPECIFICATION

MIXING SLAB, DENTAL

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification DD-M-440.

1. SCOPE

1.1 Scope. This specification covers a glass mixing slab for dental use.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, D. C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston; New York; Atlanta; Chicago; Kansas City, Mo.; Fort Worth; Denver; San Francisco; Auburn, Washington; and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

SPECIFICATIONS

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof Or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.


(Copies of Military specifications, standards and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The mixing slab shall be made from clear, colorless plate glass.

3.2 Style, design and dimensions. The mixing slab shall be rectangular in shape with flat and parallel faces and all edges beveled. The mixing slab shall be suitable for mixing dental cements and other manipulatives on both the upper and lower mixing surfaces (6 by 3 inch faces). Style, design and dimensions of the slab shall be in accordance with Figure 1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.

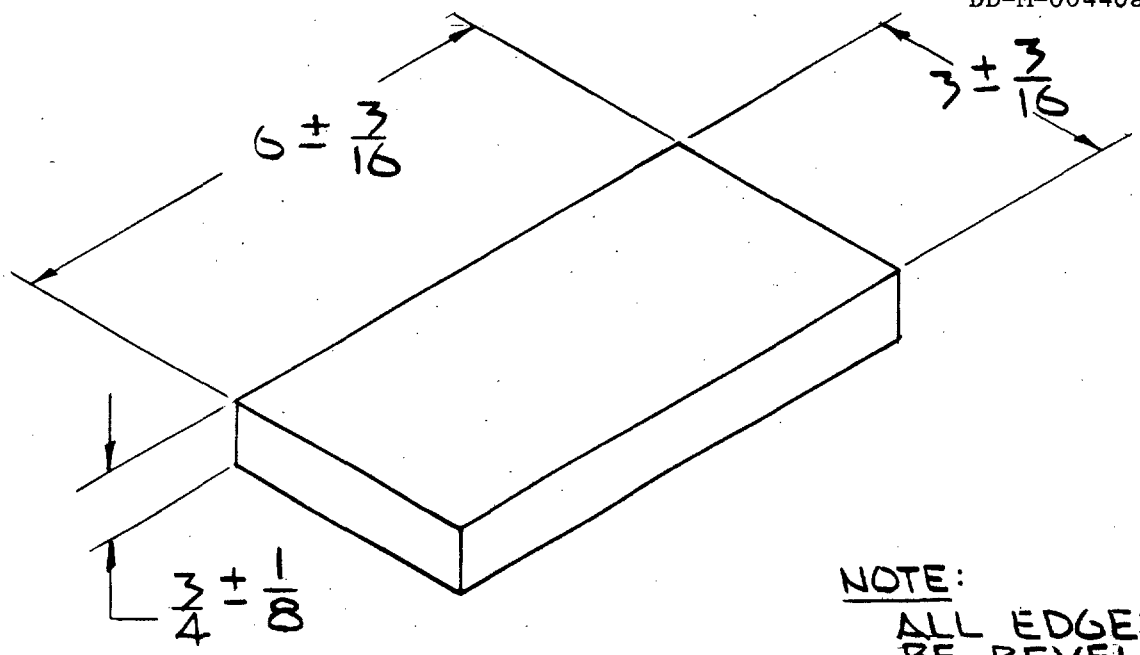

NOTE:
ALL EDGES SHALL BE BEVELED.

MIXING SLAB, DENTAL, GLASS

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.

3.3 Finish. All surfaces of the mixing slab shall be flat and smooth, and shall be highly polished. The mixing surfaces (6 inches by 3 inches) shall be free from chips, cracks, grind marks, scratches and open gaseous inclusions.

3.4 Workmanship. Workmanship shall be first class throughout. The mixing slab shall be free from defects which detract from its appearance or may impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures).

4.2 Quality conformance inspection. The examinations required to assure conformance of those items or lots of items to be offered are classified as specified in Tables I and II (see 4.2.1 and 4.3).

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in Table I. The unit of product for examination purposes shall be one mixing slab.

Table I. Examination Criteria

Type defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.

4.3 Examination. The mixing slab shall be examined for defects including, but not limited to, those listed in table II.

Table II. Classification of Defects

Categories	Defects
Critical:	None defined.
Major:	
101	Type of glass not as specified.
102	Style of mixing slab not as specified.
103	Glass not clear and colorless.
104	Opposing surfaces not flat and parallel.
105	Edges not beveled.
106	All surfaces not flat and smooth, and not highly polished.
107	Mixing surfaces (6 inches by 3 inches) not free from chips, cracks, grind marks, scratches and open gaseous inclusions.
Minor:	
201	Dimensions not as specified.
202	Sides (edges) of mixing slab not free from chips and cracks.
203	Packaging, packing and marking not as specified.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One mixing slab, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table III shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.

Table III. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	48 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be over-packed in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each unit shall be wrapped in Kraft paper or other suitable material and packaged in a box of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676 except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c.

5.2.1.2 Case liner. Each level A wood box shall be lined with a water-proof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure of wood boxes shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Unit packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 Federal Stock Number (FSN) coverage. This specification covers the following item appearing in the Federal Supply Catalog:

FSN	Item Identification
6520-556-2000	MIXING SLAB, DENTAL, 3 by 6 inches

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.

6.3 Specification changes. The margins of this specification have not been annotated with asterisks to indicate where changes from the previous issue have been made due to the extensive changes to this document.

6.4 This specification does not cover all sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the sizes which are normally procured to meet Federal Government requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6520-1294

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

☆U.S. GOVERNMENT PRINTING OFFICE: 1971-714-157/967

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements .

SPECIFICATION
DD-M-00440a (DSA-DM)

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:43Z
Check the source to verify that this is the current version before use.