DD-M-200a
AUGUST 6, 1958
SUPERSEDING
Int. Fed. Spec. DD-M-00200 (GSA-FSS)
April 25, 1957 and
Fed. Spec. DD-C-616a
June 10, 1946

FEDERAL SPECIFICATION

MEDICINE GLASS

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers medicine glasses for use in hospitals and dentists' offices.

1.2 Classification.

1.2.1 *Types.*—Medicine glasses shall be of the following types, as specified (see 6.1):

Type I.—Hospital.
Type II.—Dental.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

PPP-B-621—Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636—Boxes, Fiber.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specifications:

MIL-L-10547 — Liners, Case, Waterproof.

Military Standards:

MIL-STD-105 — Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129—Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material.—Medicine glasses shall be made of colorless transparent flint glass of a quality that will retain its luster and transparency.

3.1.1 *Boiling resistance.*—Medicine glasses

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.

shall be of such composition and so well annealed that they shall show no evidence of corrosion, chipping, scumming, or cracking, when tested as specified in 4.3.1.

3.1.2 *Thermal shock resistance.*—Medicine glasses shall not crack, when tested as specified in 4.3.2.

3.2 Style, design, and dimensions.

3.2.1 *Type I.*—Glasses shall be of the style, design, and dimensions shown in figure 1.

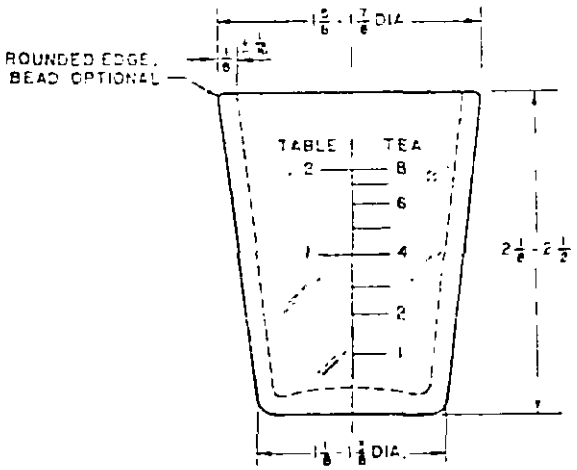


FIGURE 1.—Type I, hospital, medicine glass.

3.2.2 *Type II.*—Glasses shall be of the type known to the dental profession as "Dappen" medicine glasses. They shall be hexagonal, octagonal, or decagonal in shape, and so formed as to provide a concavity in the upper and lower surfaces of the glasses. Hexagonal glasses, when furnished, shall be of the style, design, and dimensions shown in figure 2. Decagonal and octagonal glasses, when furnished, shall be of the general design and over-all dimensions shown in figure 2.

3.3 Graduation markings, type I.—Minimum graduations required for each glass shall be as shown on figure 1. Additional graduations in ounces and cubic centimeters shall be acceptable. The scale, numbers, and all other markings shall be permanently etched, engraved, or molded on the glass, and shall be readily observed regardless of the color or character of the liquid in the glass.

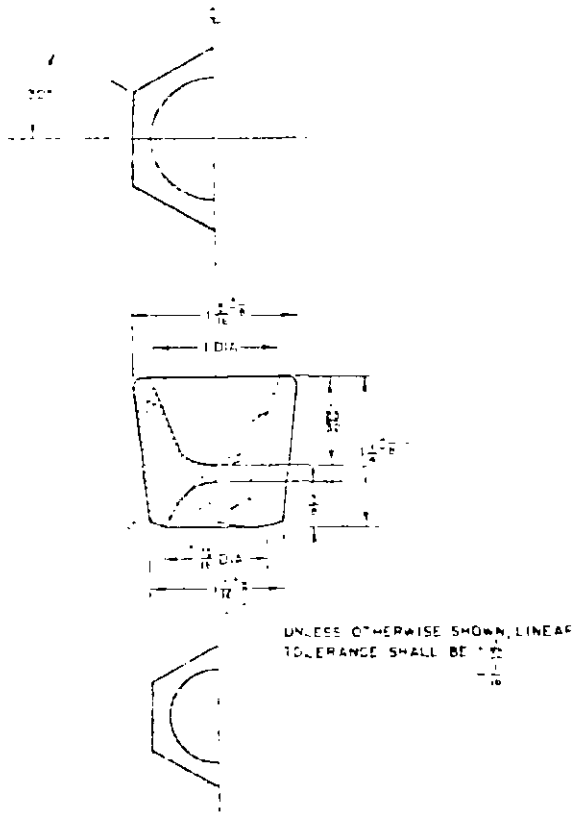


FIGURE 2.—Type II, dental, medicine glass.

3.4 Identification marking. — Each glass shall be marked with the name or registered trade-mark of the manufacturer. Markings shall be permanently etched, engraved, or molded on the glass, and shall be readily observed regardless of the color or character of the liquid in the glass.

3.5 Workmanship.—All surfaces of each medicine glass shall be highly polished and clean. Medicine glasses shall be smoothly and symmetrically finished, practically free from seeds, blisters, and other imperfections which affect their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *For visual examination.*—Sampling procedures for visual examination shall be

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.

conducted in accordance with the procedures set forth in Military Standard MIL–STD–105.

4.1.2 *For tests.* — Sample size for each major A and minor A test shall be as indicated for inspection level L–4 in Appendix to Military Standard MIL–STD–105.

4.2 **Inspection.**—The inspector shall ascertain that the medicine glasses have been examined and tested in accordance with specification requirements.

4.2.1 *Classification of defects.*—Inspection shall be conducted in accordance with the following classification of defects:

Categories and defects	
Major A	AQL 2.5 percent defective
101	Glass does not meet requirements of boiling test.
102	Glass does not meet requirements of thermal shock test.
Major B	AQL 2.5 percent defective
151	Glass not free of cracks, chips, or sharp edges.
152	Graduations omitted.
153	Graduation markings not minimum specified.
Minor A	AQL 4.0 percent defective
201	Dimensions not within specified limits.
Minor B	AQL 4.0 percent defective
201	Glass not free of striae, seeds, blisters, or other imperfections.
202	Graduations not legible or clear.
203	Identification markings not legible or omitted.
204	Glass not symmetrically formed.
	Special requirements*
501	Type shall be as specified.
502	Style and design shall be as specified.
503	Graduation markings and identification marking shall be permanent.
504	Material shall be as specified.
505	Packaging, packing, and marking shall be as specified.

*Noncompliance with any one of the special requirements is cause for rejection.

Note.—Any defect not specifically covered herein, but which adversely affects the appearance or serviceability of the medicine glasses, shall be added to the above defects in the proper classification as determined by the inspector.

4.3 **Tests.**

4.3.1 *Boiling test.*—The sample medicine glasses shall be completely immersed in distilled water in a closed vessel having a small steam vent and boiled continuously for 6 hours for type I and 4 hours for type II, boiling distilled water being added when necessary to compensate for evaporation losses. The medicine glasses shall be suspended in the water so that they do not come in contact with the containing vessel.

4.3.2 *Thermal shock test.* — The sample medicine glasses shall be immersed in tap water at 18.5° ± 2.5° centigrade (65° ± 5° Fahrenheit), allowed to remain 10 minutes, then transferred suddenly into boiling water. This operation shall be repeated five times for type I and four times for type II. Samples used for this test shall not be those subjected to the boiling test specified in 4.3.1.

4.4 **Supplier responsibilities for inspection.**—The supplier shall perform examinations and tests set forth in this specification to substantiate conformance of supplies to specification requirements. The examinations and tests shall be at the expense of the supplier. Suppliers shall have adequate test facilities, or shall arrange for test facilities acceptable to the Government to be used for executing specific prescribed tests. Records of examinations and tests performed by the supplier shall be maintained by the supplier and made available to the Government upon the Government's request, at any time, or from time to time, for a period of 2 years after the delivery of the supplies to which these records relate. The supplier shall be responsible for compliance with all requirements of this specification, and all other technical requirements of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.

TABLE I.—*Packaging quantities*

Federal stock number	Unit package	Intermediate package	Shipping container
6520–550–2000	Not required	12 units	576 units
6530–780–7000	Not required	12 units	288 units

5. PREPARATION FOR DELIVERY

The levels of preservation, packaging and packing protection used are defined in Federal Standard No. 102, (for civil agencies only).

5.1 Packaging.

5.1.1 *Unit of issue.* — One (1) glass, as specified, constitutes one unit.

5.1.2 *Packaging quantities.*—The number of units of issue indicated in table I shall be packaged in each intermediate and exterior container, as applicable, for the required level of protection specified in the procurement document.

5.1.2.1 *Packing variation permitted.* — If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Intermediate package.*—Intermediate package shall be a carton of appropriate size fabricated of not less than 200-pound-test fiberboard and constructed in accordance with Federal Specification PPP–B–636, type I, class 1. Carton shall be provided with full-height partitions fabricated of the same strength material as body of carton, so arranged that each glass is securely held in an individual cell.

5.1.4 *Level C.*—Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—Exterior container shall be a box constructed in accordance with Federal Specification PPP–B–621, table III.

5.2.1.2 *Case liner.*—Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.*—Strapping, when required, shall be in accordance with applicable box specification.

Note.—Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.*—Exterior container shall be a box constructed in accordance with Federal Specification PPP–B–636, type I, class 1, and fabricated from not less than 275-pound-test fiberboard.

5.2.3 *Level C.* — The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.

point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 *Intermediate package.*—Each intermediate package shall be marked in accordance with section 5 of Military Standard MIL–STD–129.

5.3.2 *Shipping container.*—Shipping container shall be marked in accordance with Military Standard MIL–STD–129. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

6. NOTES

6.1 **Ordering data.** — Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number and date of this specification.

(*b*) Type required (see 1.2).

(*c*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification covers the following items appearing in the Armed Services Medical Stock List:

6520–550–2000 DISH, MEDICAMENT, DENTAL.

6530–780–7000 MEDICINE GLASS, 1 oz.

6.3 This specification does not include all types, classes, grades, sizes, etc. of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.4 Transportation description.—Transportation description applicable to these items is:

Glassware. NOIBN (Specify valuation).
Carload minimum weight 24,000 pounds, subject to Rule 34, Uniform Freight Classification.
Motor volume minimum weight 24,000 pounds, subject to Rule 34, National Motor Freight Classification.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:
Army—M
Navy—Md
Air Force.

Copies of this specification may be purchased for 5 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:42Z
Check the source to verify that this is the current version before use.