A-A-50873A
30 May 1989
SUPERSEDING
A-A-50873
24 June, 1983

COMMERCIAL ITEM DESCRIPTION

BASSINET AND DRESSING TABLE COMBINATION, HOSPITAL

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-B-36560 which is cancelled.

This Commercial Item Description covers a corrosion-resisting steel hospital bassinet and dressing table combination suitable for the individual care of the newborn.

Salient characteristics:

The hospital bassinet and dressing table combination shall be suitable for use in medical facilities for the individual care of the newborn. The bassinet shall consist of a tubular framework designed to hold a removable plastic basket, a sliding shelf, and a side drawer in a suitably counter-weighted cabinet as shown in Figures 1, 2, or 3 or a combination thereof. The overall dimensions, in the compact configuration, shall be approximately 16 inches wide by 33 inches long by 35 inches high excluding the drawer pull and the basket. The unit shall move and turn easily when wheeled over a flat surface with the shelf in the closed position. The cabinet shall have approximate overall dimensions of 26 inches wide, 16-1/2 inches deep, and 9-1/2 inches high, with a drawer opening from the side. The drawer dimensions shall be approximately 22 inches wide, 15 inches deep, and 5-1/2 inches high. The cabinet bottom surface shall be at least 15 inches above the floor.

AMSC N/A FSC 6530

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

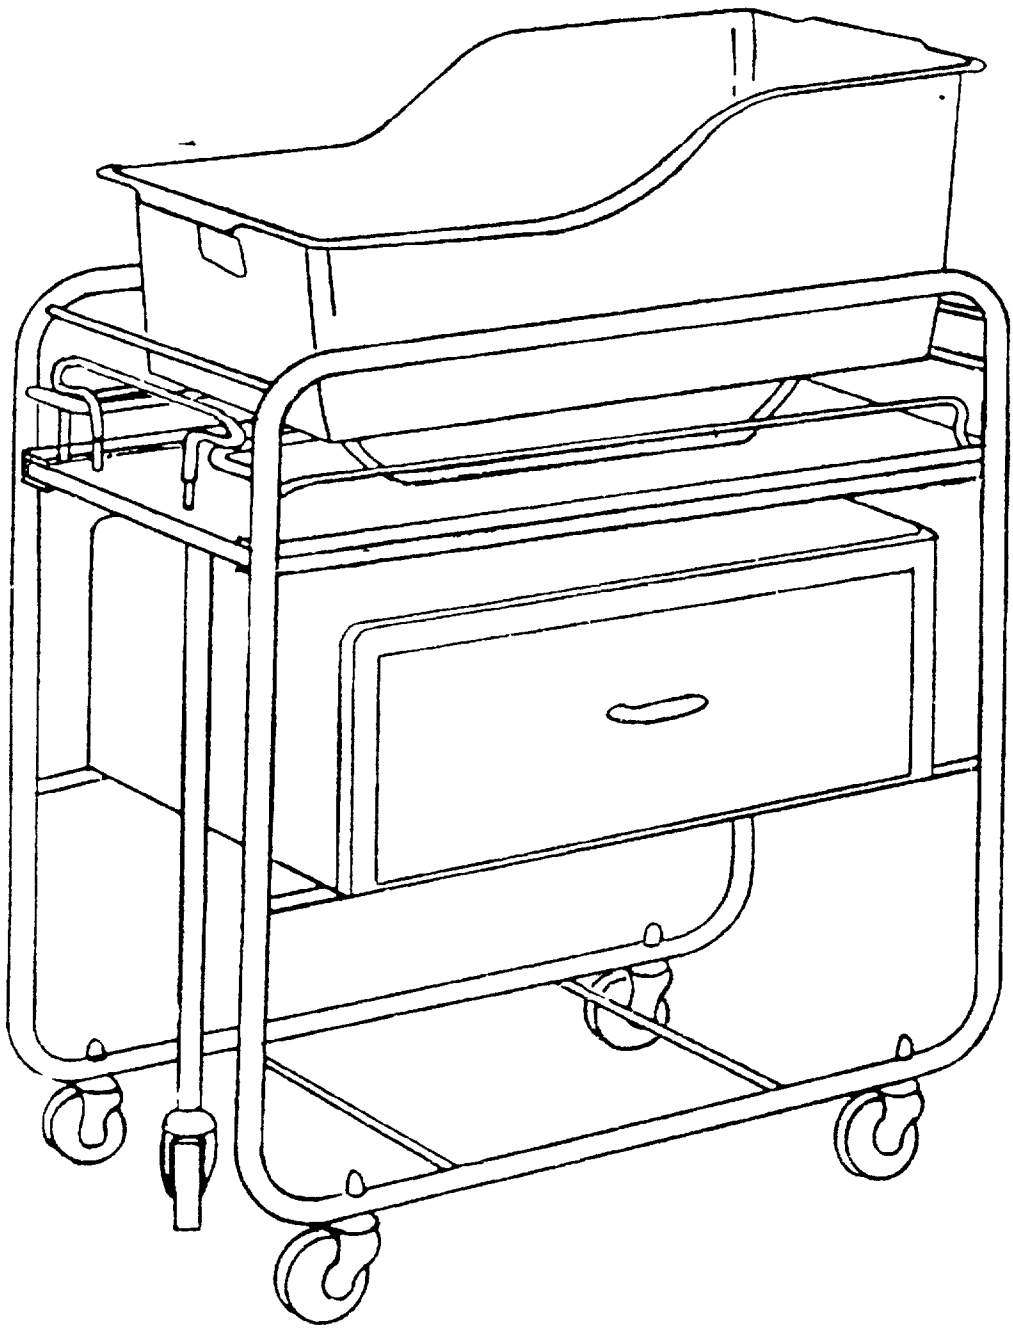


FIGURE 1. Bassinet

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

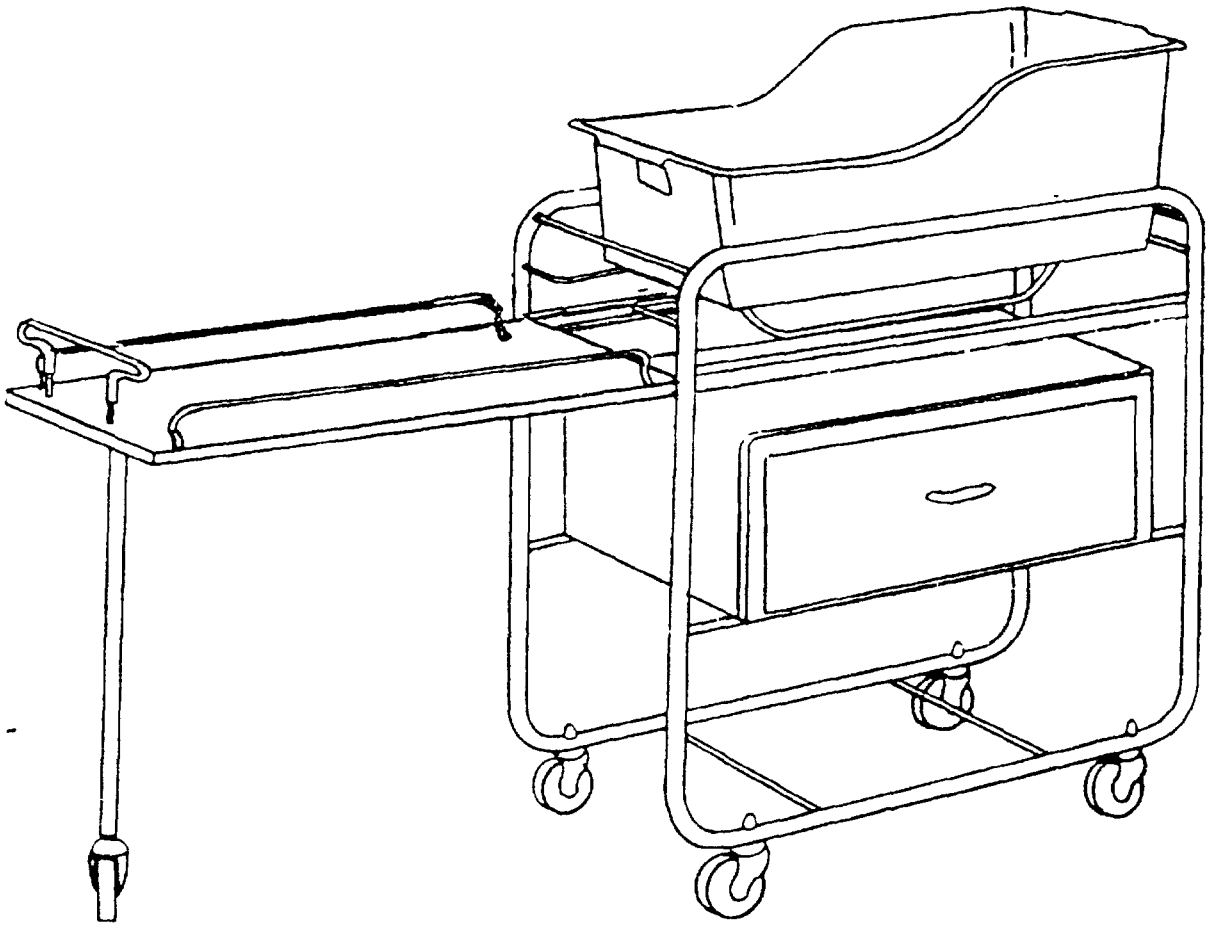


FIGURE 2 Bassinet (with tray extended)

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:48Z
Check the source to verify that this is the current version before use.

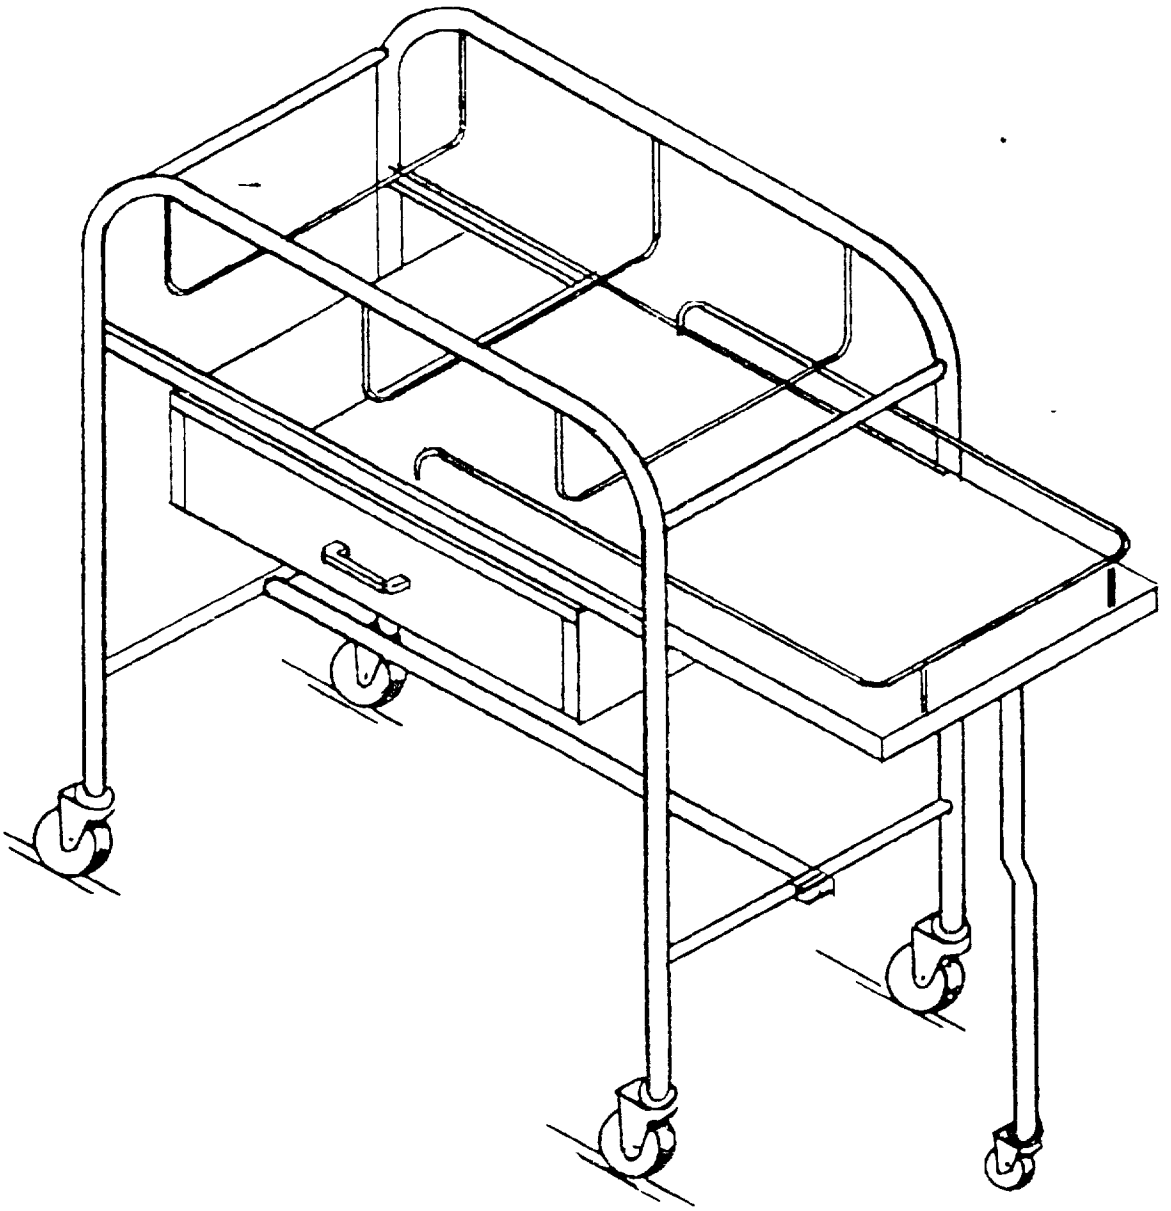


FIGURE 3 Bassinet

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:48Z
Check the source to verify that this is the currentversion before use.

The shelf shall be approximately 27 inches above the floor and shall be approximately 14 inches wide by 33 inches in length. The shelf shall be equipped with a 3 inch high guard rail. The shelf shall extend from the end of the stand, lock positively in both the open and closed positions with minimum sideplay and be supported by one or two legs. A "U" shaped leg assembly with two casters shall be acceptable. The sliding shelf shall have a safety stop so that the shelf cannot be accidently pulled out of the shelf slides.

The bassinet stand, shelf, and cabinet shall be constructed of American Iron and Steel Institute Series 300 corrosion-resisting steel. The basket support rod configuration shall be designed to provide Trendelenberg and reverse Trendelenberg positions. The rods shall be approximately 30 inches above the floor.

The bassinet stand shall have four 3-inch diameter ball bearing swivel casters. The sliding shelf shall have a minimum of one 2 inch diameter ball bearing swivel caster. The casters shall turn easily, smoothly, and quietly.

The bassinet basket shall be formed from one piece of transparent polycarbonate with integrally molded handles on each end and a vented bottom. The basket shall incorporate an identification card holder. The basket shall be intended for use with a bassinet mattress with dimensions of 27 inches long, by 13 inches, wide.

Workmanship. The hospital bassinet and dressing table combination shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One table, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 4.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one hospital bassinet and dressing table combination as specified in this description.

Defects

Bassinet and dressing table combination is not complete with all components.

Cabinet drawer or shelf fail to properly retract or extend from the frame of the carriage.

Table fails to move and turn easily and smoothly when wheeled over a flat surface.

Component parts in assembly are not properly fitted or securely fastened.

Component parts are not free of cracks or ruptures.

Edges and corners of component parts are not free of burrs or sharpness.

Welds are not free of pits, cracks, burns, and undercutting.

Surfaces of bassinet and dressing table combination are not free of scratches or mars.

Finish is not as specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests, including dimensional test shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-3. The unit of product for test purposes shall be one hospital bassinet and dressing table combination.

a. First article. Where a first article sample is required, all tests shall be performed on that unit.

b. Acceptance testing. When a first article sample has not been required, one unit shall be subjected to the performance test specified herein. If a test article sample has successfully passed all tests, performance test shall not be required at acceptance.

Tests

Shelf Sliding Action Test. With the bassinet on a smooth level floor surface, the shelf shall be slid alternately into the fully-extended position and the fully-closed position for 50 complete cycles. Any evidence of bending or looseness of the shelf support tube, or failure of the shelf lock mechanism in either the open or closed position, shall constitute a defect.

Basket Load Test. A weight of 50 pounds shall be placed in the basket. The basket shall then be lifted by the handles and held for a period of 30 seconds, supported by the handles only. Any permanent deformation, or any temporary deformation greater than 2 inches, shall constitute a defect.

Basket Drop Test. The basket shall be dropped from a height of 24 inches onto a hard concrete or tile floor surface so that the point of impact shall be a bottom corner. Any damage suffered by the basket shall constitute a defect. Minor surface scuffs or scratches caused by the drop test shall not be a defect.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6530-00-935-6590

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:48Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6530-2044

Location:
CID/BASSINET/BASSINET/H13-33

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:48Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-50873A	BASSINET AND DRESSING TABLE COMBINATION, HOSPITAL

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-0-26108:48Z
Check the source to verify that this is the current version before use.