GGG-T-671C
May 11, 1992
SUPERSEDING
GGG-T-00671B(GSA-FSS)
December 11, 1967
GGG-T-671A
August 18, 1955

FEDERAL SPECIFICATION

TROWELS

This specification is approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers trowels used in spreading and smoothing materials such as plaster, cement, and asbestos or mastic paste while in a soft state.

1.1.1 Federal specification coverage. Federal specifications do not cover all varieties of the commodity indicated by the title of the specification, or which are commercially available, but are intended to cover only those generally used by the Federal Government.

1.2 Classification.

1.2.1 Types and classes. Trowels shall be of the following types and classes as specified (see 6.2):

Type I - Plastering
Type II - Cement
  Class 1 - Midget
  Class 2 - Regular
Type III - Brick
Type IV - Pointer
Type V - Mastic (notched)
  Class 1 - Linoleum
  Class 2 - Asphalt tile
Type VI - Gauging
Type VII - Pipe covering
Type VIII - Margin
Type IX - Tuck pointer, joint filler, or caulking

2. APPLICABLE DOCUMENTS

2.1 Government documents. The following documents, of the issues in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

Federal Standards:

FED-STD-123	- Marking for Shipment (Civil Agencies)
FED-STD-376	- Preferred Metric Units for General Use by the Federal Government

Federal Specifications:

QQ-A-367	- Aluminum Alloy Forgings
PPP-P-40	- Preservation and Packing of Hand Tools and Tool Accessories For Power Driven, Metal and Woodworking Machinery

(Activities outside the Federal Government may obtain copies of Federal specifications, standards, and Commercial Item Descriptions as outlined under General Information in the Index of Federal Specifications, Standards and Commercial Item Descriptions. The Index, which includes cumulative bimonthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, DC 20402.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.

(Single copies of this specification, and other Federal specifications and Commercial Item Descriptions required by activities outside the Federal Government for bidding purposes are available without charge from General Services Administration Business Service Centers in Boston, MA; New York, NY; Philadelphia, PA; Washington, DC; Atlanta, GA; Chicago, IL; Kansas City, MO; Fort Worth, TX; Houston, TX; Denver, CO; San Francisco, CA; Los Angeles, CA; and Seattle, WA.)

(Federal Government activities may obtain copies of Federal standardization documents and the Index of Federal Specifications, Standards and Commercial Item Descriptions from established distribution points in their agencies.)

Military Standards:

MIL-STD-105	- Sampling Procedures and Tables for Inspection by Attributes
MIL-STD-129	- Marking for Shipment and Storage

(Copies of military specifications and standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Non-Government publications. The following documents form a part of this specification to the extent specified herein. Unless a specific issue is identified, the issue in effect on date of invitation for bids or request for proposal shall apply.

American Society for Testing and Materials (ASTM)

E 18	- Metallic Materials Rockwell Hardness and Rockwell Superficial Hardness of
D 4101	- Standard Specification for Propylene Plastic Injection and Extrusion Materials

(Applications for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103-1187.)

(Non-Government standards and other publications are normally available from the organizations that prepare or distribute the documents. These documents also may be available in or through libraries or other informational services.)

3. REQUIREMENTS

3.1 Illustrations. The illustrations herein are descriptive and not restrictive and are not intended to preclude the purchase of trowels otherwise conforming to this specification.

3.2 Design. Trowels shall consist essentially of a blade and handle, except that types I, II, and V trowels shall be provided with a mounting.

3.3 Materials. Materials used in construction of the trowels shall be as specified hereinafter. All forgings shall be of uniform quality and free from all defects and imperfections that might affect serviceability or durability.

3.3.1 Blades. Blades shall be of high carbon tool steel of not less than AISI 1075 for types I, II, and V trowels, and AISI 1070 to 1095 for types III, IV, VI, VII, VIII, and IX trowels.

3.3.2 Mounting. Mounting for types I, II, and V trowels shall be of permanent mold, or forged aluminum in accordance with QQ-A-367.

3.3.3 Handles.

3.3.3.1 Wood. Wood handles shall be of clear, straight-grained hardwood such as hickory, maple, birch, persimmon, or basswood. Handles shall be smoothly finished and free from cracks or splinters.

3.3.3.2 Plastic. Plastic handles shall be of high-impact strength in accordance with ASTM D 4101 and shall withstand the tests specified in 4.4.4.1 and 4.4.4.2.

3.3.3.3 Aluminum. Type I, II, and V trowels may have aluminum handles as an integral part of the mounting.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:41Z
Check the source to verify that this is the currentversion before use.

3.4 Construction.

3.4.1 Blade construction. Blades shall be smoothly and evenly ground, and when placed on a flat surface shall show no evidence of warpage. Type I, II, and V trowels shall be rectangular in shape. Types III, IV, VI, VII, VIII, and IX shall taper from heel to toe and be provided with a tang. In addition, the blade may also taper from lengthwise centerline toward edges of the blade.

3.4.1.1 Types III, IV, VI, VIII, and IX tang. The tang for types III, IV, VI, VII, VIII, and IX shall be suitably shaped to hold the handle securely.

3.4.2 Method of securing handles. Handles, where not integral with the mounting, shall be tightly fitted on the tang, and shall not turn or loosen under service conditions. For types III, IV, VI, VII, VIII, and IX with wood handles, the end of the handle where the tang enters shall be fitted with a permanently affixed metal ferrule. Except for type III, ferrule shall be not less than 1 inch long. The ferrule for type III shall be not less than 1-1/2 inches long. Wood handles for type I, II, and V trowels shall have a hole the full length of the handle and form a tight fit on the tang of the mounting. Handle shall be secured in position by a nut which may be tightened upon the threaded portion of the tang on the mounting over a suitable washer, or by riveting the end of the tang over a suitable washer.

3.4.3 Construction of mounting. The mountings for types I, II, and V trowels shall be shaped to reinforce the blade and be provided with a suitable tang, or an integral handle. The mountings shall be secured to the blade by steel or brass, flathead rivets or pins, and shall not separate from the blade when tested as specified in 4.4.2. If rivets or pins are used which extend through the blades of types I, II, and V trowels, they shall be flush with the surface of the blade. The mounting shall be free of burrs or rough edges.

3.4.3.1 Types I, II, and V tang. The tang for mounting of types I, II, and V shall be integral with the mounting, or properly shaped to accept the handle when not an integral part of the mounting.

3.5 Blade hardness. The blade shall be properly hardened and tempered to show a hardness of not less than 46 nor more than 55 on the Rockwell C scale.

3.6 Performance. The trowels shall withstand the test requirements of table I, and show no evidence of cracks, breaks, pulling out of rivets or pins, turning of edges, or permanent set when tested as specified in 4.4.2.

TABLE I. Performance test requirements

Type	Class	Movement each side of the perpendicular	Number of flexes	Strokes of shaper per minutes
		Inches		
I		2	4,000	20
II	1	1-3/4	4,000	20
	2	1-3/4	4,000	20
III		3	3,000	20
IV		1-1/2	750	20
	1	1-3/4	4,000	20
V	2	1-3/4	4,000	20
VI		1-1/2	750	20
VII		3	3,000	20
VIII		1-1/2	750	20
IX		2	1,500	20

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.

3.7 Marking. Each item shall be marked with the manufacturer's name or identifying symbol and the state or country of manufacture. The marking shall be engraved, etched, or stamped in such a manner that it will be permanent to the extent that it will remain clear and legible throughout the life of the item.

3.8 Type I, plastering. Type I trowel blades shall be securely fastened to the mounting by a minimum of 10 flathead rivets or steel pins. Mounting shall be as specified in 3.3.2 and 3.4.3. Trowel shall conform to table II, and be similar to figure 1.

TABLE II. Type I, plastering

Blade						Handle			
Length		Width		Thickness		Length		Diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inches	Inches
10-7/8	11-3/8	4-3/8	4-7/8	0.023	0.029	4-1/2	4-7/8	1.430	1-3/4

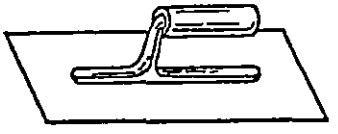


Figure 1. Type I, plastering.

3.9 Type II, cement.

3.9.1 Class 1, midget trowel. Type II, class 1 trowel blades shall be securely fastened to a mounting by a minimum of five flathead rivets or steel pins. Mounting shall be as specified in 3.3.2 and 3.4.3. Trowel shall conform to table III and be similar to figure 2.

TABLE III. Type II, cement, class 1, midget trowel

Blade						Handle			
Length		Width		Thickness		Length		Diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inches	Inches
5-3/8	5-5/8	3-7/8	4-1/8	0.023	0.029	3-7/8	4-1/8	1-3/8	1-3/4
7-3/8	7-5/8	2-7/8	3-1/8	0.023	0.029	4-1/2	4-7/8	1-3/8	1-3/4




Figure 2. Type II, cement, class 1, midget.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:41Z
Check the source to verify that this is the current version before use.

3.9.2 Class 2, regular trowel. Type II, class 2 trowels shall have mountings as specified in 3.3.2 and 3.4.3. Trowel shall conform to table IV, and be similar to figure 3.

TABLE IV. Type II, cement, class 2, regular

Blade						Handle				Number of rivets
Length		Width		Thickness		Length		Diameter		
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inches	Inches	
11-7/8	12-1/8	3-7/8	4-1/8	0.023	0.029	4-1/2	4-7/8	1-7/16	1-3/4	10
13-7/8	14-1/8	3-7/8	4-1/8	0.023	0.029	4-1/2	4-7/8	1-7/16	1-3/4	12
15-7/8	16-1/8	3-7/8	4-1/8	0.023	0.029	4-1/2	4-7/8	1-7/16	1-3/4	14

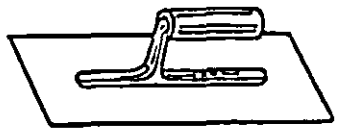


Figure 3. Type II, cement, class 2, regular.

3.10 Type III, brick. Type III trowels shall be of the Philadelphia, or wide heel London pattern, conforming to table V, and be similar to figure 4.

TABLE V. Type III, brick

Blade length, point to point		Blade width at widest point		Blade thickness at heel A		Handle length		Handle diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inches	Inches
10	10-1/2	4-7/8	5-3/8	0.065	0.085	5-1/2	6	1-1/8	1-3/8
10-1/2	11	5-1/8	5-5/8	0.065	0.085	5-1/2	6	1-1/8	1-3/8

A - Measurement to be taken 1/4-inch in from wingtip (see figure 4).

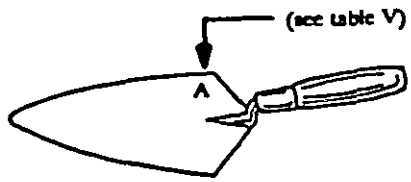


Figure 4. Type III, brick.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.

3.11 Type IV, pointer. Type IV trowels shall conform to table VI and be similar to figure 5.

TABLE VI. Type IV, pointer

Blade length point to point		Blade width at widest point		Blade thickness at heel A		Handle length		Handle diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inch	Inches
4-1/2	5	2-1/4	2-1/2	0.045	0.070	4-1/4	4-5/8	0.75	1-1/8
5-1/2	6-1/4	2-3/8	2-7/8	0.045	0.070	4-3/8	4-7/8	1.00	1-1/4

A - Measurement to be taken 1/4-inch in from wingtip (see figure 5).

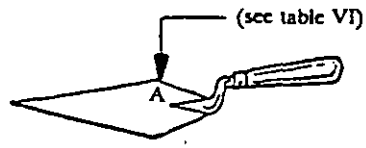


Figure 5. Type IV, pointer.

3.12 Type V, mastic (notched). Type V trowels shall be notched either U- or V-shaped on one or more sides and across the front end. The front end may be cut on an angle to provide even flow of mastic paste in corners and along walls. Trowel shall have a mounting as specified in 3.3.2 and 3.4.3, and be secured to the blade by not less than six flathead rivets or pins.

3.12.1 Class 1, linoleum. Class 1 trowels shall conform to table VII and be similar to figure 6.

TABLE VII. Type V, mastic class 1 linoleum trowel

Blade						Number of notches		Handle			
Length		Width		Thickness		Front	Side	Length		Diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inches	Inches	Inches	Inches
10-3/8	11-1/8	4-3/8	4-5/8	0.023	0.029	20	45	4-1/2	4-7/8	1-1/2	1-3/4

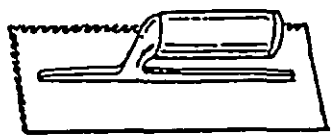


Figure 6. Type V, mastic, class 1, linoleum, and class 2, asphalt tile trowels.

3.12.2 Class 2, asphalt tile. Class 2 trowels shall conform to table VIII, and be similar to figure 6.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.

TABLE VIII. Type V, mastic, class 2, asphalt tile trowel

Blade						Number of notches		Handle			
Length		Width		Thickness		Front	Side	Length		Diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inches	Inches	Inches	Inches
10-1/4	10-7/8	4	4-5/8	0.0209	0.0269	28	70	4-1/2	4-7/8	1-1/4	1-3/4

3.13 Type VI, gauging. Type VI trowels shall conform to table IX and be similar to figure 7.

TABLE IX. Type VI, gauging

Blade						Handle			
Length		Width at widest point		Thickness at heel A		Length		Diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inch	Inches
6-5/8	7-1/4	3	3-3/8	0.065	0.085	4-3/4	5-1/2	7/8	1-1/4

A - Measurement to be taken 1/4-inch in from wingtip (see figure 7).

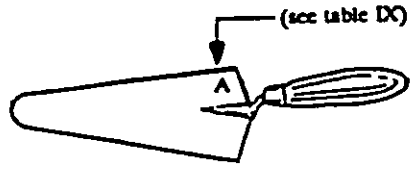


Figure 7. Type VI, gauging.

3.14 Type VII, pipe covering. Type VII trowels shall conform to table X and be similar to figure 8.

TABLE X. Type VII, pipe covering

Blade						Handle			
Length		Width at widest point		Thickness at heel A		Length		Diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inch	Inches
9-7/8	10-1/8	1-7/8	2-1/8	0.065	0.085	4-3/4	5-1/2	1	1-1/4

A - Measurement to be taken 1/4-inch in from wingtip (see figure 8).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.

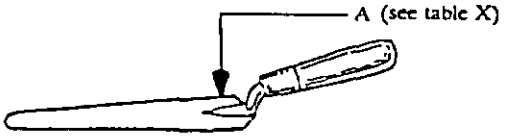


Figure 8. Type VII, pipe covering.

3.15 Type VIII, margin. Type VIII trowels shall conform to table XI and be similar to figure 9.

TABLE XI. Type VIII, margin

Blade						Handle			
Length		Width at widest point		Thickness at heel A		Length		Diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inches	Inches	Inch	Inch	Inches	Inches	Inch	Inches
4-7/8	5-3/8	1-7/8	2-1/8	0.055	0.075	4-1/4	4-3/4	7/8	1-1/8
7-7/8	8-3/8	1-7/8	2-1/8	0.055	0.075	4-1/2	5	7/8	1-1/8

A - Measurement to be taken 1/4-inch in from wingtip (see figure 9).

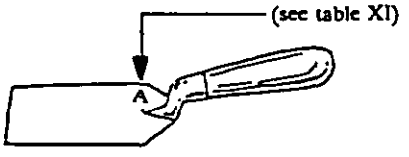


Figure 9. Type VIII, margin.

3.16 Type IX, tuck pointer, joint filler, or caulking. Type IX trowels shall conform to table XII and be similar to figure 10.

TABLE XII. Type IX, tuck pointer, joint filler, or caulking

Blade						Handle			
Length		Width		Thickness		Length		Diameter	
Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.	Min.	Max.
Inches	Inches	Inch	Inches	Inch	Inch	Inches	Inches	Inch	Inches
5-1/2	6-1/2	3/8	7/16	0.055	0.075	4-3/8	4-3/4	7/8	1-1/4
5-1/2	6-1/2	7/16	9/16	0.055	0.075	4-3/8	4-3/4	7/8	1-1/4
5-1/2	6-1/2	9/16	11/16	0.055	0.075	4-3/8	4-3/4	7/8	1-1/4
5-1/2	6-1/2	11/16	13/16	0.055	0.075	4-3/8	4-3/4	7/8	1-1/4
5-1/2	6-1/2	15/16	1-1/16	0.055	0.075	4-3/8	4-3/4	7/8	1-1/4

A - Measurement to be taken 2 inches down blade from heel (see figure 10).

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:41Z
Check the source to verify that this is the current version before use.

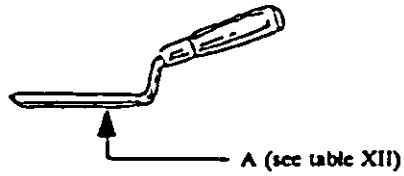


Figure 10. Type IX, tuck pointer, joint filler, or caulking.

3.17 Workmanship. Workmanship shall be of the highest grade throughout and equal in every respect to good commercial practice. The trowels shall be free from rust, burrs, fins, and any other defects which may impair their serviceability or durability.

3.18 Metric product. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, provided they fall within specified tolerances using conversion tables contained in the latest revision of FED-STD-376, and all other requirements of this Federal Specification are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Component and material inspection. In accordance with 4.1 above, the supplier is responsible for insuring that components and materials used were manufactured, tested, and inspected in accordance with the requirements of referenced subsidiary specification and standards to the extent specified, or, if none, in accordance with this specification.

4.2 Sampling procedures. Unless otherwise specified, sampling for inspection shall be performed in accordance with MIL-STD-105.

4.3 Examination.

4.3.1 Visual examination. The end items shall be examined for the defects listed in table XIII. The lot size shall be expressed in terms of trowels. The sample unit shall be one trowel. The inspection level shall be II and the acceptable quality level (AQL), expressed in terms of defects per hundred units, shall be 2.5.

TABLE XIII. Classification of visual defects

Examine	Defect
Design	Not as specified
Material	Not fabricated of specified materials Blades not of high carbon tool steel (see 3.3.1) Mounting not of permanent mold or forged aluminum
Wood handles	Not clear, straight-grained hardwood Not smoothly finished Cracks or splinters
Construction and Workmanship	Component missing or improperly assembled
Blade	Not smoothly and evenly ground; warped Not properly shaped or tapered Not proper hardness

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.

TABLE XIII. Classification of visual defects (cont'd)

Examine	Defect
Tang	Missing or of unsuitable shape
Handles	Improperly secured
Marking	Missing, incomplete, not legible

4.3.2 *Dimensional examination*. The end items shall be examined for any nonconformance with dimensional requirements. The lot size shall be expressed in terms of trowels. The sample unit shall be one trowel. The inspection level shall be II and the AQL, expressed in terms of defects per hundred units, shall be 2.5.

4.4 Testing. The end items shall be tested for the characteristics specified in 4.4.1 through 4.4.4. The lot size shall be expressed in units of trowels. The sample unit shall be one trowel. The inspection level shall be S-3 except only one trowel from each sample unit shall be tested in accordance with 4.4.2, and the AQL, expressed in terms of defects per hundred units, shall be 4.0.

4.4.1 Hardness. Testing shall be accomplished in accordance with ASTM E 18 for compliance with 3.5

4.4.2 Flexing test.

4.4.2.1 Type I, II, and V trowels. One of the edges of the trowels, in alignment with the handle, shall be gripped in a vise on a shaper with the edge of the trowel parallel with and set 5/16-inch below the top surface of the vise jaws. The opposite edge shall be engaged along its entire length by a fixture clamped in the tool postholder in the head of the shaper. The flexing test shall be as illustrated in figure 11, and conform to table I (see 3.6).

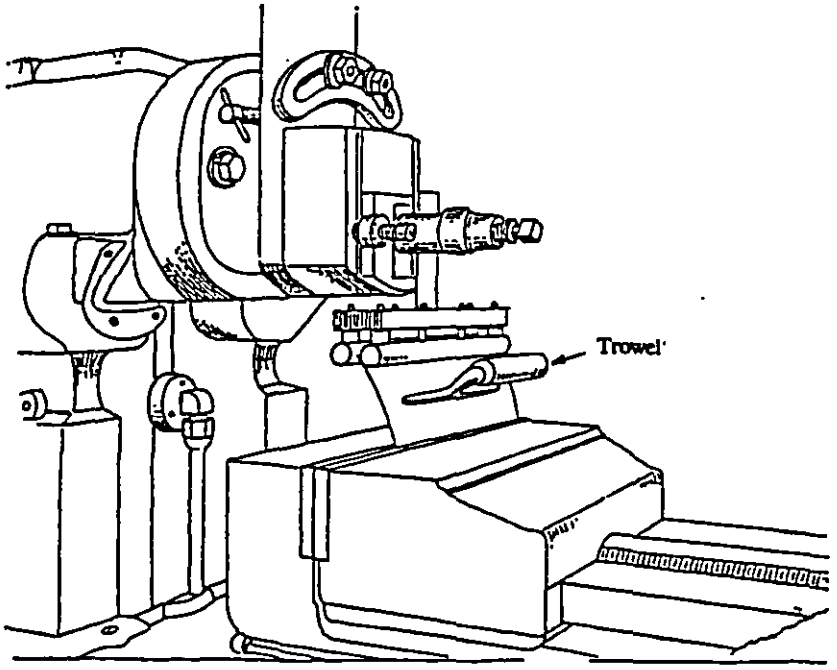


Figure 11. Method of test for types I, II, and V trowels.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.

4.4.2.2 Types III, VII, and IX trowels. The trowels shall be held in a vertical position with the point or toe 1-1/2 inches below the top surface of the vise jaws.

4.4.2.3 Types IV, VI, and VIII trowels. The trowels shall be held in a vertical position with the point or toe 1 inch below the top surface of the vise jaws.

4.4.2.4 Types III, IV, and VI through IX. The handles of types III, IV, and VI through IX trowels may be engaged by an eyebolt secured in a lathe dog which is secured to the tool post or by any similar device. The flexing test shall be as illustrated in figure 12 and conform to table I (see 3.6).

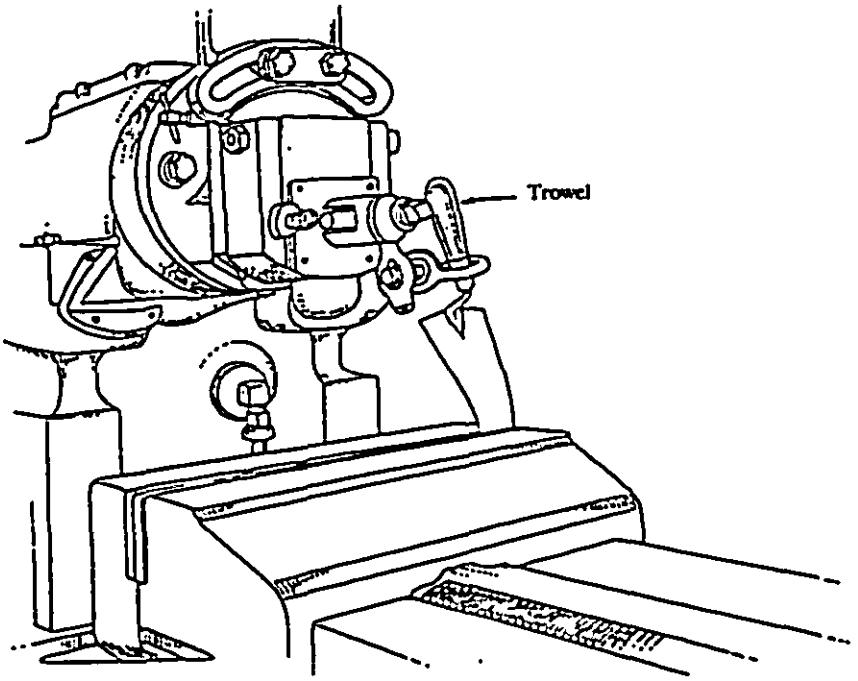


Figure 12. Method of test for types III, IV, and VI through IX trowels, inclusive.

4.4.3 Cutting test. Type III trowels shall be tested by cutting not less than six face bricks in half.

4.4.4 Plastic handle test.

4.4.4.1 Flammability test. Handle shall be clamped in a vise and a flame from blowtorch, Bunsen burner or equivalent, shall be applied to one end for 30 seconds. If this does not ignite the material, flame shall be applied the second time for 30 seconds. If the second application does not ignite the handle, it shall be considered as having passed the test. If the material ignites and the rate of burn does not exceed 2 inches per minute it shall be considered slow burning, thereby also passing the test.

4.4.4.2 Shatter test. Handle shall be placed on a solid foundation and a suitable guard shall be placed around the handle. A weight of 5 pounds shall be dropped directly upon the handle from a 3-foot height. If the handle is still intact after the two direct blows, it shall have passed the test.

4.5 Inspection of preparation for delivery requirements. An inspection shall be made to determine that the preservation, packaging, packing, and marking comply with the requirements in section 5 of this specification. Defects shall be scored in accordance with table XIV. The lot size shall be the number of shipping containers in the end item inspection lot. The sample unit shall be one shipping container. The inspection level shall be S-2 and the AQL, expressed in terms of defects per hundred units, shall be 4.0.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.

TABLE XIV. Classification of preparation for delivery defects

Examine	Defect
Marking (exterior and interior)	Omitted; incorrect; illegible; improper size, location, sequence, or method of application
Materials	Any component missing, damaged, or not as specified
Workmanship	Inadequate application of components such as incomplete closure of container flaps, loose strapping, inadequate stapling Distortion of container
Contents	Number per container is more or less than required Net weight exceeds requirements

5. PREPARATION FOR DELIVERY

5.1 Preservation, packaging, packing, and marking. Preservation, packaging, packing, and marking shall be in accordance with PPP-P-40. The level of preservation, packaging, and packing shall be A, B, or Commercial, as specified (see 6.1).

5.2 Marking.

5.2.1 Civil agencies. In addition to markings required by the contract or order, the unit packages and shipping containers shall be marked in accordance with FED-STD-123.

5.2.2 Military agencies. In addition to markings required by the contract or order, the unit packages and shipping containers shall be marked in accordance with MIL-STD-129.

6. NOTES

(This section contains information of a general or explanatory nature that may be helpful, but is not mandatory.)

6.1 Acquisition requirements. Acquisition documents must specify the following:

a. Title, number, and date of this specification.
b. Type and class required (see 1.2.1).
c. Size required (see applicable table).
d. Selection of applicable level of preservation, packaging, and packing (see 5.1).

6.2 Supersession data. Types and classes of trowels covered in this specification corresponding to those in GGG-T-671A are as follows:

GGG-T-671A	GGG-T-671C
Type I - Plastering	Type I - Plastering
Style A - Malleable iron or steel mounting	Deleted
Style B - Aluminum mounting	Type I - Plastering
Type II - Cement	Type II - Cement
Class 1 - Midget	Class 1 - Midget
Style A - Malleable iron or steel mounting	Deleted
Style B - Aluminum mounting	Type II - class 1
Class 2 - Regular	Class 2 - Regular
Style A - Malleable iron or steel mounting	Deleted
Style B - Aluminum mounting	Type II - class 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.

GGG-T-671A

Type III - Brick
Type IV - Pointer
Type V - Mastic (notched)
  Class 1 - Linoleum
    Style A - Malleable iron or steel mounting
    Style B - Aluminum mounting
  Class 2 - Asphalt tile
    Style A - Malleable iron or steel mounting
    Style B - Aluminum mounting
Type VI - Gauging
Type VII - Pipe covering
Type VIII - Margin
Type IX - Tuck pointer, joint filler, or caulking

GGG-T-671C

Type III - Brick
Type IV - Pointer
Type V - Mastic (notched)
  Class 1 - Linoleum
  Deleted
Type V - class 1
  Class 2 - Asphalt tile
  Deleted
Type V - Class 1
Type VI - Gauging
Type VII - Pipe covering
Type VIII - Margin
Type IX - Tuck pointer, joint filler, or caulking.

MILITARY INTERESTS:

Military Coordinating Activity

Army - GL

Custodians

Army - GL
Air Force - 99

Review Activity

Air Force - 84

User Activities

Army - AT
Navy - MC

CIVIL AGENCY COORDINATING ACTIVITY:

GSA - FSS

PREPARING ACTIVITY:

GSA - FSS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:41Z
Check the source to verify that this is the current version before use.