INCH-POUND

A-A-54842
30 April 1993

COMMERCIAL ITEM DESCRIPTION

SCISSORS, GENERAL SURGICAL, MAYO

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-S-36057A which is cancelled.

This Commercial Item Description covers general surgical scissors of the Mayo design suitable for use as dissecting scissors in general surgery.

Salient characteristics:

General. The scissors shall be of the following types:

TYPE I - Curved

Size 1 - 5-1/2 inches overall length.

Size 2 - 6-3/4 inches overall length.

Size 3 - 9 inches overall length.

TYPE II - Straight

Size 1 - 5-1/2 inches overall length.

Size 2 - 6-3/4 inches overall length.

Material. The scissors shall be fabricated from class 4, martensitic corrosion-resisting steel, in accordance with ASTM F899.

Hardness. The scissors shall have a Rockwell hardness Scale (HRC) of C50 to C55 with the exception of the screw which shall have a Rockwell hardness (HRC) of C40 to C45. The hardness shall be tested in accordance with ASTM E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM E140.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Style, design and dimensions. The scissors shall be in accordance with Figures 1 and 2 for style, design and dimensions.

Performance The performance of the scissors shall be in accordance with the applicable requirements of ASTM F1079. The scissors shall be capable of cutting a continuous length of at least 3/4 inch for Type I and II; Size 1, and 7/8 inch for Type I and II; Size 2, and 1-1/8 inch for Type I, size 3.

Finish. The scissors shall have a mirror finish, except inside blades shall be crocus.

Passivation. The scissors shall be properly passivated.

Corrosion resistance. The scissors shall show no evidence of corrosion or plating of copper when tested for corrosion resistance in accordance with ASTM F1089.

Identification marking and labeling. The scissors shall be legibly marked with the contractor's name or registered trademark and the word "stainless". Foreign manufactured scissors shall bear the name of the country of origin.

Workmanship. The scissors shall be free from defects which detract from their appearance or impair their serviceability.

Unit. Each (EA). One scissors, of the type specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein Unit of product for examination purposes shall be one scissors. Sampling shall be Inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one scissors. Sampling shall be Inspection level S-2 with an AQL of 1.0.

Tests Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Contractor Certification The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered material. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Numbers are covered by this document:

NSN	Item Identification	TYPE	SIZE
6515-00-364-0500	SCISSORS, GENERAL SURGICAL, Curved, Mayo, 5-1/2 inch.	I	1
6515-00-364-0520	SCISSORS, GENERAL SURGICAL, Curved, Mayo, 6-3/4 inch.	I	2
6515-00-364-0560	SCISSORS, GENERAL SURGICAL, Curved, Mayo, 5-1/2 inch.	I	3
6515-00-364-0900	SCISSORS, GENERAL SURGICAL, Straight, Mayo, 5-1/2 inch.	II	1
6515-00-364-0920	SCISSORS, GENERAL SURGICAL, Straight, Mayo, 6-3/4 inch.	II	2

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5581

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

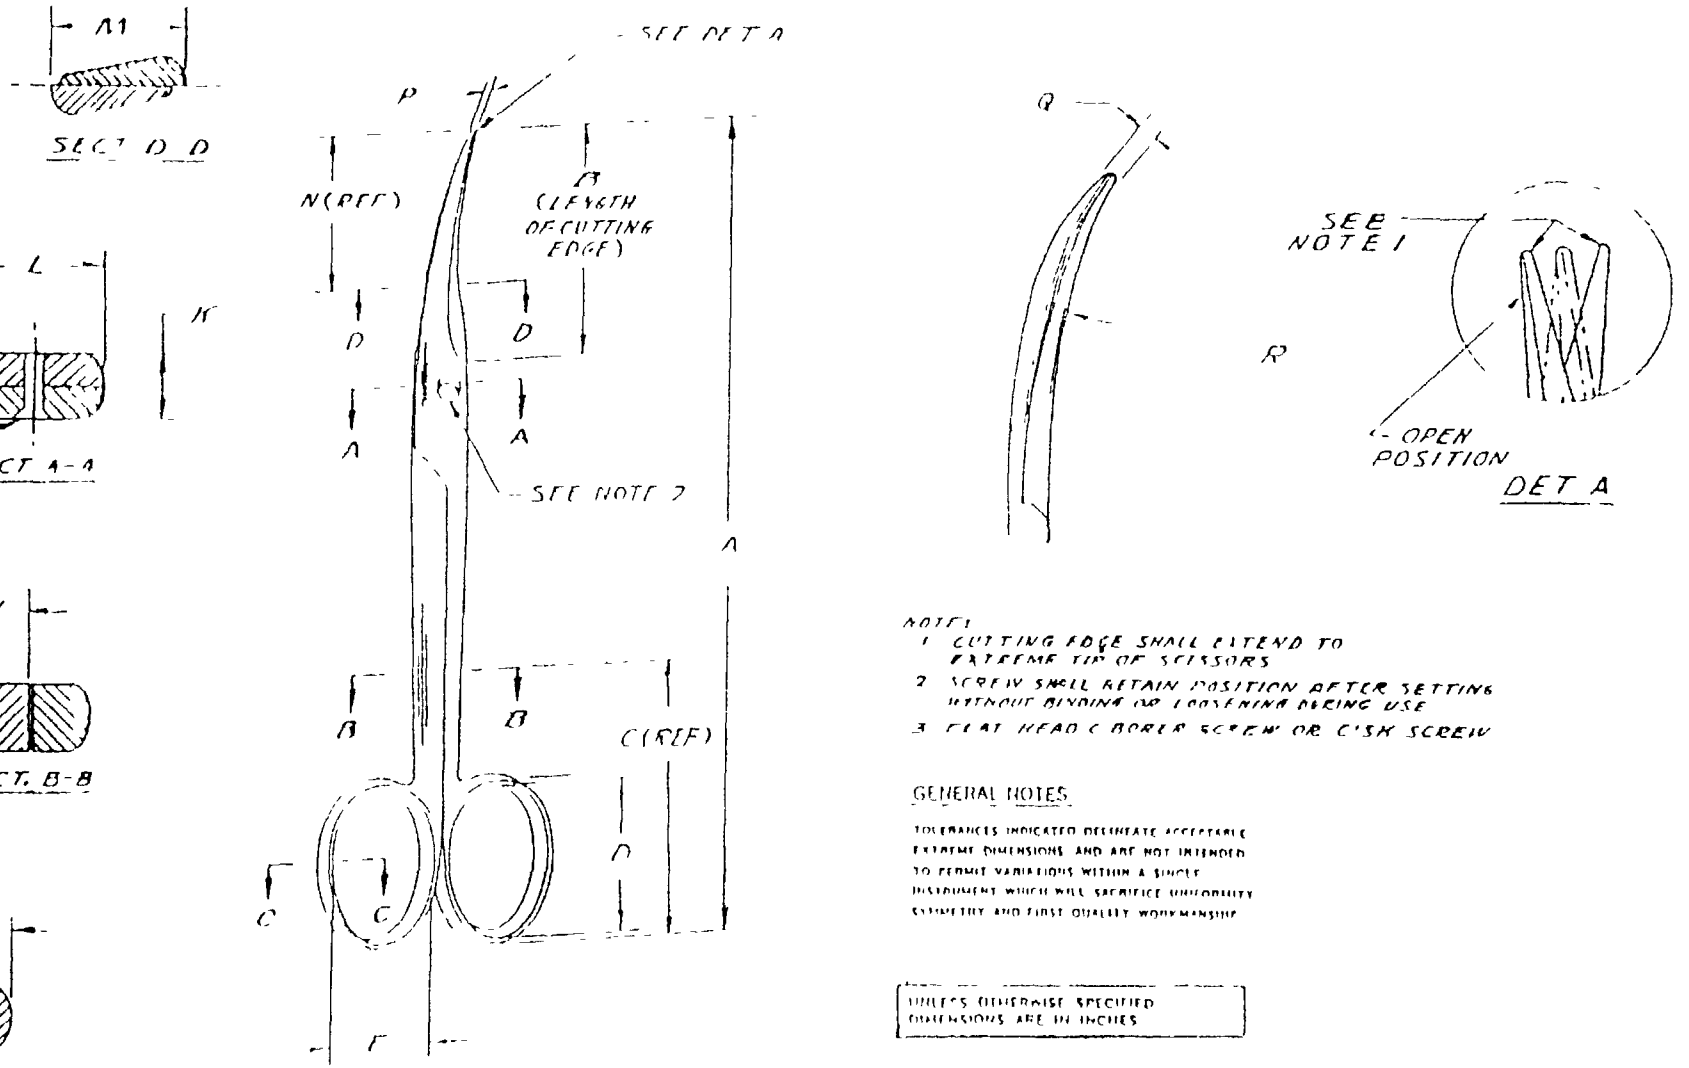

NOTES:
1. CUTTING EDGE SHALL EXTEND TO EXTREME TIP OF SCISSORS
2. SCREW SHALL RETAIN POSITION AFTER SETTING WITHOUT BINDING OR LOOSENING DURING USE
3. FLAT HEAD CROSS RECESS SCREW OR DISH SCREW

GENERAL NOTES


TOLERANCES INDICATED DESIGNATE ACCEPTABLE EXTREME DIMENSIONS AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY SYMMETRY AND FINE QUALITY WORKMANSHIP

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES

NSN	SIZE	A	B	C	D	E	F	G	H	J	K	L	M	N	P	Q	R
6515-00-364-0500	1	5-1/2	1-5/8	2-1/8	1	1/16	5/32	1/8	7/32	7/32	1/4	7/16	11/32	1 1/2	3/32	1/16	2-1/2
6515-00-364-0520	2	6-1/4	1-3/4	2-1/2	1 1/16	7/8	5/32	1/8	1/4	1/4	1/4	1/2	7/16	1-3/8	3/32	5/64	2-1/2
6515-00-364-0560	3	9	2-7/32	3	1 1/8	7/8	5/32	1/8	1/16	1/4	1/4	9/16	1/8	1-13/32	3/32	3/32	3-7/16
TOLERANCES		± 1/4	± 1/16	REF	± 1/16	± 1/16	± 1/32	± 1/64	± 1/32	± 1/32	± 1/32	± 1/32	± 1/32	REF.	± 1/64	± 1/64	± 1/8

FIGURE 1 SCISSORS, GENERAL SURGICAL, CURVED, MAYO, TYPE I

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

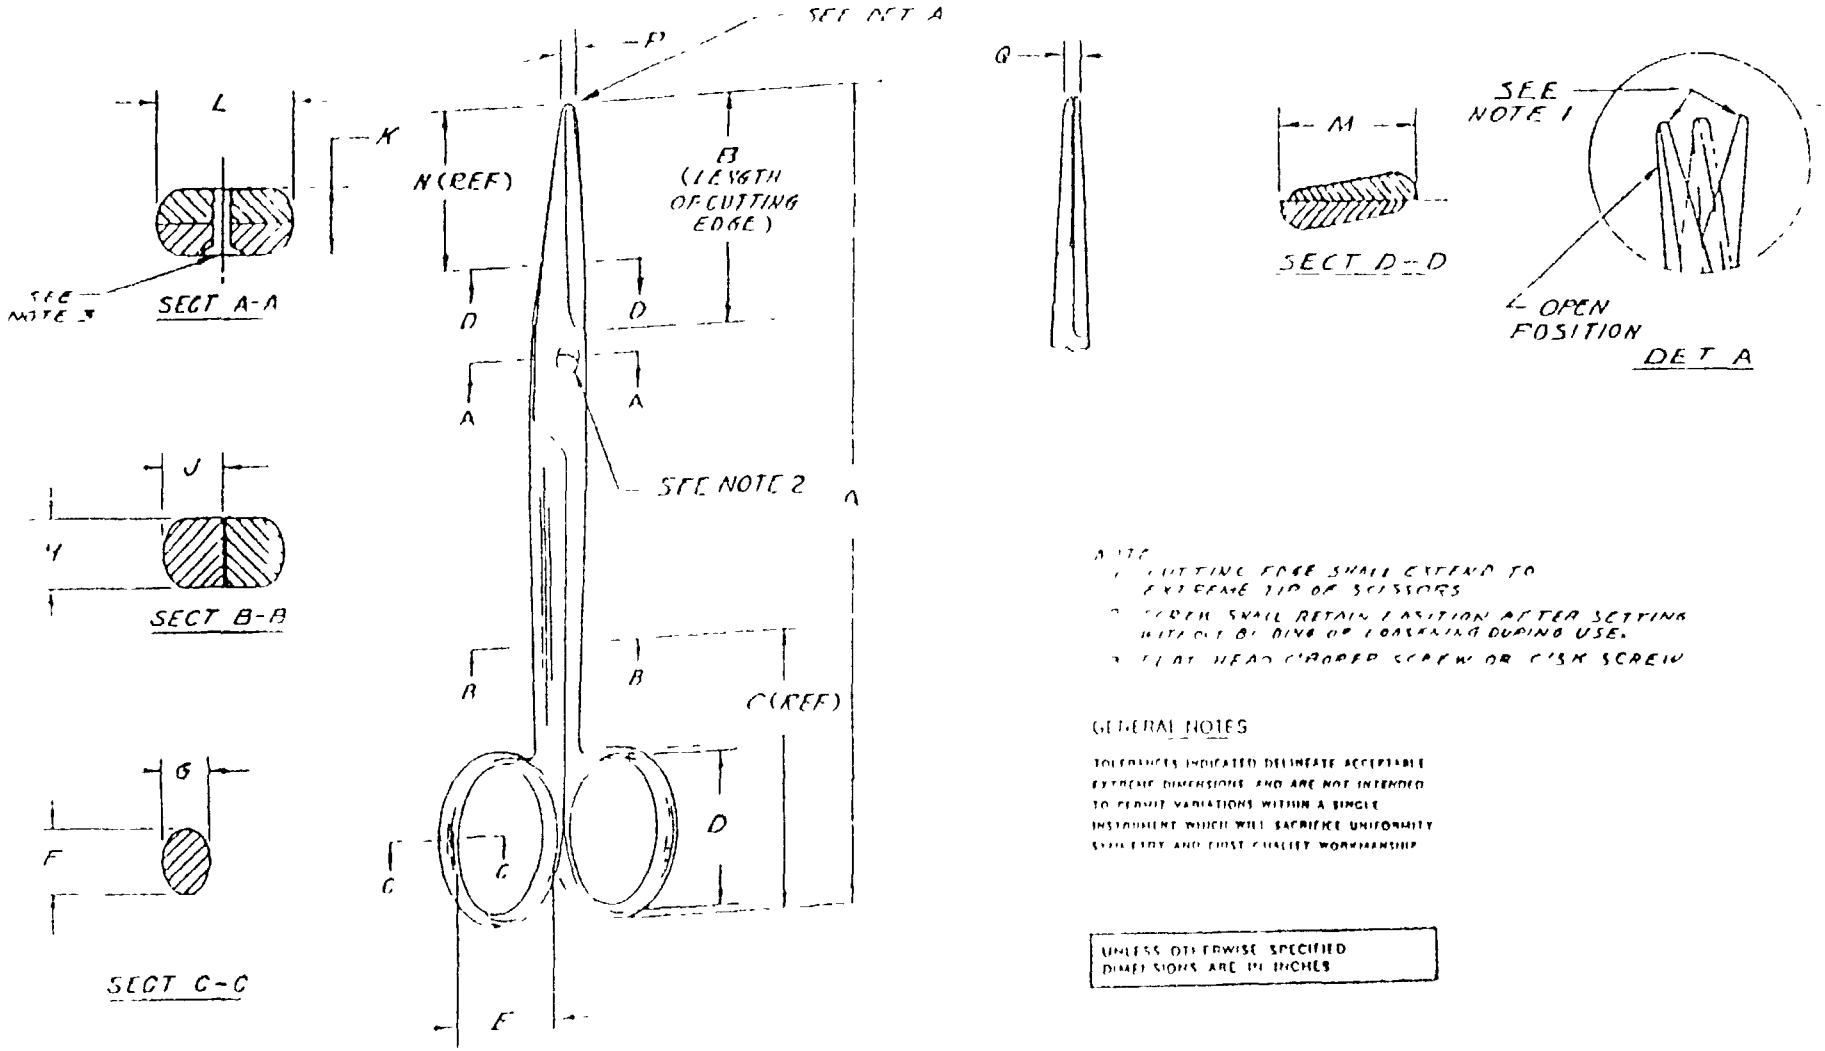

NOTE

1. CUTTING EDGE SHALL EXTEND TO EXTREME TIP OF SCISSORS
2. OPEN SHALL RETAIN POSITION AFTER SETTING WITHOUT BY DING OR LOOSENING DURING USE.
3. FLAT HEAD CROWED SCREW OR CSK SCREW

GENERAL NOTES

TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY SYMMETRY AND FIRST CLASS WORKMANSHIP

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES

ITEM	SIZE	A	B	C	D	E	F	G	H	J	Y	L	M	N	P	Q
5515-00-364-0900	1	5 1/2	1-5/8	2-1/8	1	17/32	5/32	1/8	1/16	3/16	1/4	7/16	11/32	1 1/2	1/32	1/8
5515-00-364-0920	2	6 1/4	1-7/8	2-1/2	1-1/16	7/8	5/32	1/8	1/4	1/4	1/4	1/2	7/16	1-3/8	1/32	1/16
TOLERANCES		± 1/4	± 1/4	REF	± 1/16	± 1/16	± 1/32	± 1/64	± 1/32	± 1/32	± 1/32	± 1/32	± 1/32	REF	± 1/64	± 1/64

FIGURE 2 SCISSORS, GENERAL SURGICAL, STRAIGHT, MAYO, TYPE II

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54842	2 DOCUMENT DATE (YYMMDD) 30 April 1993

3 DOCUMENT TITLE
SCISSORS, GENERAL SURGICAL, MAYO

4 NATURE OF CHANGE (*Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed*)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (*Include Area Code*) (1) Commercial (2) AUTOVON
c ADDRESS (*Include Zip Code*)	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403 Falls Church VA 22041 3466 Telephone (703) 756 2340 AUTOVON 289-2340

DD Form 1426, OCT 89 Previous editions are obsolete

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.