INCH-POUND

A-A-54861
30 April 1993

COMMERCIAL ITEM DESCRIPTION

INDICATOR, CLINICAL CHART HOLDER, METAL

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-I-36246 which is cancelled.

This Commercial Item Description covers a visual indicator, suitable for directing attention to individual clinical chart holders in military medical treatment facilities.

Salient characteristics:

The indicator shall consist of a slide receiver with a length of pressure sensitive adhesive tape on the back and a slide which may be positioned manually to expose or cover a colored "flag". The indicator shall be in accordance with figure 1.

The slide shall be a length of aluminum, "C" section channel designed to retain the slide when the unit is assembled. The back of the channel shall contain two holes located to mate with a spring loaded ball in the slide. Tabs shall be turned up at either end of the receiver to limit the travel of, and to retain the slide in the receiver when the device is assembled. The right end of the receiver shall be lined with a brilliant red paper or other suitable material, to serve as a visual indicator or "flag", wher uncovered by moving the slide to its left most position.

AMSC N/A FSC 6530

DISTRIBUTION STATEMENT A. Approved for public release: distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

The slide shall be a flat metal piece designed to fit into, and slide in, the "C" channel retainer. It shall be retained by the lip of the "C" and shall slide freely along the receiver. The slide shall cover and uncover the red "flag" on the receiver in its extreme positions. The slide shall be fitted with a knob for moving it in the receiver. The knob shall contain a spring loaded ball which shall mate with the holes in the receiver channel back to locate and hold it in its extreme position, until deliberately moved.

A length of double faced pressure sensitive tape shall cover the back of the slide receiver. The other side of the tape shall be protected with a removeable paper covering. The tape shall be adequate to provide mounting of the unit on a chart holder securely enough to permit normal operation and to prevent inadvertent removal.

Workmanship. The indicators shall be free from defects which detract from their appearance or impair their serviceability.

Unit. Package (PG). One package containing twelve (12) indicators, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination and tests. Sampling for examination and tests shall be conducted in accordance with MIL-STD-105, with an AQL of 1.0 (percent defective) and an inspection level of S-1. The unit of product for examination purposes shall be one indicator.

Tests. Test shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor Certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug, and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered material. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling and marking must be specified in the contract and/or order.

NOTES: The following National Stock Number is covered by this document:

NSN	Item Identification
6530-00-890-1882	INDICATOR, CLINICAL CHART HOLDER, METAL, 12s.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MS

Agent:

DLA-DM


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6530-2413

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

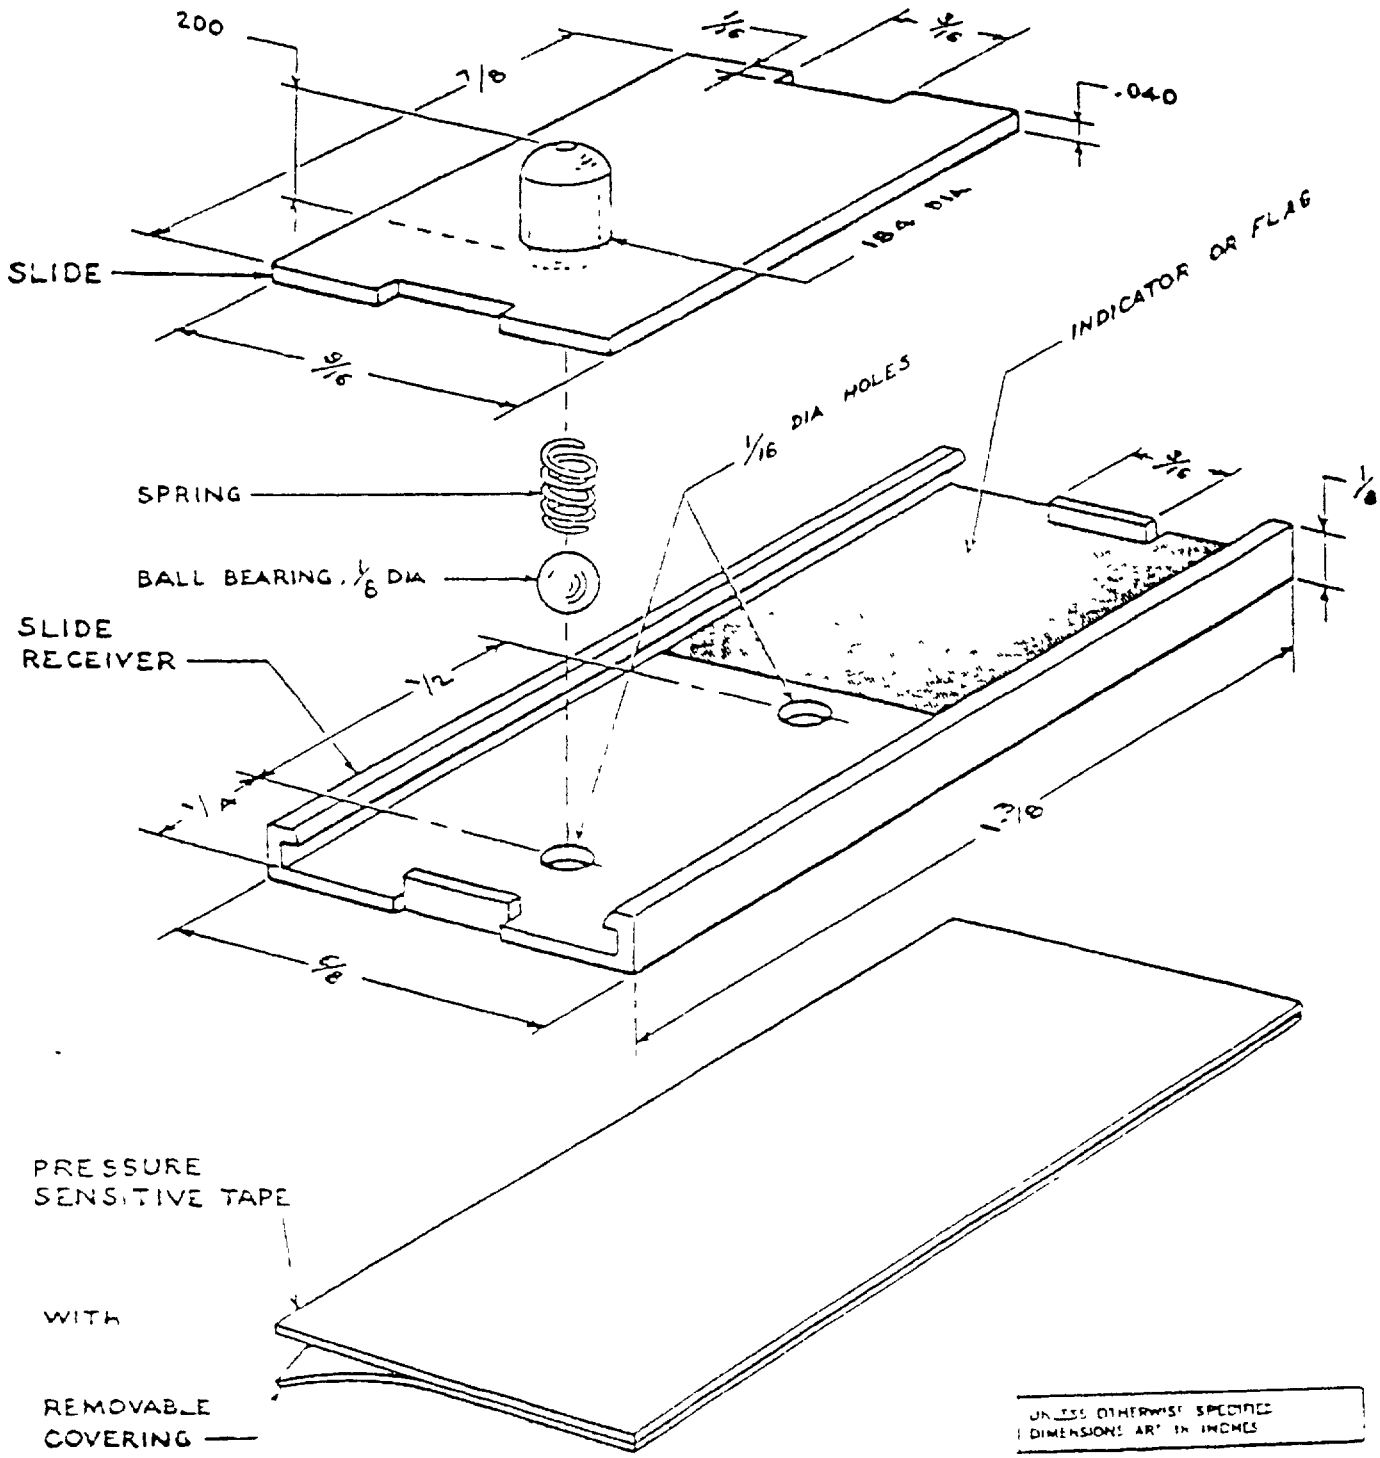

NSN 6530-00-890-1882

FIGURE 1. INDICATOR, CONNECTION MONITOR, M-TAT

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54861	2 DOCUMENT DATE (YYMMDD) 30 April 1993

3 DOCUMENT TITLE
INDICATOR, CLINICAL CHART HOLDER, METAL

4 NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)*

5 REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON
c ADDRESS (Include Zip Code)	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403 Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 *Previous editions are obsolete* 198/290

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.