METRIC

A-A-54864
15 May 1993

COMMERCIAL ITEM DESCRIPTION

BRONCHOSCOPE, Flexible, Fiber Optic, Transnasal or Transoral

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a bronchoscope with the following salient characteristics:

Salient characteristics:

The instrument shall be a 5 millimeter (mm) flexible fiberoptic bronchoscope specifically designed for either transoral or transnasal passage in diagnostic and therapeutic exploration of the bronchial tree. The bronchoscope shall be supplied with the following components and their respective quantities:

Component	Quantity
4.8 Fr biopsy specimen forceps	1
Disposable cytology brushes	5
Bite protector	1
Cleaning brush	1
Operating/maintenance manuals	2
Carrying case	1
Diaphragm seals	
Eyepiece cover and rubber eyeguard	1

Features. The bronchoscope shall have the following design and performance features. The bronchoscope shall have a 5.0 mm maximum tip diameter, an outside shaft diameter of 4.9 mm to 5.3 mm, a working length of approximately 55 centimeter (cm), and a biopsy channel diameter of 2.00 +/- 0.2 mm. The extreme distal diameter of the deflecting tip shall be approximately 4.8 mm allowing for deep atraumatic entry into subsegmental bronchial areas.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

The instrument shall have a deflection control knob conveniently located on the scope body distal to the eyepiece. The deflecting section shall have an approximate length of 32 mm with a bend radius of approximately 10 mm. The instrument shall feature a total deflection range of 220 degrees minimum, 160 degrees minimum upward deflection span and 60 degrees minimum downward deflection span.

The instrument shall have a fiber optic image bundle producing large, bright, sharp images. The bundle shall be attached to the scope just distal to the eyepiece. This bundle shall be a minimum of 1.5 meters in length with an integral bakelite type connecting end that securely attaches into a light source (see Note 2). The extreme distal tip of the bundle shall be protected with a heat shield to protect the bundle from separation.

The bronchoscope shall have a 67 degree minimum optical field of view and shall feature forward vision and fixed focus optical properties. The optical bundle shall have a 16X minimum magnification through the eyepiece and the instrument shall have a depth of field of 5.0 mm to 50 mm. The instrument shall feature a +2 to -8 diopter ocular adjustment.

The bronchoscope shall feature an automatic aspirator for lavage, aspiration, and introduction of medication with and without the forceps in place. The bronchoscope shall have a 2.0 mm +/- .2 mm operating channel for biopsy, medication, lavage, suction and local anesthesia. The component biopsy forceps and the disposable cytology brushes shall easily pass through the 2.0 +/- .2 mm channel even when the distal tip deflected 90 degree.

Accessories. The biopsy forceps shall be flexible with a double acting design for taking adequate specimens with minimum chance of bleeding. The 4.8 French biopsy forceps shall have a 1.6 mm diameter and a nominal working length of 101 cm. The forceps shall be designed with a finger ring control.

The cytology brushes shall have flexible shafts consisting of tightly twisted stainless steel wires. The plastic brush sheaths shall be free of cuts, nicks or imperfections. The brushes shall be designed with a finger ring control for ease in insertion and removal. The extreme distal tip shall be rounded to prevent inadvertent damage to tissues. The brush segments on the distal end shall be tightly woven into the twisted steel shaft preventing inadvertent separation during use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

The bite protectors shall be of molded plastic with a central hole for introduction of the bronchoscope.

The instrument shall come with a heavily padded "brief case style" case of sufficient size to contain the bronchoscope and all component parts.

Materiel. The body of the bronchoscope shall be fabricated of high impact plastic for strength and comfort. The metal portions of the bronchoscope shall be fabricated of a suitable corrosion resisting steel.

Style, design and dimensions. The bronchoscope shall be in accordance with Figure 1 in this specification for style, design and dimensions.

Passivation. The metal components of the bronchoscope shall be properly hardened and passivated as a final operation.

Sterilization. The bronchoscope shall be capable of withstanding ethylene oxide sterilization up to 140°F. The bronchoscope shall be completely immersible for cleaning and disinfection.

Workmanship. The bronchoscope shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One bronchoscope with accessories as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in specification where such inspection are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one bronchoscope as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one bronchoscope.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:39Z
Check the source to verify that this is the current version before use.

NOTE 1: The following National Stock Number and its respective Item Identification is covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-01-173-7054	BRONCHOSCOPE, Flexible, Fiberoptic, Transnasal, Transoral, 58 cm, 220 Minimum Degree Tip, Deflection, 16X Minimum Magnification, 1.8 mm Channel.

NOTE 2: The following National Stock Numbers and their respective Item Identifications are to be used in conjunction with this item:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-01-153-9649	LIGHT, Endoscopic Instrument, Fiber Optic
6515-01-181-8711	LIGHT, Endoscopic Instrument, Fiber Optic

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5454
Location: c:\word\eric\bronscop

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

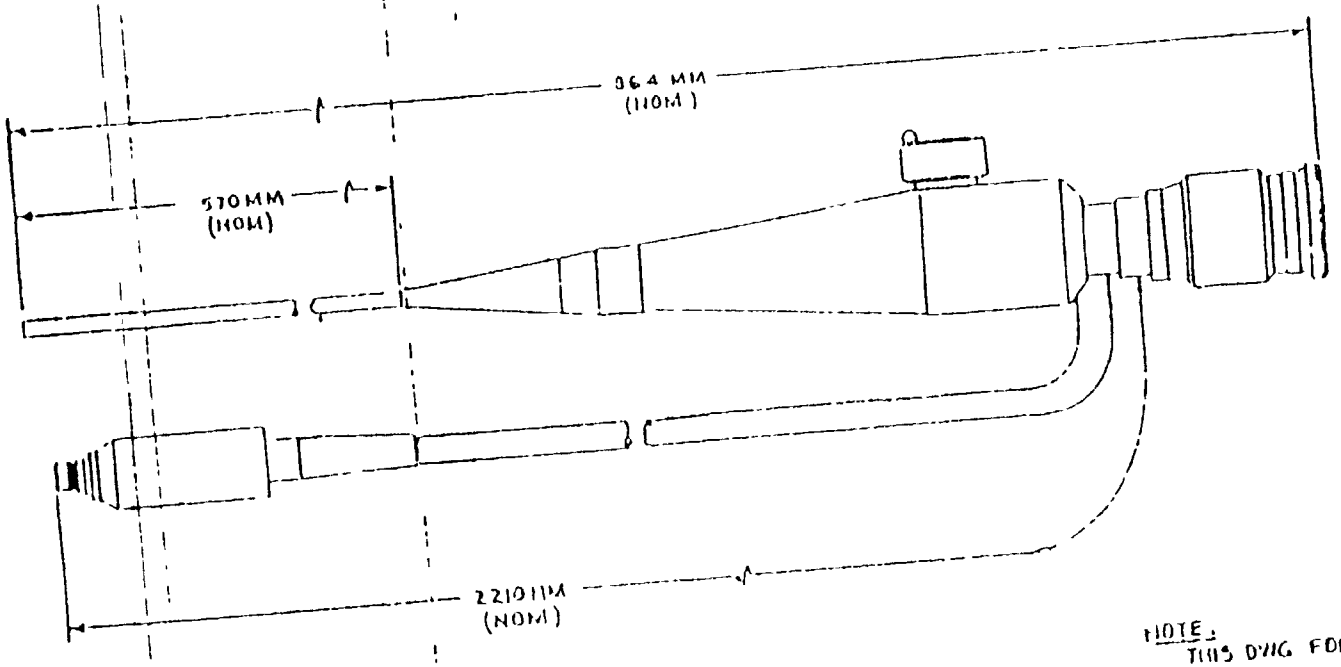

NOTE:
THIS DWG FOR STYLE AND DESIGN ONLY

NSN 6515-01-173-7054

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN MILLIMETERS

FIGURE 1 BRONCHOSCOPE, FLEXIBLE, FIBEROPTIC, TRANSNASAL/TRANSORAL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given.

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
A-A-54864	15 May 1993

3 DOCUMENT TITLE

BRONCHOSCOPE, Flexible, Fiber Optic, Transnasal or Transoral

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215)7372870	444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT. Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 *Previous editions are obsolete*

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:39Z
Check the source to verify that this is the current version before use.