INCH-POUND

A-A-54881
4 June 1993

COMMERCIAL ITEM DESCRIPTION

ELECTRODE ASSEMBLY, FETAL

The General Services Administration has authorized the use of this Commercial Item Description.

This Commercial Item Description covers a fetal electrode assembly.

Salient Characteristics:

The electrode assembly shall be specifically designed for internal fetal heart rate monitoring. It shall monitor the fetal heart rate through the attachment of the electrode to the "presenting part" of the fetus.

The electrode assembly shall be a stainless steel, single spiral electrode with two pre-attached wound leadwires. The leadwires shall be housed in two plastic tubes, one inside the other. The outer plastic tube shall be capable of guiding the inner plastic tube. The leadwires shall be 18 to 19 inches long and the outer and inner plastic tubes shall be 11 to 12 inches long.

The electrode assembly shall be sterile and disposable.

The electrode assembly shall be capable of being inserted approximately 2mm into the skin of the fetus.

The electrode shall be applied to the fetus with minimal trauma to the mother and the fetus.

The electrode assembly shall be packaged in a peel-open container that guarantees sterility of the item unless the package has been opened or damaged.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

The spiral electrode shall have less than or equal to a 35° angle at the tip of the electrode, as shown in figure 1.

Sterility, pyrogenicity, toxicity. The electrodes shall be nonpyrogenic and nontoxic in accordance with the United States Pharmacopeia (USP). The electrodes shall be sterile in accordance with USP or Association for the Advancement of Medical Instrumentation (AAMI) requirements. Sterility assurance level shall be 0.000001.

Workmanship. The electrode assembly shall be free from defects which detract from its appearance of impair its serviceability.

Unit. Package (PG). One package containing fifty individually packaged sterile electrodes, as specified, constitutes one unit. The individual package shall be a suitable container capable of maintaining sterility of contents unless the package is damaged or opened.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

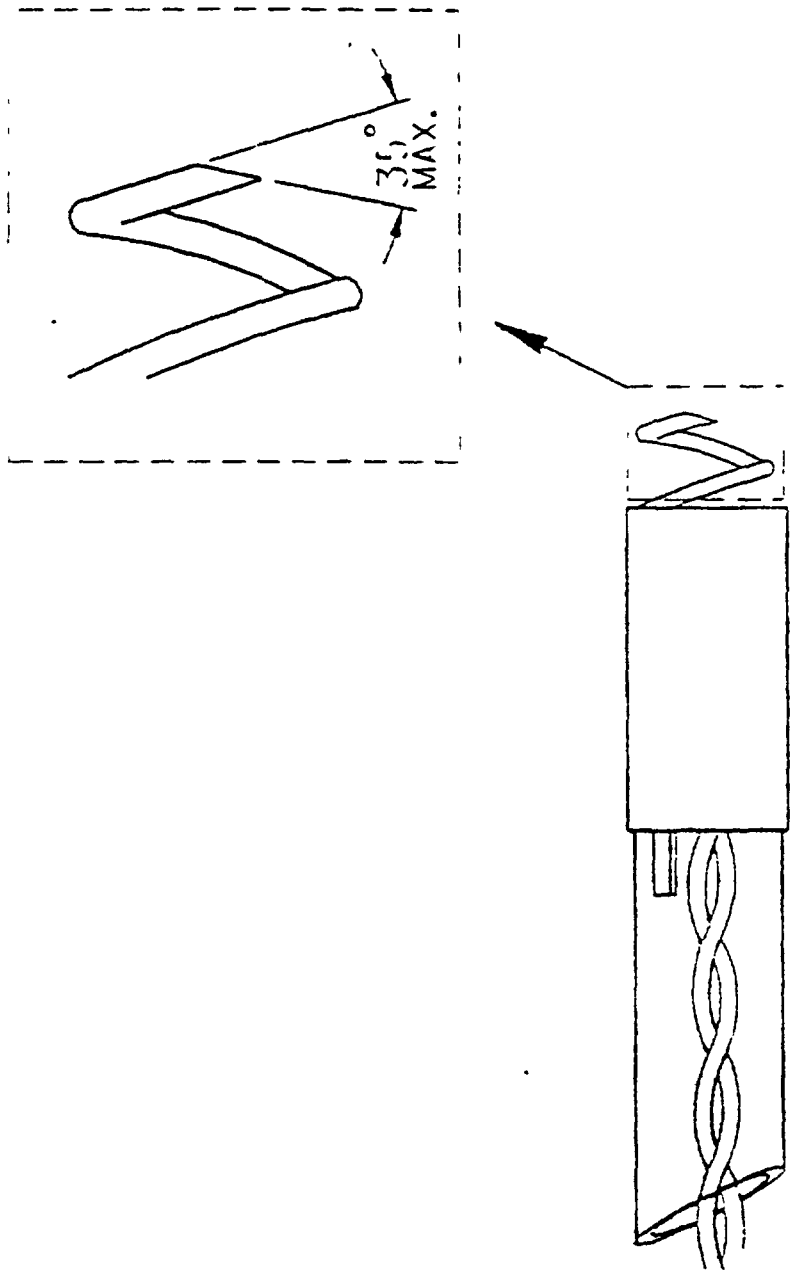


FIGURE 1 – TIP DETAIL, ELECTRODE ASSEMBLY, FETAL – NSN 6515-01-146-4257

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-1. The unit of product for examination purposes shall be one electrode.

Sampling for tests. Sampling for tests, including dimensional test, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-1. The unit of product for test purposes shall be one electrode.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics. Tests shall include, but shall not be limited to, the following:

Angle test. The angle at the tip of the electrode, as shown in figure 1, shall be equal to or less than 35°.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document.

6515-01-146-4257

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

A-A-54881

MILITARY INTERESTS:

Custodians:

Air Force - 03
Army - MD
Navy - MS

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

FDA-MPQAS
USPHS
VA - OSS

Project Number: 6515-5425
Location: ELEC16C.DOC

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

1. RECOMMEND A CHANGE:	1. DOCUMENT NUMBER A-A-54881	2. DOCUMENT DATE (YYMMDD) 4 June 1993

3. DOCUMENT TITLE
ELECTRODE ASSEMBLY, FETAL

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME DEFENSE PERSONNEL SUPPORT CENTER ATTN: DPSC-MSE	b. TELEPHONE (Include Area Code) (1) Commercial: AC 215-737-2870 (2) AUTOVON: AV 444-2870
c. ADDRESS (Include Zip Code) 2800 SO. 20TH STREET PHILADELPHIA, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous editions are obsolete — 9670/1426

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.