INCH-POUND

A-A-54884
18 June 1993

COMMERCIAL ITEM DESCRIPTION

CATHETER AND NEEDLE UNIT, INTRAVENOUS
(Catheter into Needle)

The General Services Administration has authorized the use of this Commercial Item Description as a repacement for Military Specification MIL-C-37203 which cancelled.

This Commercial Item Description covers catheter and needle units suitable for prolonged intravenous infusion therapy.

Salient characteristics:

Material. The catheter and extension tube shall be fabricated from clear polyvinylchloride. All plastic components coming in contact with intravenous medication shall meet the requirements of United States Pharmacopeia (USP) for Class IV plastics. The protective conduit shall be fabricated from clear flexible plastic. The needle shall be fabricated from Type 304 stainless steel in accordance with ASTM Designation F899. The needle hub shall be fabricated from Type 304 stainless steel or plastic meeting USP Class II requirements. The needle guard and needle cover shall be fabricated from rigid plastic. The three place connector shall be fabricated from rigid plastic. The injection sites shall be fabricated from natural rubber.

Style and design. The catheter and needle unit shall consist of an outer needle (short bevel design) and indwelling catheter, an extension tube with a Luer hub, a protective conduit, an actuator to advance the catheter, an inline locking needle guard, a needle and a cap for the Luer end.

The catheter shall be radiopaque in accordance with ASTM Designation F640. The radiopaque material may be incorporated into the plastic either as striped or throughout the whole catheter cannula.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

The needle guard shall permanently lock the needle hub after catheter placement and shall completely encase the needle to prevent the needle bevel from piercing the catheter.

The indwelling catheter shall be permanently attached to the extension tube and the actuator.

The Luer fittings shall meet the requirement of ISO 594. The style and design of the unit shall be in accordance with Figure 1.

Catheter flexibility. With the needle removed, the catheter shall be wrapped 90 degrees around a 1/2 inch diameter rod without kinking or cracking. Water shall then be admitted through the catheter hub and observed for restricted flow from the distal tip.

Catheter security of assembly. The catheter shall not tear or separate from the extension tube when the catheter is subjected to the following minimum tensile forces:

GAUGE	LOAD (pounds)
15	2.5
18	2.0

Catheter leakage. With the needle removed, the distal tip of the catheter shall be sealed and 20 psig water admitted through the catheter hub. The junction of the catheter to catheter hub shall not leak when observed for 2 minutes.

Heavy metals extractability. Plastic and rubber components coming in contact with intravenous solution or patient's blood shall be tested. The quantity of lead and cadmium shall not exceed 5 parts per million (ppm) and the amount of barium shall not exceed 10 ppm when tested in accordance with the USP.

Sterility, pyrogenicity and toxicity. The catheter and needle unit shall be nonpyrogenic and nontoxic in accordance with USP. The unit shall be sterile in accordance with USP or AAMI requirements. Sterility assurance level shall be 0.000001.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Instructions. Each catheter and needle units shall contain instructions for use.

Workmanship. The catheter and needle unit shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing ten individually packaged sterile catheter and needle units of the gauge size specified, constitutes one unit. An individual package shall be a sealed peel-open type capable of maintaining sterility of contents unless the package is damaged or opened.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one catheter and needle unit as specified. Sampling shall be inspection level II with an Acceptable Quality Level (AQL) of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified. Unit of product for test purposes shall be one catheter and needle unit. Sampling shall be inspection level S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commerical Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

NOTE: The following National Stock Numbers and their respective Item Identifications is covered by this document:

National Stock Numbers	Item Identifications
6515-00-138-2307	CATHETER AND NEEDLE UNIT INTRAVENOUS, 15 gauge Catheter, Radiopaque, 21 inches
6515-00-187-2388	CATHETER AND NEEDLE UNIT INTRAVENOUS, 18 gauge Catheter, Radiopaque, 21 inches

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

A-A-54884

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5429
Location: c:mark\needle2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

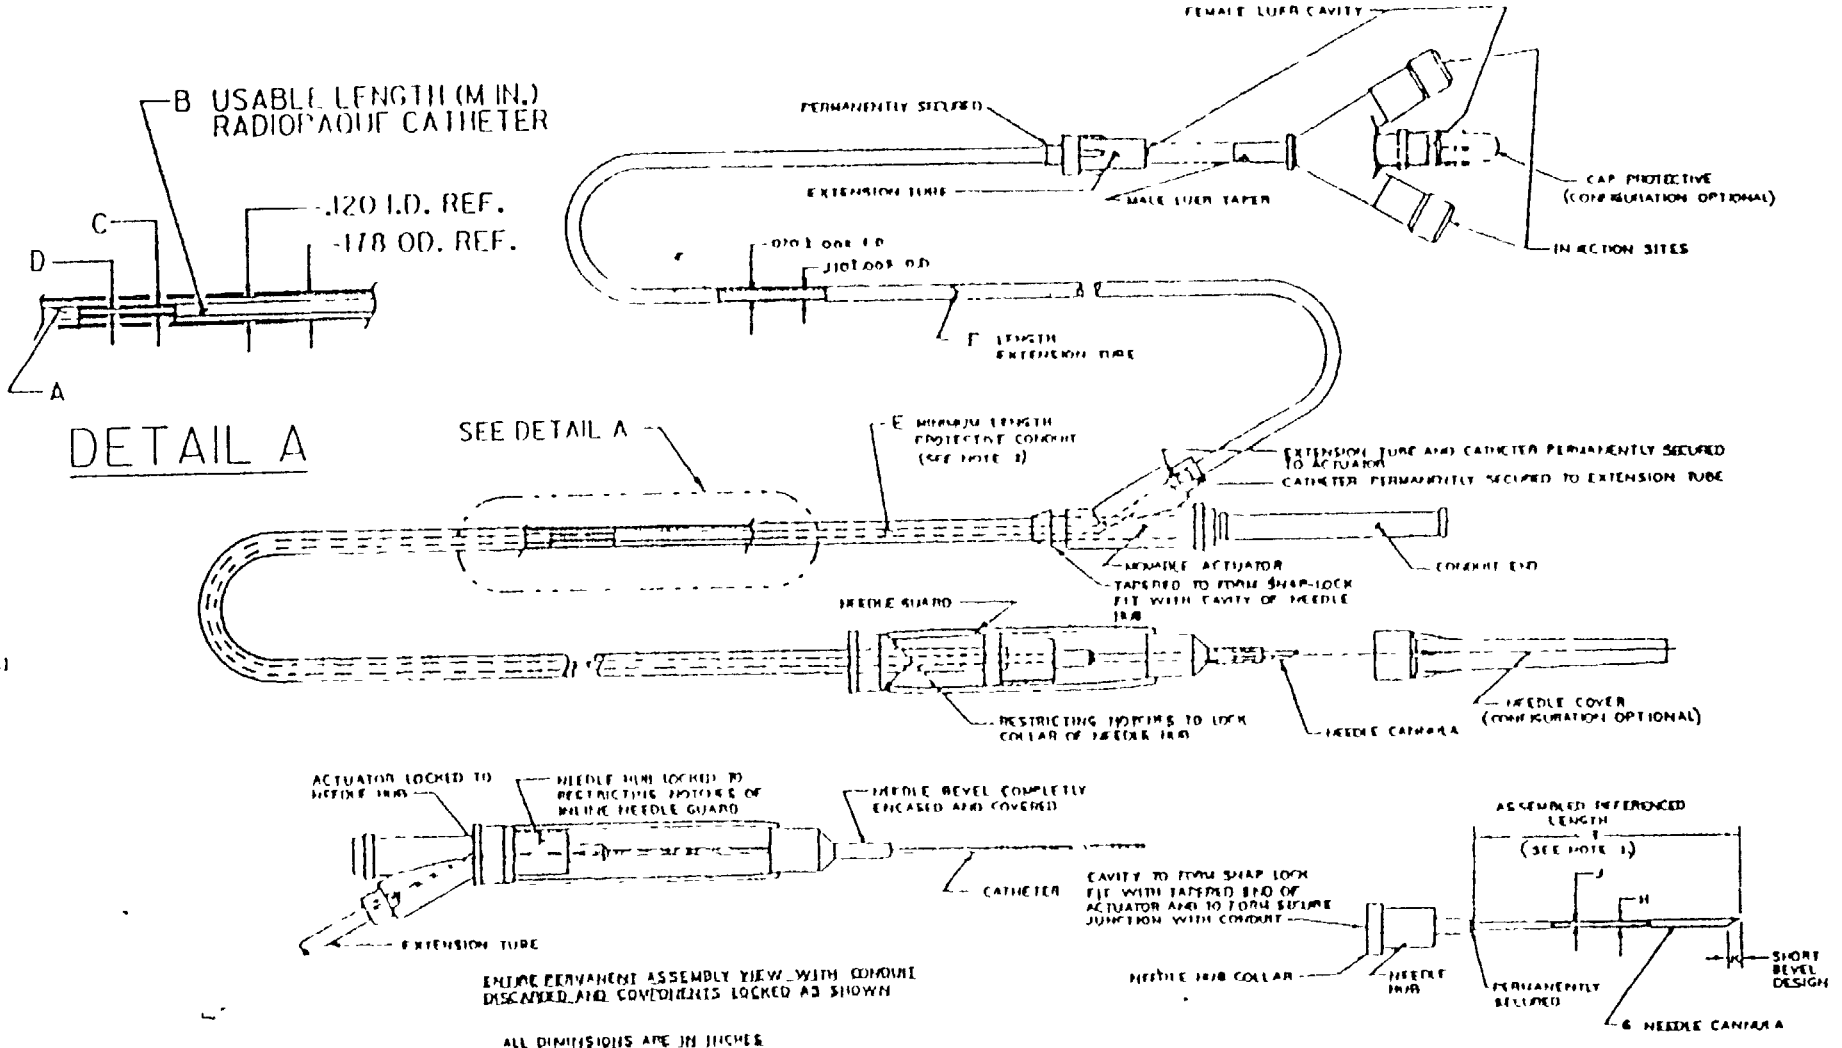

NSN	CATHETER A GAGE	CATHETER B LENGTH	CATHETER C O.D.	CATHETER D I.D.	PROTECTIVE CONDUIT E LENGTH	EXTENSION TUBE F LENGTH	NEEDLE G GAGE	NEEDLE H O.D.	NEEDLE J I.D.	NEEDLE K	3-PLACE CONNECTOR
6515-00-107 2389	18	21	.048	.033	25	22 1/2	17	.038	.030	172	REQUIRED
6515-00-138 2307	15	21	.067	.050	25	22 1/2	14	.083	.073	225	REQUIRED
TOLERANCES			±.002	±.002		± 1/16		±.001	±.001	±.010	

NOTE:
1. WITH NEEDLE FULLY EXTENDED OUT OF INLINE NEEDLE GUARD THERE SHALL BE 1 1/2 ± 1/16 INCHES OF USABLE NEEDLE (FINE LENGTH).
2. CONDUIT SHALL POSSESS A LONGITUDINAL FINE SLIT ALONG ENTIRE LENGTH FOR CATHETER ADVANCEMENT

A-A-54884

FIGURE 1 CATHETER AND NEEDLE UNIT, INTRAVENOUS, RADIOPAQUE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given
2. The submitter of this form must complete blocks 4, 5, 6, and 7
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER	2 DOCUMENT DATE (YYMMDD)
	2-2-54864	18 June 1993

3 DOCUMENT TITLE
CATHETER AND NEEDLE UNIT INTRAVENOUS (Catheter into Needle)

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible Attach extra sheets as needed)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	d TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME	b TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center ATTN: DPSC-MSE	(215)7372870	444-2870
c ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403 Falls Church VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:39Z
Check the source to verify that this is the current version before use.