A-A-50976
25 June 1985

COMMERCIAL ITEM DESCRIPTION

# HOLDER, RUBBER DAM, DENTAL, (Metal, "U" Shaped)

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-H-36575A.

This commercial item description covers two sizes of rubber dam holders suitable for use during dental operative procedures.

Size 1 - Adult.
Size 2 - Child.

Salient characteristics:

Description: The size 1 "U" shaped rubber dam holder shall be for use on adults and the size 2 holder shall be for use on children. The holders shall consist of a frame, two (2) straps, and instructions for use.

Frame. The frame of the holder shall be made from half-hard brass rod. The outer periphery of the frame shall have seven permanently attached solid or hollow brass pins for proper engagement and retention of the rubber dam. The free end of each vertical side of the frame shall have a permanently attached offset ball-shaped solid brass spherical knob for protection of the patient's eyes, and a blunt-headed solid brass hook suitable for engaging and retaining the neck strap. The assembled frame shall be chromium over nickel plated and shall have a bright, polished finish. The design and construction of the frame shall be as shown in figure 1.

Strap. The strap shall be an adjustable, elastic neck strap for use with the frame to provide tension for the required cheek retraction. The strap webbing shall be made of a blue or black dyed, cotton-rayon, polyester, or nylon elastic webbing containing 14 to 20 strands of natural rubber. The strap loops shall be made of stainless steel. The strap lock shall be made of stainless steel, or, as an alternate, plated or blue enameled brass or carbon steel. The loops shall be for attachment of the strap to the frame. The lock shall hold positively and shall be readily adjustable to permit increasing or decreasing the strap length. The design and construction of the strap shall be as shown in figure 1.

Tests.

Resistance to boil. Before testing, the holders shall be scrubbed with soap and water, rinsed thoroughly in distilled water, and dried. After being cleaned, the holders shall be placed in a glass container in which distilled water is added, boiled for 30 minutes, and allowed to remain submerged for an additional 24 hours. Upon removal, no corrosion shall be present after lightly wiping with a gauze sponge.

Elongation and rupture. The test for elongation shall be determined by manually stretching 2.0 inches of webbing to a minimum of 3.8 inches. Any rupture of rubber strands shall be determined both during and after the test. Any evidence of rupture shall be cause for rejection.



DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Markings. The holder shall be legibly and permanently marked with name or registered trademark of the manufacturer.

Workmanship. Rubber dam holder shall be free from defects which detract from its appearance or impair its serviceability, such as sharp burrs capable of lacerating or puncturing skin during handling and use. All soldered joints, such as for the pins, hooks, and knobs shall be cleanly and properly finished.

Unit. Each (EA). One rubber dam holder, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspections. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item. Inspection shall be conducted to determine compliance with specification requirements.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more test characteristics. The unit of product for test purposes shall be one holder. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.



Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

6520-00-935-7143 HOLDER, RUBBER DAM, DENTAL, "U" SHAPED, Adult.

6520-00-935-7144 HOLDER, RUBBER DAM, DENTAL, "U" SHAPED, Child.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

CIVIL AGENCY COORDINATING ACTIVITY:

VA-OSS

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

05459


Project No. 6520-1622




Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

| SIZE | A | B | C | D |
|---|---|---|---|---|
| 1- ADULT | 3 1/2 | 1 3/4 | 5 1/16 | 4 1/8 |
| 2- CHILD | 3 1/4 | 1 1/16 | 4 9/16 | 3 3/4 |

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
TOLERANCES ON
FRACTIONS ± 1/16 DECIMALS ± ~ ANGLES ± 3°

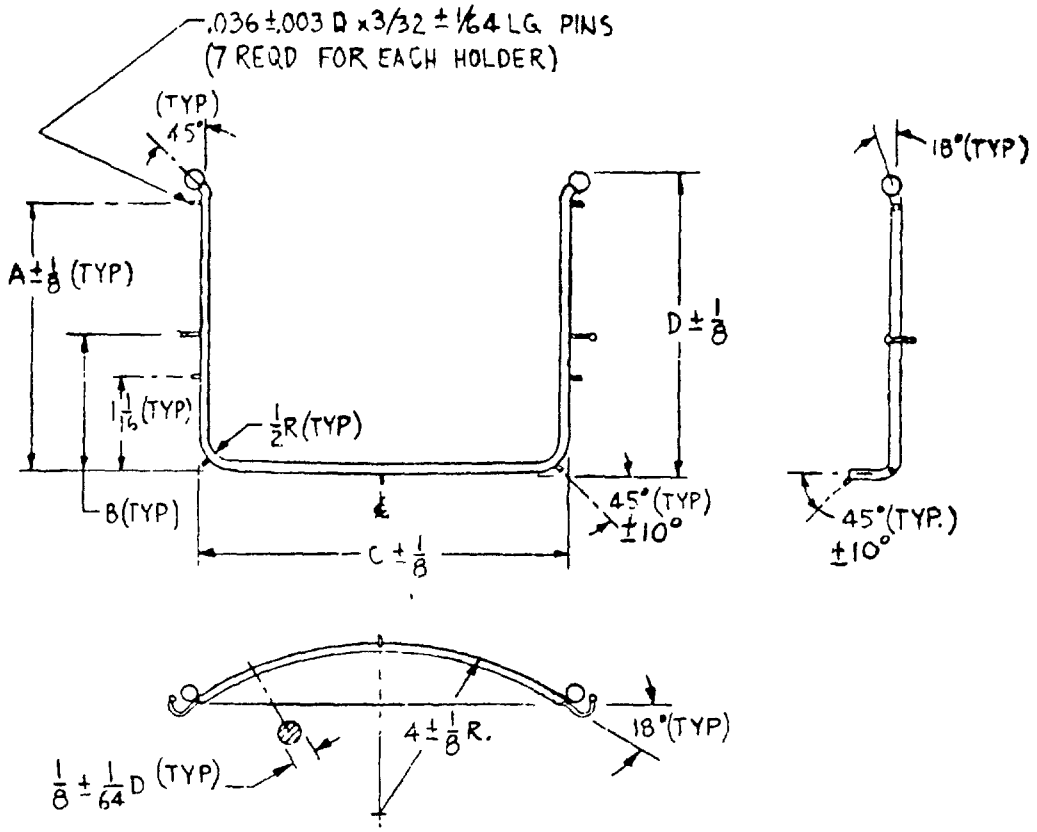


FRAME

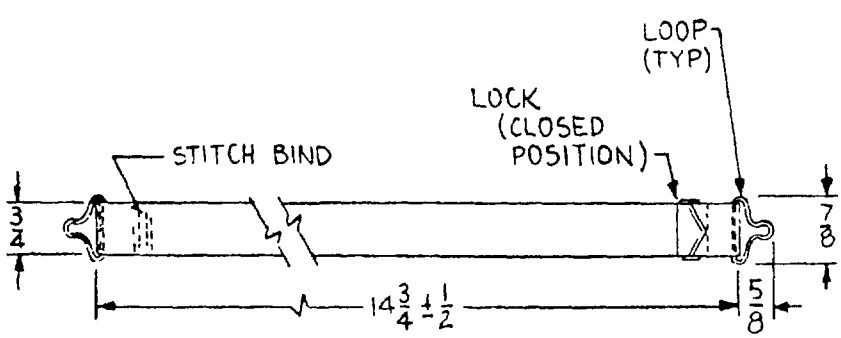


STRAP

FIGURE 1 HOLDER, RUBBER DAM

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.