A-A-51011A
25 October 1989
SUPERSEDING
A-A-51011
13 September 1985

COMMERCIAL ITEM DESCRIPTION

SCREEN, X-RAY PROTECTIVE

(Frame Mounted, Mobile)

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-S-36463 which is cancelled.

This Commercial Item Description covers a frame mounted mobile x-ray protective screen.

Salient characteristics:

The x-ray protective screen shall be a mobile radiation protective device suitable for use in protecting the patient against scattered radiation during chest, skull, and spine radiography, or to drape over table for extremities. The screen shall be radiographic lead impregnated vinyl sheeting supported by a caster mounted frame (see figure 1 for a typical design).

The screen shall be radiographic lead impregnated vinyl sheeting 24 inches wide by 96 inches long, made from lead impregnated vinyl with a smooth, washable finish on both sides. The sheeting shall be uniformly impregnated with a sufficient amount of lead, or a compound of lead, to provide a lead equivalent of 0.5 mm minimum when the sheeting is doubled over the top cross member of the mobile frame. The screen may be faced one or both sides with colored vinyl resin. If the screen is layered, bonding shall be continuous and permanent so that no separation will occur.

The screen shall be folded in two and mounted on an all-welded chrome-plated frame. The screen top shall have a minimum adjustable height range of 33-1/4 inches to 47-3/4 inches. The screen shall be securely supported at the desired height. The frame shall be free of burrs and sharpness. The chrome plating shall be free from scratches, pits, rough areas, and other surface defects.

AMSC N/A FSC 6525
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

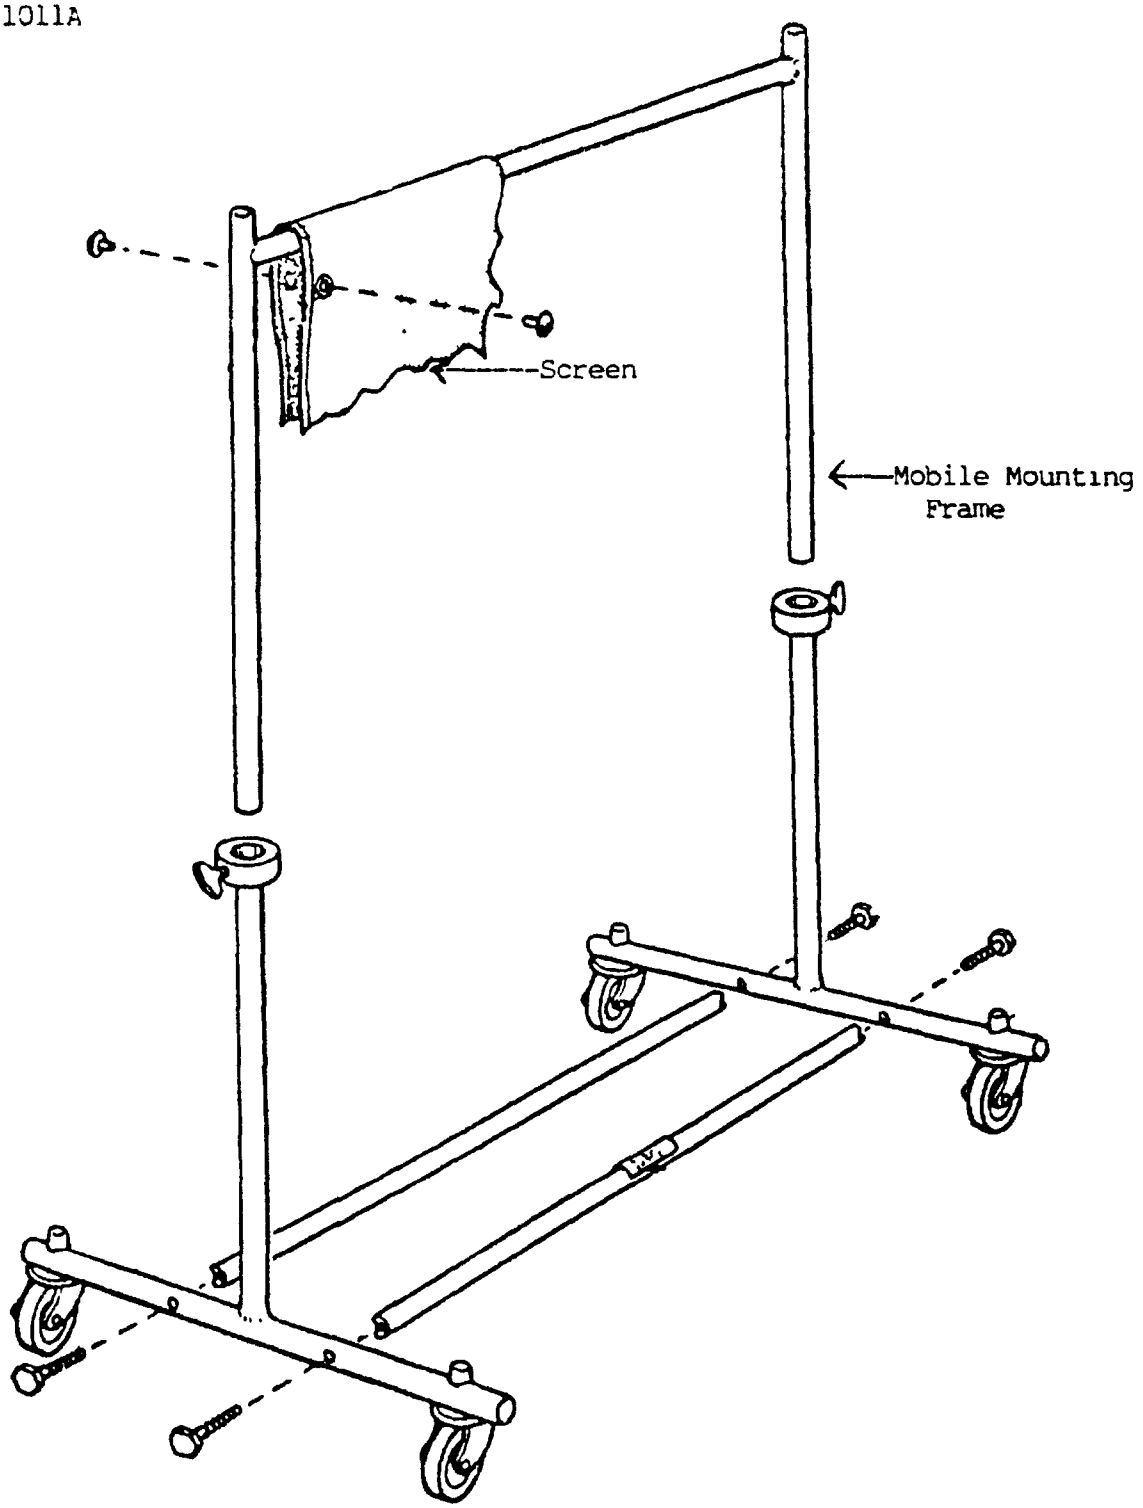


FIGURE 1. Typical screen design.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

The screen frame shall be mounted on four electrically conductive, smooth-rolling, quiet, swiveling casters which shall be a minimum of 3 inches in diameter.

The screen shall be free of cuts, tears, holes, perforations, and blisters. The surfaces of the screen shall be smooth, uniform, and free from tack, lumps, embedded foreign matter, and pits.

Welds shall be thorough, non-porous, and free from pits, cracks, or other imperfections. All welds shall be cleaned. All exposed welds shall be ground and finished smooth to match adjoining surfaces.

The screen and frame shall be clean and free of oil, grease, dirt, or other contamination.

Workmanship. The x-ray protective screen shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One x-ray protective screen, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests, including dimensional test, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-3. The unit of product for test purposes shall be one x-ray protective screen.

Tests

Lead equivalency. An x-ray radiograph shall be taken in two random areas of the vinyl sheeting. The resulting x-ray exposures shall be examined and compared with standard exposures taken through a lead step wedge. A lead equivalency of less than 0.25 millimeters of lead on either test sample, shall constitute a defect.

Density uniformity. The vinyl sheeting shall be tested by x-ray exposure at 100 kvp in a minimum of two random places on each screen. Any essentially different density shall constitute a defect.

Rigidity test. With the x-ray protective screen in the normal position, and the base held firmly, a force of 50 pounds shall be applied at any point, and in any direction, on the top member of the screen. Play in any direction, exceeding two inches, shall constitute a defect.

Rolling test. The x-ray protective screen shall be placed on a smooth horizontal tile or concrete floor. The casters shall be clean. A horizontal force shall be applied gently to the top member of the screen, at any point, and in any direction. The force shall be gradually increased until the screen rolls or upsets. If the screen upsets, it shall constitute a defect.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6525-00-753-9598

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6525-0698

Location:
CID/SCREEN/X-RAY PROTECTIVE/H13-35

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS - In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge (*DO NOT STAPLE*), and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4956 WASHINGTON D C
POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51011A	SCREEN, X-RAY PROTECTIVE, (Frame Mounted, Mobile)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI – Optional)*	b. WORK TELEPHONE NUMBER *(Include Area Code) – Optional*
c. MAILING ADDRESS *(Street, City, State, ZIP Code) – Optional*	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 1426 PREVIOUS EDITION IS OBSOLETE.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

Source: https://assist.dla.mil – Downloaded: 2025-10-26T08:49Z
Check the source to verify that this is the current version before use.