A-A-51482
13 June 1986

COMMERCIAL ITEM DESCRIPTION

WIRE SNARE, NO. 24 STUBS WIRE GAGE, CARBON STEEL

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a snare wire used with tonsil snares of the Tyding design.

Salient characteristics:

General. Shall be a wire snare used to surgically remove tonsils when assembled to tonsil snares of the Tyding design.

Materials. The wire snare shall be manufactured from cold drawn carbon steel in accordance with the chemical composition and mechanical requirements of ASTM A228 or austenitic corrosion-resistant steel of the chemical composition specified in ASTM F899.

Characteristics. The wire shall be No. 24 Stubs iron wire gage with a diameter of 0.0220 ± 0.0003 inch. As an alternate, the wire shall be 0.55 ± 0.01 mm (0.0217 ± 0.0004 inches) when the wire is labeled in SI units. The wire shall be in accordance with Figure 1.

Physical Properties.

Tensile strength. Carbon steel wire shall have a tensile strength of 345,000 to 382,000 pounds per square inch (psi) when tested as specified herein.

Austenitic corrosion-resistant wire shall have a tensile strength of 290,000 psi minimum when tested as specified herein.

Uniformity and finish. The finished wire snare shall be uniform in diameter and temper and shall have a smooth, bright finish, free from cracks, pits, die marks, scale and corrosion.

Workmanship. The wire snare shall be free from defects which detract from its appearance or impair its serviceability.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Package (PG). One package, containing 12 wire snares, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as follows. For dimensions, the Inspection shall be S-1 and a 2.5% AQL. The tensile strength (austenitic or carbon steel) and coiling (carbon steel only - ASTM A228) tests shall be conducted with at least 3 specimens per lot of material from which the finished snare is manufactured with no defects permitted. The unit of product for test purposes shall be one wire snare.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of composition testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the test method, and the test results.

Chemical analysis. In the absence of certificates of quality, the chemical analysis of the material used in the fabrication of the wire shall be performed in accordance with method III of Federal Standard No. 151.

Tensile strength. Samples of straight specimens of wire, 15 inches in length, shall be tested in accordance with ASTM A318. The specimens of wire used in the test shall be of the same lot of material from which the finished wire snares are fabricated.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE 1: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-00-149-1102	WIRE SNARE, No. 24 Stubs Wire Gage Carbon Steel, 12s

NOTE 2: The tonsil snare with which this wire snare is to be used is covered by NSN 6515-00-149-1103.

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.)

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA - OSS
PHS

PGC 46839

Project No. 6515-3516

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

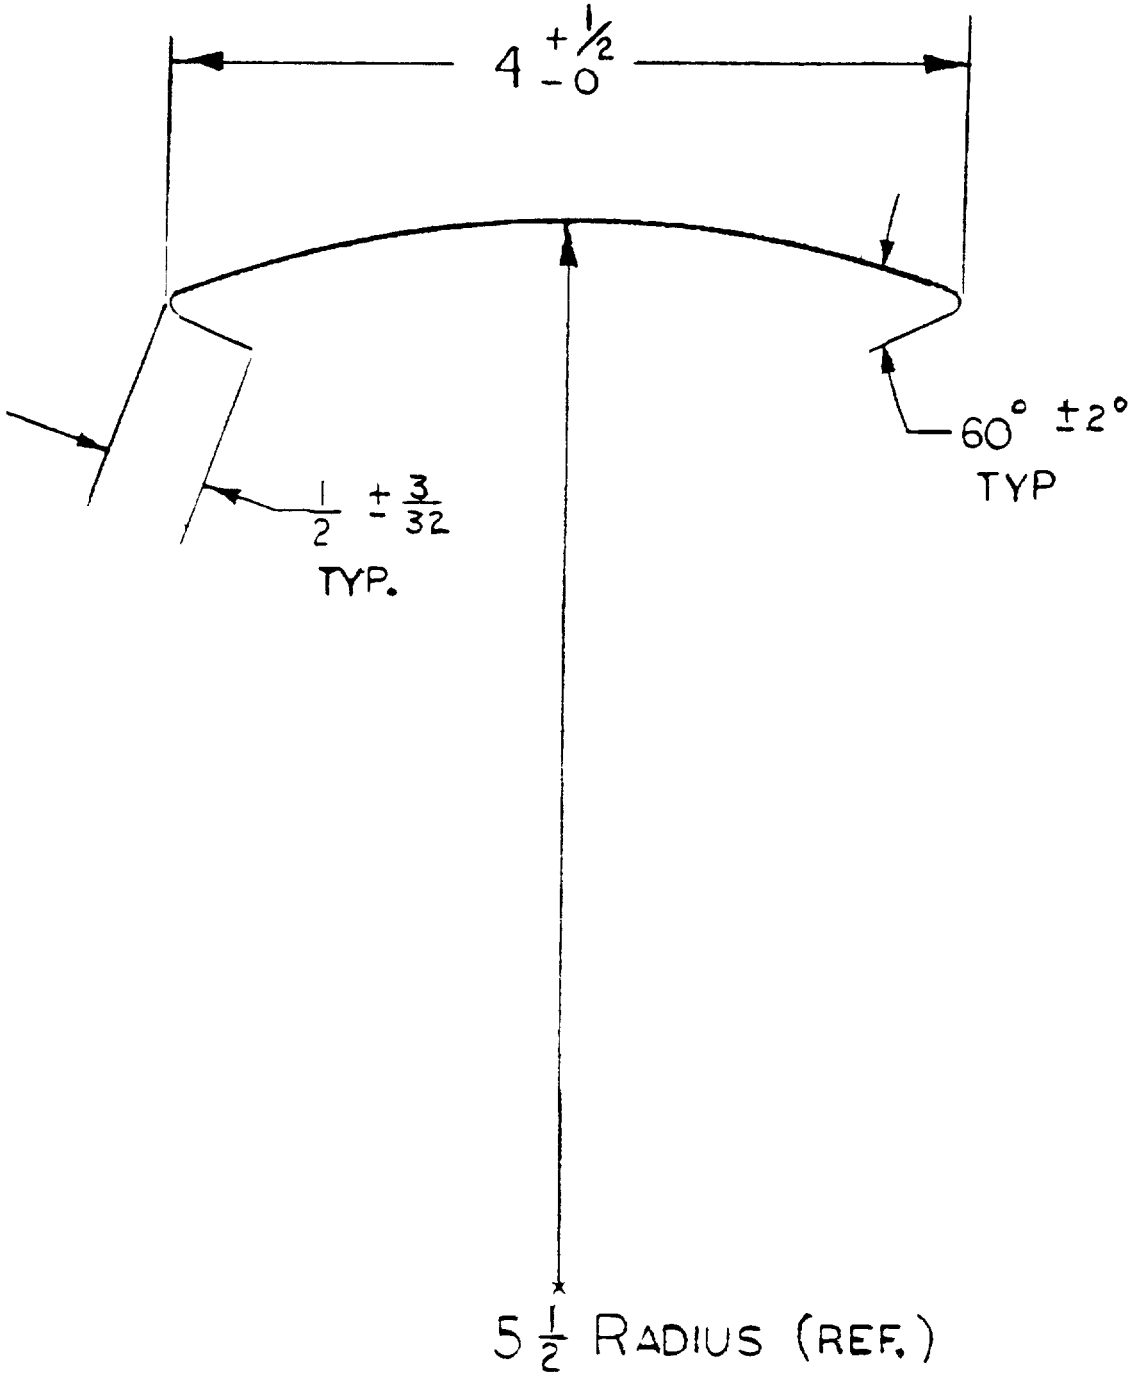

DIMENSIONS IN INCHES

FIGURE 1

WIRE SNARE, NO. 24 STUBS WIRE GAGE, CARBON STEEL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC-ATTS
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:56Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-51482	Wire,Snare, No.24, Stubs

3a. NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark on* ☐ VENDOR ☐ USER ☐ MANUFACTURER ☐ OTHER *(Specify)* _____
b. ADDRESS *(Street, City, State, ZIP Code)*	

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Incl Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 20260-26T08:56Z
Check the source to verify that this is the current version before use.