A-A-51483
23 June 1986

COMMERCIAL ITEM DESCRIPTION

BLADE and FRAME, DENTAL LABORATORY SAW (Plastic and Gypsum Materials)

The General Services Administration has authorized the use of this commercial item description in preference to Federal Specification GG-B-00406B.

This commercial item description covers an adjustable saw frame and blade suitable for dental laboratory procedures.

Class 1 - Saw Frame
Class 2 - Saw Blade

Salient characteristics:

The saw frame shall be suitable for use with the saw blade to form an adjustable saw (frame plus blade) suitable for cutting plastics and hardened gypsum products in the dental laboratory.

Frame. The frame bow shall be fabricated of a suitable steel plated to render corrosion resistant. The bow support and tang shall be a zinc-base alloy die casting. The thumb screw shall be rolled stainless steel or cold rolled steel treated to be corrosion resistant. The handle shall be fabricated of smooth, seasoned, close-grained hardwood, and shall have a painted or lacquered finish. The saw frame shall be easily adjustable and shall consist of a bow, bow support with tang, and handle. The frame shall securely hold the blade and shall maintain rigidity during use. All parts of the frame shall be held together when the blade is not in place. The blade bearing surfaces of the holding devices on the rod and tang shall be serrated to provide gripping surfaces for the blade. The handle shall be securely attached to the tang by means of a heavy duty ferrule. The frame shall be of the design and dimensions shown in Figure 1. The bow and blade bearing surfaces of the holding devices shall have a polished finish. The bow support (and tang) and bow holding device shall have a smooth finish. Each frame shall be legibly and permanently marked with name or registered trademark of the manufacturer. Instruments of foreign (other than U.S.) manufacture shall also be marked with the name of the country of origin.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Blade. The blade shall be fabricated of heat treated steel. The blade shall be spiral in design so as to cut in any direction without turning the frame. The blade shall have blank ends for clamping into the holding devices of the frame. The blade shall be of the design and dimensions shown in figure 2. The blade shall have a Rockwell hardness of C60 minimum when determined in accordance with ASTM Designation E18 (Rockwell) or E92 (Vickers or Diamond Pyramid).

Workmanship. All parts shall be symmetrically made, smoothly and properly finished, and shall be free from defects which detract from their appearance or may impair their serviceability.

Unit.

Class 1- Each (EA). One saw frame, as specified, constitutes one unit.

Class 2 - Package (PG). One package containing twelve blades, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

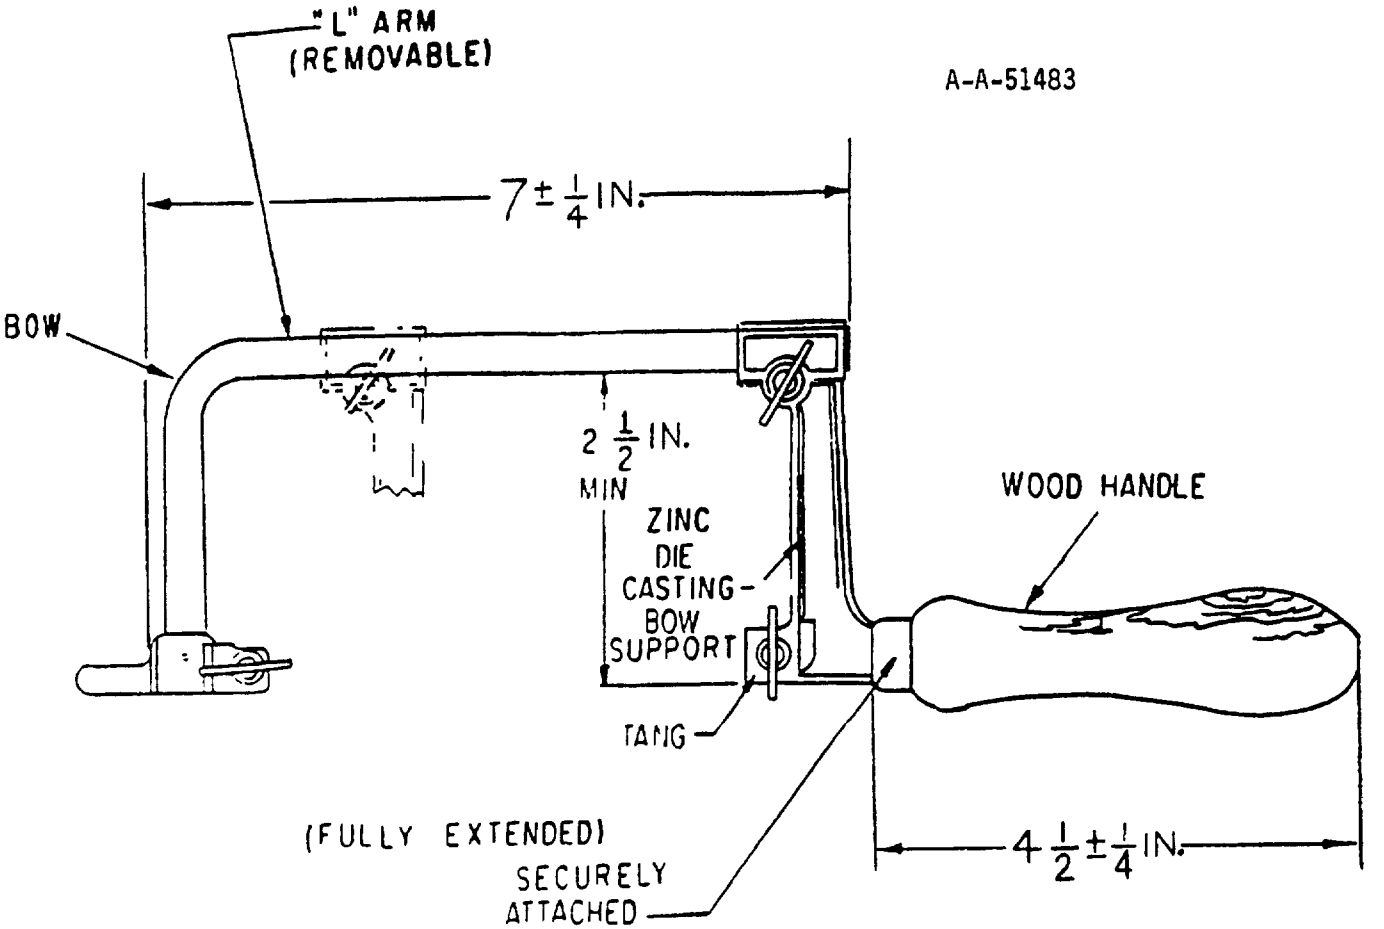


FIGURE 1 : DENTAL LABORATORY SAW, FRAME

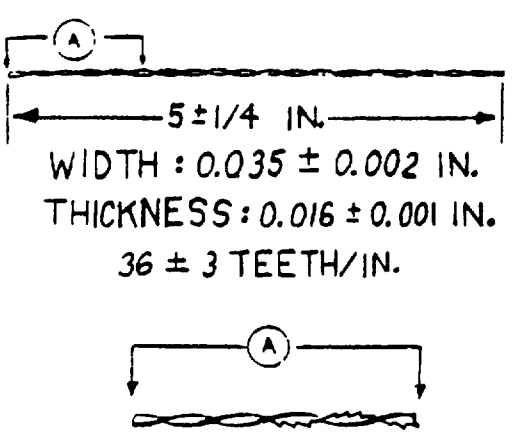


FIGURE 2 : DENTAL LABORATORY SAW, BLADE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection . Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one saw frame or package of blades. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drugs and Cosmetic Act. If the product covered by this document has been determined by U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

Stock Number	Item Identification	Designation
6520-00-553-8150	FRAME, DENTAL LABORATORY SAW	Class 1
6520-00-553-8250	BLADE, DENTAL LABORATORY SAW, Spiral, No. 2 Blade, 12s	Class 2

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTEREST:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Civil Agency Coordinating Activity:
VA-OSS

05434

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

Project No. 6520-1904

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-ATTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51483	BLADE and FRAME, DENTAL LABORATORY SAW

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.