A-A-51488B
31 December 1990
SUPERSEDING
A-A-51488A
31 MAY 1988

COMMERCIAL ITEM DESCRIPTION

FLUORIDE APPLICATION TRAY, DENTAL

The General Services Administration has authorized the use of this Commercial Item Description.

This Commercial Item Description covers dental fluoride application trays suitable for the simultaneous application of fluoride gel to the upper and lower dentition.

Salient characteristics:

The three sizes of the dental fluoride application trays shall be as specified below.

Small
Medium
Large

The trays shall be a disposable one piece application tray with anterior handles consisting of a maxillary and mandibular tray joined by a common hinge.

The trays shall be suitable to contain the fluoride gel and for the simultaneous application of the fluoride gel to the upper and lower dentition. The buccal, lingual, and posterior walls shall form a closed tray to preclude dripping gel into the throat, insure coverage of dentition and accommodate the residual fluoride gel.

Material. The trays shall be formed of sheet stock 1/4 inch thick, 5 ± 1 pound/feet 3 density, soft closed-celled polyethylene foam.

The trays shall be anatomically contoured and constructed to provide total coverage of all dentition. To create a close apposition of the fluoride to the tooth surface, the inside of the tray shall be of anatomical tooth configuration, or shall have a heat bonded polyester foam lining.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

The trays shall be formed with a decrease in trough depth from the anterior segment to the posterior segment. The minimum wall thickness of the tray shall be 1/16 inch measured at the center of the anterior buccal wall of the mandibular or maxillary tray. The hinge strap shall be designed and constructed to minimize the contact between the straps and the near sides of the tongue to prevent gagging. The handles shall be a minimum of 1 inch in length and 1/2 inch in width. The design and dimensions of the trays shall be in accordance with figure 1.

The handles shall be clearly labeled to indicate which is the upper or lower tray for correct orientation and shall be coded for size. The trays shall have no sharp or rough edges.

Adequate and accurate instructions for use shall be included with each package of trays to include size code designations.

Workmanship. The trays shall be free of visible contamination, such as dirt, burns, cuts, holes, shaved areas, excess trim or other defects which detract from their appearance or impair their serviceability.

Unit. Package (PG) One package containing thirty trays of one size only, as specified, constitutes one unit. The unit package shall be a resealable type package and shall contain instructions for use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more examination characteristics. The unit of product for examination purposes shall be one package, as specified. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5 (percent defective), except dimension shall be conducted at inspection level S-2, AQL 1.0 (percent defective).

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conform to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric Products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

offeror/contractor shall comply, and be responsible for compliance by its subcontractors/supplies, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to appliance carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document

National Stock Number	Item Identification	Size
6520-01-317-1133	FLUORIDE APPLICATION TRAY, DENTAL, Small, Disposable, 30s	Small
6520-01-317-1134	FLUORIDE APPLICATION TRAY, DENTAL, Medium, Disposable, 30s	Medium
6520-01-317-1135	FLUORIDE APPLICATION TRAY, DENTAL, Large, Disposable, 30s	Large

Ordering data. Intermediate/exterior package quantities, labeling and marking must be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity.

DoD-MB

Agent:


DLA-DM

Civil Agency Coordinating Activities.

VA-OSS
PHS
FDA-MPQAS

Project No. 6520-2391
Location: WORD/FLAPTR/KD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

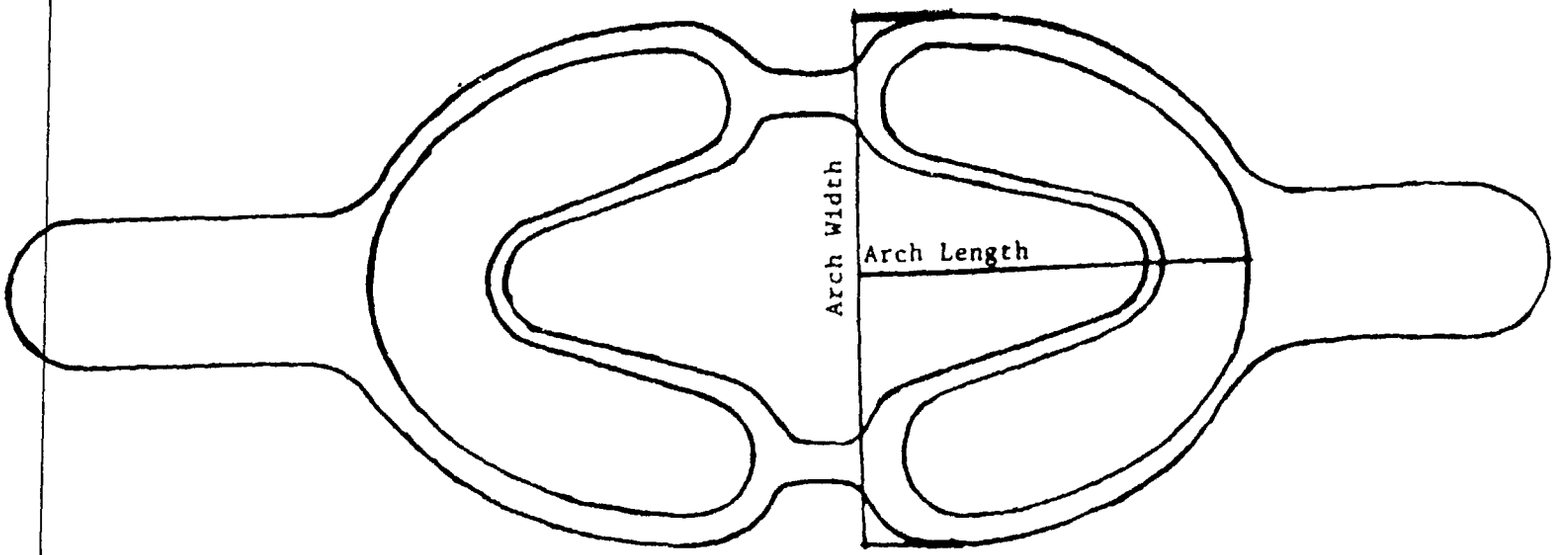

Size	Arch		Trough
	Width	Length	Depth Range
Small	2 - 1/4 ± 1/8	1-5/8 ± 1/4	1/8 - 15/32
Medium	2 - 1/2 ± 1/4	2 ± 1/4	5/32 - 9/16
Large	2 - 3/4 + 1/8 - 1/4	2 - 1/4 ± 1/4	1/4 - 19/32

1/ All dimensions are in inches.
Width is taken at widest part.
Length is taken at midline.
Measurements are taken with optional liner removed.

FIGURE 1. FLUORIDE APPLICATION TRAY, DENTAL

The fluoride application tray is typical in style and design and is not intended to restrict or preclude the purchase of fluoride application trays which are otherwise in accordance with the requirements of this document.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC-MSTE
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51488B	FLUORIDE APPLICATION TRAY, DENTAL

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR ☐ USER ☐ MANUFACTURER ☐ OTHER *(Specify)*: _____
b. ADDRESS *(Street, City, State, ZIP Code)*	

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 2020-10-26T08:56Z
Check the source to verify that this is the current version before use.