A-A-54573
17 January 1992

COMMERCIAL ITEM DESCRIPTION

SCISSORS-DAGGER, TRACHEOTOMY, UNIVERSITY OF KANSAS DESIGN, CURVED BLADES, 5-3/16 INCH LONG

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-S-36750 which is cancelled.

This Commercial Item Description covers one type of scissors-dagger, suitable for use in cricothyroidotomies concerning infants and adults.

Salient characteristics:

General. The scissors-dagger shall be of the University of Kansas design and suitable for use in cricothyroidotomies concerning pediatric and adult surgical procedures. Shall be designed to cut a nick in the skin and to incise the cartilage of the trachea. Shall have specially curved cutting blades with angulated pointed tips. Tips shall be suitable for piercing into the trachea without causing enlarged openings. Tips shall possess a special bevel on both blades, with the last third of the bevel forming a non-sharp edge blending into its sharp portion. Cutting action shall be such that skin is grasped and cut cleanly without causing the skin to be pushed away from the cutting blades.

Material. The scissors-dagger shall be fabricated from class 4, type 420 martensitic corrosion-resistant steel in accordance with ASTM F899.

Hardness. The scissors-dagger shall have a Rockwell hardness (HRC) of C50 to C55 when tested for hardness in accordance with ASTM E18 or E92 whichever is applicable. As an alternate, the screw shall have a Rockwell hardness (HRC) scale of C40 to C45 when tested for hardness in accordance with ASTM E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM E140.

Style, design and dimensions. The scissors-dagger shall be in accordance with Figure 1 for style, design and dimensions.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.

Tip protectors. The scissors-dagger shall be provided with a protective covering to protect the tips and blades of the instrument when not in use.

Performance The performance of the scissors-dagger shall be in accordance with applicable requirements of ASTM F1079.

Finish. The scissors-dagger shall have a mirror or mirror and satin finish.

Passivation. The scissors-dagger shall be properly passivated.

Corrosion resistance. The scissors-dagger shall show no evidence of corrosion or plating of copper when tested for corrosion resistance in accordance with ASTM F1089.

Identification marking and labeling. The scissors-dagger shall be legibly marked with the contractor's name or registered trademark and the word "stainless". Foreign manufactured scissors-dagger shall bear the name of the country of origin.

Workmanship. The scissors-dagger shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One scissors-dagger, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purposes shall be one scissors-dagger. Sampling shall be Inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for test purposes shall be one scissors-dagger. Sampling shall be Inspection level S-2 with an AQL of 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal State, and local statutes, ordinances, and regulations.

Recovered material. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

NOTE: The following National Stock Number is covered by this document:

NSN	Item Identification
6515-00-935-7092	SCISSORS-DAGGER, TRACHEOTOMY, University of Kansas Design, Curved Blades, Angulated Pointed Tips, 5-3/16 Inch Long.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project No. 6515-5210

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.

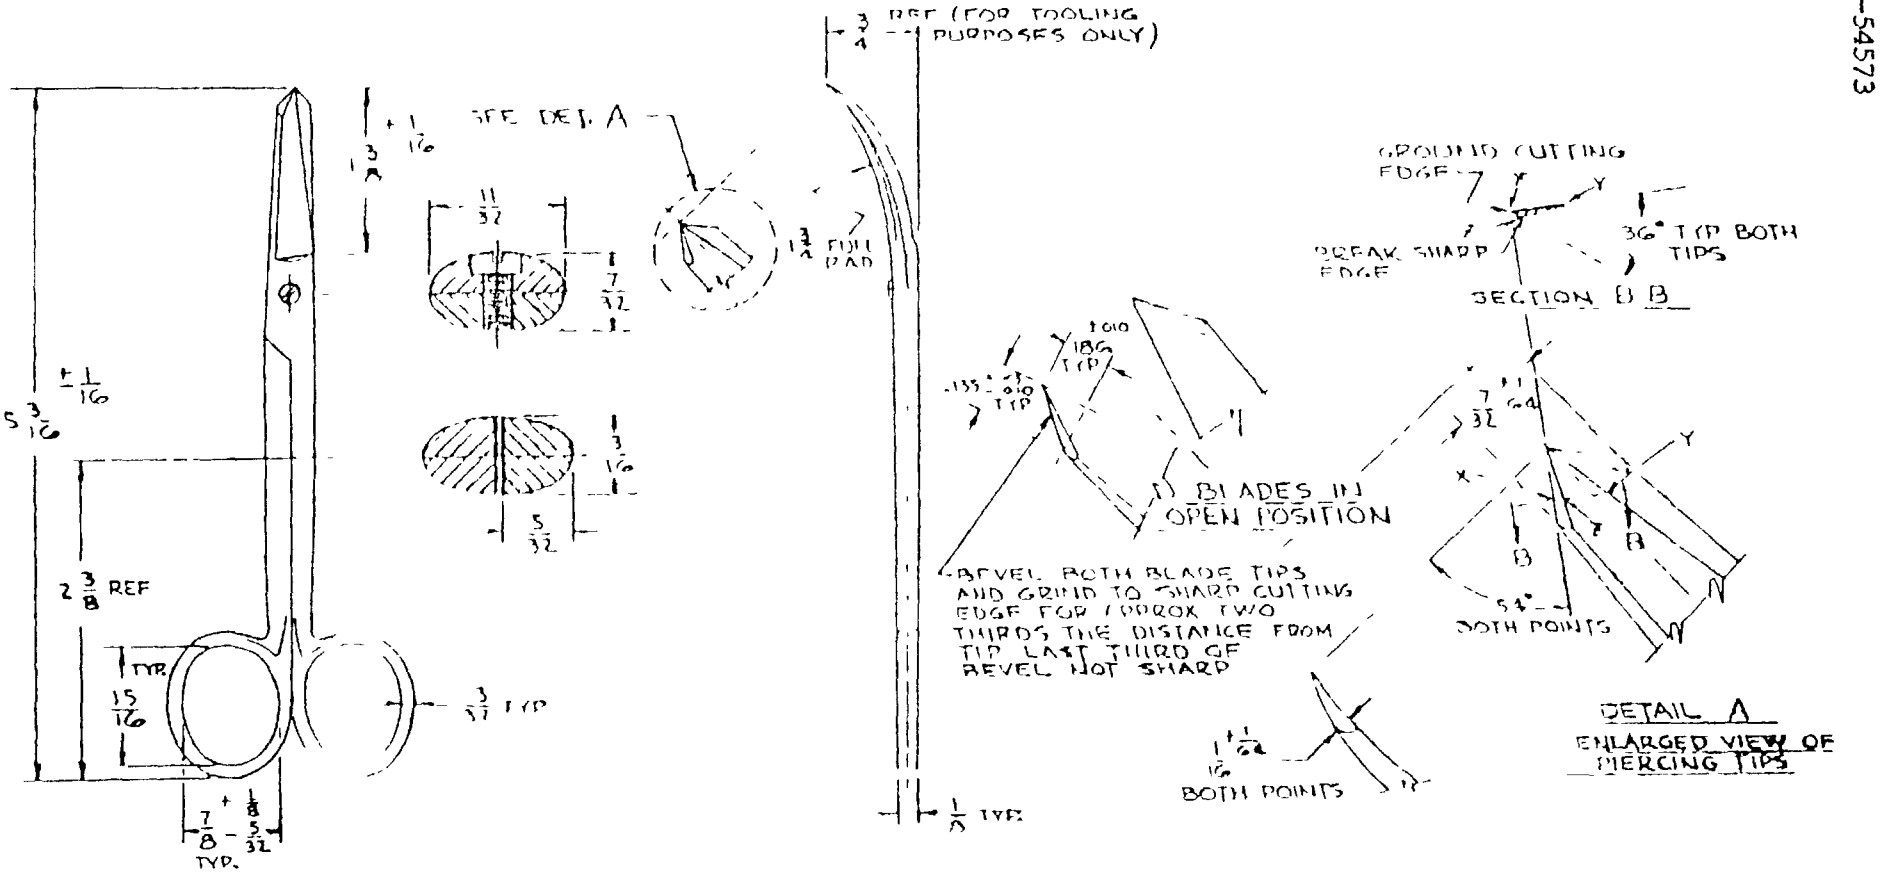

NOTE

TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP

NSN 6515-00-935-7092

FIGURE 1 SCISSORS-DAGGER-TRACHEOTOMY, CURVED BLADES, ANGULATED POINT TIPS, 5-3/16 IN. LONG, UNIVERSITY OF KANSAS DESIGN

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1 The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given

2 The submitter of this form must complete blocks 4, 5, 6, and 7

3 The preparing activity must provide a reply within 30 days from receipt of the form

NOTE This form may not be used to request copies of documents nor to request waivers, or clarification of requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements

I RECOMMEND A CHANGE:	1 DOCUMENT NUMBER A-A-54573	2 DOCUMENT DATE (YYMMDD) 17 January 1992

3 DOCUMENT TITLE
SCISSORS-DAGGER, TRACHEOTOMY, UNIVERSITY OF KANSAS DESIGN, CURVED BLADES, 5-3/16 INCH LONG

4 NATURE OF CHANGE (Identify paragraph number and include proposed rewrite if possible Attach extra sheets as needed)

5 REASON FOR RECOMMENDATION

6 SUBMITTER

a NAME (Last, First, Middle Initial)	b ORGANIZATION	
c ADDRESS (Include Zip Code)	c TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7 DATE SUBMITTED (YYMMDD)

8 PREPARING ACTIVITY

a NAME Defense Personnel Support Center	b TELEPHONE (Include Area Code) (1) Commercial (215)737-2870	(2) AUTOVON 444-2870
c ADDRESS (Include Zip Code) ATTN: MSE 2800 S. 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403 Falls Church VA 22041 3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 Previous editions are obsolete 198/290

Source: https://assist.dla.mil - Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.