A-A-54596
28 February 1992

COMMERCIAL ITEM DESCRIPTION

CURETTE, PERIODONTAL (Columbia)

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for MIL-C-42015 which is cancelled.

This commercial item description covers double-ended periodontal curettes of the Columbia design.

Salient characteristics:

Classification: The curettes shall be of the following numbers:

Columbia, No. 2L and 2R
Columbia, No. 4L and 4R
Columbia, No. 13 and 14

Material. Materials shall be stainless steel in accordance with the American Society for Testing and Materials (ASTM) Designation F899 for composition only.

Operative ends. The operative ends shall be class 4, type 440A, 440B, or 440C stainless steel.

Handle. Handle A and D (see figures 1-3) shall be plated brass. Brass shall conform to class 8, copper alloy No. 260 or 330, as specified in ASTM Designation B135 for composition only. The brass handles shall be chromium over nickel plated. Handle B shall be fabricated of martensitic stainless steel, type 430F stainless steel in accordance with ASTM A473 for composition only. Handle C shall be fabricated of austenitic stainless steel, type 303.

Hardness. After proper stress relieving, the Rockwell Hardness of the operative ends shall be C52 to C56 for type 440A, C54 to C58 for type 440B, and C56 to C60 for type 440C, when tested in accordance with ASTM Designation E18 (Rockwell) or E92 (Vickers or Diamond Pyramid).

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Style, design and dimensions. The curettes shall be double-ended, of Columbia design, of the Columbia instrument (2L, 2R, 4L, 4R, 13 or 14) as specified. The curettes shall be fine bladed, and suitable for use during subgingival curettage, as well as during polishing of cementum. The curettes shall be furnished with the handle and shank design A, B, C or D, in accordance with figures 1-3, for the applicable Columbia instrument number.

The curettes shall be of three-piece construction, consisting of a handle with two operative ends. The operative ends shall be permanently secured to the handle. The junction of the operative end to the handle shall be smoothly finished and free of crevices. There shall be no movement, loosening, or separation between the operative end and handle when the operative end is subjected to the pull test, specified herein.

Corrosion resistance. The curettes shall show no evidence of corrosion when being subjected to the boil and copper sulfate tests of ASTM Designation F1089.

Identification marking. The curettes shall be permanently and legibly marked on the front face, smooth portion of the handle with "Columbia" and the applicable Columbia instrument number, the name or registered trademark of the manufacturer, and the word "stainless". As an alternate to the word stainless, the use of a registered trade name identifying the steel as stainless, shall be acceptable, provided prior approval is received from the cognizant officer.

Finish. The operative ends, including shanks, shall have a smooth mirror or smooth bright finish, except for the surfaces that form the cutting edges which shall have a finely honed finish. The operative ends (entire blade) shall have a sharp cutting edge. Honed portion of operative end shall have a sharp cutting edge. Honed portion of operative end shall be blended at junction of shank to from a smooth contour. Finger grip portions of handles shall be serrated or knurled. Handles shall have a mirror or bright finish, except for the serrated or knurled portions. Finger grip portions of the handles shall be free from barbs and shall provide adequate finger grip during use.

Workmanship. The curettes shall be free from defects, including surface defects, which may detract from their appearance or impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Unit. Each (EA). One curette, of the number (2L, 2R, 4L, 4R, 13 or 14) as specified, shall constitute one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after the delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The curette shall be examined to determine compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 at inspection level S-1, with and AQL of 1.0 (percent defective).

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Pull test. The handle and shank of the operative end shall be securely held in separate chucks or other holding devices. A slowly increasing pull out force, increasing from 0 to 85 pounds (minimum), shall be applied to the shank of the operative end. The force shall be maintained at the high value for a minimum of 1 second. The instrument shall then be examined for movement, looseness, or separation of the operative end with respect to the handle. The test shall be repeated for each operative end of the double-ended instrument.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met. If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable. The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

National Stock Number	Item Identification
6520-01-046-7334	Curette, Periodontal, Columbia University No. 2L and 2R
6520-01-046-7335	Curette, Periodontal, Columbia University No. 4L and 4R
6520-01-047-9801	Curette, Periodontal, Columbia University No. 13 and 14

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS


Project No. 6520-2515
Location: DC Disk #2
(CURETTE)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.


3-A-3455/96

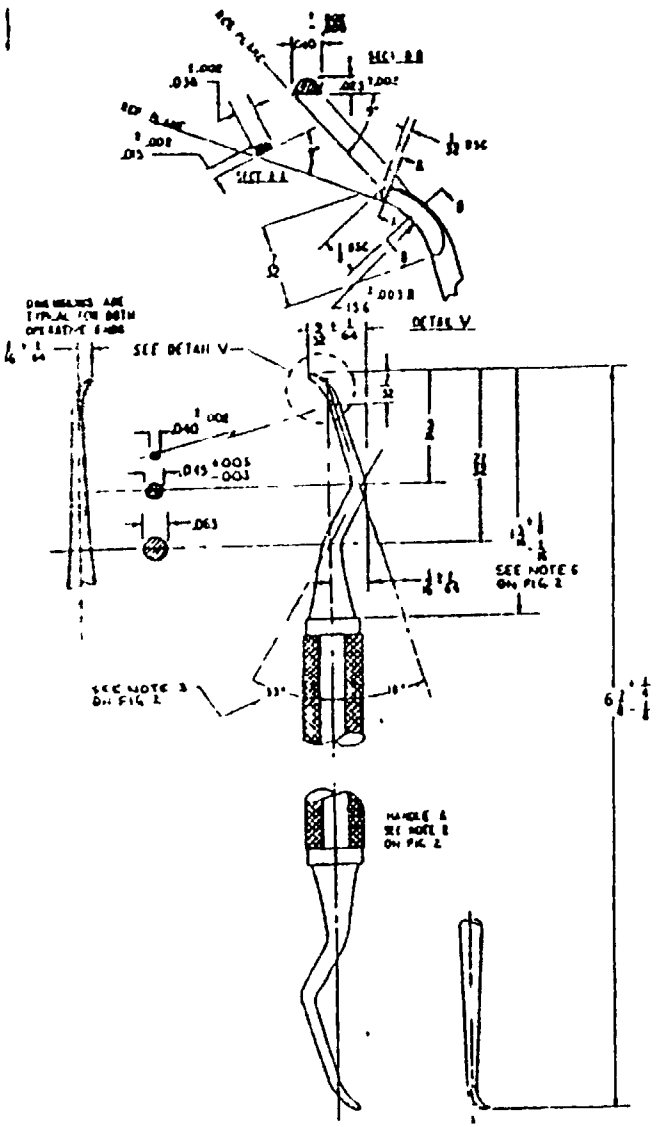

STYLE 1 COLUMBIA NO. 2L AND 2R
NSN 6520-01-046-7334

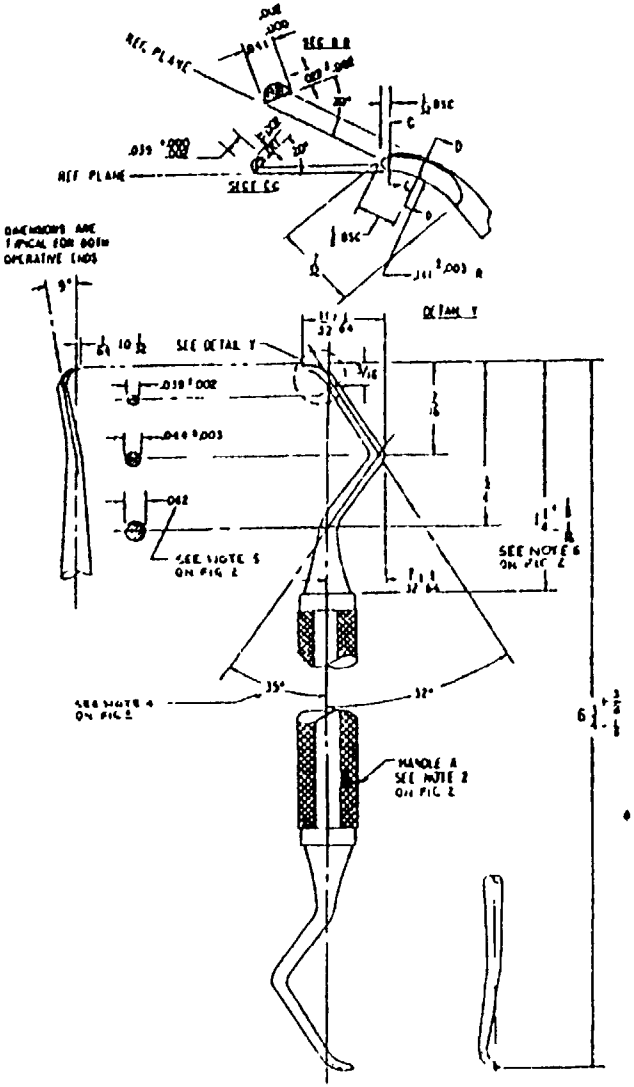


STYLE 2 COLUMBIA NO. 4L AND 4R
NSN 6520-01-046-7335

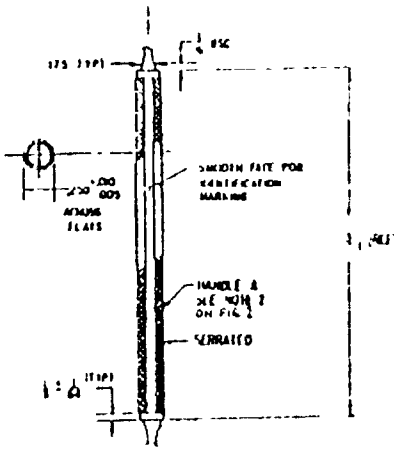

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 1/32	± .005	= 2°

FIGURE 1 CURETTES, PERIODONTAL (COLUMBIA)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

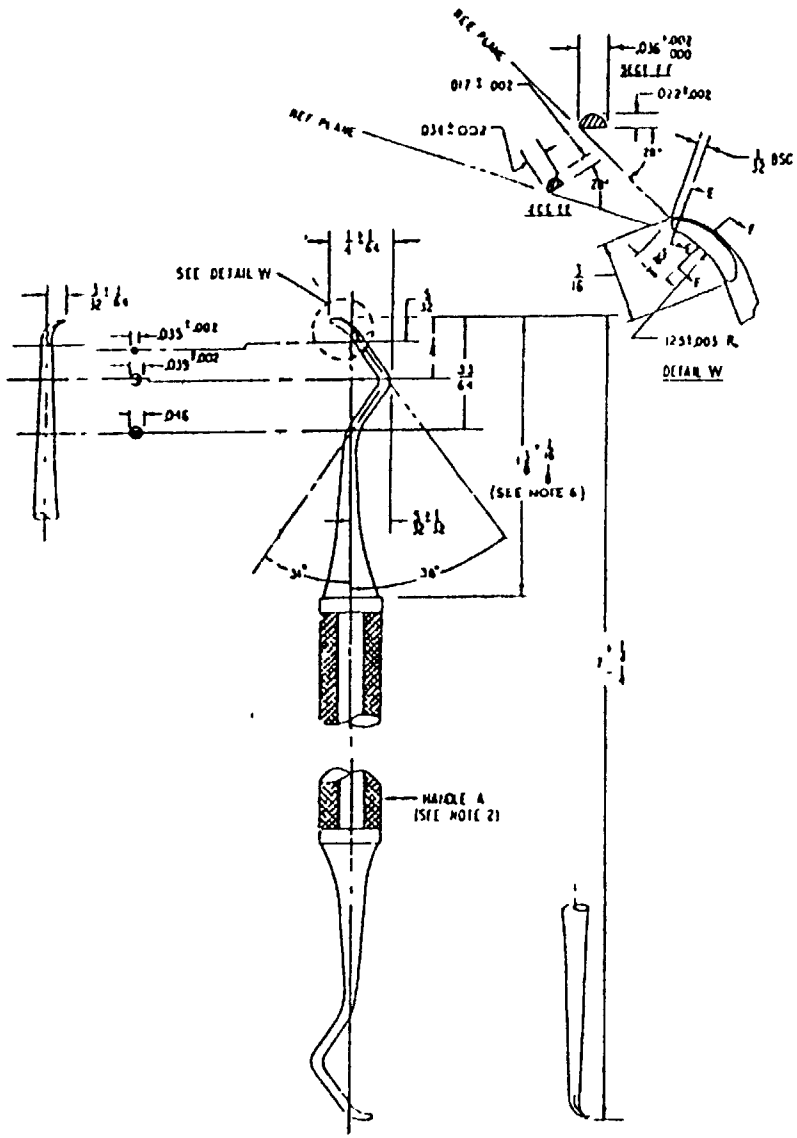

STYLE 3 COLUMBIA NO. 13 AND 14
NSN 6520-01-047 9801

NOTE:

1 - DIMENSION LABELED "BSC" ARE BASIC WITHOUT TOLERANCE USED AS A BASIS FROM WHICH PERMISSIBLE VARIATIONS ARE ESTABLISHED BY TOLERANCES ON OTHER DIMENSIONS.

2 - SEE SHEET 3 OF 3 FOR ALTERNATE HANDLES B, C AND D WITH RESPECTIVE SHANK DESIGNS AND DIMENSIONS

3 - AS AN ALTERNATE SHALL BE 40±2 DEGREES

4 - AS AN ALTERNATE SHALL BE 45±2 DEGREES

5 - AS AN ALTERNATE SHALL BE .081±.002

6 - AS AN ALTERNATE SHALL BE $1\frac{1}{2}{}^{+\frac{1}{8}}_{-\frac{1}{8}}$ FOR HANDLE C

FIGURE 2 CURETTES, PERIODONTAL (COLUMBIA)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

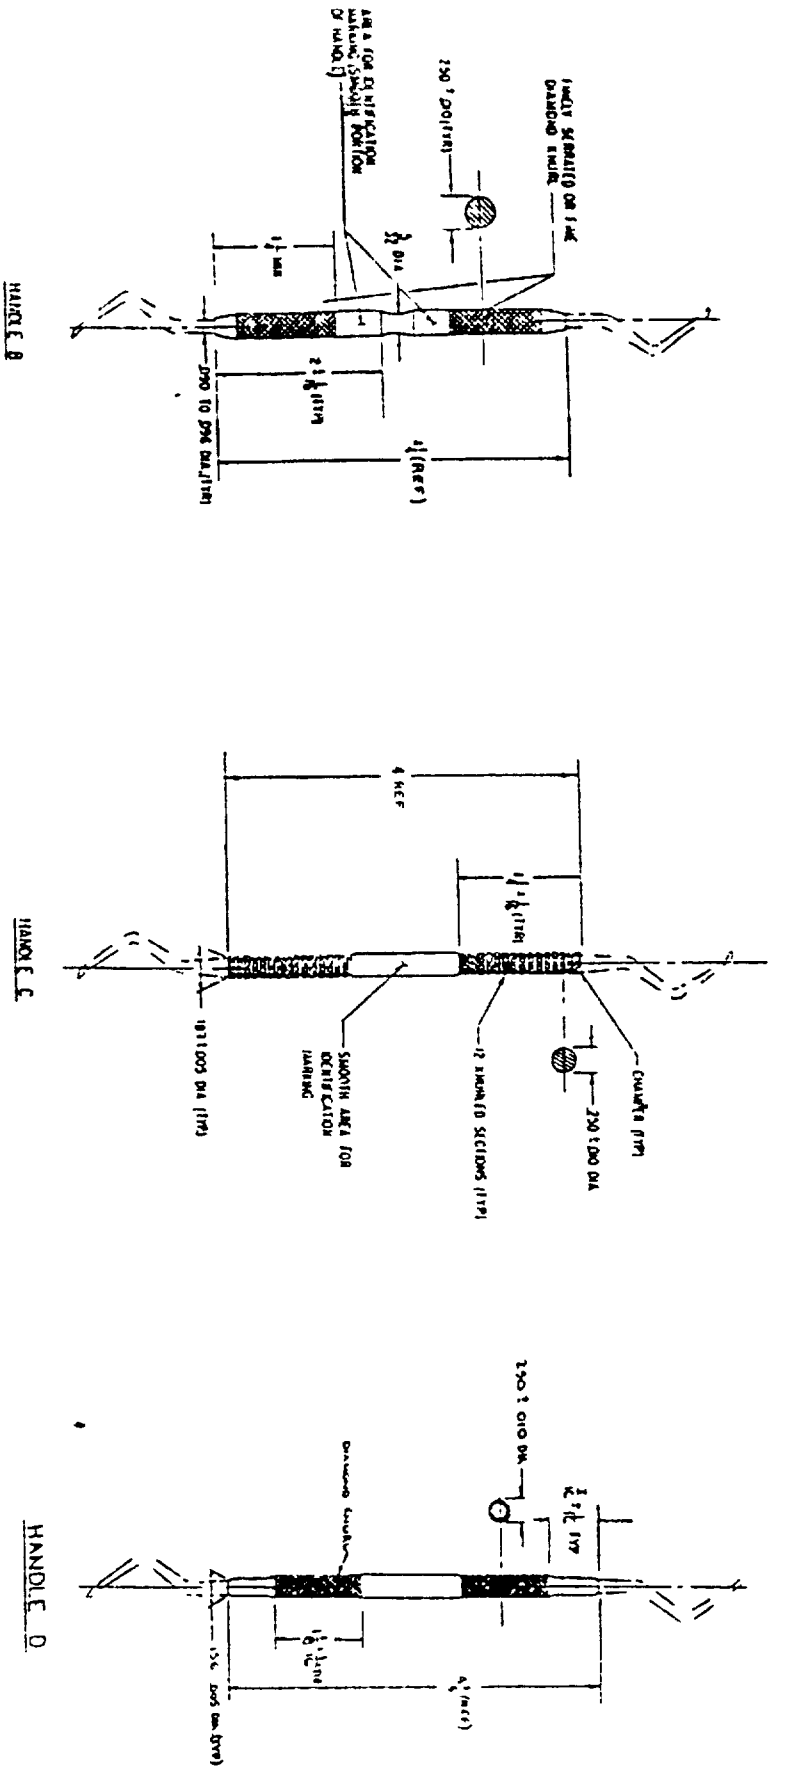


FIGURE 3 CURETTES, PERIODONTAL (COLUMBIA)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I. RECOMMEND A CHANGE:	1. DOCUMENT NUMBER: A-A-54596	2. DOCUMENT DATE (YYMMDD): 92-02-28

3. DOCUMENT TITLE: CURETTE, PERIODONTAL (Columbia)

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable) / 7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME: Defense Personnel Support Center	b. TELEPHONE (Include Area Code) (1) Commercial: (215)737-2870 (2) AUTOVON: 444-2870
c. ADDRESS (Include Zip Code): ATTN: DPSC-MSE, 2800 S. 20th Street, Philadelphia, PA 19101	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS CONTACT: Defense Quality and Standardization Office, 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466, Telephone (703) 756-2340, AUTOVON 289-2340

DD Form 1426, OCT 89 — Previous editions are obsolete — 96/296

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:36Z
Check the source to verify that this is the current version before use.