RR-B-00120b (VAM1)
October 12, 1967
Int. Rev. of Fed Spec.
RR-B-120a
April 24, 1958

INTERIM FEDERAL SPECIFICATION

BASIN, EMESIS; BASIN, WASH; (CORROSION-RESISTING STEEL)

This Interim Federal Specification was developed by the Veterans Administration, Department of Medicine and Surgery, Supply Service, Marketing Division, Medical-Dental-Scientific Supplies, Marketing Center, P. O. Box 76, Hines, Illinois 60141, based upon currently available technical information. It is recommended that Federal Agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers emesis and wash basins for use in hospitals, physicians offices, and first-aid stations in applications suitable for each type.

1.2 Classification

1.2.1 Types, classes, and capacities. Basins shall be of the following types, classes and capacities, as specified (see 6.1).

Type I. - Emesis

Type II - Wash
- Class 1 - Deep.
  - 7-quart capacity
  - 9-quart capacity
- Class 2 - Shallow
  - 4-1/4 quart capacity
  - 5-1/4 quart capacity

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids or request for proposal, form a part of this specification:

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

FEDERAL SPECIFICATIONS

QQ-S-766 - Steel Plates, Sheets and Strip-Corrosion Resisting
PPP-B-585 - Boxes, Wood, Wirebound
PPP-B-601 - Boxes, Wood, Cleated - Plywood
PPP-B-621 - Boxes, Wood, Nailed and Lock-Corner
PPP-B-636 - Box, Fiberboard

FEDERAL STANDARDS:

Fed. Std. No. 102 - Preservation, Packaging, and Packing Levels.

Fed. Std. No. 123 - Marking for Domestic Shipments (Civilian Agencies).

Fed. Test Method Std. No. 151 - Metals;
Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.,

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military Specifications

MIL-L-10547 - Liners, Case, Waterproof

Military Standards

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes

MIL-STD-129 - Marking for Shipment and Storage

(Copies of Military Specifications and Standards, required by contractors in connection with specific procurement functions, should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

3. Requirements.

3.1 Material

3.1.1 Sheet and Strip. Sheet and strip used in the construction of the basins shall be corrosion-resisting steel, conforming to class 301, 302 or 304 of Federal Specification QQ-S-766. Material shall meet the chemical requirements specified therein, when tested as specified in 4.4.1.

3.2 Construction

3.2.1 Type 1. Type 1 basin shall be of the conventional kidney shape, formed seamlessly from one piece of 0.031-inch (No. 22, U.S. Standard) corrosion-resisting steel, which shall not be reduced below 0.023 inch thick at any point in the finished basins. Basin shall have half-round open-bead edge and the joint of side walls with flat bottom shall be rounded. Design and dimensions shall be as shown in figure 1.

3.2.2 Type II. Type II basin shall be formed seamlessly, from one single piece of 0.031-inch (No. 22, U.S. Standard) corrosion-resisting steel, which shall not be reduced below 0.025 inch thick at any point in the finished basins. Design and dimensions of type II basins shall conform to the requirements of figure 2 for the specified class and capacity.

3.3 Tolerances. A plus or minus tolerance of 6 percent will be allowed in capacity. Dimensional tolerances shall be as indicated in the figures. Tolerances shall be applied in such a way as not to interfere with the proper stacking of the basins of like size and design.

3.4 Finish. The finish shall be smooth on all edges and surfaces, and shall be free of rough grind marks, pits, scales, die marks, and other defects. The final finish on all outside surfaces shall be equivalent to a No. 7 high luster polish. The interior surface may be finished by electropolishing or equivalent to a No. 4 commercial finish. The final finish shall leave a uniform, bright, and shiny surface which can be easily cleaned.

3.4.1 Cleaning. As a final operation, the basins shall be thoroughly cleaned to remove foreign particles, such as dirt, grease, graphite, and metal.

3.5 Identification marking. Each basin shall be impressed with the manufacturer's name or registered trade-mark, when specifically required in the invitation for bids or request for proposal, the contract or purchase order number and the letters U.S. shall be impressed (see 6.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

3.6 Workmanship. Workmanship shall be first class throughout. The basins shall be free from rough grind marks, trimming marks, pits, scales, or other defects or imperfections. All surfaces shall have a smooth finish and shall be free from sharp edges. Basins shall be free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspection set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component of material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling

4.2.1 For examination. Sampling for examination shall be conducted in accordance with Military Standard MIL-STD-105.

	Inspection level	AQL (defects per hundred units)
For visual examination:		
Major defects	II	1.0
Total (major and minor combined) defects	II	4.0
For dimensional examination	L5	2.5

4.3 Examination. The basins shall be examined to determine compliance with all requirements contained in this specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects:

Categories and defects*	
Major	
101	Joint of side walls and flat bottom not rounded (Type I).
102	Basins will not stack properly
103	Bead edge not free of sharpness and burrs
104	Identification marking incomplete or illegible
Minor	
201	Basin not free of dirt, grease, graphite, metallic particles, and other foreign particles.
202	Surface not free of pit, scales, scratches, and grinding and trimming marks.
203	Inside surface penetrated by marking impression.

*Examination shall not be restricted to the classified defects listed above.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.1 or 112.1 of Federal Test Method Standard No. 151.

5. PREPARATION FOR DELIVERY

For civil agency procurement, Federal Standard No. 102 should be referred to for definitions and applications of the various levels of packaging and packing protection for supplies and equipment.

5.1 Packaging. Packaging shall be level A, B, or C as specified (see 6.1).

5.1.1 Unit of issue. One basin, of the stock number specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

5.1 Packaging quantities. The number of units of issue indicated in Table I shall be packaged in each unit, intermediate and shipping container, as applicable, for the required level of protection specified in procurement document.

Type	Unit Package	Intermediate Package	Shipping Container
	Units	Units	Units
I - Emesis	1	6	72
II - 7-Quart	1	6	18
9-Quart	1	6	18
4-1/4-Quart	1	6	36
5-1/4-Quart	1	6	36

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each unit shall be completely wrapped in kraft paper of suitable weight. Wrapping shall be adequately secured to prevent accidental opening.

5.1.3.2 Intermediate package. Intermediate package shall be a carton of appropriate size and design constructed in accordance with Federal Specification PPP-B-636, Type CF, Class Domestic. Carton shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to, the contents. Closure of carton shall be adequate to prevent accidental spillage of contents.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

5.1.4 Level C. The units shall be packaged in accordance with the suppliers commercial practice, which will afford the degree of protection required for shipment within the continental limits of the United States.

5.2 Packaging

5.2.1 Level A

5.2.1.1 Exterior container. Shipping container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; PPP-B-621, table III, or PPP-B-636, type CF, class weather-resistant. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-STD-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4,of PPP-B-636. Strapping when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and distribution.

5.2.2 Level B

5.2.2.1 Exterior container. Exterior container shall conform to Federal Specification PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load and constructed in accordance with Federal Specification PPP-B-621, table I; PPP-B-585, style 3, for class 2 use; or PPP-B-636, type CF, class domestic and method I closure shall be utilized.

5.2.3 Level C. The number of units to be overpacked in a shipping container shall be in accordance with standard commercial practice. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

5.3.1 For civilian agencies

5.3.1.1 Interior packages. In addition to any special marking specified in the contract or order, each unit package, and shipping container shall be marked in accordance with Federal Standard No. 123.

5.3.2 For Military Agencies

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2.2 Shipping container. Shipping container shall be marked in accordance with Military Specification MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Table, number, and date of this specification.
(b) Type, class, and capacity required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(d) Specify if special marking is required.

6.2 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.4 Transportation description. Transportation description applicable to these items is:

Sheet-steel ware, not otherwise indexed by name.
Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification.

Sheet-steel articles, not otherwise indexed by name.
Truckload minimum weight 20,000 pounds.


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

Notice. - When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:


Army - M Q
Navy - Md
Air Force

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

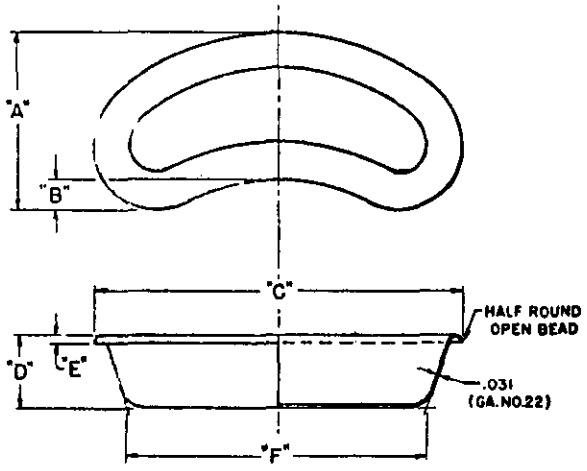

A	B	C	D	E	F
$5\frac{1}{2}\pm\frac{1}{8}$	$\frac{7}{8}\pm\frac{1}{16}$	$10\pm\frac{1}{8}$	$2\frac{1}{16}\pm\frac{1}{16}$	$\frac{7}{32}\pm\frac{1}{32}$	$7\frac{7}{8}$ APPROX.

FIGURE 1.

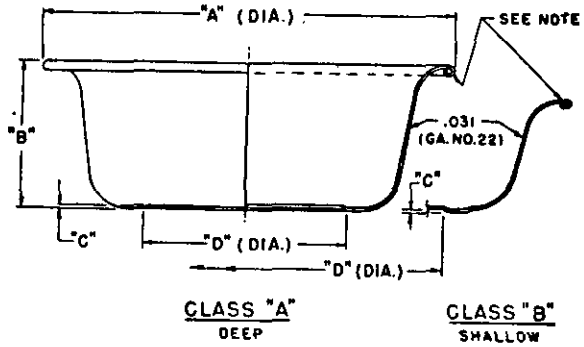

CLASS	A	B	C	D	CAP IN QTS.
1	$13\frac{3}{4}\pm\frac{1}{8}$	$4\frac{1}{2}\pm\frac{1}{8}$	$\frac{3}{32}\pm\frac{1}{64}$	$7\frac{3}{8}\pm\frac{1}{8}$	7
	$14\frac{5}{8}\pm\frac{1}{8}$	$4\frac{13}{16}\pm\frac{1}{32}$	$\frac{3}{32}\pm\frac{1}{64}$	$7\pm\frac{1}{8}$	9
2	$12\frac{1}{2}\pm\frac{1}{4}$	$3\frac{1}{2}\pm\frac{1}{4}$	$\frac{3}{32}\pm\frac{1}{32}$	$5\frac{1}{8}\pm\frac{1}{8}$	$4\frac{1}{4}$
	$13\frac{7}{8}\pm\frac{1}{4}$	$3\frac{3}{4}\pm\frac{1}{4}$	$\frac{3}{32}\pm\frac{1}{32}$	$5\frac{3}{16}\pm\frac{1}{8}$	$5\frac{1}{4}$

NOTE:
MANUFACTURER MAY USE EITHER A TIGHT ROUND ROLLED BEAD, OR A TIGHT FLAT DOUBLE ROLLED BEAD, APPROX. $\frac{3}{16}$ THICK.

FIGURE 2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.