RR-B-120a
APRIL 24, 1958
SUPERSEDING
Fed. Spec. RR-B-120
January 14, 1955

FEDERAL SPECIFICATION

BASIN, EMESIS; BASIN, WASH; (CORROSION-RESISTING STEEL)

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers emesis and wash basins for use in hospitals, physicians' offices, and first-aid stations in applications suitable for each type.

1.2 Classification.

1.2.1 *Types, classes, and capacities.*—Basins shall be of the following types, classes and capacities, as specified (see 6.1).

Type I.—Emesis.

Type II.—Wash.
- Class 1.—Deep.
  - 7-quart capacity.
  - 9-quart capacity.
- Class 2.—Shallow.
  - 4¼-quart capacity.
  - 5¼-quart capacity.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

QQ-S-766 — Steel, Corrosion-Resisting, Plates, Sheets, Strips, and Structural Shapes.

PPP-B-585—Boxes; Wood, Wirebound

PPP-B-601—Boxes, Wood, Cleated, Plywood.

PPP-B-621—Boxes, Wood, Nailed and Lock-Corner.

PPP-B-636—Boxes, Fiber.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.

Fed. Std. No. 123.—Marking for Domestic Shipments (Civilian Agencies).

Fed. Test Method Std. No. 151—Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

441890/58/306

FSC 6530, 7240

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

Military Specifications:

MIL–B–10377—Box, Wood, Cleated, Veneer, Paper Overlaid.

MIL–B–10547 — Liners, Case, Waterproof.

Military Standards:

MIL–STD–105 — Sampling Procedures and Tables for Inspection by Attributes.

MIL–STD–129—Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by the contractor in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS


3.1 Material.

3.1.1 *Sheet and strip.*—Sheet and strip used in the construction of the basins shall be corrosion-resisting steel, conforming to class 1 or 2 of Federal Specification QQ–S–766. Material shall meet the chemical requirements specified therein, when tested as specified in 4.3.1.

3.2 Construction.


3.2.1 *Type I.*—Type I basin shall be of the conventional kidney shape, formed seamlessly from one piece of 0.031-inch (No. 22, U. S. Standard) corrosion-resisting steel, which shall not be reduced below 0.027 inch thick at any point in the finished basins. Basin shall have half-round open-bead edge and the joint of side walls with flat bottom shall be rounded. Design and dimensions shall be as shown in figure 1.

3.2.2 *Type II.* — Type II basin shall be formed seamlessly, from one single piece of 0.031-inch (No. 22, U. S. Standard) corrosion-resisting steel, which shall not be reduced below 0.027 inch thick at any point in the finished basins. Design and dimensions of type II basins shall conform to the requirements of figure 2 for the specified class and capacity.

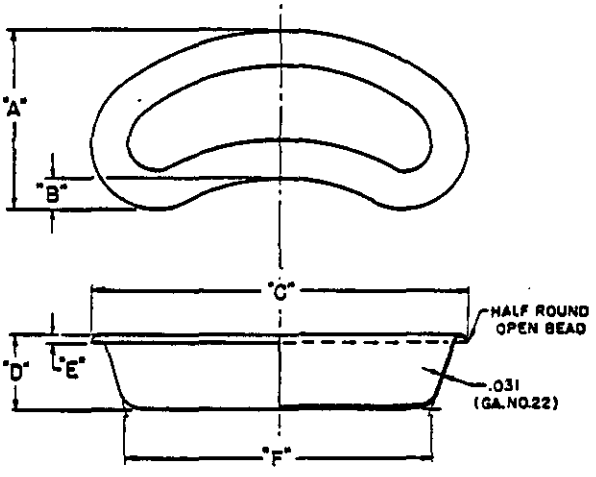

A	B	C	D	E	F
$5\frac{1}{2} \pm \frac{1}{8}$	$\frac{7}{8} \pm \frac{1}{16}$	$10 \pm \frac{1}{8}$	$2\frac{1}{16} \pm \frac{1}{16}$	$\frac{7}{32} \pm \frac{1}{32}$	$7\frac{7}{8}$ APPROX.

FIGURE 1.

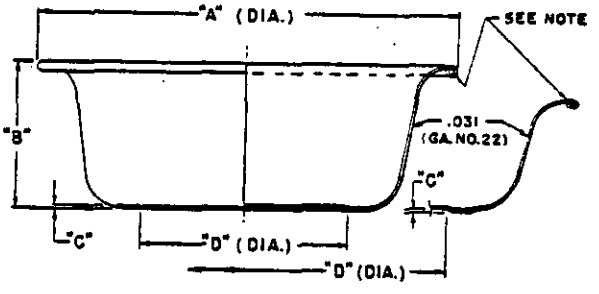

CLASS "A" DEEP

CLASS "B" SHALLOW

CLASS	A	B	C	D	CAP IN QTS.
1	$13\frac{3}{4} \pm \frac{1}{8}$	$4\frac{1}{2} \pm \frac{1}{8}$	$\frac{3}{32} \pm \frac{1}{64}$	$7\frac{3}{8} \pm \frac{1}{8}$	7
	$14\frac{3}{8} \pm \frac{1}{8}$	$4\frac{13}{16} \pm \frac{1}{32}$	$\frac{3}{32} \pm \frac{1}{64}$	$7 \pm \frac{1}{8}$	9
2	$12\frac{1}{2} \pm \frac{1}{4}$	$3\frac{1}{2} \pm \frac{1}{4}$	$\frac{3}{32} \pm \frac{1}{32}$	$5\frac{1}{8} \pm \frac{1}{8}$	$4\frac{1}{4}$
	$13\frac{7}{8} \pm \frac{1}{4}$	$3\frac{3}{4} \pm \frac{1}{4}$	$\frac{3}{32} \pm \frac{1}{32}$	$5\frac{3}{16} \pm \frac{1}{8}$	$5\frac{1}{4}$

NOTE: MANUFACTURER MAY USE EITHER A TIGHT ROUND ROLLED BEAD, OR A TIGHT FLAT DOUBLE ROLLED BEAD, APPROX. $\frac{3}{16}$ THICK.

FIGURE 2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

3.3 Tolerances.—A plus or minus tolerance of 6 percent will be allowed in capacity. Dimensional tolerances shall be as indicated in the figures. Tolerances shall be applied in such a way as not to interfere with the proper stacking of the basins of like size and design.

3.4 Finish.

3.4.1 *Grinding.*—The entire inside and outside surfaces shall be finished with a No. 200 emery, after all surface imperfections have been removed by previous grinding. This last grinding shall produce a uniform finished surface with all imperfections and marks of previous grinds removed. The thickness of the sheet forming the basins shall not be reduced below the thickness specified in 3.2.1 and 3.2.2, by grinding to remove surface imperfections.

3.4.1.1 *Electropolishing.*—The interior of the basin may be finished by electropolishing. The electropolishing shall result in a uniform, bright, and shiny surface which may be easily cleaned.

3.4.2 *Cleaning.*—As a final operation, the basins shall be thoroughly cleaned to remove foreign particles such as dirt, grease, graphite, and metal.

3.4.3 *Resistance to corrosion.*—When tested as specified in 4.3.2, slight surface corrosion of the specimen which can be washed off shall not be considered cause for rejection, but if the specimen should rust or show continuous bleeding from pits, it shall be considered as having failed to pass the test.

3.5 Identification marking. — Each basin shall be impressed with the manufacturer's name or registered trade-mark. All impressions shall be made at even pressure so as not to penetrate the inside surface of the basin. Markings shall be legible and distinct.

3.5.1 *Marking for Military Medical Supply Agency Procurement.* — In addition to the manufacturer's name or registered trademark, the bottom of the basins shall be die-stamped, or otherwise permanently marked with the Medical Services symbol conforming to figure 3. The letters shall be ¼ inch high and the caduceus shall be of appropriate size.

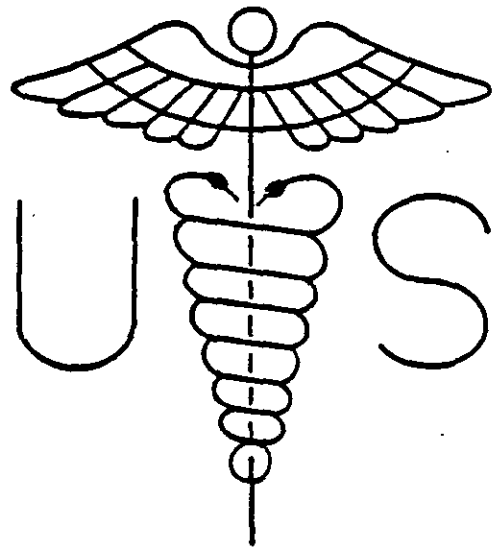


FIGURE 3.—Medical Services symbol.

3.6 Workmanship.—Workmanship shall be first class throughout. The basins shall be free from rough grind marks, trimming marks, pits, scales, or other defects or imperfections. All surfaces shall have a smooth finish and shall be free from sharp edges. Basins shall be free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *For visual examination.*—Sampling procedures for visual examination shall be conducted in accordance with the procedures set forth in Military Standard MIL–STD–105.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

4.1.2 *For tests.*—Sample size for tests shall be as indicated for inspection level L–2 in Appendix to Military Standard MIL–STD–105, except that the acceptance number shall be zero (0) for all sample sizes, and a minimum of three samples shall be taken.

4.2 Inspection.—The inspector shall ascertain that the basins have been inspected and accepted in accordance with specification requirements.

4.3 Tests.

4.3.1 *Chemical composition.* — Tests for chemical analysis shall be conducted in accordance with method 111 or 112 of Fed. Test. Method Std. No. 151. In lieu of the above, a certificate of quality, showing results of tests performed to indicate that material is as specified in 3.1.1, may be furnished.

4.3.2 *Salt-spray.*—Salt spray test shall be conducted in accordance with method 811 of Fed. Test Method Std. No. 151, for a period of 48 hours.

4.4 Suppliers responsibilities for inspection.—The supplier shall be required to perform examinations and tests set forth in this specification to substantiate conformance of supplies to specification requirements. The examinations and tests shall be at the expense of the supplier. Suppliers shall have either adequate test facilities for executing specific prescribed tests, or shall make arrangements for the utilization of test facilities acceptable to the Government. Records of examinations and tests performed by the supplier shall be maintained by the supplier and made available to the Government upon the Government's request, at any time, or from time to time, for a period of two years after the delivery of the supplies to which the same relate. The supplier shall be responsible for compliance with all requirements of this specification, and all other technical requirements of the contract.

5. PREPARATION FOR DELIVERY

(The levels of preservation, packaging, and packing protection used are defined in Fed. Std. No. 102.)

5.1 Packaging.

5.1.1 *Unit of issue.*—One basin, of the stock number specified, constitutes one unit.

5.1.2 *Packaging quantities.*—The number of units of issue indicated in table I shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in procurement document.

TABLE I.—*Packaging quantities*

Federal Stock Number	Unit package	Intermediate package	Shipping container
	Units	*Units*	*Units*
6530–770–9220	1	6	72
6530–771–0105	1	6	18
6530–771–0225	1	6	18
7240–771–0945	1	6	36

5.1.2.1 *Packing variation permitted.* — If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Unit package.*—Each unit shall be completely wrapped in kraft paper of suitable weight. Wrapping shall be adequately secured to prevent accidental opening.

5.1.3.2 *Intermediate package.*—Intermediate package shall be a carton of appropriate size and design constructed in accordance with Federal Specification PPP–B–636, type

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

I, class 1. Carton shall be designed with suitable interior fittings or shall contain sufficient cushioning material to insure against shifting of, or damage to, the contents. Closure of carton shall be adequate to prevent accidental spillage of contents.

5.1.4 *Level C.*—Each unit shall be wrapped in kraft paper or flexible corrugated fiberboard as required for protection of the unit from damage in handling or storage. Packaging in suitable paperboard carton with adequate cushioning material is acceptable.

5.2 Packing.

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—Exterior container shall be designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 3 use; PPP–B–601, table II, using type III, class 1 plywood; PPP–B–621, table IV; or Military Specification MIL–B–10377, table II.

5.2.1.2 *Case liner.*—Each level A box shall be lined with a waterproof case conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.* — Strapping, when required, shall be in accordance with applicable box specification.

Note.—Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.*—Exterior container shall conform to Federal Specification PPP–B–601, table I, using type III, class 1 plywood; or shall be designed for type 3 load and constructed in accordance with Federal Specification PPP–B–621, table II; PPP–B–585, style 3, for class 2 use; or Military Specification MIL–B–10377, table I.

5.2.3 *Level C.*—The number of units to be overpacked in a shipping container shall be in accordance with standard commercial practice. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 *For civilian agencies.*

5.3.1.1 *Interior packages.*—Marking shall be in accordance with Federal Standard No. 123, and shall include the stock number and item identification as specified in the contract or purchase order.

5.3.1.2 *Shipping container.*—Marking shall be in accordance with Federal Standard No. 123.

5.3.2 *For Military agencies.*

5.3.2.1 *Interior packages.*—Each unit package and each intermediate package shall be marked in accordance with section 5 of Military Standard MIL–STD–129.

5.3.2.2 *Shipping container.*—Shipping container shall be marked in accordance with Military Standard MIL–STD–129. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

6. NOTES

6.1 Ordering data. — Procurement documents should specify the following:

(*a*) Title, number, and date of this specification.

(*b*) Type, class, and capacity required (see 1.2).

(*c*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.

6.2 This specification covers the following items appearing in the Armed Services Medical Stock List:

6530–770–9220—BASIN, EMESIS, Corrosion-Resisting Steel.
6530–771–0105 — BASIN, WASH, Corrosion-Resisting Steel, 7 qt.
6530–771–0225 — BASIN, WASH, Corrosion-Resisting Steel, 9 qt.
7240–771–0945 — BASIN, WASH, Corrosion-Resisting Steel, 4¼ qt.

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no samples will be necessary prior to award to determine compliance with this specification. If, for any particular purpose, samples with bids are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid sample should be definitely stated, the specification to apply in all other respects.

6.4 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.5 Transportation description.—Transportation description applicable to these items is:

Sheet-steel ware, not otherwise indexed by name.
Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification.

Sheet-steel articles, not otherwise indexed by name.
Truckload minimum weight 20,000 pounds.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:
Army—M Q
Navy—Md
Air Force.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:08Z
Check the source to verify that this is the current version before use.