RR-B-00191e(DSA-DM)
October 6, 1971
SUPERSEDING
Revision of
Int. Fed. Spec.
RR-B-00191d (VAMI)
October 12, 1967 and
(see Section 6).

INTERIM FEDERAL SPECIFICATION

BEDPAN

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification RR-B-191.

1. SCOPE

1.1 This specification covers a corrosion-resisting steel bedpan, suitable for use where patients are confined to bed.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:09Z
Check the source to verify that this is the current version before use.

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Federal

FED-STD-66	Steel: Chemical Composition and Hardenability.
FED-STD-123	Marking for Domestic Shipment (Civilian Agencies).
Fed. Test Method Std. No. 151	Metals, Test Methods.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, D. C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The bedpan shall be fabricated from AISI 304 corrosion-resisting steel conforming to Federal Standard No. 66, when tested as specified in 4.4.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:09Z
Check the source to verify that this is the current version before use.

3.2 Design and construction. Design shall be as shown in figure 1 or 2, and as hereinafter specified. The bedpan shall be formed from two pieces of corrosion-resisting steel not less than 0.031 inch thick, (No. 22, United States Standard [USS] gage), which shall not be reduced below 0.027 inch thickness except for a maximum of 5 percent of the total area, which shall not be reduced below 0.022 inch thickness at any point. The material shall be joined by welding. The bedpan shall have a tight, flat, single, rolled edge all around the opening at the top, and shall be rolled tightly to eliminate all crevices. The bottom of the bedpan shall be embossed and concave. Dimensions shall be as shown in the figures.

* 3.3 Welding. Welding shall be durable, sound in every detail and in accordance with latest practices recommended by the American Welding Society. All welds shall be produced by qualified welding operators with satisfactory welding equipment using satisfactory filler metal or electrode where applicable to provide the best possible weld. Surfaces to be welded shall be free from grease, oil, oxides or any other foreign matter; any cleaning method which will remove these substances and leave the surface clean is satisfactory. All weld joints shall blend into the adjacent metal in gradual, smooth curves. Welds shall not be oxidized. All welds shall be continuous with no visible voids, pin holes, or cracks, and have more strength than required for purpose intended.

* 3.4 Finish. The inside and outside surfaces shall be ground to produce a uniform finished surface equivalent to a No. 4 commercial finish, with all imperfections and all marks of previous grinds removed. The thickness of the sheet forming the bedpan shall not be reduced below the thickness specified by grinding to remove surface imperfections.

* 3.5 Cleaning. As a final operation, the bedpan shall be thoroughly cleaned to remove any substances, such as dirt, grease, graphite, and metal.

3.6 Identification marking. Each bedpan shall be impressed on the bottom with the manufacturer's name or registered trademark, the contract or purchase order number, Federal Stock Number and the letters U.S. All impressions shall be made at even pressure so as not to penetrate the inside surface of the bedpan.

3.7 Workmanship. Bedpans shall be free from defects which may affect their appearance or serviceability. Bedpans shall be free of rough grind marks, trimming marks, pits, scales, and other defects or imperfections. All surfaces shall have a smooth finish and shall be free of sharp edges.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:09Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the Federal Stock Number, the Item Identification, the name of the component or material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specifications requirements.

4.2 Sampling.

4.2.1 For examination, Sampling for examination shall be conducted in accordance with MIL-STD-105, and Table I.

Table I.

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Minor defects	II	4.0
For dimensional examination	S-3	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:09Z
Check the source to verify that this is the current version before use.

4.3 Examination. The tables shall be examined to determine compliance with all requirements contained in this specification.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the following classification of defects, as shown in Table II.

Table II

Categories	Defects
Major	
101	Welding joining two pieces not sound, or not free of spatter or porosity.
102	Opening at top does not have a tight, flat, single rolled edge.
103	Rolled edge not free of sharpness, and burrs.
104	Bottom not concave and embossed.
105	Bedpan does not rest on a flat surface without rock or wobble.
* 106	Existance of crevice, undercut pinhole or crack at either surface of welded joint.
Minor	
201	Welded joint not properly ground; does not blend with adjacent surfaces.
202	Unit not free of dirt, grease, graphite, metallic particles, or other foreign substances.
203	Surface not free of pits, scales, scratches, and grinding or trimming marks.
204	Inside surface of the bottom penetrated by marking impressions.
205	Identification marking incomplete or illegible.

* Examination shall not be restricted to the classified possible defects listed above.

4.3.2 Dimensional examination. The bedpans shall be examined for defects in dimensions. Any dimension not within the tolerances specified herein shall be classified as a defect.

4.4 Tests. Tests shall be conducted as necessary, to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:09Z
Check the source to verify that this is the current version before use.

4.4.1 Chemical composition. Tests for chemical analysis shall be conducted in accordance with method 111.2 or 112.2 of Fed. Test Method Std. No. 151. Four ounces of each lot of metal used in the construction of the bedpans shall be selected for chemical analysis.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A, or C as specified (see 6.2).

5.1.1 Unit of issue. One bedpan, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in the following table shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table III. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	12 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Unit package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.2).

5.2.1 Level A.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:09Z
Check the source to verify that this is the current version before use.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with Fed. Std. No. 123.

5.3.2 Military activities.

5.3.2.1 Interior packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. Military hospitals and medical facilities.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:09Z
Check the source to verify that this is the current version before use.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specifications.
(b) Selection of applicable levels of packing (see 5.1 and 5.2).
(c) Selection of design (see 3.2).

6.3 This specification covers the following item listed in the Federal Supply Catalog:

FSN	Item Identification
6530-771-7025	Bedpan, Corrosion-Resisting Steel

6.4 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

6.5 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

* 6.6 Also superseding Int. Fed. Spec. RR-B-00191c (DSA-DM) January 25, 1967 and Int. Revision of Fed. Spec. RR-B-191b, September 18, 1962 and Fed. Spec. RR-B-191a, October 26, 1956 and Int. Fed. Spec. RR-B-00191a (GSA-FSS) March 22, 1956 and Fed. Spec. RR-B-191, October 11, 1940.

Custodians:
Army - MD
Navy - MS
Air Force - 03


Preparing activity:
Defense Supply Agency - DM


Project No. 6530-1235


Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026t0-26T12:09Z
Check the source to verify that this is the current version before use.

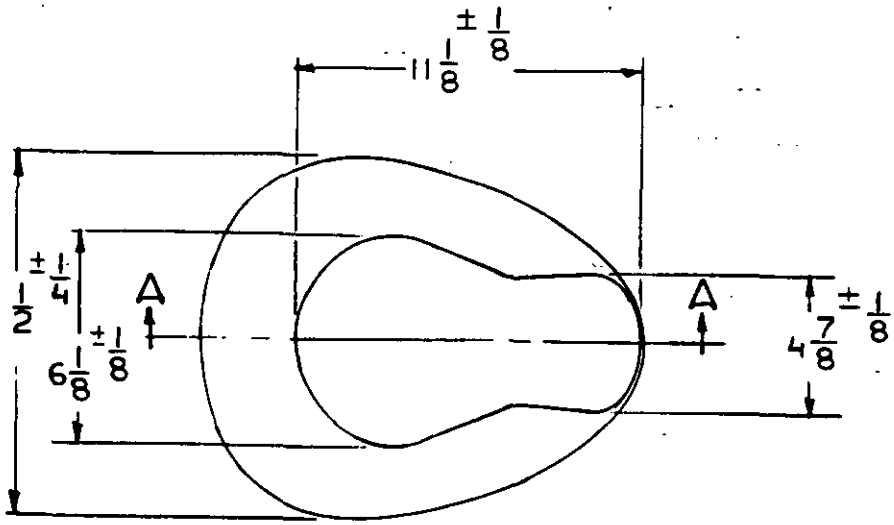



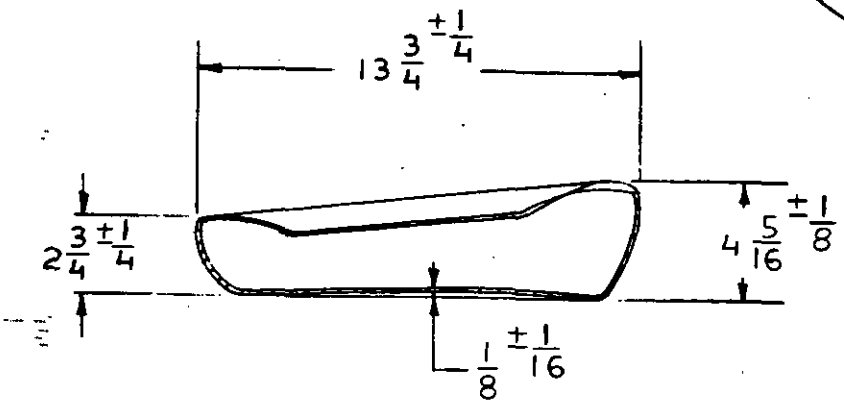


SECTION A-A

GENERAL NOTES:
UNLESS OTHERWISE SPECIFIED:


1. REMOVE BURRS AND BREAK ALL SHARP EDGES
2. DIMENSIONS ARE IN INCHES.

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:09Z
Check the source to verify that this is the current version before use.

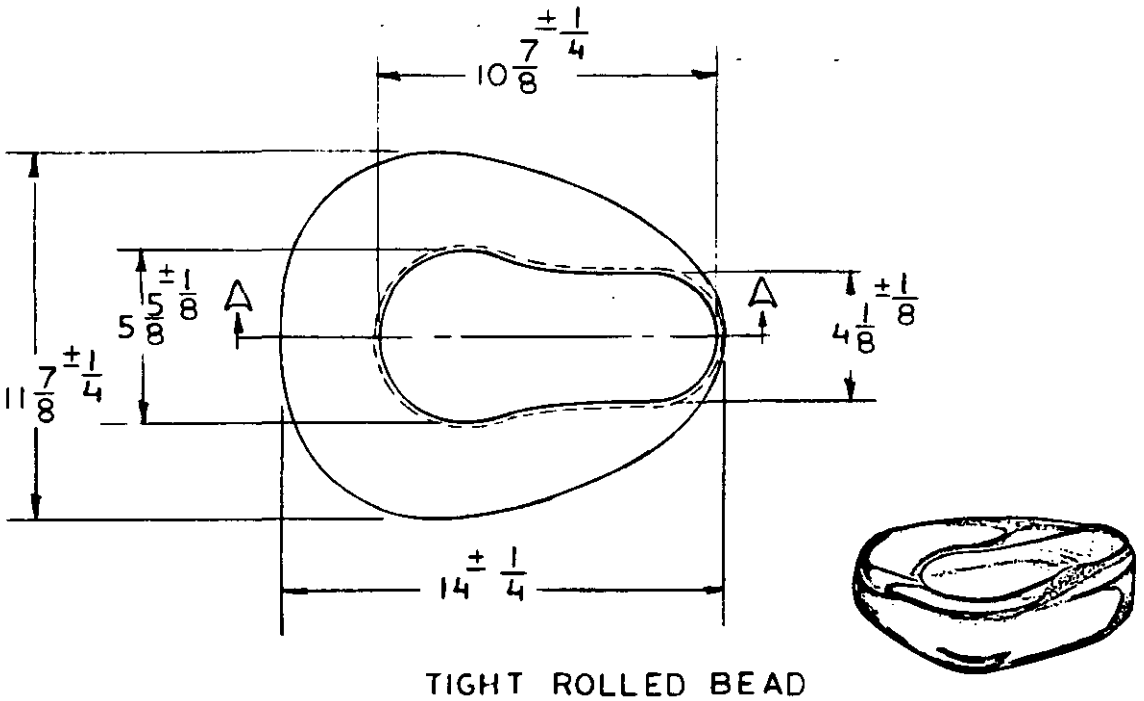

TIGHT ROLLED BEAD AROUND OPENING CLOSED FLAT IN NOSE AREA

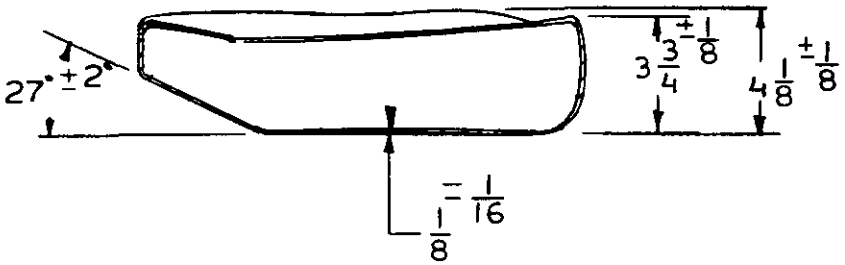

SECTION A-A

GENERAL NOTES

UNLESS OTHERWISE SPECIFIED:

1. REMOVE BURRS AND BREAK ALL SHARP EDGES
2. DIMENSIONS ARE IN INCHS.

FIGURE 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:09Z
Check the source to verify that this is the current version before use.