A-A-51328
21 February 1986

COMMERCIAL ITEM DESCRIPTION

CANNULA, LARYNGEAL

The General Services Administration has authorized the use of this commercial item description in preference to Federal Specification GG-C-124.

This commercial item description covers three types of metal laryngeal cannulae suitable for the suction or the aspiration of the bronchial tract.

Salient characteristics:

Types. The three types of laryngeal cannulae are designated as follows:

Type	Description
I	Laryngeal cannula, Abranam
II	Laryngeal cannula, Jackson
III	Laryngeal cannula, Yankauer

Characteristics:

Type I (Abranam). The type I cannula shall be a curved, flexible laryngeal cannula of the Abraham design with bulbous tip. The type I cannula shall be in accordance with Figure 1.

Type II (Jackson). The type II cannula shall be a curved aspirating tube of the Jackson design. The type II cannula shall be in accordance with Figure 2.

Type III (Yankauer). The type III cannula shall be a suction tube of the Yankauer design. The type III cannula shall be provided with a removable tip.

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

AMSC N/A

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

The type III cannula shall be in accordance with Figure 3. The proximal end of the type III cannula shall be a tapered tip which makes a secure connection with 7/32 i.d. inch rubber hose. As an alternate, the cannula may be provided with a tip adapter which makes a secure connection with 7/32 i.d. inch rubber hose.

Material. The cannula and tip of the type I (Abraham) cannula shall be manufactured from copper and plated with nickel. The hub of the type I cannula shall be manufactured from a suitable brass and plated with chromium over nickel. The type II and type III cannulae shall be manufactured from Class 3, Type 304 or Type 316 austenitic corrosion-resistant steel of the composition given in American Society of Testing and Material (ASTM) Standard F899.

Leakage. The type III cannula shall be tested for leakage as follows: The distal end of the lumen shall be sealed. The adapter, if present, shall be attached and the cannula filled with water. The water shall be pressurized to 45 pounds per square inch (psi) and maintained at 45 psi for 5 minutes. There shall be no leakage from any part of the cannula or from the adapter.

Corrosion. Type I cannula shall be tested for resistance to salt spray in accordance with Federal Specification GG-I-526. Type II and Type III cannulae shall be tested for resistance to boil in accordance with Federal Specification GG-I-526. The cannulae shall show no evidence of corrosion when tested as specified.

Luer Lock hub (Type I) only. The Luer lock hub cavity and flange shall meet the dimensional and performance requirements of American National Standards Institute/Health Industry Manufacturers Association (ANSI/HIMA, Standard MD70.1. The hub cavity shall be plated to the entrance of the lumen.

Markings. Cannulae shall bear the manufacturer's name or registered trademark. Cannulae of foreign manufacture shall bear the name of the country of manufacture. The Type II and Type III cannulae shall bear the word "stainless."

Workmanship. The workmanship of the cannulae shall be first class throughout. There shall be no metal chips or foreign matter on the exterior nor in the lumen of the cannulae. The plating of the type I cannula shall be uniform and free from cracks or peeling. There shall be no defects which impair the serviceability, appearance, or life of the cannulae.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Materials. The supplier shall be responsible for performing test to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One cannula, as specified, constitutes one uni

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and service conform to prescribed requirements.

Records. Records of examinations and tests performed by or for t contractor shall be maintained by the contractor and made available the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a perio of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, Level II, AQL 2.5. The un of product for examination purposes shall be one cannula.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one cannula. Sampling shall be S- with an AQL of 1.0.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

Type	NSN
I	6515-00-314-0600
II	6515-00-385-1100
III	6515-00-386-7600

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB


Agent:

DLA-DM

05263

Project No. 6515-3474

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

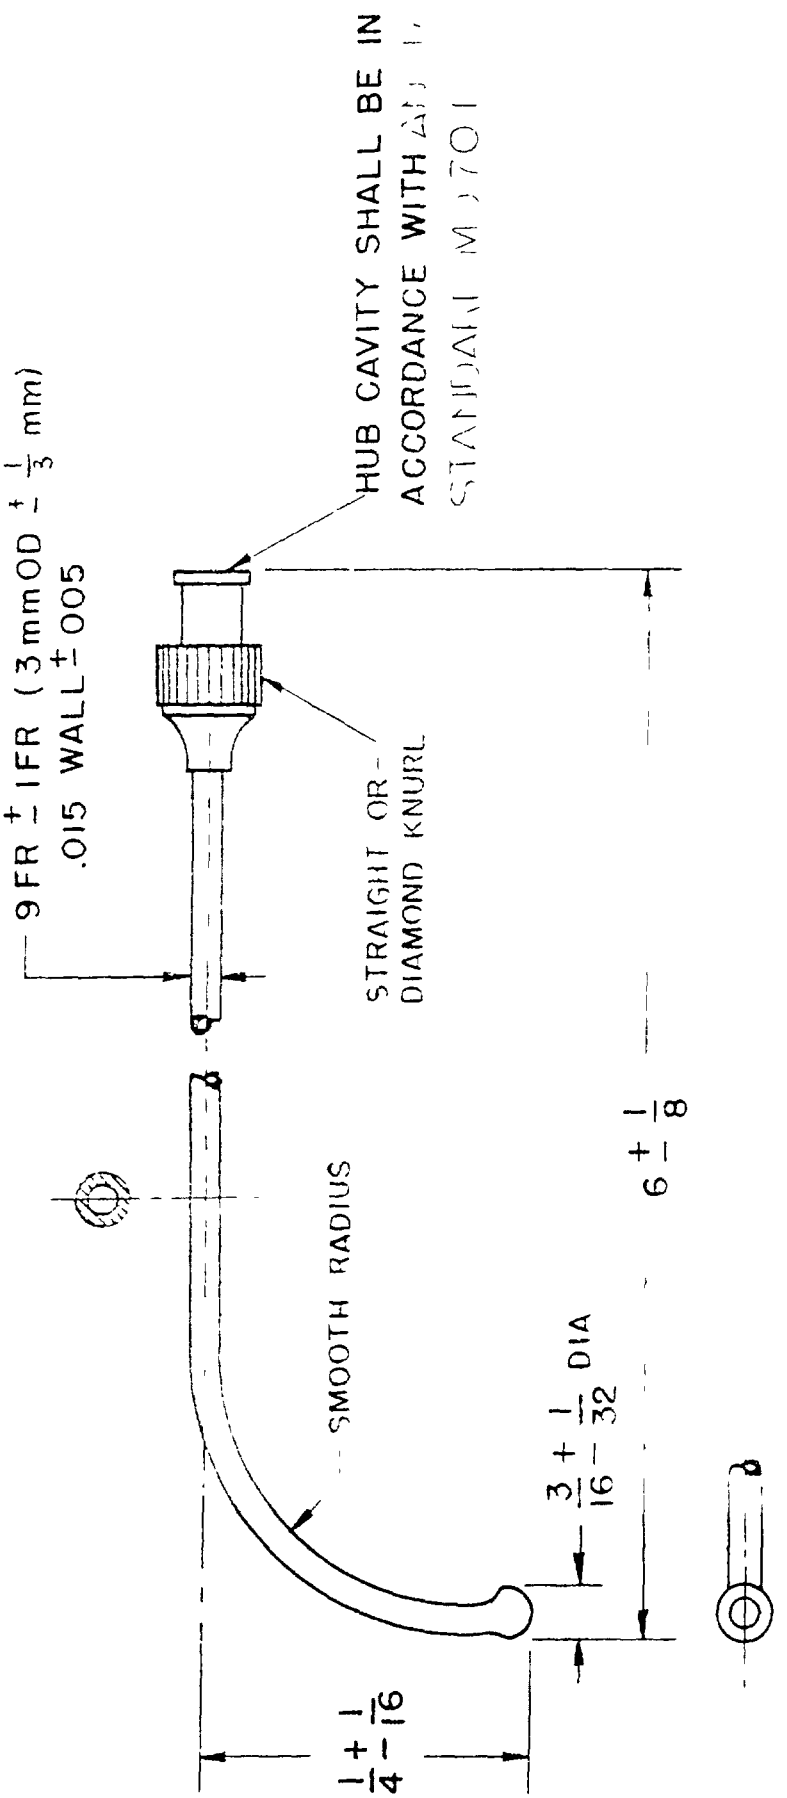


TYPE I

ARRAHAM DESIGN (FLEXIBLE TUBE)


FIG. 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

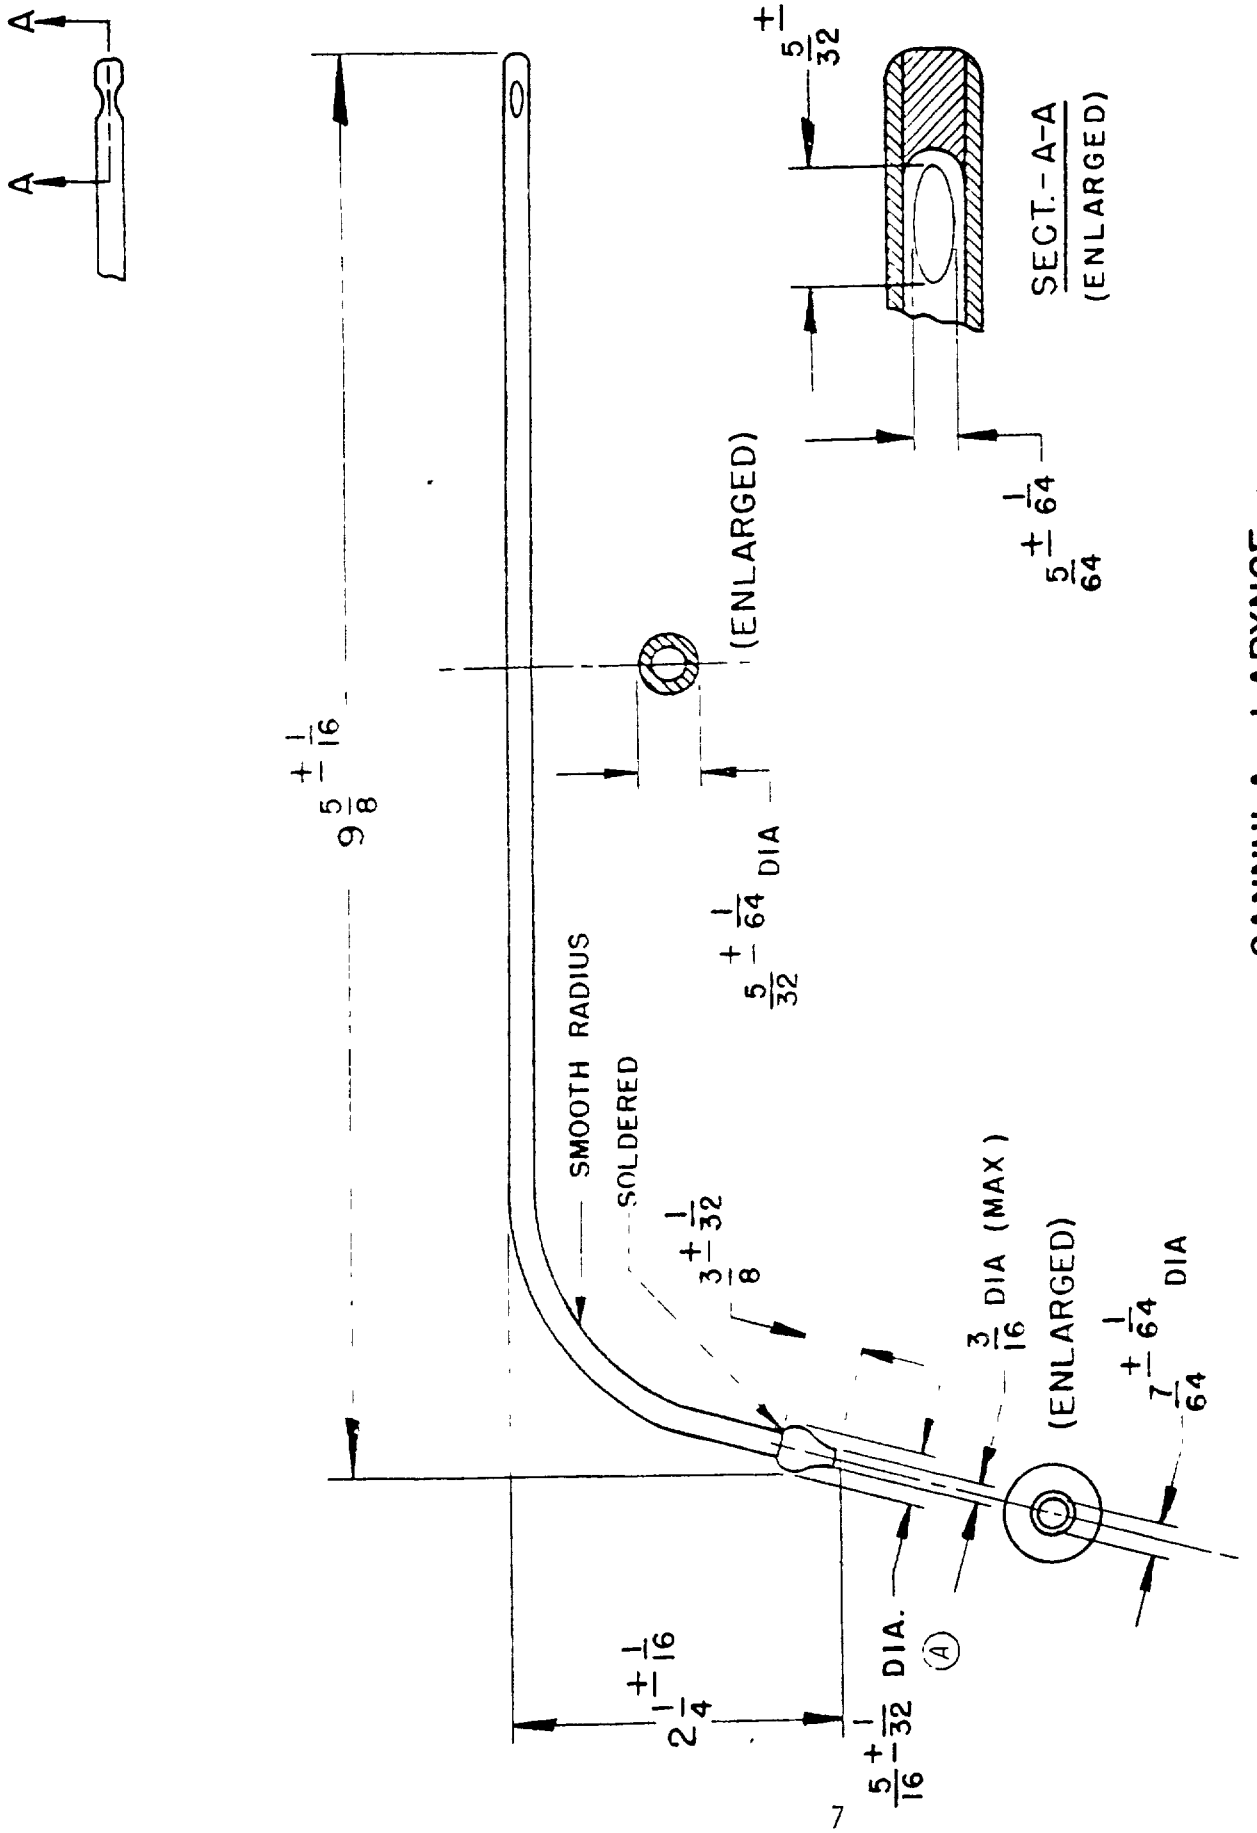

CANNULA, LARYNGEAL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

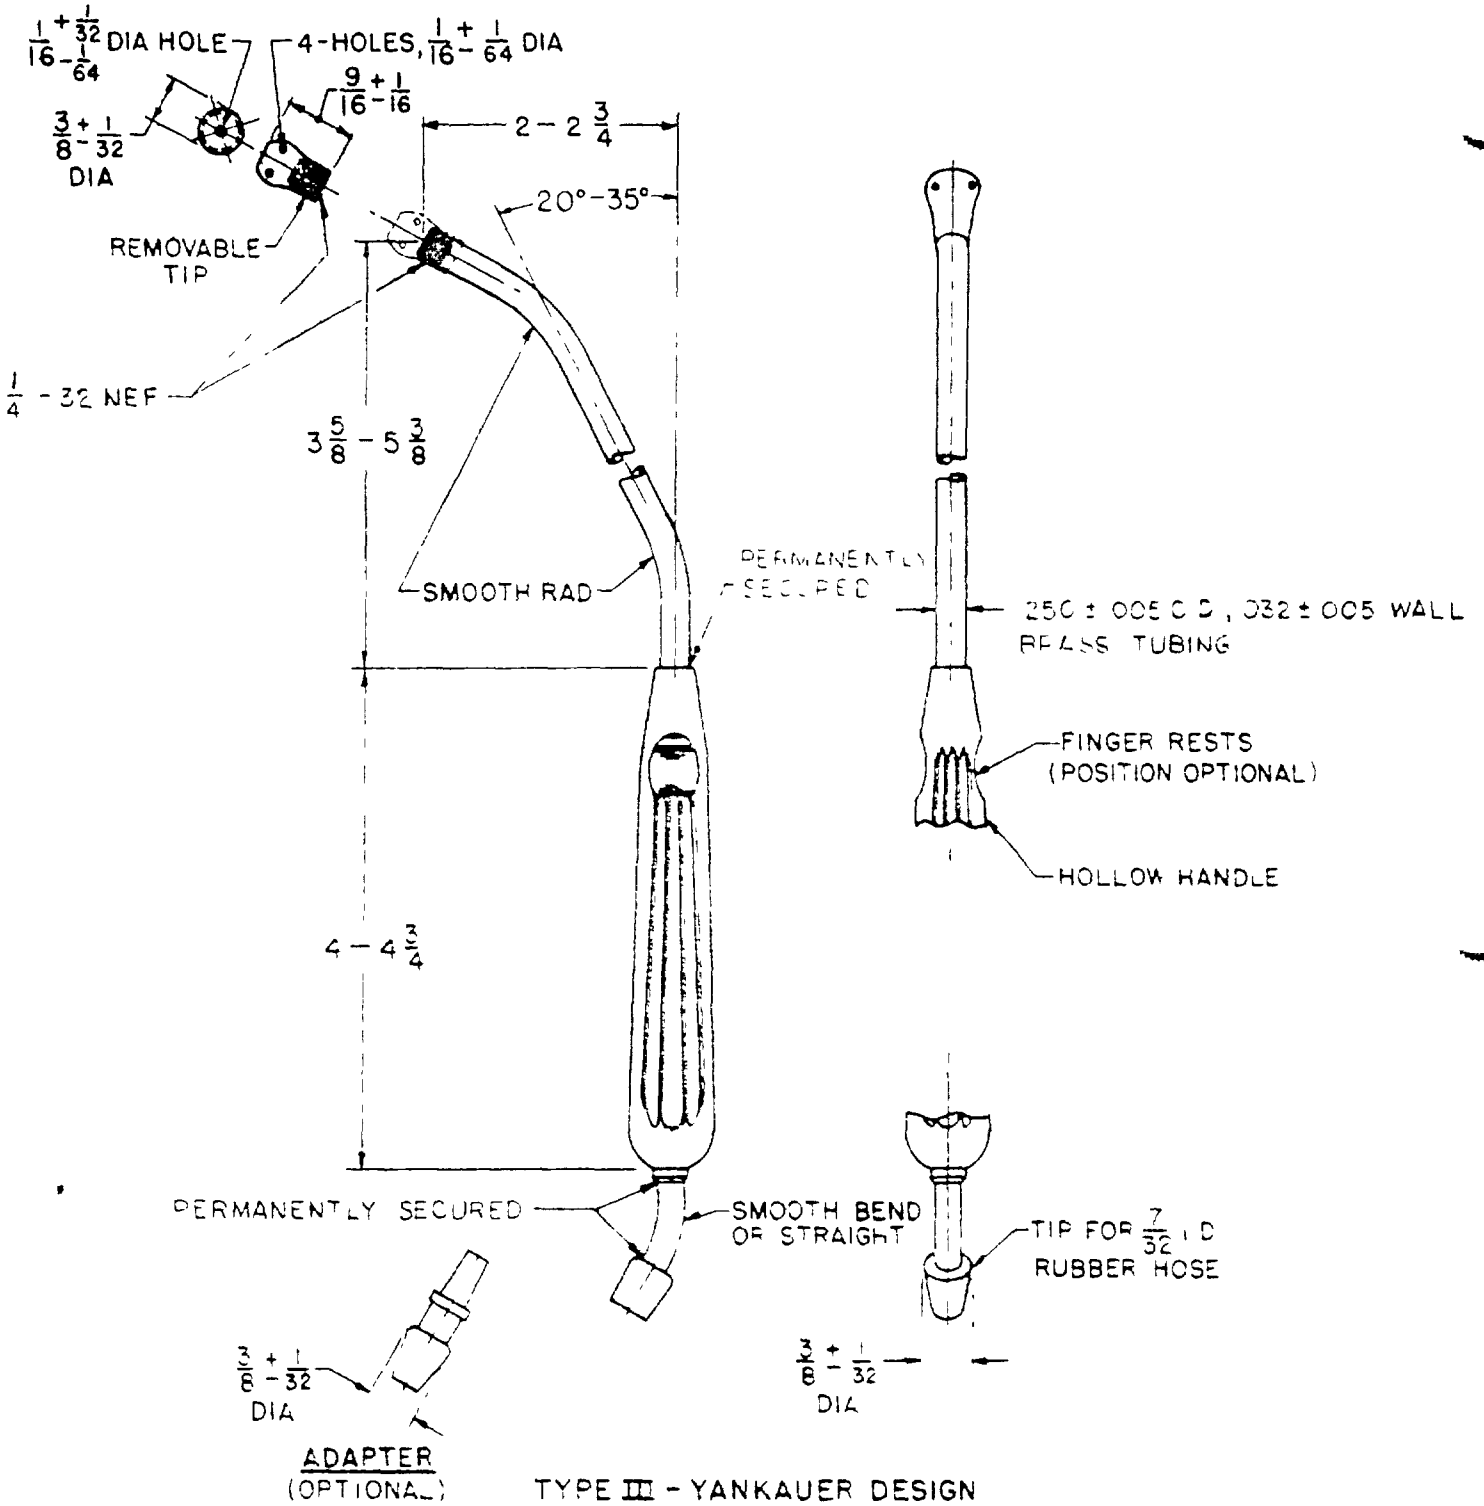

TYPE III - YANKAUER DESIGN SUCTION TUBE

FIG 3

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.