A-A-51330
14 March 1986

COMMERCIAL ITEM DESCRIPTION

BLOOD PLATELET ADMINISTRATION-POOLING SET

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers an administration or pooling "Y" set for transfusing blood platelets.

Salient characteristics:

General. Shall be a sterile, disposable administration or pooling "Y" set for transfusing blood platelets. The administration-pooling set shall consist of a "Y" plastic tubing assembly composed of plastic tubing, fittings and various components. The set shall be assembled as shown on Figure 1.

Materials. The tubing shall be fabricated from polyvinyl chloride. The connecting spike shall be fabricated of acrylonitrile-butadiene-styrene terpolymer. The "Y" connector shall be fabricated of polyvinylchloride. The mal and female Luer lock adapters, female Luer lock cover and needle adapter protecto shall be fabricated of a suitable plastic.

Style and design. The tubing shall have a nominal ID of 0.125 inches with a nominal wall of 0.032 inches. Shore A durometer shall be 80 ± 3 as measured by ASTM D-2440, 10 seconds at 23°C.

The connecting spike piercing tip shaft effective length above protector seat shall not be greater than 1.05 inch to protect from piercing bag sidewall during use. Base diameter should provide tight leakproof seal with blood bag entry port diameter of 0.220 + .002 inch. Taper from cone tip to shaft transition to base should be smooth with no steps. The piercing tip shall have a conical design with three equally spaced (120°) slots to assure no blockage under suction. Smoothly rounded finger wings shall be provided for easy insertion or removal of the spike into or from the blood bag. The tubing connector shall have internal tubing connection to provide the most open lumen. Length of connection below the wings shall be long enough to provide adequate finger grip of 0.75 inches. A protector seat with a diameter greater than the base of the functional shaft shal be provided between the base of the shaft and finger wings.

The Luer taper and Luer locking engagements of the male and female Luer lock adapters shall meet the requirements of ANSI/HIMA MD70...

The "Y" connector shall have smooth, internal surfaces to minimize turbulance and flow resistance.

The filter screen shall fit tightly in the tubing and shall be composed of polyester monofilament with square weave of 200 mesh per inch, equivalent to 74 microns (± 10%) opening size. The effective filter shall be 3 square millimeters

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release, distribution is unlimited.
AMSC N/A

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

The needle adapter protector cover shall provide a cover to maintain security of the needle adapter end of the check valve prior to use and shall be easily removed without compromising the adapter. Contact with the needle adapter protector shall be by molded levels with a tortuous air path to permit priming the set without removal of the cover.

Performance. A plastic spike protector shall be provided to maintain security of the spike prior to use and shall be easily removable without compromising the spike.

Low volume disc check valves shall be provided to reduce fluid hold up and to assure rapid response to pressure changes. The free floating disc valve shall be open but shall close with reverse flow. The spring-loaded disc check valve shall be closed and shall open under 2 to 4 psi pressure. The hold up volume in each valve shall be 0.2 ml maximum.

The female Luer lock cover shall provide security of the female Luer adapter before use, but shall be easily removable without compromising the adapter.

The fluid path in the tubing and components and internal surfaces of covers shall be sterile, non-pyrogenic and non-toxic when tested in accordance with the United States Pharmacopeia (USP). The tubing, covers and components in direct contact with the blood or fluid flow shall meet the requirements of the USP for Class IV plastics.

Workmanship. The blood platelet administration pooling set shall be free from defects which detract from its appearance or impair its serviceability.

PRODUCT QUALITY LEVEL

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with the requirements specified.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with the requirements specified.

Unit. Package (PG). One package containing forty-eight blood platelet administration-pooling sets, each set individually packaged in a container capable of maintaining sterility of fluid path, as specified, constitutes the unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one blood-platelet administration-pooling set.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or comments thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	Item Identification
6515-01-139-9158	BLOOD PLATELET ADMINISTRATION-POOLING SET, Disposable, 48s: Sterile

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:

VA-OSS

PGC 58363

Project No. 6515-3356

Location S1-10-28

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

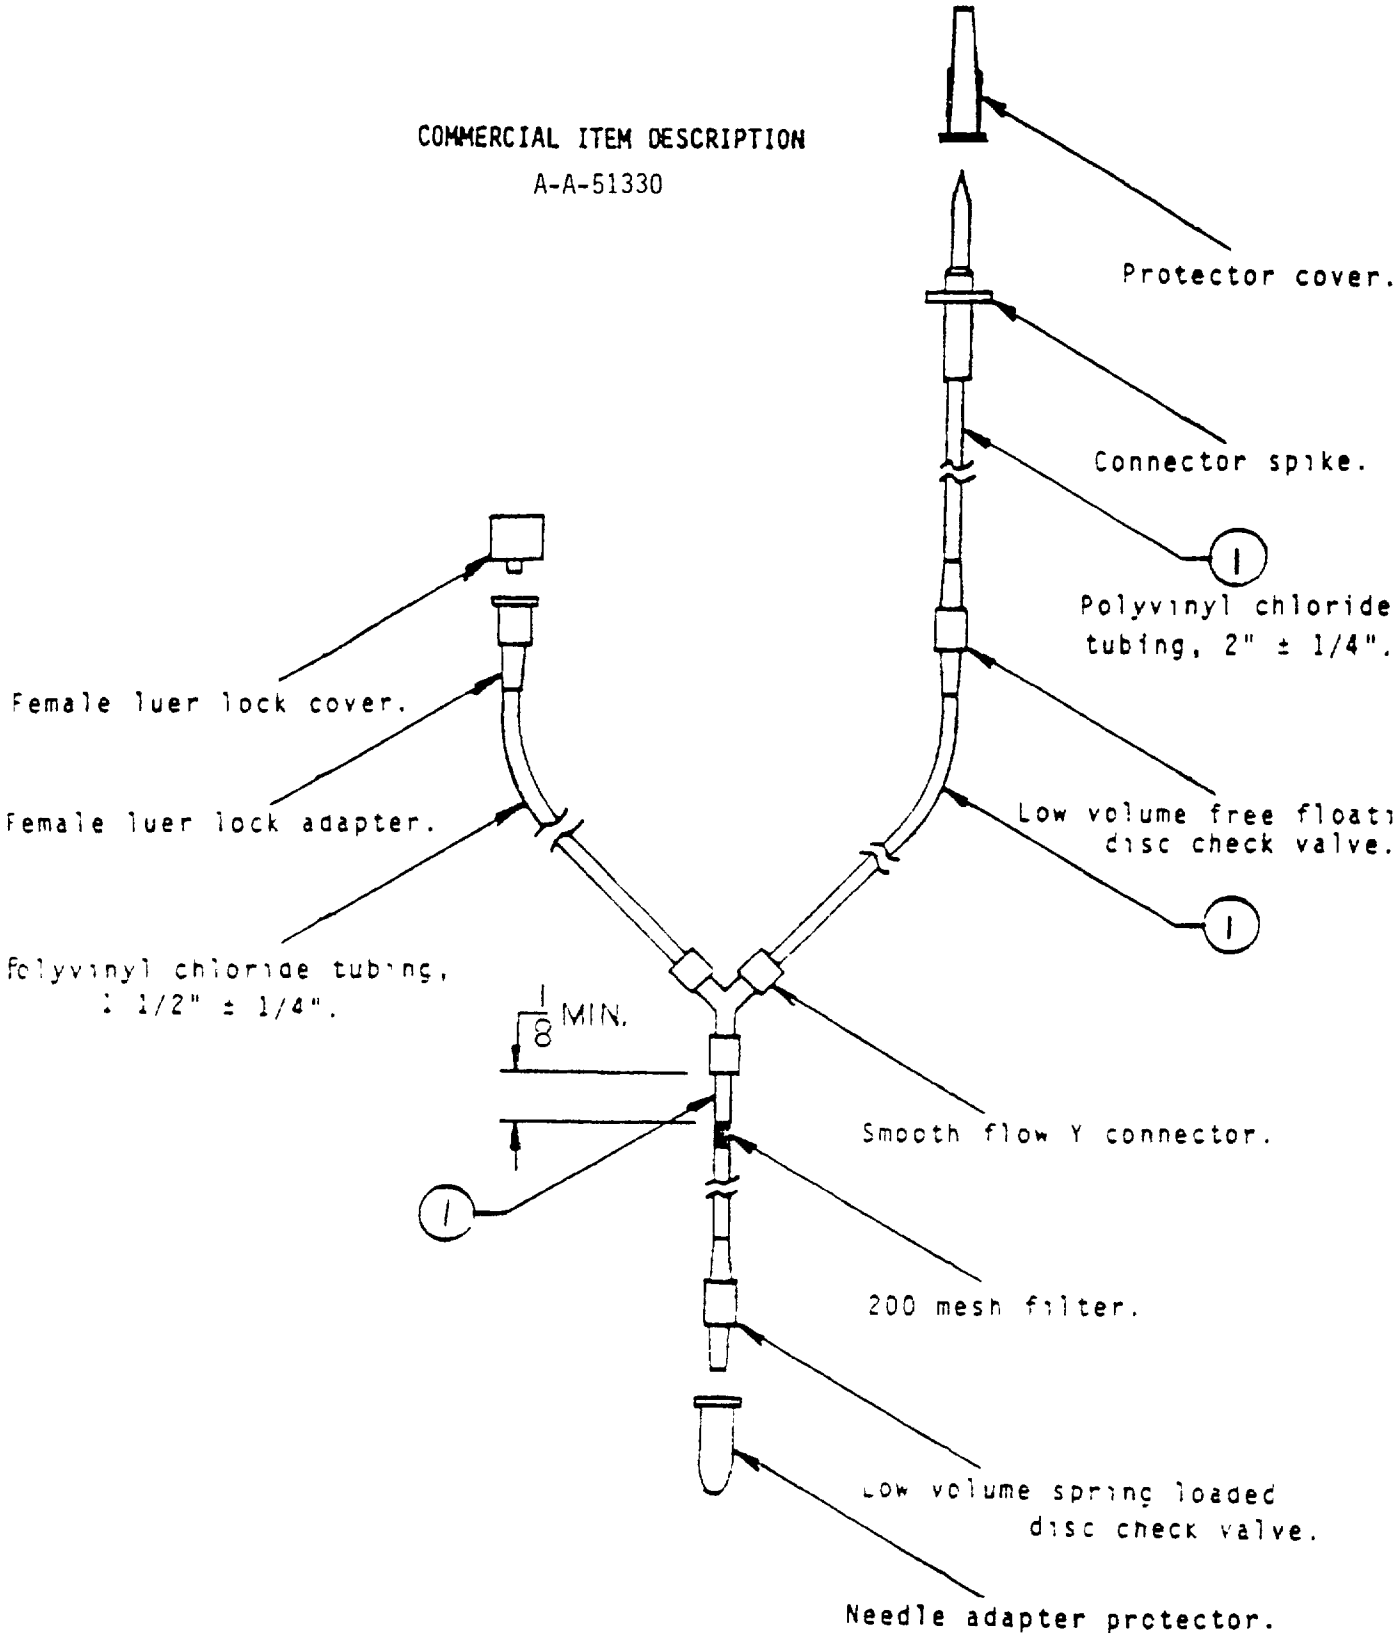


FIGURE 1

Blood Platelet, Administration-Pooling Set

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.