MIL-A-36051A
11 July 1973
SUPERSEDING
MIL-A-36051
18 May 1961

MILITARY SPECIFICATION

ANOSCOPE, HIRSCHMAN

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers anoscopes of the Hirschman design, suitable for use in proctological procedures.

* 1.2 Anoscopes shall be of the following sizes, as specified (see 6.1).

Size 1 - Medium (3/4 inch O.D.)
Size 2 - Small (5/8 inch O.D.)

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Boxes, Fiberboard.
PPP-B-676	Box, Setup.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case, and Sheet Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENT

3.1 General Requirements. The anoscopes shall be in accordance with the applicable requirements of GG-I-526 and the following option exercises under that specification:

3.2 Material. The anoscope shall be fabricated of Class 3, Type 304 material, except, that the obturator assembly, as an alternate, may be fabricated from Class 3, Type 303.

3.3 Hardness. Rockwell hardness shall be B-75 minimum.

3.4 Style, design and dimensions. Shall be an anoscope of the Hirschman design, complete with handle and obturator, and suitable for use in proctological procedures. Shall be in accordance with Figure 1. Handle to cannula and obturator joints shall be permanently secured by silver soldering or brazing.

3.5 Finish. Finish shall be mirror, except for handle, obturator knob and stem which may be satin.

3.6 Passivation. The entire anoscope shall be properly passivated.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

3.7 Identification marking. Each anoscope shall be permanently and legibly marked in accordance with the requirements of Specification GG-I-526. In addition to GG-I-526 requirements, instruments of foreign manufacture shall also be marked "stainless". Also, each anoscope shall be permanently and legibly marked with abbreviated size designation (M for medium and S for small) and matched pair coding as shown in Figure 1.

3.8 Workmanship. Workmanship shall be first class throughout. Anoscopes shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS


4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

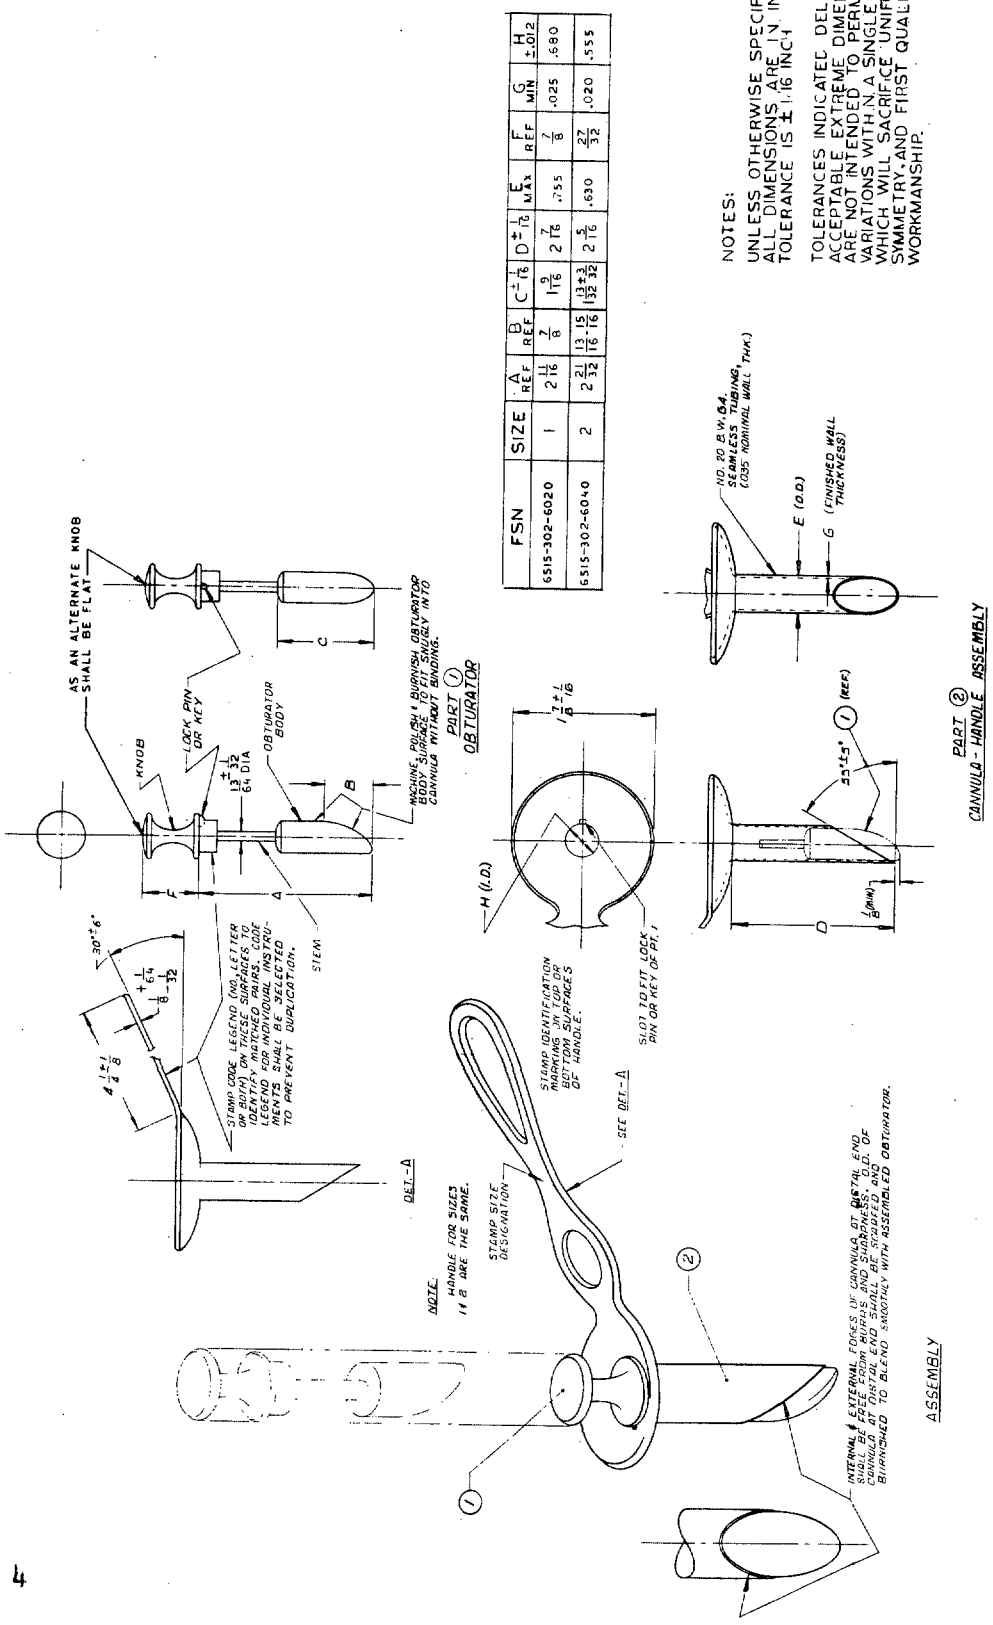

ANOSCOPE-HIRSCHMAN

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in Table I. The unit of product for examination purposes shall be one anoscope.

Table I. Sampling Criteria for Examination

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. The unit of product for test purposes shall be one anoscope.

Table II. Sampling Criteria for Tests

Component	Characteristic	Requirement	Test procedure	Inspection level	AQL
Anoscope	Composition analysis	3.2 and GG-I-526	GG-I-526	*	
	Hardness	3.3 and GG-I-526	GG-I-526	S-2	2.5
	Dimensions	3.4	-	S-2	2.5
	Boil Test	GG-I-526	GG-I-526	S-2	2.5

* Four ounces of each lot of metal used in the construction of the anoscope shall be selected for chemical analysis.

4.3 Examination. The anoscope shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in Tables I and III. Examination, however, shall not be restricted to defects listed in Table III. Any anoscope in the sample containing one or more defects shall be rejected and if the number of defective items in the sample exceeds the acceptance number for that sample, the lot represented by the sample shall be rejected.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects.

Categories	Defects
Critical	None defined.
Major	
101	Matched pair coding on handle and obturator not present, not legible or not permanent.
102	Size marking (M or S) not present or not correct for stock number under consideration.
103	Edges and corners of component parts not free from burs and sharpness.
104	Component parts not free from cracks.
105	Obturator fails to fit smoothly, easily and snugly within the cannula (without excess clearance).
106	External surface of cannula and tip of obturator not mirror finish, smooth and free from surface roughness.
107	Tip of obturator fails to protrude beyond the end of the cannula (in assembled position).
108	Obturator tip fails to properly align with beveled distal end of the cannula (in the assembled position).
109	Handle alignment with respect to truncated distal end of cannula not correct (see Figure 1).
110	Joints not secure and/or not properly silver soldered or brazed.
111	Soldered or brazed joints and adjacent surface not free of flux.
112	Finish not free from coarse grind marks or excessively scratched surfaces.
Minor	
201	Finish not mirror or mirror and satin.
202	Identification marking not present, legible and permanent (except matched pair coding and size marking).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be Level A or C as specified (see 6.2).

5.1.1 Unit of issue. One anoscope as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	48 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Preservative shall not be applied.

5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive material.

5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method 1C-2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-566, PPP-B-676 or PPP-B-636, class domestic. Commercial colors are acceptable on intermediate cartons and closure shall be adequate to prevent spilling of contents under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3c. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.1.2 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard box shall be waterproof in accordance with paragraph 30.4 of PPP-B-636.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Fiberboard box shall be closed by method II of PPP-B-636. Special requirements of applicable table shall apply for PPP-B-636 box.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

5.3.1 Interior packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The anoscopes are intended to facilitate examination and treatment of the rectum.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Size required (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 This specification is intended to cover the following items appearing in the Federal supply Catalog:

National Stock No.	Item Identification
6515-00-302-6020	ANOSCOPE, Hirschman, Medium
6515-00-302-6040	ANOSCOPE, Hirschman, Small

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

Custodians:
Army - MD
Navy MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1747

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.