MIL-D-36140A
25 September 1967
SUPERSEDING
MIL-T-36140(BuMed)
13 March 1963

MILITARY SPECIFICATION

DRAIN, SURGICAL RUBBER, T-TYPE

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers sterile and nonsterile drains suitable for use in surgical drainage of the ureter or gall bladder.

1.2 Classification. Drains shall be of the following sizes as specified:

Size 12 - 12 French
Size 14 - 14 French
Size 16 - 16 French
Size 18 - 18 French
Size 22 - 22 French

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

MMM-A-250	Adhesive, Water Resistant, for Sealing Fiberboard Boxes.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-Up, Paperboard.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper (for Carton Sealing).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

Fed. Test Method Std. No. 601 Rubber; Sampling and Testing.

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. Drains shall be natural latex containing not less than 90 percent rubber hydrocarbon by volume, when tested as specified in 4.4.1.

3.2 Design and construction. Drains shall be fabricated in the form of a 'T', shall be fabricated without seam or joint, and shall be in accordance with figure 1.

3.3 Accelerated aging and breaking strength. Drains shall not become brittle or tacky when tested as specified in 4.4.2. Tubes shall not decrease in breaking strength and ultimate elongation by more than 25 percent, when tested as specified in 4.4.3.


3.4 Sterility. Drains shall be sterile when tested for sterility as specified in 4.4.4.

3.5 Safety (nontoxicity). Drains shall be safe (nontoxic) when tested for safety as specified in 4.4.5.

3.6 Identification marking. Each drain shall be legibly and permanently marked with name of manufacturer or registered trademark, French size, and date of manufacture (year, month). Sterile drains shall be marked accordingly.

3.7 Workmanship. Workmanship shall be first class throughout. Drains shall be free from defects which detract from their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.

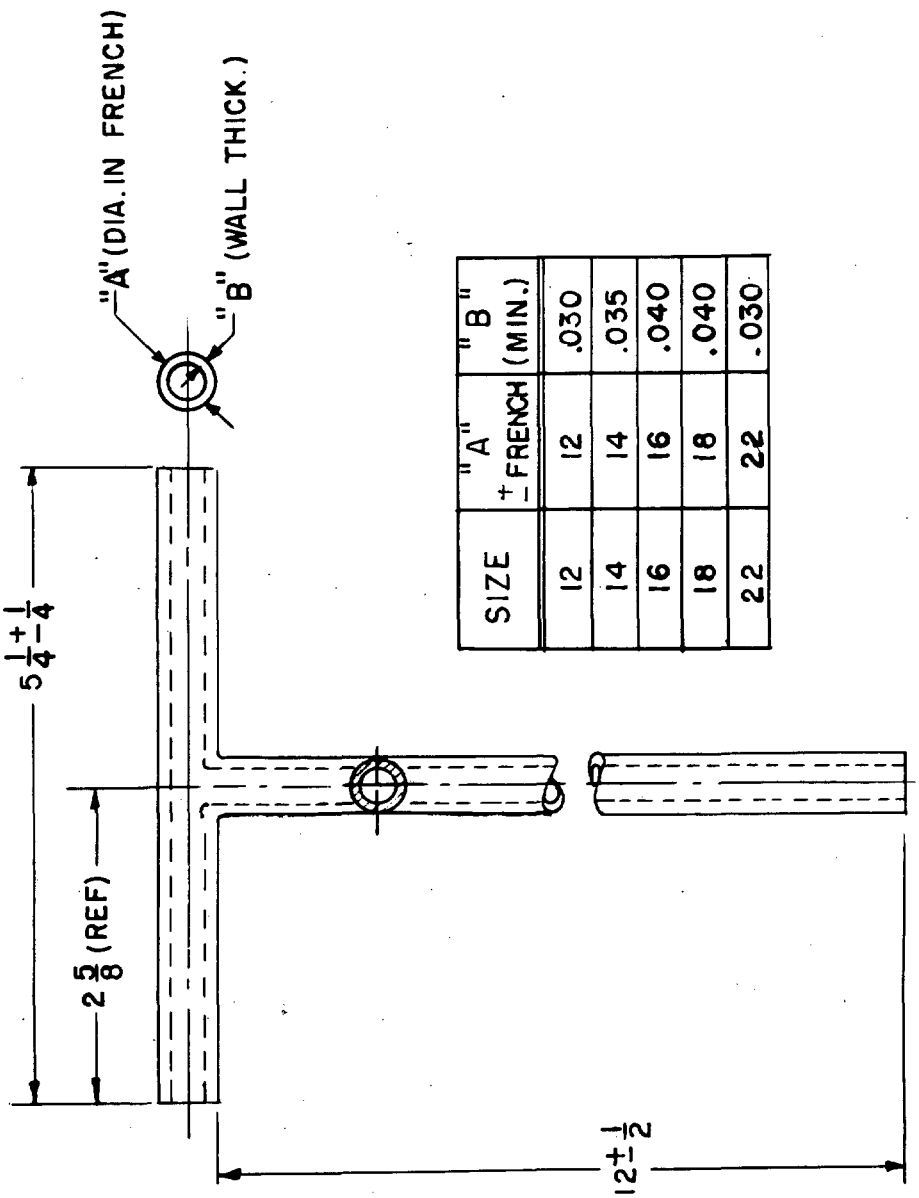

SIZE	"A" ± FRENCH	"B" (MIN.)
12	12	.030
14	14	.035
16	16	.040
18	18	.040
22	22	.030

FIGURE 1. SURGICAL RUBBER DRAINS, T-TYPE

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.

3.8 Certificates of sterility and safety tests. Where applicable, a certificate listing all lot or control numbers, shall state that representative sample from each lot or control have been tested and found to be sterile and have passed the safety test. This certificate shall include specific tests performed and the test results. For destination inspection only, one copy of certificate shall be submitted by the destination inspection only, one copy of certificate shall be submitted by the contractor directly to the Chief, Quality Control and Maintenance Division, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, Code ATQ, 2800 South 20th Street, Phila. Pa. 19101, and one copy shall be forwarded with each shipment to the consignee.

3.9 Manufacturer's record. Where applicable, the manufacturer shall place a code or lot number, on the paper label or on the printed carton, which can be verified against the manufacturer's records of all tests made on nontoxic sterile drains. These records shall be made available for inspection by any duly authorized Government representative. No shipment shall be made until all tests shave been completed, verified, and recorded in the permanent records of the manufacturer.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facility or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to insure that supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be in accordance with MIL-STD-105.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.

4.2.2 For tests.

4.2.2.1 Percent rubber hydrocarbon. Sufficient samples shall be taken from each lot to perform the test. Failure of any sample to comply with test requirements shall be cause for rejection of the lot represented.

4.2.2.2 Accelerated aging. Sufficient samples shall be selected from each lot to perform the test. Failure to comply with test requirements shall be cause for rejection of the lot represented.

4.2.2.3 For sterility, and safety tests. Sampling procedures for sterility and safety tests shall be conducted as indicated in the current edition of the U.S.P., for transfusion and infusion assemblies.

4.2.3 Where possible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination. The tubes shall be examined to determine compliance with all requirements contained in this specification.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

4.4.1 Rubber hydrocarbon by volume. Test for rubber hydrocarbon shall be conducted in accordance with method 16111 of Federal Test Method Standard No. 601.

4.4.2 Accelerated aging test. Tubes shall be subjected to method 7221 of Federal Test Method Standard No. 601.

4.4.3 Breaking strength. The breaking strength and ultimate elongation shall be conducted in accordance with methods 4111 and 4121 of Federal Test Method Standard No. 601. In using method 4111 to determine the breaking strength, the value defined as 'breaking force' will be used as the value for breaking strength.

4.4.3.1 Specimens. For ultimate elongation and breaking strength tests, straight specimens shall be used.

4.4.4 Sterility tests. Drains shall be tested for sterility in accordance with the current edition of the U.S.P., for transfusion and infusion assemblies.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.

4.4.5 Safety test. Drains shall be tested for safety in accordance with the current edition of the U.S.P., for transfusion and infusion assemblies.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One package (6 sterile tubes) or one nonsterile tube, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in the following table shall be packaged in each unit, intermediate, and exterior container as applicable, for the required level of protection specified in the procurement document.

Table I. Packaging Quantities

Size	Unit Package	Intermediate Package		Exterior Container	
		Nonsterile	Sterile	Nonsterile	sterile
12	1 unit	12 units	6 units	576 units	96 units
14	1 unit	6 units	6 units	144 units	48 units
16	1 unit	6 units	6 units	144 units	48 units
18	1 unit	6 units	6 units	144 units	144 units
22	1 unit	6 units	6 units	144 units	48 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Sterile tubes.

5.1.3.2 Individual container. Each unit shall be mounted on a substantial cardboard or plastic fitting and placed in a polyethylene bag or combination polyethylene and paperback, tear-type, envelope of appropriate size. Excess air shall be evacuated from the container and closure so as to maintain sterility until manually opened. The sealed container shall be designed so to permit ready dispensing of the T-type drain by sterile techniques.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.

5.1.3.3 Unit package. Unit package shall be a carton of appropriate size constructed in accordance with PPP-B-676, except that commercial colors will be acceptable. Closure shall be adequate to prevent accidental opening.

5.1.3.1.1 Nonsterile tubes.

5.1.3.1.2 Unit package. Each unit shall be packaged (not coiled) in a carton of suitable size and design or in a waxed or glassine envelope. Carton or envelope shall be secured to prevent accidental opening.

5.1.3.1.2.1 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2-inch wide tape conforming to PPP-T-76. Closing of bottom flap with ahdesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type I, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant. Closure and strapping shall be in accordance with appendix of applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic. Closure shall be in accordance with appendix of applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, constructed so as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Individual container (sterile). Labeling shall conform with the requirements of the Federal Food, Drug and Cosmetic Act, in addition, marking shall bear the following:

(a) Instructions describing the proper sterile techniques for dispensing the T-tube from the container.

(b) Identification of the T-tube as to length of cross bar and French size.

(c) Contractor's name or trademark.

(d) The legend "Sterile".

5.3.2 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.3 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.

(b) Selection of applicable levels of packing (see 5.1 and 5.2).

6.2 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet Military requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

CATEGORY: N

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

MIL-D-36140A

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 68 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
AUG 66

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.