MIL-P-36073A (DSA-DM)
18 May 1971
SUPERSEDING
MIL-P-36073 (BUMED)
17 July 1961

MILITARY SPECIFICATION

PAD HOSPITAL STRETCHER

This specification is mandatory for use by all Departments and Agencies.

1. SCOPE

1.1 This specification covers one type of latex foam rubber hospital stretcher pad with a removable cover of double coated, electrically conductive, rubber sheeting.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

V-F-106	Fasteners, Slide, Interlocking.
V-T-276	Thread, Cotton.
V-T-295	Thread, Nylon.
ZZ-C-450	Cloth, Coated (Rubber and Plastic) and Plastic Sheeting (Rolls), for Hospital Use.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

Military

MIL-R-5001	Rubber; Latex Foam Sponge.

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

Fed Std 751	Stitches, Seams and Stitching.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications, standards, and drawings, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

NATIONAL FIRE PROTECTION ASSOCIATION (NFPA)

No. 56	Flammable Anesthetics

(Application for copies should be addressed to National Fire Protection Association, 60 Batterymarch Street, Boston, Mass. 62110).

3. REQUIREMENTS

3.1 Material.

3.1.1 Rubber sheeting. Rubber sheeting shall be double coated material conforming to ZZ-C-450 for type I, and shall have electrical resistance not exceeding one megohm when tested as specified in 4.3.1. Sheeting shall be from 0.015 inch to 0.020 inch thick. Color shall be black.

3.1.2 Latex foam rubber. Latex foam rubber shall conform to Specification MIL-R-5001 for type I, medium, grade C, 1-1/2 inches thick.

* 3.1.3 Cotton thread. Thread for all stitching shall be nylon conforming to V-T-295 for Type III, Size 2, black.

3.1.4 Slide fastener. Slide fastener shall conform to Specification V-F-106 for type I, style 6, without lock, bridge top stop, closed bottom stop, size L, single slider, single pull, short tab pull. Metallic parts shall be brass or aluminum alloy 568 finished in (d) or (f) finish, respectively. Tape shall be black.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.

* 3.2 Construction. The stretcher pad shall be in strict accordance with figure 1. The pad shall be of foam rubber and shall have a removable cover of rubber sheeting. The cover shall encase the foam rubber neatly and smoothly. The cover shall be provided with a slide fastener extending the full length of the pad on one side to permit easy removal of the rubber pad. The slide fastener shall be attached with double stitching. As an alternate to figure I construction, the cover shall be a four-piece construction as follows:

A one-piece top panel.
A one-piece bottom panel.
A one-piece border extending around two ends and along one side.
A closure section including the slide fastener extending along the other side.

All seams shall be turned in, and the slide fastener shall be attached with double stitching.

* 3.2.1 Stitching, Seams, and Stitches. All stitching shall be by machine. Stitches shall conform to type 301 of Fed Std 751. There shall be 6 to 8 stitches per inch. Seams shall be as shown in figure I.

* 3.3 Identification marking. Each pad shall bear the manufacturer's name or registered trademark, and contract or purchase order number, printed or stenciled in black indelible ink on a cloth label permanently attached to the underside of the pad.

* 3.4 Workmanship. Workmanship shall be first class throughout. The pads shall be free from defects which detract from their appearance or may impair their serviceability. Uncoated areas of rubber sheeting less than 1/8 inch by 1/16 inch in area, occuring only on the inside of the cover as a result of the manufacturing process, shall be considered acceptable.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, and auditory, investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the foam rubber, thread and sheeting, may be furnished by the contractor for the pads in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the component or material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and Table I.

Table I. Sampling for Examination*

	Inspection level	AQL (defects per hundred units)
For visual examination		
Major defects	II	1.0
Minor defects	II	2.5

* Acceptance number shall be zero. Not less than three samples shall be taken regardless of lot size.

4.2.2 Components. Sufficient samples of components shall be selected to perform the tests specified in 4.4.2.

4.2.3 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as shown in Table II.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.

Table II. Sampling for Tests

Component Unit of product	Characteristic	Req.	Test procedure	Insp. level	AQL (percent defective)
Rubber, Sheeting, thread fasteners, latex foam	Conductivity	3.1.1	4.3.1	S-1	*
	Physical properties	3.1.1; 3.1.2; 3.1.3; 3.1.4	4.3.2	S-1	*

*Acceptance number shall be zero, and not less than three samples shall be taken.

4.2.4 Classification of defects. Examination shall be conducted in accordance with the following classification of defects as shown in Table III.

Table III. Categories and Defects

Categories	Defects
Major	
101	Foam rubber not free of tears.
102	Foam rubber not free of malformations affecting serviceability.
103	Rubber sheeting not free of cuts, tears, and holes.
104	Slide fastener does not open and close fully; not free of jamming.
105	Slide fasteners not free of sharp edges.
106	Stitching not free of breaks and open seams.
107	Material not free of objectionable odor.
108	Rubber sheeting not free of uncoated areas greater than 1/8 inch by 1/16 inch.
109	Rubber sheeting not free of peeling, blisters, cracks, and pits.
Minor	
201	Rubber sheeting not free of dirt or grease.
202	Seam not the type(s) specified.
203	Seam twisted or not neatly pleated.
204	Number of stitches per inch not as specified (check both seam types carefully).
205	Rubber sheeting not free of needle chews.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.

Table III. Categories and Defects (Cont'd.)

206	Sheeting not free of raw edges at seam.
207	Thread ends not trimmed.
208	Covering puckered, loose.
209	Identification marking not present, not legible, not complete, not as specified.
210	Stitch type not 301.
211	Pad not free of seams not specified.

* Examination shall not be restricted to the classified possible defects listed above.

4.3 Tests. Tests shall be conducted, as specified herein, to determine compliance with specification requirements.

4.3.1 Conductive rubber. Test for electrical conductivity shall be conducted as described in section 2541 of NFPA No. 56.

4.3.2 Components. Rubber sheeting, latex foam rubber, cotton thread, and slide fasteners shall be tested in accordance with the test procedures outlined in their respective specifications.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One pad, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	6 units

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Unit package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling. Prior to placing into the box, each pad shall be rolled or folded in such a manner as to insure against damage to the pad.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.

6. NOTES

* 6.1 Intended use. The hospital stretcher pad is intended for replacement use with Federal Stock Number 6530-792-4605, STRETCHER, Hospital, Wheeled, Corrosion-Resisting Steel.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packing (see 5.1 and 5.2).

6.3 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

* 6.4 This specification covers the following item appearing in the Federal Supply Catalog:

Item	FSN
Pad, Hospital Stretcher	6530-687-8410

* 6.5 The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

Custodians:
Army - MD
Navy - MS
Air Force - 03


Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6530-1192

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.

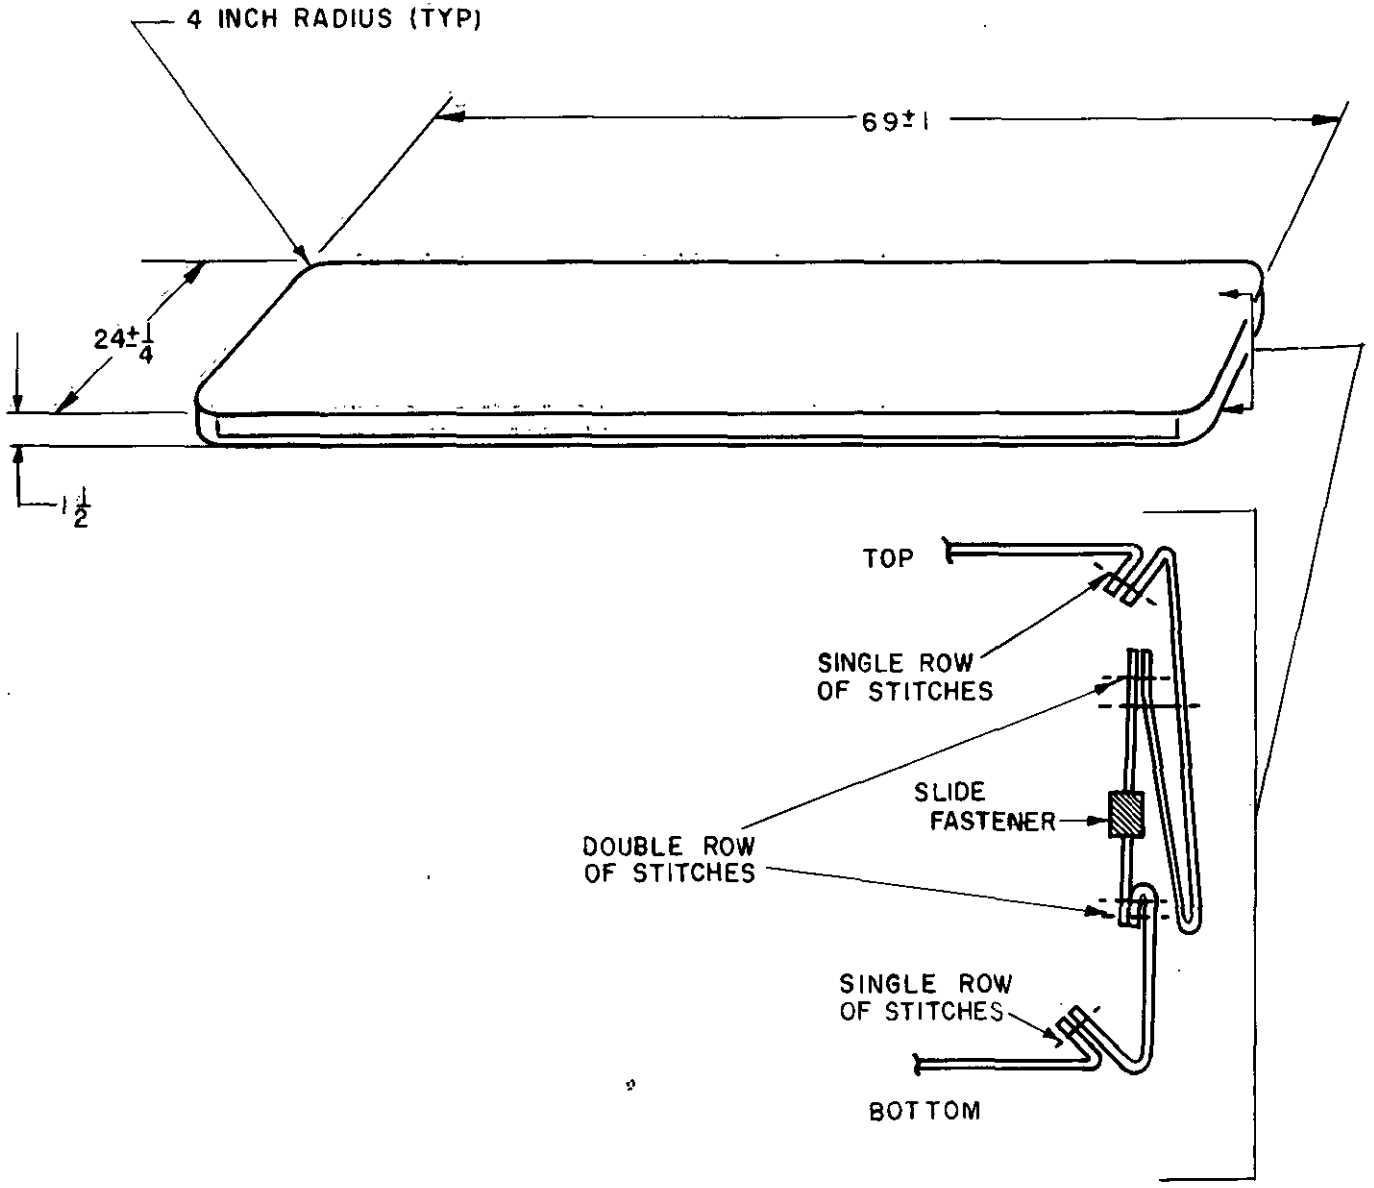

PAD HOSPITAL STRETCHER

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements.

SPECIFICATION

MIL-P-36073A (DSA-DM)

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 66 1426

REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:04Z
Check the source to verify that this is the current version before use.