MIL-R-36052A
10 October 1968
SUPERSEDING
MIL-R-36052
18 May 1961

MILITARY SPECIFICATION

RETRACTOR, VAGINAL, SIMS

This specification is mandatory for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 This specification covers one type of medium sized Sims vaginal retractor, suitable for use in gynecological examination and operative procedures.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids, form a part of this specification to the extent specified herein:

SPECIFICATIONS

* Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.

Military

MIL-P-116	Preservations, Methods of.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.

(Copies of specifications and standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

* 3.1 Material. The retractors shall be fabricated of class 3, composition 302, 303, and 304 material in accordance with Specification GG-I-526, Rockwell hardness shall be B75 minimum.

3.2 Style, design, and dimensions. Retractor shall be of the Sims design, suitable for use in gynecological surgery. Style, design, and dimensions shall be in accordance with figure 1.

3.3 Finish. Finish shall be mirror, or mirror and satin in accordance with Specification GG-I-526.

* 3.4 Identification marking. Instruments made in U.S.A. shall be marked with the name or registered trademark of the contractor, "stainless". Instruments of foreign manufacturer shall be marked with the name of the country of origin, "stainless", and name or registered trademark of the contractor.

3.5 Additional requirements. Except as specified herein, the retractors shall comply with the applicable requirements and tests of Specification GG-I-526.

3.6 Workmanship. Workmanship shall be first class throughout. Retractors shall be free from defects which detract from their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

Table I. Sampling Criteria

Component	Characteristic	Req.	Test procedure	Unit of product	Insp. level	AQL(percent defective
Retractor (end item)	Hardness	GG-I-526	GG-I-526	1-retractor	S-3*	**
	Boil test	GG-I-526	GG-I-526	1-retractor	S-3*	**
	Dimensions	3.2	-------	1-retractor	S-3	4.0

* A minimum of three units shall be tested regardless of lot size.
** Acceptance number shall be zero for all sample sizes.

4. QUALITY ASSURANCE PROVISIONS

4.1 Supplier responsibilities for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own or any other inspection facilities and services acceptable to the Government. Inspection records of the examination and test shall be kept complete and available to the Government as specified in the contract or order. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling for lot acceptance.

* 4.2.1 Inspection lot. The inspection lot shall be determined in accordance with MIL-STD-105.

4.2.2 Sampling for examination. A random sample of retractors shall be selected from each lot offered to the Government in accordance with MIL-STD-105. Examination for dimensions shall be in accordance with MIL-STD-105, and as indicated in table I.

4.2.3 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table I.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

4.2.4 Raw materials. Four ounces of each lot of metal used in the construction of the retractor shall be selected for chemical analysis.

4.2.5 Sample unit usage. Where possible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination. The retractor shall be examined to determine compliance with all requirements contained in this specification.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One retractor, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in the following table shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table II. Packaging quantities

Unit package	Intermediate package	Exterior container
1 unit	Not required	48 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

* 5.1.3 Level A.

* 5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

* 5.1.3.2 Preservative. Not required.

* 5.1.3.3 Intimate wrap. Each unit shall be wrapped in neutral tissue or other suitable anticorrosive materials.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

* 5.1.3.4 Unit package. Each unit shall be packaged in accordance with MIL-P-116, method 1A-15.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

* 5.2 Packing.

5.2.1 Level A.

* 5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-601, table III, using type I, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant. Closure and strapping shall be in accordance with appendix of applicable box specification.

5.2.2 Level B.

* 5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load and constructed in accordance with PPP-B-621, table I; or PPP-B-636, type CF, class domestic. Closure shall be in accordance with appendix of applicable box specification.

* 5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

* 5.3 Marking.

* 5.3.1 Interior packages. Each unit package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

6.2 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.

6.3 Transportation description. Transportation description applicable to this item is:

Surgical instruments NOIBN in boxes.

Carload minimum weight 10,000 pounds subject to Rule 34 of the Uniform Freight Classification.

Truckload minimum weight 10,000 pounds per National Motor Freight Classification.

Notice. When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

* Note: The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.


Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation shall be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.

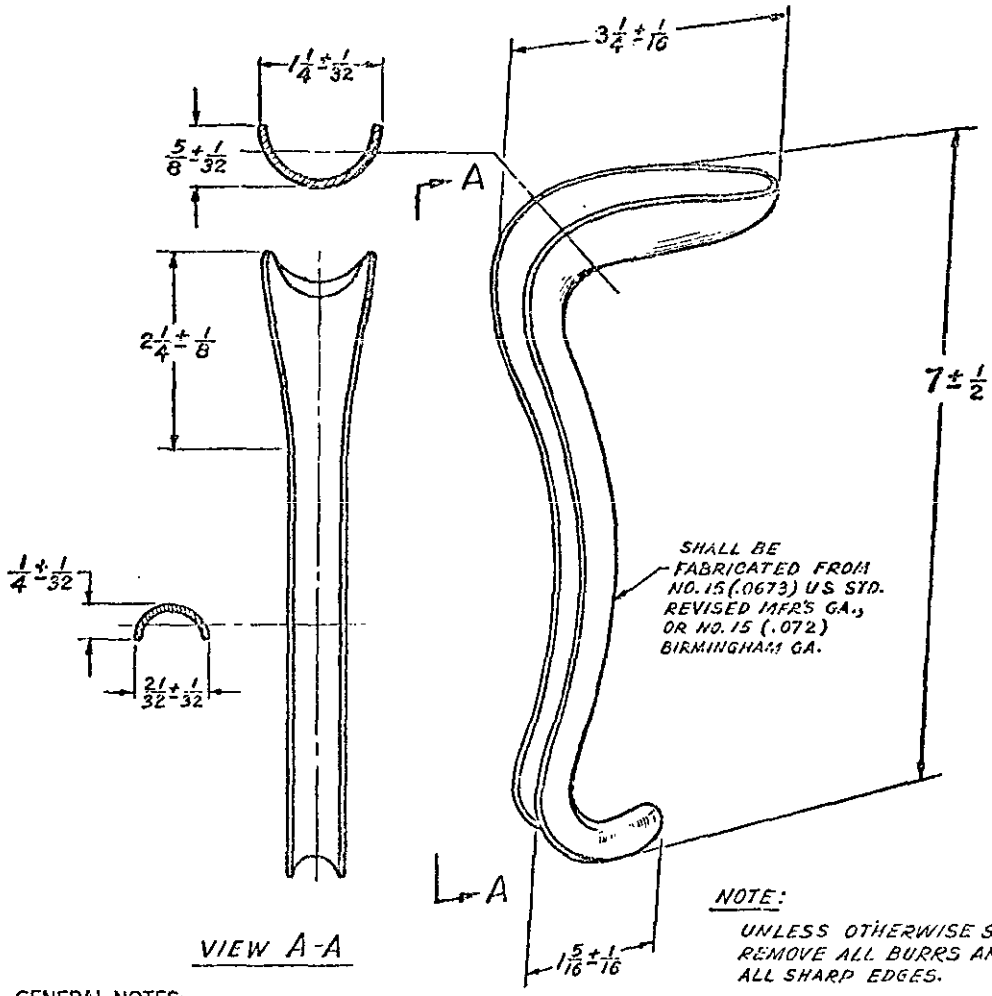

VIEW A-A

NOTE:

UNLESS OTHERWISE SPECIFIED. REMOVE ALL BURRS AND BREAK ALL SHARP EDGES.

DIMENSIONS ARE IN INCHES.

GENERAL NOTES:

TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP.

FIGURE I

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:01Z
Check the source to verify that this is the current version before use.