MILITARY SPECIFICATION

SPLINT ATTACHMENT, LEG, PEARSON

1. SCOPE

1.1 This specification covers a Pearson attachment for use in immobilization of fractures and treatment of injuries to the lower extremities of personnel.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids form a part of the specification to the extent specified herein:

SPECIFICATIONS

Federal

TT-C-490	Cleaning Methods and Pretreatment of Ferrous Surfaces for Organic Coatings.
TT-E-527	Enamel, Alkyd, Lustreless.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-Up, Paperboard.

Military

MIL-L-10547	Liners, Case, Waterproof.
MIL-P-8585	Primer Coating, Zinc Chromate, Low-Moisture-Sensitivity.

STANDARDS

Federal

Fed. Std. No. 66	Steel: Chemical Composition and Hardenability.
Fed. Std. No. 595	Colors.

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:07Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer).

3. REQUIREMENTS

3.1 Material

3.1.1 Rod. The rod portion of the attachment shall be fabricated of cold-rolled AISI 1042 or 1045 carbon steel, conforming to Federal Standard No. 66.

3.1.2 Other parts. All other parts of the attachment shall be fabricated of the highest grade material and suitable for the purpose intended.

3.2 Style, design and construction. The leg splint attachment shall be the Pearson type. A metal hinge shall be attached to each open end. The hinge shall be freely movable and shall lock the attachment to a fixed place on the side of a Thomas leg splint. The leg splint attachment shall be in accordance with figures 1, 2 or 3.

3.3 Finish.

3.3.1 Cleaning. Cleaning shall be accomplished as specified for type I in Specification TT-C-490.

3.3.2 Primer. After cleaning, all accessible surfaces shall receive a zinc-chromate primer conforming to color Y of Specification MIL-P-8585.

3.3.3 Enamel coating. Two coats of lustreless olive drab enamel conforming to Specification TT-E-527 and to color X34087 of Federal Standard No. 595, shall be applied after the priming (see 6.2). All enamel coats shall be sprayed on to accomplish a complete and uniform coverage of the coated parts, and shall be baked to give a smooth, hard and tough finish, which shall be free from runs and which shall resist cracking and chipping.

3.4 Identification marking. Attachment shall be permanently and legibly stamped with manufacturer's name or registered trademark.

3.5 Workmanship. Workmanship shall be first class throughout. Attachment shall be free from defects which detract from their appearance or may impair their serviceability. All edges and corners shall be rounded, ground smooth, or otherwise treated to eliminate burs and sharp or ragged edges. Any sharp edges or burs on rivets shall be removed. All rivets shall be securely set without any cracking of formed heads or malformation of rivet, and shall allow smooth working of the rotating hinge.

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:07Z
Check the source to verify that this is the current version before use.

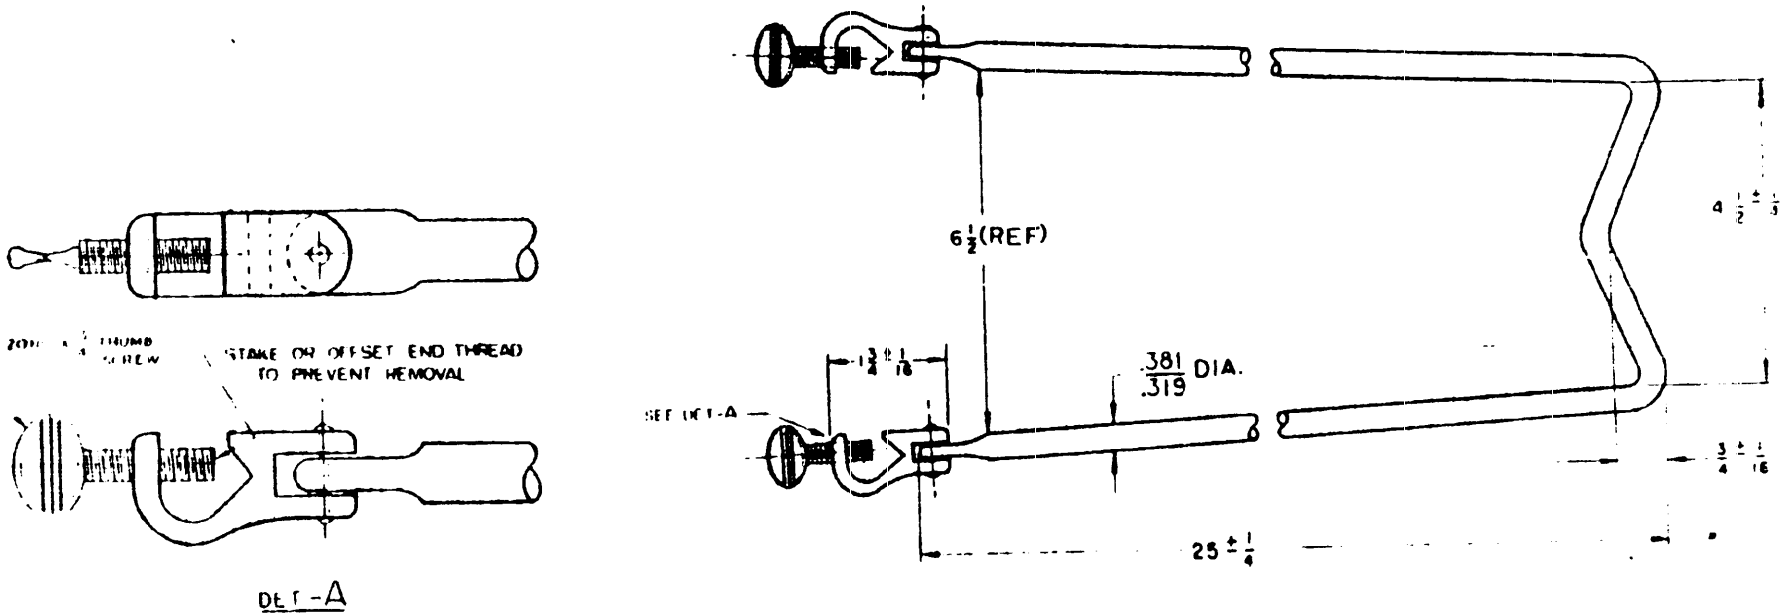


FIG-1 ATTACHMENT, LEG SPLINT, PEARSON

Source: https://assist.dla.mil -- Downloaded: 2026/10-21T08:07Z
Check the source to verify that this is the current version before use.

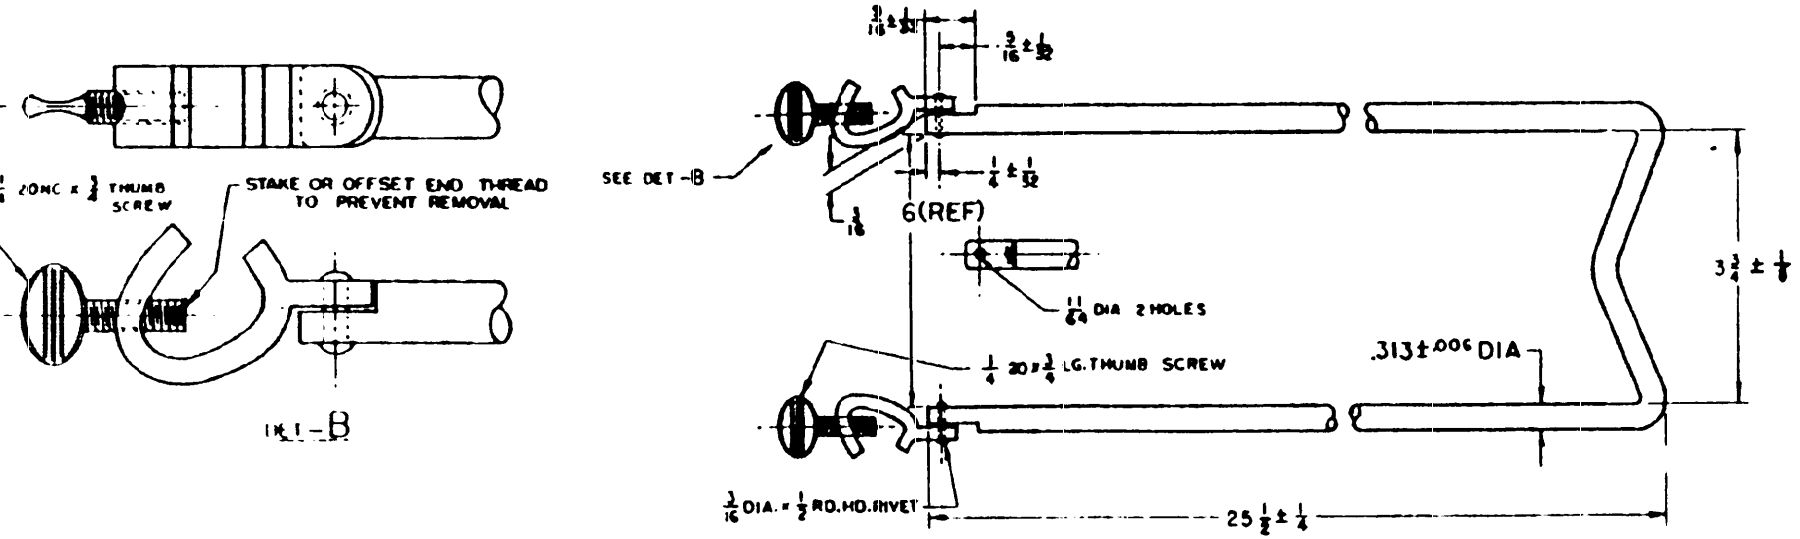


FIG-2 ATTACHMENT, LEG SPLINT, PEARSON

Source: https://assist.dla.mil -- Downloaded: 20260-21T08:07Z
Check the source to verify that this is the current version before use.


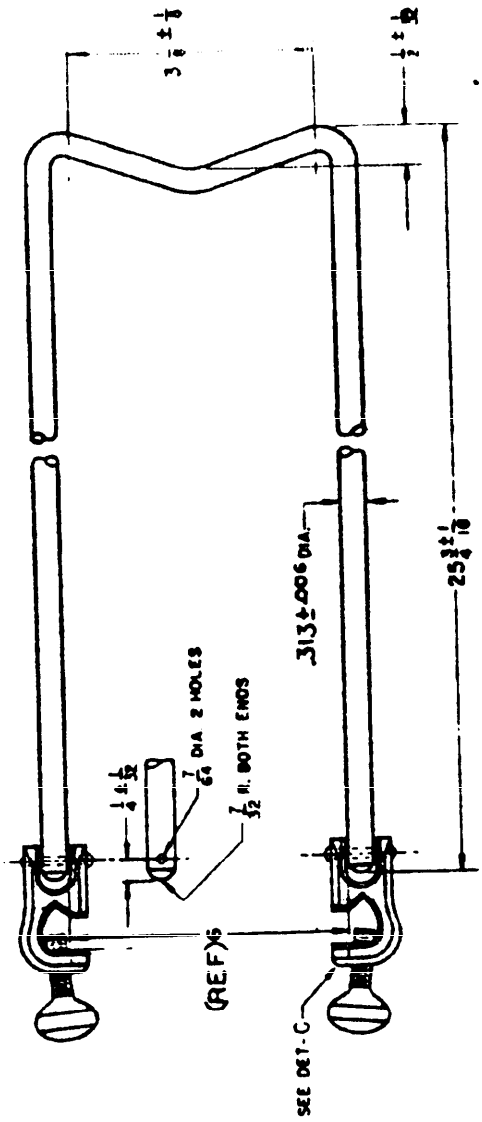


FIG-3 ATTACHMENT, LEG SPLINT, PEARSON

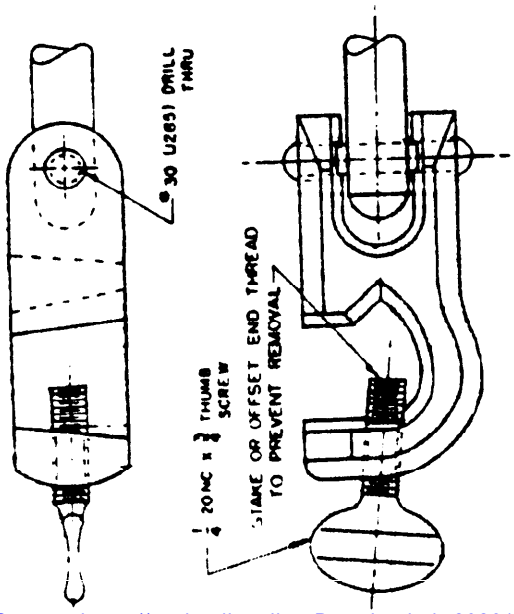

DET - C

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:07Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Supplier responsibilities for inspection. The supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own or any other inspection facilities and services acceptable to the Government. Inspection records of the examination and tests shall be kept complete and available to the Government as specified in the contract or order. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection as used in this specification, is defined as both examination (such as visual, auditory, etc., investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with Standard MIL-STD-105.

4.2.2 For tests. Sufficient samples of the components shall be selected to perform tests as required by the applicable subsidiary specifications or by tests specified herein. When sample size is not specified, the sample size for each test shall be as indicated for inspection level L2 in Standard MIL-STD-105, except that the acceptance number shall be zero (0) for all sample sizes, and a minimum of three (3) samples shall be taken regardless of lot size. No test result shall fall below or exceed the maximum values specified.

4.2.3 Where possible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination. The attachments shall be examined to determine compliance with all requirements contained in this specification.

4.4 Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 20260-21T08:07Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY.

5.1 Packaging.

5.1.1 Level A.

5.1.1.1 Unit package. Each splint shall be packaged in a carton of appropriate size constructed in accordance with Specification PPP-B-566 or PPP-B-676 except that commercial colors shall be acceptable. Closure of carton shall be adequate to prevent spillage of contents under normal handling.

5.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Twenty-four (24) splints packaged as described in 5.1.1.1 shall be packed in an exterior container designed for type 2 load, and constructed in accordance with Specification PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type III, class 1 plywood; or PPP-B-621, table III.

5.2.1.2 Case liner. Each level A box shall be lined with a waterproof case liner conforming to Specification MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 Strapping. Strapping, when required, shall be in accordance with applicable paragraphs of appendix thereto.

NOTE: Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

Source: https://assist.dla.mil -- Downloaded: 20261O-21T08:07Z
Check the source to verify that this is the current version before use.

5.2.2 Level B.

5.2.2.1 Exterior container. Twenty-four (24) splints, packaged as specified in 5.1.1.1 shall be packed in an exterior container conforming to Specification PPP-B-601, table I, using type III, class 1 plywood, or shall be designed for type 2 load, and constructed in accordance with Federal Specification PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type I, class 1.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or order.

5.3 Marking.

5.3.1 Unit package. Each unit package shall be marked in accordance with Standard MIL-STD-129. Waterproofing of labels shall be required only when carton utilized is fabricated of water resistant material. Contract number and contractor's name shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with Standard MIL-STD-129. In addition, the letter "L" shall precede the Federal stock number. One space shall be allowed between the letter "L" and the first digit of the stock number. The terms "Stock number" or "FSN" shall not be indicated. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 Availability of color standards. The color standards of the color referenced in 3.3.3 are available from Commanding General, Aberdeen Proving Ground, Maryland, Attention: Coating and Chemical Laboratory.

6.3 This specification does not include all types, classes, grades, sizes, etc. of the commodity indicated by the title of this specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Military requirements.

Source: https://assist.dla.mil -- Downloaded: 20261O-21T08:07Z
Check the source to verify that this is the current version before use.

6.4 Transportation description. Transportation description applicable to this item is:

Wire Goods or Wire Work, No. I, Flat, in Boxes

Carload minimum weight: 20,000 pounds subject to Rule 34 of the Uniform Freight Classiciation.

Truckload minimum weight: 20,000 pounds per National Motor Freight Classification.

Notice. When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

Custodians:
Army-Med
Navy-Bu'ed
Air Force-AFCSG

Preparing Activity:
Defense Medical Supply Center.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:07Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:07Z
Check the source to verify that this is the current version before use.