MILITARY SPECIFICATION SHEET

ELECTRON TUBE, RADIATION COUNTER
TYPE 7840

This amendment forms a part of Military Specification Sheet MIL-E-1/1388C(EC), dated 19 July 1978.

PAGE 2

TABLE, METHOD 6201, NOTES column: Add ",17, 19".

TABLE, METHOD 6211, NOTES column: Add ",20, 21".

TABLE, Quality conformance inspection, part 1, METHOD 6221, NOTES column: Add ",17".

PAGE 5

NOTE 17: Delete and substitute: "17. Sampling shall be in accordance with MIL-STD-105, General Inspection Level II for both normal and tightened inspection, with an AQL of 6.5, and witnessed by DCAS/DCASR."

Add the following new NOTES:

"19. Spurious pulses of amplitude greater than four volts shall not occur after four minutes of operation.

"20. A new Gieger-Mueller tube (one that has not been used for a month or more) should be counted at 1400V with standard reference source SBRS on shelf in position 1 of the tube-mount assembly for 15 minutes before starting voltage is measured.

"21. Starting voltage test circuit:

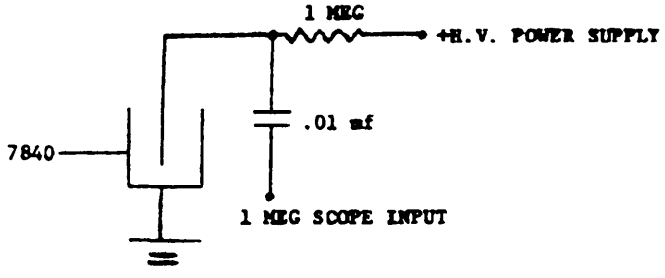

"

Preparing activity:
Navy - EC

(Project 5960-N171)

FSC 5960

Source: https://assist.dla.mil -- Downloaded: 2026-10-15T14:37Z
Check the source to verify that this is the current version before use.