A-A-53179
14 September 1987

COMMERCIAL ITEM DESCRIPTION

CHISEL, BONE

The General Services Administration has authorized the use of this Commercial Item Description.

This commercial item description covers a Stille type bone chisel suitable for use in orthopedic and plastic surgical procedures.

Salient characteristics: Shall be in accordance with the applicable requirements of Federal Specification GG-I-526 and as specified herein.

Material. The chisel shall be fabricated from type 420, martensitic stainless steel, as specified in Table 2 of ASTM F899 for composition only.

Hardness. After proper stress-relieving, the Rockwell hardness of the operative ends shall be C 48 to C 54 when tested in accordance with ASTM E 18 (Rockwell) or E 92 (Vickers or Diamond Pyramid).

Style, design, and dimensions. The chisel shall be a solid one-piece chisel suitable for use in orthopedic and plastic surgical procedures. The distal tip shall be straight on one side and the opposite side shall be angled at the tip to form a bevel. The proximal end of the chisel shall be suitable for absorbing shock when used with a mallet. The handle shall be of a design to facilitate secure grip while in use. The style, design, and dimensions shall conform to Figure 1.

Finish. The finish of the chisel shall be a satin finish, except for the sharpened edges of the beveled portions which shall have a fine honed finish. The chisel cutting edges shall be sharp and shall be free from defects, such as coarse grind marks, cracks, burrs, and feathers when viewed under 4 power (4X) magnification.

Corrosion-resistance. The chisel shall be properly passivated and shall meet the copper sulfate and boil test requirements of GG-I-526, as specified therein. The salt spray test shall not apply.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

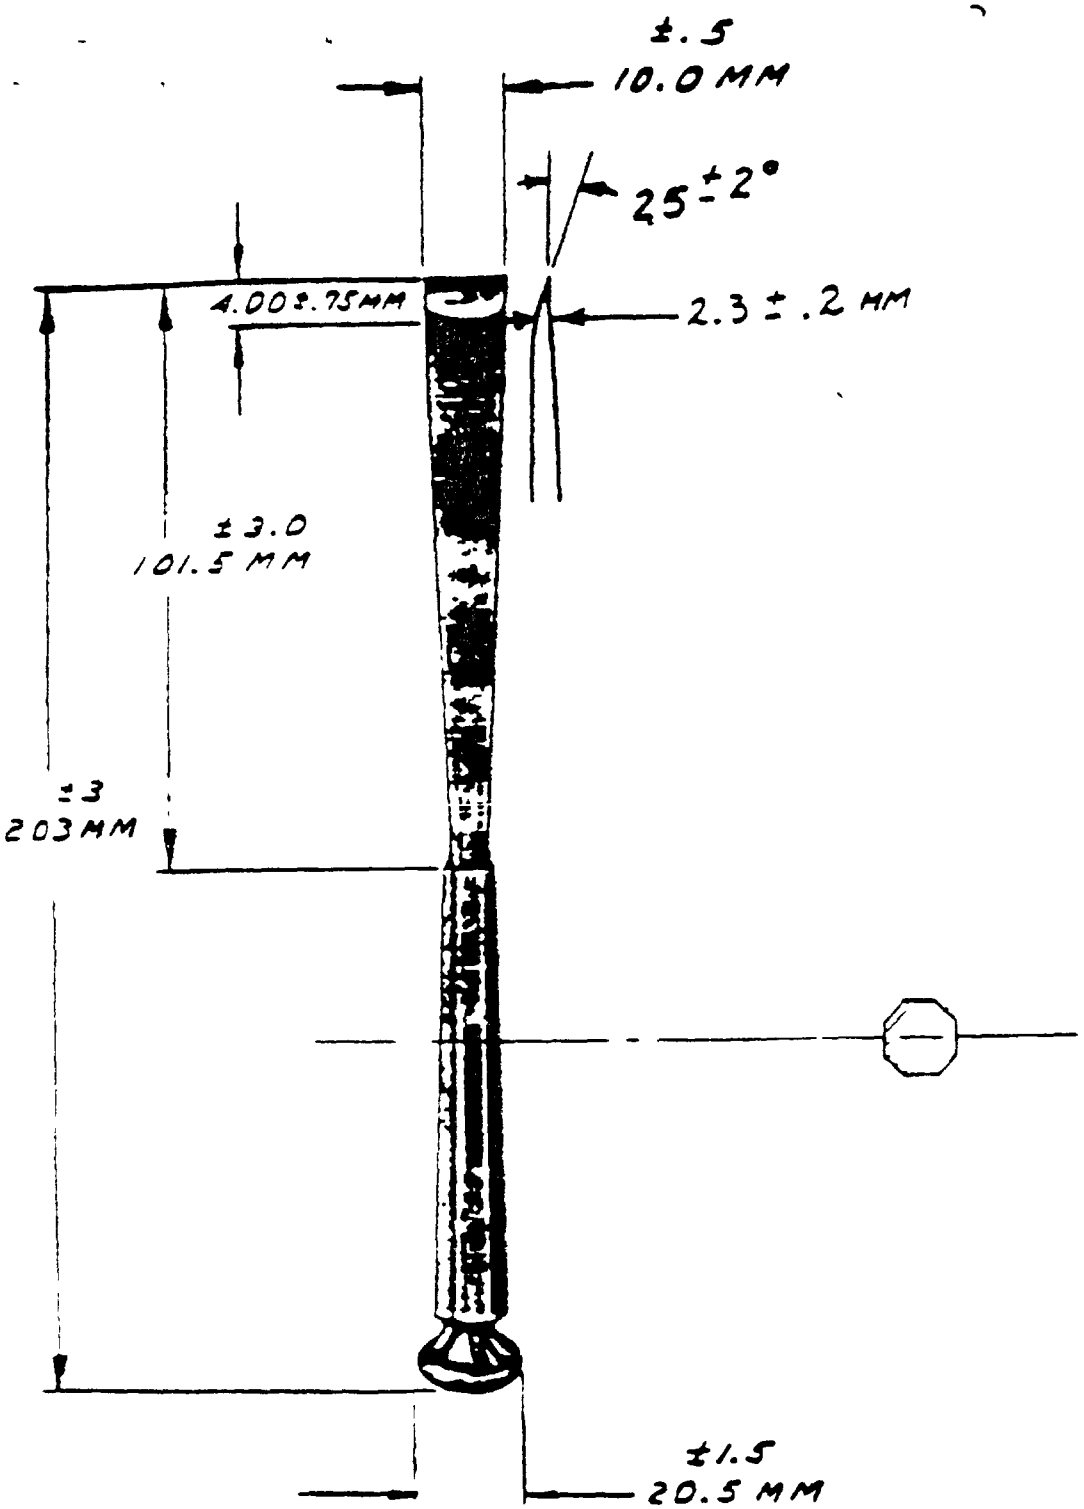


FIGURE 1. Chisel, bone, Stille, 10 mm.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

Identification marking. In addition to the marking requirements of GG-I-526, each chisel shall be marked with the size in mm. The word "Stainless" shall also be marked on the chisel of foreign manufacture. As an alternate to the word "Stainless", the use of a registered trademark identifying the steel as stainless shall be acceptable, provided prior approval is received from the cognizant contracting officer. All marking shall be legible and permanent.

Workmanship. The chisel shall be free from defects which detracts from its appearance or impairs its serviceability.

Unit. Each (EA). One chisel, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one chisel. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

National Stock Number	ITEM IDENTIFICATION
6515-01-139-7605	CHISEL, BONE

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:
VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4098

51299

Location: NCR CID DISK 3

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements All users of military standardization documents are invited to provide suggestions This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN DPSC-ATTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-53179	CHISEL, BONE

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5 PROBLEM AREAS

a Paragraph Number and Wording

b Recommended Wording

c Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.