COMMERCIAL ITEM DESCRIPTION

CANNULA, SUCTION, SURGICAL (Adson)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers curved Adson suction cannulae for use during plastic or reconstructive surgical procedures.

Salient characteristics:

Sizes. Cannulae shall be furnished in the following sizes, as specified in the contract or purchase order:

Size	Outside diameter
9	9 French (0.118 ± 0.015 inches)
11	11 French (0.144 ± 0.015 inches)

Material. The cannula shall be fabricated from Class 3 austenitic corrosion-resistant steel in accordance with ASTM F899.

Hardness. The cannula shall have a Rockwell hardness of B75 minimum. Hardness shall be tested in accordance with ASTM E18, or ASTM E92 and E140.

Style and design. The cannula shall be in accordance with Figure 1. The tubing connector end shall be designed to make a mechanically and functionally secure connector with 1/4 inch i.d suction tubing.

Each cannula shall be furnished with a cleaning stylet. The stylet shall have a 0.022 to 0.032 outside diameter austenitic corrosion-resistant steel wire of sufficient length that the stylet tip extends through the distal tip of the cannula. The distal tip of the stylet may have a steel ball permanently attached to it. The proximal end of the stylet shall have a knob permanently attached to it. The knob shall be knurled or hatched, and shall have a taper portion which seats in the proximal end of the cannula.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

All edges of the cannula shall be chamfered or rounded such that the cannula is free from any sharp edges.

Passivation. The cannula shall be properly passivated.

Finish. The finish of the cannula shall be satin or matte. The finish of the cannula shall be uniform and free from burrs, pits, scale, cracks, and grind or tool marks.

Identification markings. The cannula shall bear the name or registered trademark of the manufacturer, the word "stainless" and the French size. Cannulas of foreign manufacture shall bear the name of the country of manufacture.

Workmanship. The cannula shall be free from defects which detract from its appearance or impair its serviceability. The surface of the cannula shall be smooth and the lumen void of obstructions.

PRODUCT QUALITY LEVEL.

Visual and dimensional examination. The cannula shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One cannula, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for visual examination shall be in accordance with MIL-STD-105. The unit of product for examination shall be one cannula. Sampling shall be Level II with an AQL of 6.5.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one cannula. AQL shall be 1.0 percent defective. Inspection level shall be S-2.

Corrosion-resistance. Cannulas shall be tested for corrosion-resistance in accordance with the Resistance to Boil test of Federal Specification GG-I-526.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-7575	CANNULA, SUCTION, ADSON, Curved, 9 Fr With Obturator
6515-01-139-7576	CANNULA, SUCTION, ADSON, Curved, 11 Fr With Obturator

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4044

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

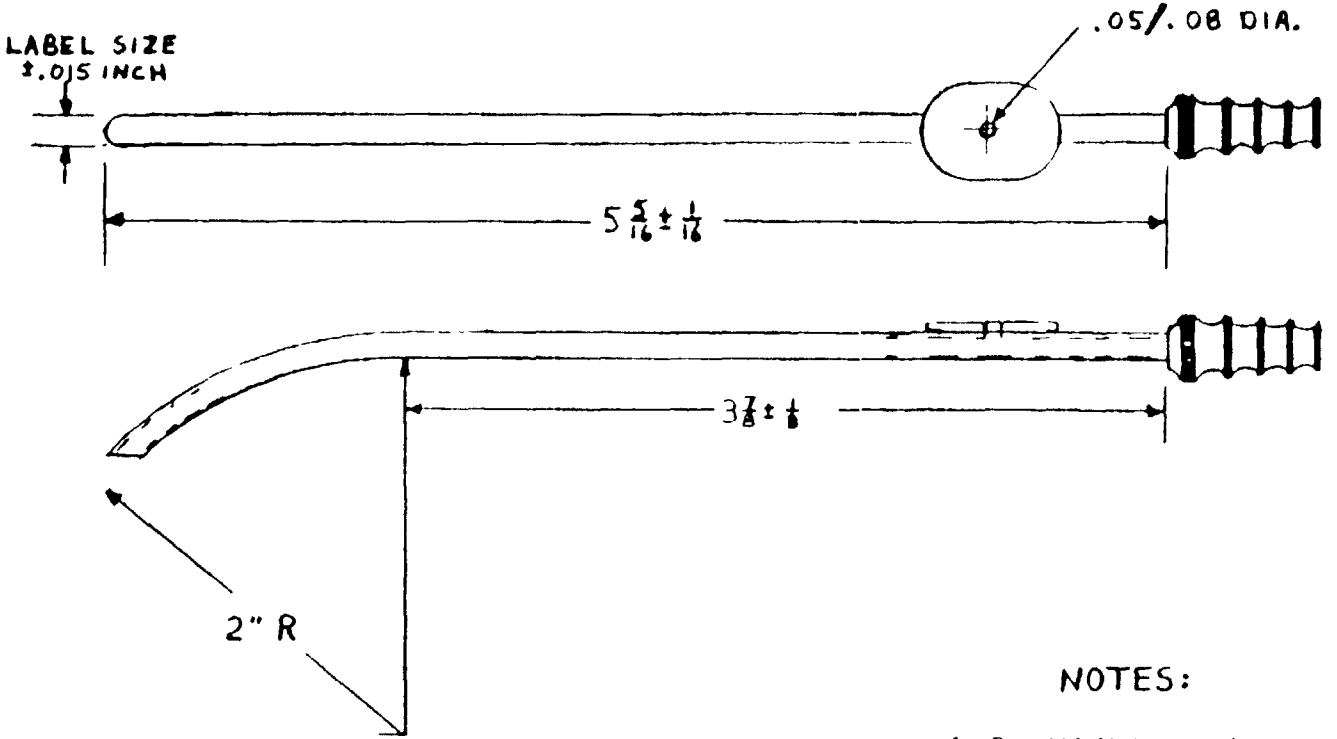

NOTES:

1. CANNULA MAY HAVE SECOND THUMBREST PLATE OPPOSITE THE ONE SHOWN.
2. ALTERNATE TUBING CONNECTOR CONFIGURATIONS ARE PERMITTED.
3. DO NOT SCALE.

FIGURE 1. CANNULA, SUCTION, ADSON, CURVED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO. 4966 WASHINGTON D. C.

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
Attn: DPSC-RSTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-53194	CANTULA, SUCTION, SURGICAL (Adson)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION (Mark one)
	☐ VENDOR
	☐ USER
b. ADDRESS (Street, City, State, ZIP Code)	☐ MANUFACTURER
	☐ OTHER (Specify)

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER (Last, First, MI – Optional)	b. WORK TELEPHONE NUMBER (Include Area Code) – Optional
c. MAILING ADDRESS (Street, City, State, ZIP Code) – Optional	8. DATE OF SUBMISSION (YYMMDD)

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

(FOLD ON THIS LINE)

(CUT ALONG THIS LINE)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.