A-A-53203A
17 May 1990
SUPERSEDING
A-A-0053203(DM)
21 September 1987

COMMERCIAL ITEM DESCRIPTION

DIALYSIS PROCEDURAL SET, ACUTE PERITONEAL

The General Services Administration has approved the use of this commercial item description.

This commercial item description covers a sterile, disposable, periotoneal dialysis procedure set.

Salient characteristics:

General. The set shall be a sterile, disposable, periotoneal dialysis procedural set suitable for treatment of acute renal shutdown and periotoneal lavage. The set shall contain, at a minimum, the following items, which shall be placed in sequence of use:

Quantity	Item
1	20(±2) x 30(±2) inch drape with 3x5 inches centered fenestration
6	4-ply gauze sponges; 4x4 inches
1	5 ml ampule of 1% Lidocaine, USP
1	5/8 inch 25 gage syringe needle
1	1-1/2 inch 22 gage syringe needle
1	3-1/2 inch 15 gage syringe needle
1	5 ml syringe, with short slash markings every 0.2 ml and long slash markings at every ml.

AMSC/NA FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:16Z
Check the source to verify that this is the current version before use.

Quantity	Item
1	Scissors
1	No. 11 scalpel blade
1	Rubber band
1	Safety pin
1	11 French periotoneal catheter with retaining disc and hand grips *
1	Fluid administration and drainage system *
1	Prep solution container
2	Prep sponges

* The fluid administration and drainage system and periotoneal catheter shall consist of the components in accordance with Figure 1.

Material. The catheter shall be fabricated of a rigid plastic which meets the requirements of the USP for Class IV plastics. All other plastic components in contact with fluids shall meet the requirements of the USP for Class II plastics. Remaining components shall meet USP requirements for class I plastics. The drape shall be fabricated of a non-woven, water repellant material. The stylet shall have a trocar point and be made of a suitable corrosion-resistant steel in accordance with ASTM Designation F899. Scalpel blade shall be stainless steel carbon or steel in a peel open package.

Style and design. The stylet shall have a contoured hand grip to provide control for aseptic manipulation of the stylet. Luer fittings shall be in accordance with ANSI/HIMA MD70.1. Scissors shall be disposable, general use and fabricated of metal. Rubber band and safety pin shall be of suitable size to function properly. The drip chamber shall provide approximately 8 drops per ml.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:16Z
Check the source to verify that this is the current version before use.

Each set shall be provided in a sterile, peel-open package designed to strip cleanly on opening without contaminating the set contents.

Sterility, pyrogenicity and toxicity. The complete set shall be sterile, non-pyrogenic, and safe (non-toxic) in accordance with the USP. Sterility assurance level shall be 0.000001.

Shelf life. The dialysis procedural set shall have a shelf life of at least 30 months with at least 24 months remaining at time of delivery to the government.

Workmanship. The dialysis procedural set shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing four dialysis sets, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:16Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Leakage and security of assembly. Fluid path components connected as shown on Figure 1 and tested for leakage and security of assembly by being subjected to an internal pressure of 8 p.s.i.g., minimum except for the drip chamber which shall be subjected to 1/2 psig pressure. No leakage or separation shall occur for 60 seconds test duration.

Tubing clamps shall be operated at least 10 times to stop and open air flow while subjected to an internal pressure of 8 p.s.i.g., minimum. Following the test, the tubing shall be examined for cuts.

Durability. The piecing device shall be tested for durability by inserting into, and removing from, the rubber stopper of a 1 liter parenteral fluid bottle. The device shall be tested with 3 bottles, each bottle tested twice.

Certification of biocompatibility. A certificate of compliance, stipulating offered items meet the requirements specified herein, shall be acceptable in lieu of actual lot testing, provided that the contractor has supplied acceptable items to the Government within the past three years, and that there has been no changes to material formulation and method of processing. The certificate shall include the current contract number and applicable NSN, the date of actual testing, the test method and results, the name and title of the person evaluating test results, and a statement to the effect that material formulation and processing have not changed since the testing was performed.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, inspection level S-1 and acceptance number zero. Sampling for sterility shall be in accordance with the USP.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to thee producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subscontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-253-3826	DIALYSIS PROCEDURAL SET, Acute Peritoneal, Disposable, 4's

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:16Z
Check the source to verify that this is the current version before use.

A-A-53203A

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4542

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:16Z
Check the source to verify that this is the current version before use.

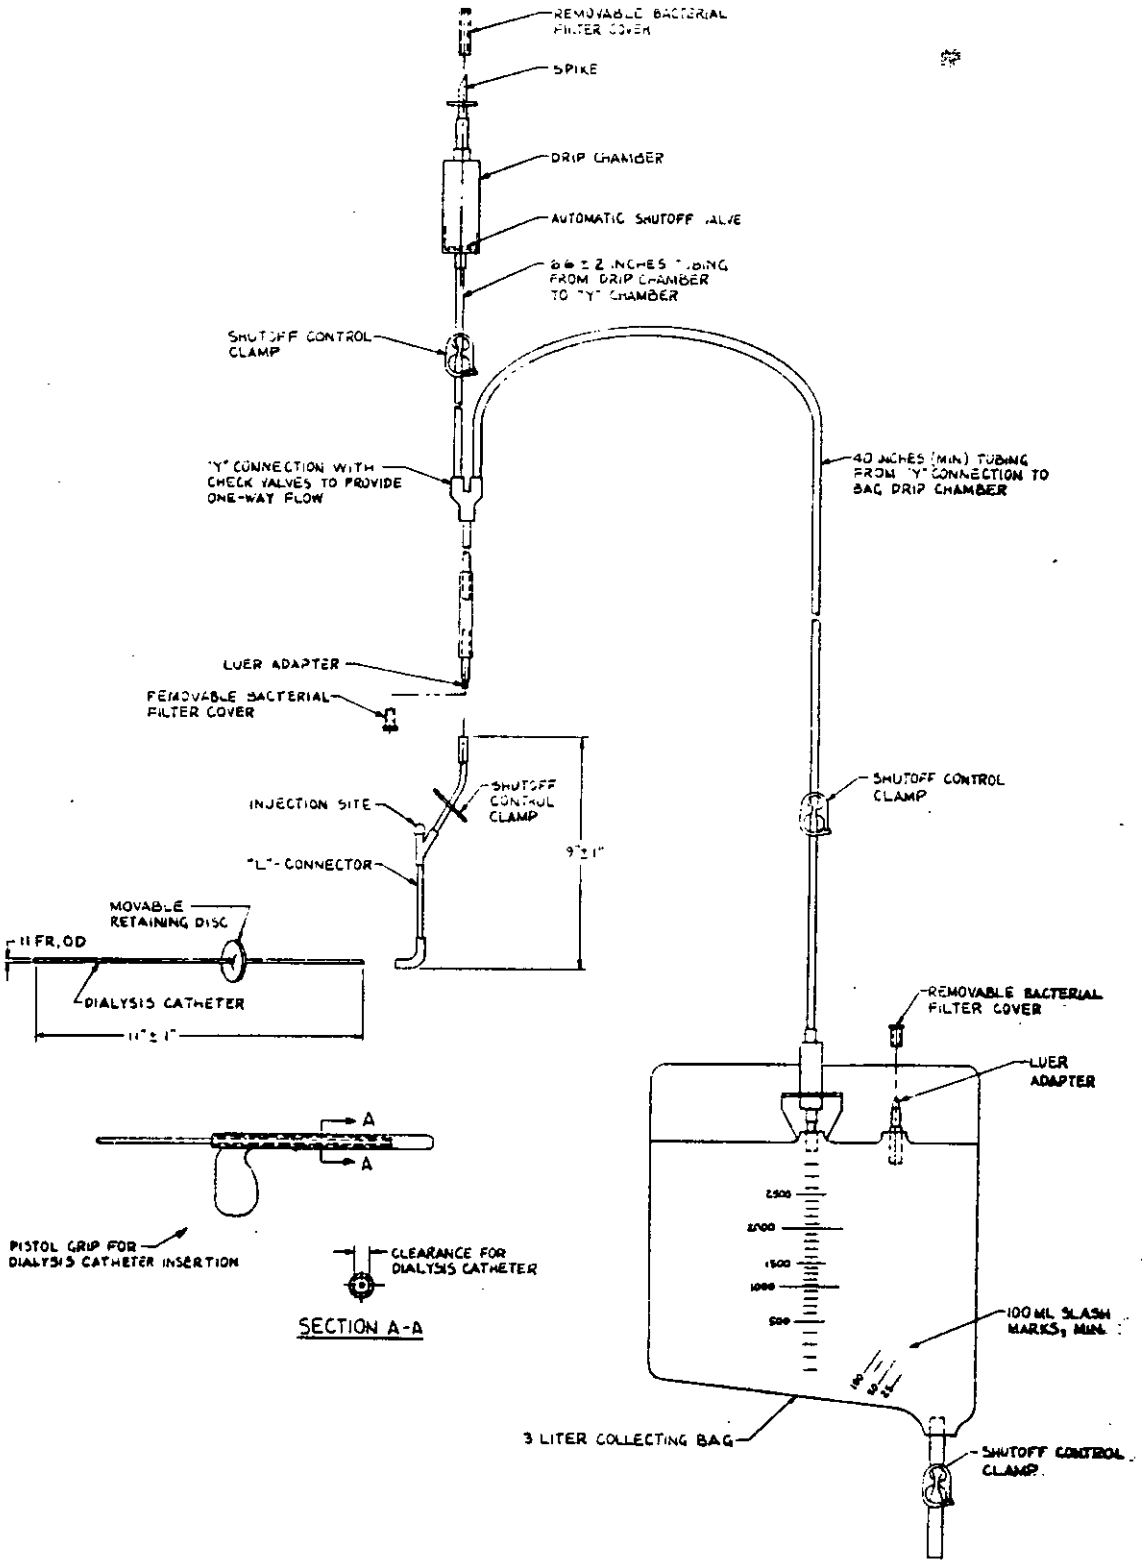


FIGURE 1 DIALYSIS PROCEDURAL SET

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:16Z
Check the source to verify that this is the current version before use.