FEDERAL SPECIFICATION

CART, CLINICAL CHART HOLDER (MOBILE)

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers the following sizes of mobile chart-holder carts constructed of corrosion-resistant steel. Carts shall be suitable for accommodating aluminum clinical chart holders as described in Federal Specification GG–H–555.

1.2 Classification.

1.2.1 *Sizes.*—Carts shall be of the following sizes as specified in the invitation for bids:

Size 1.—Capacity 45 Chart Holders.
Size 2.—Capacity 30 Chart Holders.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification.

Federal Specifications:

FF–C–86—Casters, Truck.
GG–H–555—Holders, Clinical Chart.
QQ–S–766 — Steel, Corrosion-Resisting, Plates, Sheets, Strips and Structural Shapes.
PPP–B–601—Boxes, Wood, Cleated-Plywood.

Military Specifications:

JAN–P–106—Packaging and Packing for Overseas Shipment — Boxes; Wood, Nailed.
JAN–P–125—Packaging and Packing for Overseas Shipment—Barrier Materials, Waterproof, Flexible.

Military Standard:

MIL–STD–129—Marking for Shipment and Storage.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the GSA Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.

(Copies of Military specifications and standards required by contractors in connection with specific procurement functions should be obtained from the procuring agency or as directed by the contracting officer.)

3. REQUIREMENTS


3.1 Material.

3.1.1 *Steel, corrosion-resisting.*—Steel shall conform to Federal Specification QQ–S–766 for class I, condition A.

402166/56/No. 68

FSC Class 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

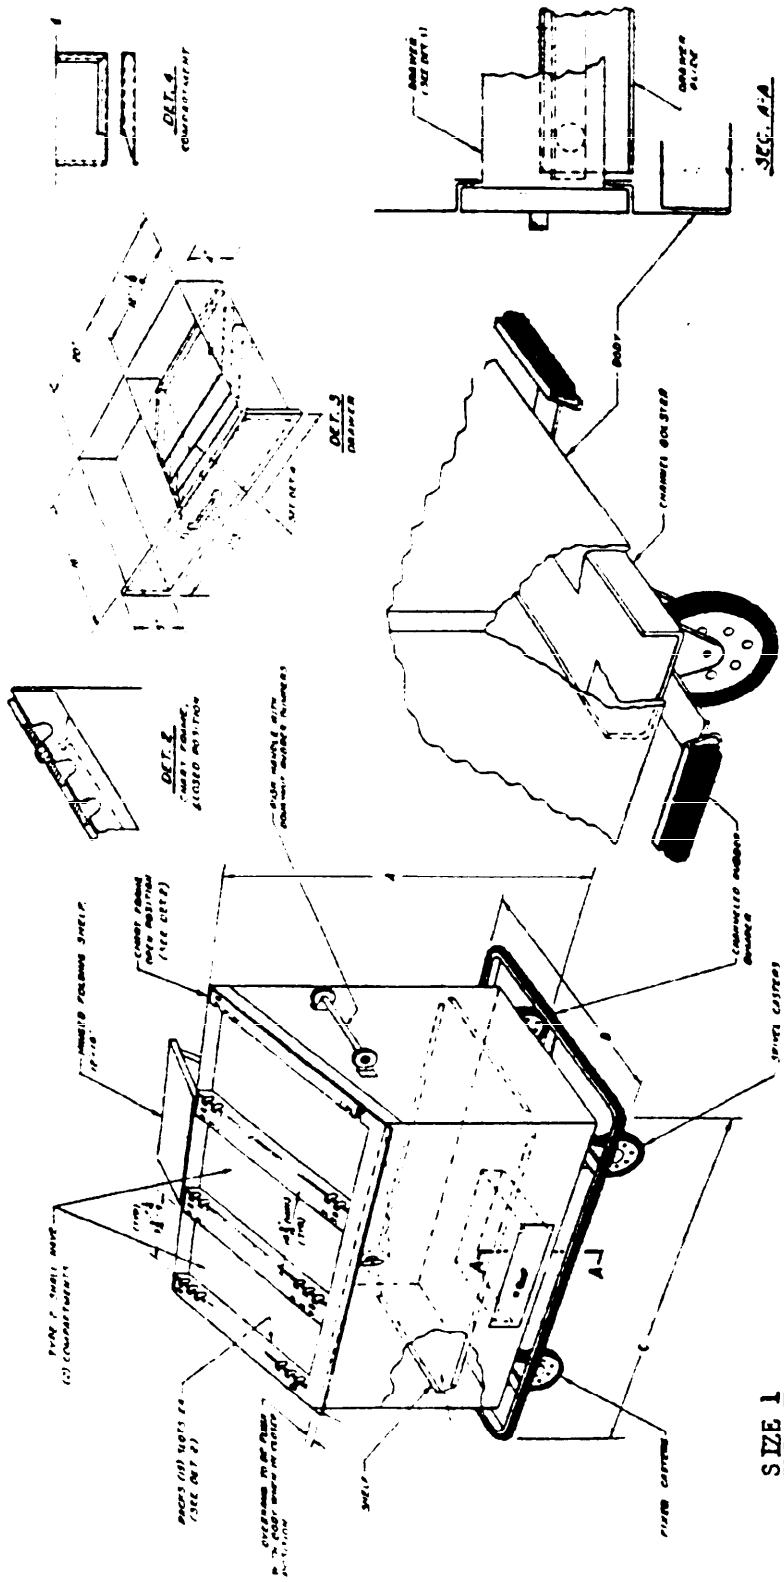

SIZE 1
(As shown)

Note:
Size 2, Similar In General
Design Except As Noted Above

SIZE	A	B	C	CAPACITY
	Inches	Inches	Inches	
1	45	25	44	45 Charts
2	45	25	33	30 Charts

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:49Z
Check the source to verify that this is the current version before use.

3.1.2 *Casters.*—Rigid casters shall be flat plate type I, class B, and swivel casters shall be flat plate type II, class B, Federal Specification FF-C-86.

3.1.3 *Rubber bumper.*—The rubber compound used in the bumper form specified shall be free from any significant quantities of carbon filler or from any other admixture that would visibly mar, streak, or discolor ordinary hospital side-walls by transference on contact therewith during normal operation. It shall be of the rubber compound type known commercially as "Non-Marking", in a gray color, with a Shore Durometer hardness of from 50 to 70, and of a quality free from any reclaimed rubber formulations. The rubber bumpers furnished under this specification are not required to be electrically conductive.

3.2 **Construction.**—Chart-holder carts shall consist of a four-wheel corrosion-resisting steel, mobile, cabinet-type cart with rows of racks (three rows of racks for size 1, two rows of racks for size 2) located at such an angle that names on chart holders are visible from a sitting position. Carts shall have a capacity as specified in 1.2.1 and shall be provided with a drawer and drop-type writing shelf. Construction for size 1 cart shall be in conformance with figure 1. Size 2 cart shall be similar in general design, modified as specified below to have a smaller capacity of chart holders.

3.2.1 *Welding.*—Chart-holder carts shall be welded throughout, and shall be sound, well-fused and free from blisters or blowholes developing strength equal to the part welded. Welding rod shall be of similar chemical composition to part welded. All welds shall be cleaned and free from twists or strains, and all exposed welds shall be ground smooth to eliminate pitmarks and seams, and shall be polished to blend with the color of the adjacent surfaces.

3.2.2 *Size.*—Carts shall be of approximately the following overall dimensions:

3.2.2.1 *Size 1 cart:*

	Length	Width	Height, rear
Body	34½ inches	20 inches	
Overall	44 inches	25 inches	45 inches

3.2.2.2 *Size 2 cart:*

	Length	Width	Height, rear
Body	23½ inches	20 inches	
Overall	33 inches	25 inches	45 inches

3.2.3 *Body.*—The front, back, and sides of the cart shall be constructed of not less than 0.0375-inch-thick corrosion-resisting steel. The ends of the front and back shall have a vertical right-angle flange fitting into an offset recess on the side panels to form a smooth joint. Panels shall be electrically welded together 2 inches on centers. All sides shall be suitably hemmed or flanged with right-angle flange forming support for drawer glides. The top edge of the front and back panel shall be hemmed or flanged. A channel, formed of 0.037-inch-thick corrosion-resisting steel shall be spot-welded across the full length of the inside of the back for reinforcing the body where the folding shelf bracket is mounted. The channel shall be hat-shaped in section, the web being 3 inches long minimum, the channel flanges ½ inch, and the mounting flanges of sufficient length to span the shelf-bracket attaching bolts. Flanges of channel shall span shelf bracket to reinforce shelf. The body shall be fitted with an inner full-length, full-width shelf with turned up flanges on back and sides electrically welded 2 inches on centers all around the inside of the body. The shelf shall be 0.0375 inch thick with cutout corners. It shall be suitable for preventing loss of papers inadvertently dropped from the chart holders. Vertical body seams adjacent to push handles shall be closely spot welded.

3.2.4 *Drawer.*—A drawer shall be located in the center of the cart directly below the inner shelf. The drawer shall be made of

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

0.0375-inch-thick corrosion-resisting steel, having inside measurements of approximately 20 inches long by 16 inches deep by 4 inches high, and have a double walled, sound deadened front measuring approximately 21½ inches long by 5 inches high. Drawer shall be compartmented in conformance with the drawing and shall be equipped with racks for holding blank forms, etc., for charts. Drawer front shall be fitted with a self-closing thumb latch to prevent its rolling open when the cart is in use and shall have a metal chromium-plated handle. Drawer shall travel on suspension channels with built-in roller or ball-bearings. Drawer front shall close against rubber bumpers and shall be flush with the frame of the cart resting in rabbets formed integrally with the cart front, along the top and bottom of the drawer opening. The sides of the drawer openings shall have sheet angles, approximately ¾ inch by ½ inch, welded on the inside of the body front and flush with the edges of the opening. The angles shall be corrosion-resisting steel not less than 0.037 inch thick. The leg extending laterally inward from the front of the cart shall be hemmed and shall extend back to, and be tack-welded to, the top and bottom rabbets. The crevice between the angle and the edge of the opening shall be eliminated by welding and/or flow-soldering and grinding. Slides 0.050 inch thick shall have ball-bearing rollers. The thumb latch shall be located to the left of the drawer handle and shall be so designed that movement of the latch to the right will release the drawer.

3.2.5 *Chassis.*—Body shall be continuously welded or tack-welded to corrosion-resisting holster channels 0.078 inch thick, located to support the body, the bumper assembly, and to provide a mounting for the flat plate casters. Construction shall result in a sturdy, rigid assembly. Tack welding shall provide sufficient welds to hold the bolsters and body firmly.

3.2.6 *Bumper.*—The cart shall be provided with a continuous non-marking rubber bumper (see 8.1.3) at the base fastened by means of screws through a metal insert inside the rubber to a one-piece 1¼-by ½-by 0.109-inch corrosion-resisting steel channel surrounding the entire cart connected by means of 2- by 5/16-inch spacers welded or bolted to the channel and to the chassis bolster channels.

3.2.7 *Push handle.*—Push handle shall be of one-inch outside diameter by 0.0625-inch wall corrosion-resisting steel tubing welded to 0.078-inch-thick corrosion-resisting steel-formed brackets, fitted with doughnut-shaped nonmarking rubber bumpers. Push handle shall be securely fastened to swivel end of the cart. Push handle shall be not less than 10 inches long, excluding bumpers, and shall be attached to cart body at a height of 30 inches from the floor. Body of cart where push handle is attached, shall be reinforced on the inside with a corrosion-resisting steel sheet not less than 0.109 inch thick which shall span the attaching bolts.

3.2.8 *Casters.*—The cart shall be mounted on two fixed-plate and two swivel-plate casters with 8-inch-diameter by 1⅛-inch-face replaceable rubber-tired wheels having a minimum load capacity of 300 pounds per wheel, and conforming to Federal Specification FF–C–86 for types I and II, class B. Casters shall be heavily cadmium plated. Attaching bolts and nuts shall be of corrosion-resisting steel. The lateral span of the casters shall be not less than 14 inches, center to center.

3.2.9 *Shelf.*—A drop-type writing shelf approximately 16 inches long by 12 inches wide formed of 0.037-inch corrosion-resisting steel shall be mounted on the back of the case, level with the top, midway between the ends. All edges of the shelf shall be turned down 1 inch and hemmed, corners rounded, welded and ground. Shelf shall be hinged at cart side and supported by two hinged, folding, self-locking, corrosion-resisting steel brackets having arms approximately 8 inches long. Shelf shall close to approximately 1½ inch width overall in the down position.

Source: https://assist.dla.mil -- Downloaded: 20260-26T11:49Z
Check the source to verify that this is the current version before use.

3.2.10 *Racks.*

3.2.10.1 *Size 1 cart.*—The top of the cart shall consist of racks located at approximately a 40-degree angle to hold three rows of 15 chart holders in visible formation. Four racks of cast aluminum or suitable alloy, equally spaced and slotted to receive the chart holders, shall be securely fastened to the top of the carrier body. All racks shall have 15 equally spaced ¾-inch-wide by ¾-inch-deep wells in top for suspending book-form hinged chart holders in a vertical position. A minus tolerance of ⅛ inch will be permitted in dimensions of wells. Intermediate racks shall have these wells at each side and end racks shall have wells on one side only. Wells at side may run through entire width of end casting.

3.2.10.2 *Size 2 carts.*—The top of the cart shall consist of racks located at approximately a 40-degree angle to hold two rows of 15 chart holders in visible formation. Three racks of cast aluminum or suitable alloy, equally spaced and slotted to receive the chart holders, shall be securely fastened to the top of the carrier body. All racks shall have 15 equally spaced ¾-inch wide by ¾-inch deep wells in top for suspending book-form hinged chart holders in a vertical position. A minus tolerance of ⅛ inch will be permitted in dimensions of wells. Intermediate rack shall have these wells at each side, and end racks shall have wells on one side only. Wells at side may run through entire width of end casting.

3.2.11 *Chart frame.*—A one-piece welded frame, 0.109 inch thick, shall cover these racks and the edge of the cart. This frame shall be movable laterally and notched out so that when it is in the down position, the slots shall line up vertically with the wells in the racks and the chart holders shall be readily removable. When the frame is in the up position, the solid portions of the frame shall cover the well openings, closing them to prevent removal of the charts. The frame shall be held close to the racks, and guided to its movement over the racks by at least three corrosion-resisting steel studs extending through elongated holes or slots in the frame. The studs shall extend through the racks and be fastened securely below. The chart frame lock mechanism shall be so designed as to preclude opening the frame, except by unlocking frame with key, without actually destroying the frame or lock. The frames shall be readily removable and this movement controlled by a two-way key-in handle chromium-plated lock. The lock handle shall operate a disc lever driving rods attached to cans operating against ball or needle bearing rollers so as to readily drive the frame up or down, opening or closing the rack slots without lifting or pushing the frame. The mechanism shall be designed to lock the frame in the up or closed slot position. As an alternate design, the rack slots may be closed by locking bars which are actuated by one two-way key-in handle chromium-plated lock, located at one side of the cart, the locking bars so confined and controlled that rotation of the lock handle in one direction closes all of the slots and locks them closed, and rotation in the opposite direction opens the slots and locks them open.

3.2.12 *Identification marking.*—Each cart shall be permanently and legibly marked with the name or registered trade-mark of the manufacturer, OIN No., and stock number. Decalcomanias shall not be employed.

3.3 Holder, clinical chart.—Unless otherwise specified, carts shall be supplied without clinical chart holders. However, carts shall be constructed to accommodate chart holders as described in Federal Specification GG-H-555.

3.4 Finish.—All exterior corrosion-resisting steel surfaces shall be free from pitmarks and scale. All corrosion-resisting steel surfaces that are or may be exposed in normal use of the cart shall be finished in No. 4 commercial finish. All welds shall be cleaned

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:49Z
Check the source to verify that this is the current version before use.

and ground, and exterior welds shall be polished to match the surrounding surfaces. Wheels shall be cadmium plated.

3.5 **Workmanship.**—Workmanship shall be first class throughout. The finished units shall be clean, well-made, and free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 **Sampling.**—Unless otherwise specified, samples will be submitted in accordance with instructions furnished by the procuring activity.

4.2 **Inspection.**—Inspection may be made throughout the entire process of manufacture. The passing as satisfactory of any detail of construction or materials shall not relieve the contractor of responsibility for faulty workmanship or materials which may be discovered at any time prior to final acceptance. Final inspection of the finished article shall be made either at point of production or at point of delivery designated in the contract or purchase order of procuring agency. In case of factory inspection, every facility shall be afforded inspectors, by the manufacturer, for the prosecution of their work.

4.3 **Tests.**—Tests shall be conducted in accordance with the applicable specifications, as necessary, to determine compliance with this specification.

5. PREPARATION FOR DELIVERY

(For definitions and levels, see 6.1)

5.1 **Packaging.**

5.1.1 Each clinical chart holder cart shall be completely wrapped in Kraft paper of not less than 30 pounds basic weight (500 sheets 24 inches by 36 inches), or equal and securely taped closed with Kraft gummed paper tape, or equal. The clinical chart holders shall then be assembled in the cart, and secured in such a manner as to insure against shifting, displacement, marring of surfaces, or breakage.

5.1.2 The casters shall be disassembled from the cart and placed in a suitable corrugated carton of approximate size, with sufficient cushioning material (Kimpak, cellulose, excelsior, die cut pads, cells, etc.) to insure against shifting or breakage.

5.2 **Packing.**—Each unit shall be carefully wrapped in a protecting covering with all corners adequately protected against marring. The complete outfit shall be packed in a standard commercial shipping container of proper size and so constructed as to withstand storage, handling and reshipment without the necessity of repacking.

5.3 **Marking.**—Unless otherwise specified, shipping containers shall be marked with the name and size of the commodity as defined by the contract or order under which shipment is made, the quantity contained therein, the name of the contractor, the number of the contract or order, the name and address of the consignee, and the gross weight.

5.4 **Preparation for delivery (Military).**

5.4.1 *Packaging.*

5.4.1.1 *Unit of issue.*—One (1) cart of the size specified constitutes one unit.

5.4.1.2 *Level A.*—Casters shall be removed. Casters and components shall be adequately protected and packaged in a carton of suitable size and design and packed within the unit. Drawer shall be closed and secured in position. All exterior finished surfaces shall be protected by wrapping with Kraft paper and cushioning with flexible corrugated fiberboard or other suitable materials. Wrapping and cushioning material shall be secured by tying with cotton cord or tape, or by sealing with Kraft gummed paper tape. Work shall be accomplished in such a manner as to insure against marring, scratching, or damage to the unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.

5.4.1.3 *Level C.*—Package shall be as specified in 5.1.

5.4.2 *Packing.*

5.4.2.1 *Level A.*—Each unit shall be overpacked in accordance with Military Specification JAN-P-106 or Federal Specification PPP-B-601 (table II; type III, class 1 plywood). The unit shall be adequately secured within the exterior container by means of bolts, wood braces, or other interior fittings, to insure against shifting or breakage. Each unit shall be protected by a shroud fabricated of waterproof barrier material conforming to Military Specification JAN-P-125. The exterior container design shall include three skids of not less than 1½ inches in thickness applied crosswise of base, so positioned as to facilitate handling with a fork-lift truck and to maintain unit in an upright position. Closure shall comply with appendix of applicable specification. Strapping will not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage.

5.4.2.2 *Level C.*—Pack shall be as specified in 5.2

5.4.3 *Marking.*

5.4.3.1 *Interior packages.*—Each container shall be marked to identify contents.

5.4.3.2 *Shipping container.*—Shipping container shall be marked in accordance with Military Standard MIL-STD-129. Service color marking and symbol are not required on containers for level A packs when addressed to domestic establishments, for the Medical Services of the Armed Forces.

6. NOTES

6.1 Federal Standard 102 shall be referred to for definitions and applications of the various levels of packaging protection for supplies and equipment.

6.2 Ordering data.—Procurement documents should specify the following:

(*a*) Title, number, and date of this specification.
(*b*) Size required.
(*c*) Sampling required (see 4.1).
(*d*) Place of final inspection (see 4.2).
(*e*) Selection of applicable levels of packaging and packing.

6.3 It is believed that this specification adequately describes the characteristics necessary to secure the desired material, and that normally no sample will be necessary prior to award to determine compliance with this specification. If for any particular purpose, samples with bid are necessary, they should be specifically asked for in the invitation for bids, and the particular purpose to be served by the bid samples should be definitely stated, the specification to apply in all other respects.

6.4 This specification does not include all sizes, etc., of the commodities indicated by the title of the specification or which are commercially available, but are intended to cover the size, etc., which are normally procured to meet Federal Government requirements.

6.5 Transportation description.—Transportation description applicable to this item is:

Barrows, trucks or wagons, not otherwise indexed by name, hand, with fixed bodies or with platforms and standing ends, sides, stakes or standards.
Carload minimum weight 24,000 pounds, subject to Rule 34, Uniform Freight Classification.
Truckload minimum weight 24,000 pounds.

6.6 This specification covers the following items appearing in the Armed Services Medical Stock List:

6530-774-1310 Cart, Clinical Chart Holder, Mobile, Capacity 30 Chart Holders
6530-774-1315 Cart, Clinical Chart Holder, Mobile, Capacity 45 Chart Holders.

Source: https://assist.dla.mil -- Downloaded: 20261O-26T11:49Z
Check the source to verify that this is the current version before use.

Patent notice.—When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:
Army—M
Navy—Md S
Air Force—AF.

Copies of this specification may be purchased for 10 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:49Z
Check the source to verify that this is the current version before use.