GG-L-00110a(DSA-DM)
May 17, 1971
Interim Revision of
Fed. Spec GG-L-110
July 31, 1958

INTERIM FEDERAL SPECIFICATION

LANCET, FINGER BLEEDING

This interim Federal Specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above.

The General Services Administration has authorized the use of this interim Federal Specification as a valid exception to Federal Specification GG-L-110.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers disposable sterile lancets to be used for finger punctures to obtain blood for hematologic studies.

1.2 Classification.

1.2.1 Types and styles. The lancets covered by this specification shall be of the following types and styles (see Figure 1), as specified:

Type I	Type III
Type II	Type IV
Style 1	Type V
Style 2	Type VI
Style 3	Type VII

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

SPECIFICATIONS

•Federal

MMM-A-250	Adhesive, Water-Resistant (for Sealing Waterproofed Paper).
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.
PPP-T-76	Tape, Pressure-Sensitive Adhesive-Paper (for Carton Sealing).
QQ-S-766	Steel Plate, Sheet, and Strip - Corrosion Resisting.

Military

MIL-B-116	Preservation, Methods of.
MIL-B-117	Bags, Interior Packaging.
MIL-S-36586	Sterilization Test Strip Set, Bacterial Spore.

STANDARDS

Federal

Fed. Test Method Std. No. 151 Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D. C. 20402.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the currentversion before use.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston; New York; Atlanta; Chicago; Kansas City, Mo.; Fort Worth; Denver; San Francisco; Auburn, Washington; and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of Military specifications, standards and drawings required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The lancets shall be made of corrosion-resisting steels in the 300 or 400 series of classes conforming to Federal Specification QQ-S-766, except that hardness shall be Rockwell B70 to 110. The surface finish shall be number 4 or 7 of QQ-S-766.

3.2 Design and fabrication. The design and fabrication of the finger bleeding lancet shall be in strict accordance with Type I, Type II (Styles 1, 2, or 3), Type III, Type IV, Type V, Type VI, or Type VII, as shown in Figure 1.

3.3 Sterility. The lancet shall be sterile, when tested as specified in 4.4.1. When tested as specified in 4.4.1, there shall be no evidence of bacterial growth.

3.4 Manufacturer's record. The manufacturer shall place a lot control number on the paper label, or on the printed carton, which can be verified against the manufacturer's records of all tests made which shall be available for inspection by any duly qualified medical officer of the Armed Forces, National Institutes of Health, or any official of the Federal Food and Drug Administration. No shipment shall be made until all the tests have been completed, verified, and recorded in the permanent records of the manufacturer.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.

3.5 Certificates. Certificates of sterility, as specified below, shall be submitted. For destination inspection, certificates shall be submitted by the contractor directly to Technical Operations Division, Directorate of Medical Materiel, Defense Personnel Support Center, 2800 South 20th Street Philadelphia, Pa. 19101, Attention: Quality Assurance Branch, and one copy of each shall be forwarded with each shipment to the consignee. For source inspection, certificates shall be furnished to the procuring activity via the Government inspector.

3.5.1 Certificate of sterility. A certificate of sterility, listing all sterility lot or control numbers, shall state that samples from each sterility lot or control have been tested for sterility, as required in 3.3 and 3.5, and were found to be sterile. The certificate shall reference the method used in determining sterility.

3.6 Workmanship. Workmanship shall be first class throughout. Lancets shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may utilize his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026l0-26T11:48Z
Check the source to verify that this is the currentversion before use.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in Table I. The unit of product for examination purposes shall be one lancet.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (percent defective)*
Major	I	1.0
Minor	I	2.5

* If acceptance number is not exceeded, lot shall be acceptable. If rejection number is equalled or exceeded, inspection at Level II may be performed to determine final acceptance or rejection.

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II. Where possible, the same sample shall be used for the determination of two or more test characteristics.

Table II. Sampling for Tests

Component	Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Lancet	Sterility	3.3	4.4.1	S-2	*
Lancet	Hardness	3.1	4.4.2	S-1	*
Corrosion-resistant steel stock	Composition	3.1	4.4.3	**	*

* Acceptance number shall be zero for all sample sizes.
**One composite sample per lot of stainless steel.

4.3 Examination. The lancet shall be examined to determine compliance with specification requirements. Examination shall be conducted in accordance with MIL-STD-105 and the following classification of defects. Examination shall include but shall not be limited to the defects listed in Table III.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.

Table III. Classification of Defects

Categories	Defects
Major	
101	Point is not sharp.
102	Lancet is not free from burrs.
103	Lancet is not free from foreign matter.
104	Point is bent or deformed.
Minor	
201	Shape and style somewhat different than specified.
202	Surface finish not as specified.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Sterility test. Testing for sterility on the surfaces of the lancet shall be in accordance with the method specified in the USP Procedural Details for Sterility Tests of Class B, Type II, Inoculated Products. As an alternate, testing for sterility shall be in accordance with the method specified in the USP Procedural Details for Sterility Tests, Class B, Type II, Inoculated Carrier, except that the inoculated carrier shall contain sterilization test strips carrying spores of Bacillus subtilis var. globigii and Bacillus stearothermophilus, Type B of MIL-S-36586.

4.4.2 Hardness. Hardness shall be determined in accordance with ASTM Method E-18 as listed in Federal Test Method Standard No. 151.

4.4.3 Chemical composition. The chemical composition shall be determined on a 4-ounce sample of the metal in accordance with Methods 111.2 and 112.2 of Federal Test Method Standard No. 151.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One hundred lancets, as specified, constitute one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:48Z
Check the source to verify that this is the current version before use.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	288 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

5.1.3.3 Individual package. Each lancet shall be individually packaged in a tear type container of appropriate size and design. The container shall be capable of maintaining sterility of contents unless damaged or opened. The container shall have no corrosive effect on the lancet. Closure shall be made in such a manner as to cause destruction of the container when opened.

5.1.3.4 Unit package. One hundred individually packaged lancets shall be packaged in a box of appropriate size constructed in accordance with PPP-B-676, except that commercial colors are acceptable. Closure shall be adequate to prevent spilling of contents under normal handling. Each box shall be further packaged in bag conforming to MIL-B-117, type 1, class E, style 2.

5.1.3.5 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2 inch wide tape conforming to PPP-T-76. Closing of bottom flaps with adhesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.

5.2 Packing.

5.2.1 Level A .

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B .

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure of wood boxes shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II of PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Individual package. In addition to any commercial markings, each individual package shall be marked with lot (control) number, item identification, type, size, name of manufacturer and the legend: "STERILITY GUARANTEED UNLESS PACKAGE IS DAMAGED OR OPENED" or similar statement.

5.3.2 Unit package. Each unit package shall be marked in accordance with MIL-STD-129. Lot (control) number, contract or purchase order number and name of contractor shall be shown. In addition, the method of sterilization (G-Gas, S-Steam, D-Dry Heat Sterilization) shall be shown following the level of packaging and date of packaging. Example "A-1/71-G". Final sterilization shall be on or after indicated packaging date.

5.3.3 Intermediate package. Each intermediate package shall be marked as specified in 5.3.2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

5.3.4 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129. Lot (control) number and the method of sterilization as specified in 5.3.2 shall be shown.

6. NOTES

6.1 Intended use. The finger lancet is intended to puncture the skin of the finger tip in order to draw a small specimen of blood for hematologic studies.

6.2 Ordering data. Procurement documents should specify the following:

(a) Title, number and date of this specification.
(b) Applicable levels of packaging and packing (see 5.1 and 5.2).
(c) Federal stock number.

6.3 This specification does not cover all types, classes, grades or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet requirements.

6.4 This specification is applicable to the following Federal Supply Catalog item:

Federal Stock No.	Item Identification
6515-431-2890	LANCET, FINGER BLEEDING, 100s.

Custodians:
Army - MD
Navy - MS
Air Force - 03


Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM


Project No. 6515-1559

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.


Source: https://assist.dla.mil -- Downloaded: 202640-26T11:48Z
Check the source to verify that this is the current version before use.

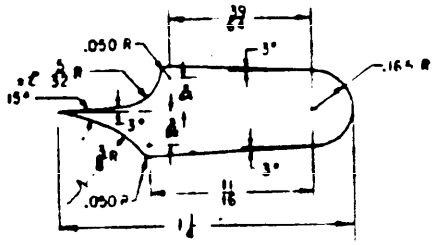

TYPE I

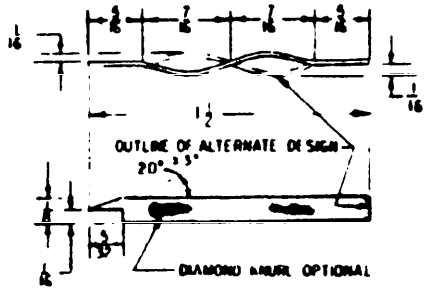


TYPE II STYLE 1

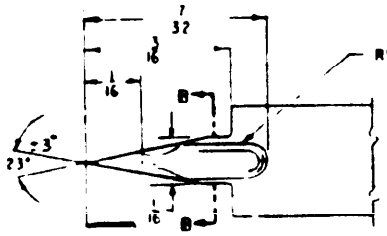

TYPE II STYLE 3




SECT B-B

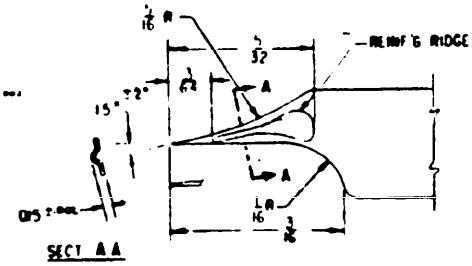


SECT A-A


TYPE II STYLE 2



SECT C-C



SECT D-D

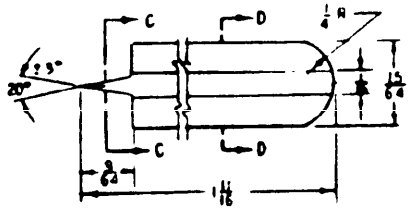

TYPE III

GENERAL NOTES:

1. ALL POINTS MUST BE SHARP
2. UNLESS OTHERWISE NOTED MAT'L THICKNESS SHALL BE .007 - .010
3. DIMENSIONS AND DESIGN FOR TYPE II STYLES 1, 2, AND 3 ARE SIMILAR EXCEPT AS NOTED

FIGURE 1 Types and Styles

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.

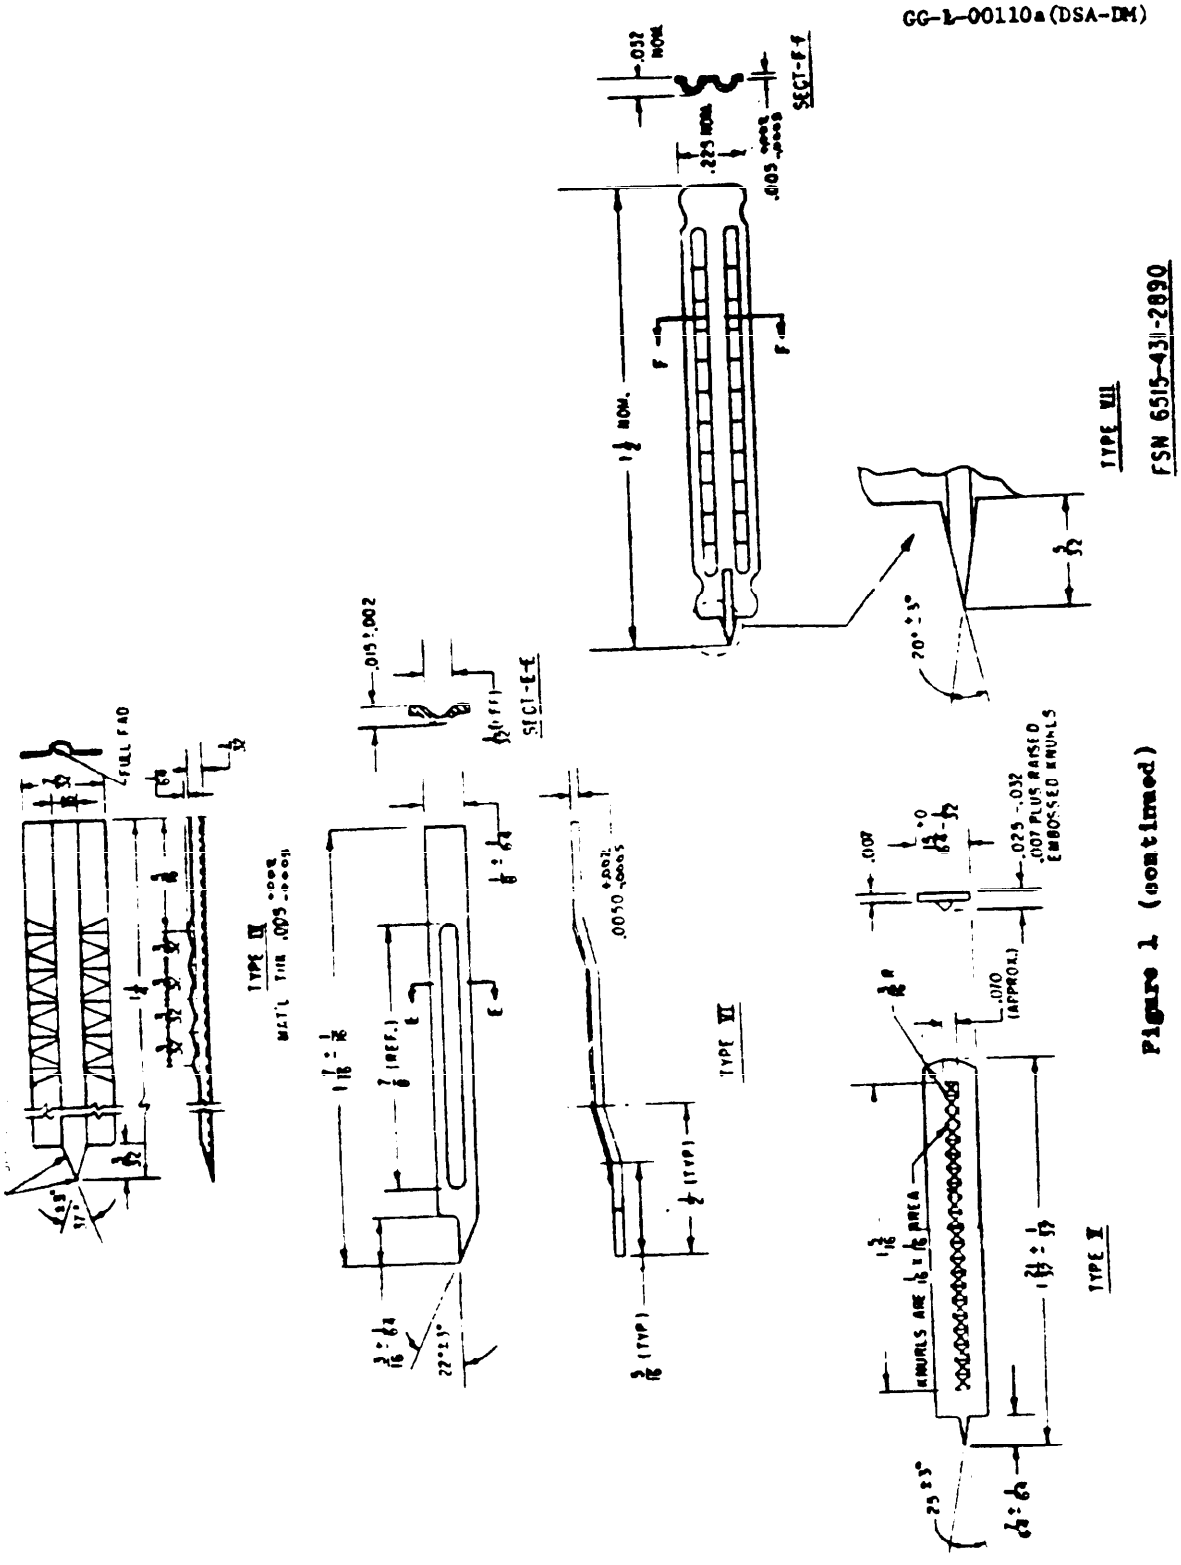


Figure 1 (continued)

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION
GG-L-00110a (DSA-DM)

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
MAR 68

EDITION AUG 66, WILL BE USED UNTIL EXHAUSTED

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:48Z
Check the source to verify that this is the current version before use.