FEDERAL SPECIFICATION

LANCET, FINGER BLEEDING

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers disposable sterile lancets to be used for finger punctures to obtain blood for hematologic studies.

1.2 Classification.

1.2.1 *Types and styles.*—The lancets covered by this specification shall be of the following types and styles, as specified:

Type I. —(See figure 1.)
Type II.—(See figure 2.)
Style 1.—(See figure 2.)
Style 2.—(See figure 2.)
Style 3.—(See figure 2.)
Type III.—(See figure 3.)
Type IV.—(See figure 4.)
Type V. —(See figure 5.)

2. APPLICABLE SPECIFICATIONS, STANDARDS, AND OTHER PUBLICATIONS

2.1 Specifications and standards.—The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

QQ–S–766 — Steel, Corrosion-Resisting, Plates, Sheets, Strips, and Structural Shapes.
PPP–B–566 — Boxes, Folding, Paperboard.
PPP–B–585—Boxes, Wood, Wirebound.
PPP–B–601—Boxes, Wood, Cleated-Plywood.
PPP–B–621—Boxes, Wood, Nailed and Lock-Corner.
PPP–B–636—Boxes, Fiber.
PPP–B–676 — Boxes, Set-Up, Paperboard.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.
Fed. Test Method Std. No. 151—Metals; Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specifications:

MIL–B–117—Bags, Interior Packaging.
MIL–B–10377—Box, Wood, Cleated, Veneer, Paper Overlaid.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

MIL–L–10547 — Liners, Case, Waterproof.

Military Standards:

MIL–STD–105 — Sampling Procedures and Tables for Inspection by Attributes.

MIL–STD–129 — Marking for Shipment and Storage.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. — The following document forms a part of this specification. Unless otherwise indicated, the issue in effect on date of invitation for bids shall apply.

U. S. Pharmacopoeial Convention Publication:

Pharmacopeia of the United States.

(Application for copies should be addressed to the Mack Printing Company, Easton, Pa.)

3. REQUIREMENTS

3.1 Material.

3.1.1 *Corrosion-resisting steel.*—The corrosion-resisting steel shall conform to class 4 or 7 of Federal Specification QQ–S–766, except hardness shall be Rockwell B–70 to 110.

3.2 Design and fabrication.—Design and fabrication of finger bleeding lancet shall be in strict accordance with type I, type II, styles 1, 2, or 3, type III, type IV, or type V as shown in figures 1 through 5.

3.3 Package.—Each individual lancet shall be packaged individually in such a manner that the sterility is maintained until the individual package is opened. The wrapper shall leave no corrosive effect on the lancet.

3.4 Identification marking.—Each individual sterilized package shall be commercially identified as to contents and name of manufacturer, and shall bear the required legend for sterility in accordance with statute.

3.5 Sterilization.—The lancet shall be sterile, when tested as specified in 4.3.1. The package lancet shall be sterilized by high-pressure steam, and shall be dried after sterilization, or shall be sterilized by gas. When tested as specified in 4.3.1, there shall be no evidence of bacterial and mold growth.

3.6 Certificate of sterility.—Unless otherwise specified, a certificate of sterility, listing all lot or control numbers, stating that samples from each sterilizer charge have been tested, in accordance with the method specified herein, and found to be sterile, shall be forwarded by the contractor to the procuring activity (see 6.3). This certificate shall include specific tests performed and the tests results.

3.7 Lot (control) numbers.—The manufacturer shall maintain lot (control) numbers to identify each lot. The lot (control) numbers shall be entered in the manufacturer's original and permanent records of sterilization and shall also appear on each shipment, as hereinafter specified. The manufacturer's records shall be made available for inspection by any duly authorized Government representative.

3.8 Workmanship.—Workmanship shall be first class throughout. Lancets shall be free from defects which detract from their appearance or may impair their serviceability.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 Sampling.

4.1.1 *For visual examination.*—Sampling procedures for visual examination shall be conducted in accordance with the procedures set forth in Military Standard MIL–STD–105.

4.1.2 *For tests.*

4.1.2.1 *For sterility test.*—Sampling for sterility test shall be as indicated for Liquids

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

and Suspension under Sterility Tests in the current edition of the Pharmacopeia of the United States.

4.1.2.2 *For chemical composition.*—Four ounces of metal, representative of each lot used in the manufacture of the end item, shall be selected for determining chemical composition.

4.1.2.3 *For other tests.*—Sample size for each test shall be as indicated for inspection level L2 in Appendix to Military Standard MIL–STD–105, except that the acceptance number shall be zero for all sample sizes, and a minimum of two samples shall be taken regardless of lot size. The unit of product for inspection purposes shall be one lancet.

4.2 **Inspection.**—The inspector shall ascertain that the lancets have been examined and tested in accordance with specification requirements.

4.3 **Tests.**

4.3.1 *Sterility.*—Aseptically transfer the whole lancet, with sterile instruments, to culture tubes each containing 20 milliliters (ml.) of Fluid Thioglycollate Medium and incubate at 30° Centigrade (C.) to 32° C. for not less than 7 days. In addition, similarly transfer whole lancet to culture tubes containing 20 ml. of Fluid Sabouraud Medium and incubate at 22° C. to 25° C. for not less than 10 days. The media shall be prepared as described under "Sterility Tests" in the current edition of the Pharmacopeia of the United States. At the end of incubation periods, the cultures shall be examined for evidence of bacterial and mold growth.

4.3.2 *Hardness.* — Hardness shall be determined in accordance with method 243 of Federal Test Method Standard No. 151.

4.4 **Supplier responsibilities for inspection.**—The supplier shall perform examinations and tests set forth in this specification to substantiate conformance of supplies to specification requirements. The examinations and tests shall be at the expense of the supplier. Suppliers shall have adequate test facilities or shall arrange for test facilities acceptable to the Government to be used for executing specific prescribed tests. Records of examinations and tests performed by the supplier shall be maintained by the supplier and made available to the Government upon the Government's request, at any time, or from time to time, for a period of 2 years after the delivery of the supplies to which these records relate. The supplier shall be responsible for compliance with all requirements of this specification, and all other technical requirements of the contract.

5. PREPARATION FOR DELIVERY

Levels of preservation, packaging, and packing protection used are defined in Fed. Std. No. 102 (for civil agencies only).

5.1 **Packaging.**

5.1.1 *Unit of issue.*—One hundred lancets, as specified, constitute one unit.

5.1.2 *Packaging quantities.*—The number of units of issue indicated in table I shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

TABLE I.—*Packaging quantities*

Federal stock number	Unit package	Intermediate package	Shipping container
6515–431–2890	1 unit	12 units	288 units

5.1.2.1 *Packing variation permitted.*—If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

5.1.3 *Level A.*

5.1.3.1 *Unit package.*—Each unit shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP–B–676. Closure shall be adequate to prevent spillage of contents under normal handling. Carton shall be further packaged in a bag conforming to Military Specification MIL–B–117, type I, class d.

5.1.3.2 *Intermediate package.*—Intermediate package shall be a carton of appropriate size constructed in accordance with Federal Specification PPP–B–566, PPP–B–636 or PPP–B–676. Closure shall be adequate to prevent spillage of contents under normal handling.

5.1.4 *Level B.*

5.1.4.1 *Unit package.*—Each unit shall be packaged in a carton of appropriate size constructed in accordance with Federal Specification PPP–B–676. Closure shall be adequate to prevent spillage of contents under normal handling.

5.1.4.2 *Intermediate package.*—Intermediate package shall be a carton of appropriate size and design, or a complete wrapping of kraft paper of suitable weight. Closure shall be adequate to prevent spillage of contents under normal handling.

5.1.5 *Level C.*—Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose within the continental limits of the United States of America.

5.2 **Packing.**

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—Exterior container shall be designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 3 use; PPP–B–601, table II, when using type III, class 1 plywood; PPP–B–621, table III; or Military Specification MIL–B–10377, table II.

5.2.1.2 *Case liner.*—Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.*—Strapping, when required, shall be in accordance with applicable box specification.

Note.—Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.*—Exterior container shall conform to Federal Specification PPP–B–601, table I, using type III, class 1 plywood, or shall be designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3, for class 2 use; PPP–B–621, table I; or Military Specification MIL–B–10377, table I.

5.2.3 *Level C.* — The subject commodity shall be packed in substantial commercial containers of the type, size and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 **Marking.**

5.3.1 *Interior packages.*—Each unit carton and barrier, and each intermediate package shall be marked in accordance with section 5 of Military Standard MIL–STD–129. Lot (control) number shall be shown.

5.3.2 *Shipping container.*—Shipping container shall be marked in accordance with Military Standard MIL–STD–129. Lot (control) number shall be shown. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Ordering data.—Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(a) Title, number, and date of this specification.

(b) Certificate of sterility required (see 3.6 and 6.3).

(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

(1) Level B packaging is intended to provide economical but limited protection, and should be specified only when it is determined the lancets will be held in covered storage approximately twelve months from date of initial packaging.

6.2 Storage surveillance.—Items packaged in accordance with level B requirements must be inspected to determine condition when not used within the time period indicated in (6.1) (c) (1). Items not used within the time period specified must be repackaged in accordance with level B requirements in this specification or with level A requirements if storage beyond an additional year is anticipated.

6.3 For Military Medical Supply Agency procurement.

6.3.1 Source inspection.—When inspection is made at source, certificate of sterility, required in 3.6, shall be submitted to cognizant inspector for transmittal to Head, Quality Control Division, Technical Department, Military Medical Supply Agency, 84 Sands Street, Brooklyn 1, New York.

6.3.2 Destination inspection. — When inspection is made at destination, certificate of sterility, required in 3.6, shall be submitted by contractor directly to Head, Quality Control Division, Technical Department, Military Medical Supply Agency, 84 Sands Street, Brooklyn 1, New York, and a copy shall be forwarded with shipment to the consignee.

6.4 This specification covers the following item appearing in the Armed Services Medical Stock List:

6515–431–2890 LANCET, FINGER BLEEDING, 100s.

6.5 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of the specification, or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.6 Transportation description.—Transportation description applicable to this item is:

Surgical Instruments, NOIBN.
Carload minimum weight 10,000 pounds, subject to Rule 34, Uniform Freight Classification.
Motor volume minimum weight 10,000 pounds, subject to Rule 34, National Motor Freight Classification.

Notice. — When Government drawings, specifications, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:
Army—M
Navy—Md
Air Force.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

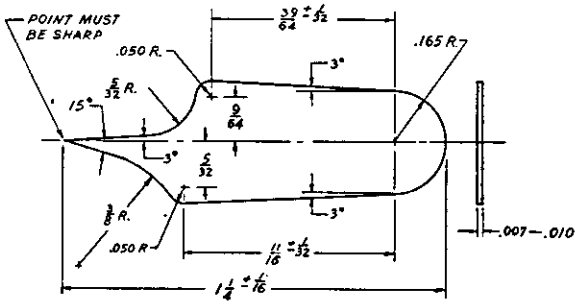


FIGURE 1.—Type I.

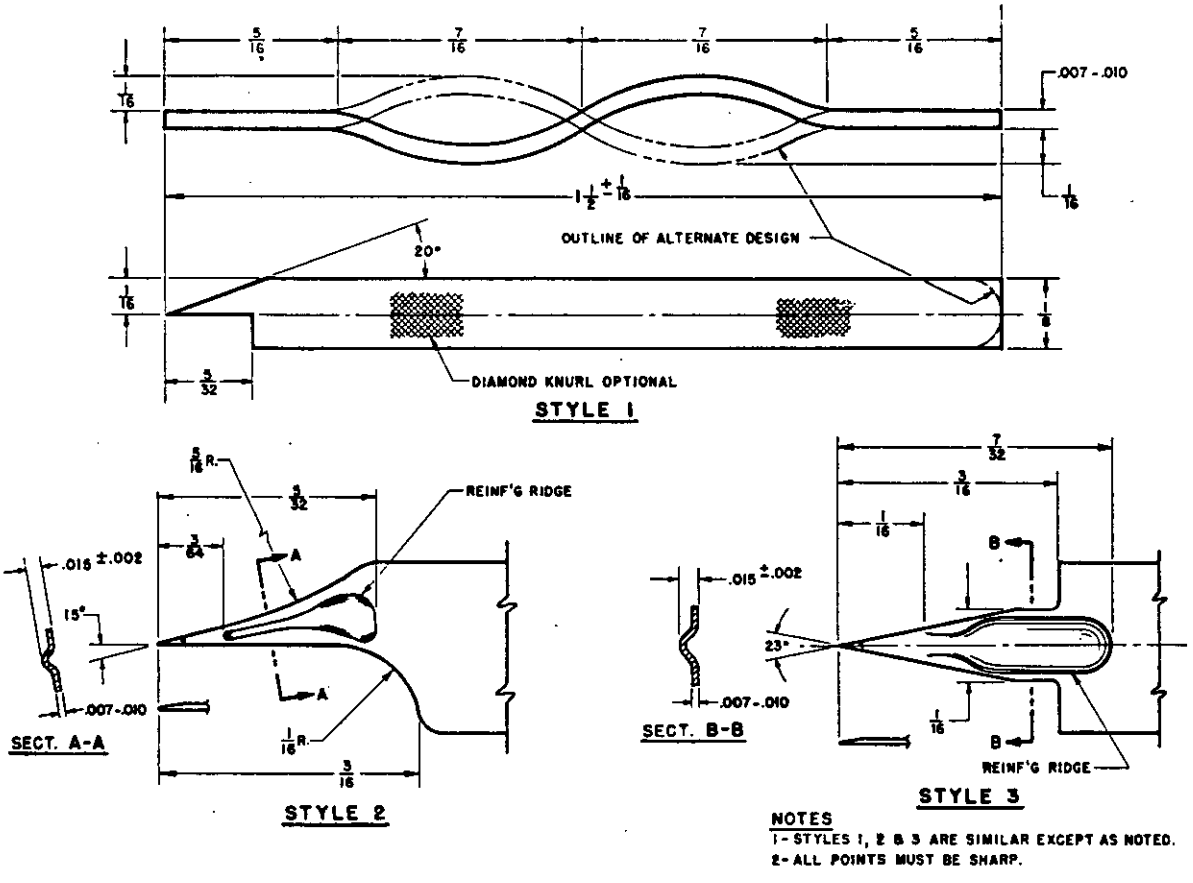


FIGURE 2.—Type II, styles 1, 2, and 3.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.

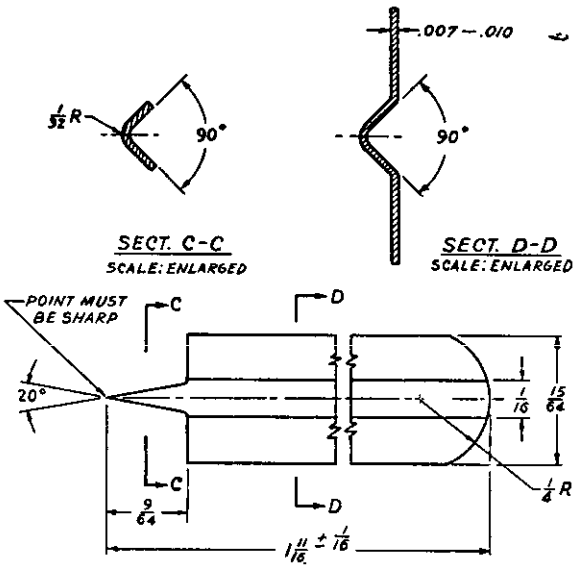


FIGURE 3.—Type III.

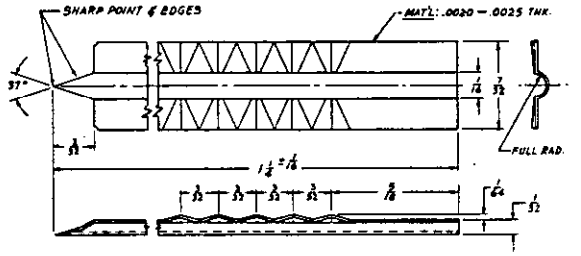


FIGURE 4.—Type IV.

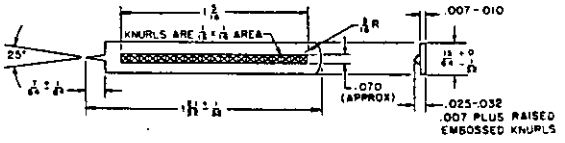


FIGURE 5.—Type V.

Copies of this specification may be purchased for 5 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:48Z
Check the source to verify that this is the current version before use.