GG-F-00336G(DSA-DM)
23 June 1976
SUPERSEDING
Int. Fed. Spec.
GG-F-00336f(DSA-DM)
11 May 1972, and
Fed Spec. GG-F-336c
September 16, 1960

INTERIM FEDERAL SPECIFICATION

FILE AND REAMER, PULP CANAL, DENTAL, STANDARDIZED

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, PA 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal specification GG-F-336c.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers standardized pulp canal files and reamers for use in endodontic procedures.

1.2 Classification. Files and reamers shall be of the following types and classes, as specified (see 6.1).

1.2.1 Types and classes.

Type I - Files.
  Class 1. - 25 mm operative end.
  Class 2. - 21 mm operative end.

Type II - Reamers.
  Class 1. - 25 mm operative end.
  Class 2. - 21 mm operative end.

1.2.2 Sizes. Files and reamers shall be of the sizes indicated in tables II and III, as specified (see 6.1).

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

1.2.3 Assortment. File assortment shall consist of 15 files, 1 each of sizes 1 through 100 of the files listed in table III, except as specified in 3.2.1. (see 6.1).

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of the specification to the extent specified herein:

Federal Specifications:

PPP-B-566	-	Boxes, Folding, Paperboard.
PPP-B-636	-	Boxes, Shipping, Fiberboard.
PPP-B-676	-	Boxes, Setup.

Federal Standards:

Fed. Std. No. 123	-	Marking for Shipment, (Civil Agencies).
Fed. Std. No. 151	-	Metal, Test Methods.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, DC 20402.

(Single copies of this specification and other Federal Specifications required by activities outside the Federal Government for bidding purposes are available without charge from Business Service Centers, at the General Services Administration Regional Offices in Boston, New York, Washington, DC, Atlanta, Chicago, Kansas City, MO, Fort Worth, Denver, San Francisco, Los Angeles, and Seattle, WA.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

Military Specification:

MIL-P-116	-	Methods of Preservation.

Military Standards:

MIL-STD-105	-	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	-	Marking for Shipment and Storage.

(Copies of specifications, standards and publications required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

American Society for Testing and Materials (ASTM):

A 370	-	Methods and Definitions for Mechanical Testing of Steel Products.
A 564	-	Specification for Hot-Rolled and Cold-Finished Age-Hardening Stainless and Heat Resisting Steel Bars and Shapes.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103.)

3. REQUIREMENTS

3.1 Material.

3.1.1 Operative end.

3.1.1.1 Composition. Operative ends of the files and reamers shall be fabricated of AISI 302 stainless steel or alloy type 631 stainless steel conforming to American Society for Testing and Materials (ASTM) Designation A 564 for composition only. As an alternate, operative end of files sizes 60 through 100 only and reamers sizes 55 through 100 only shall be fabricated of 18-2 Mn stainless steel. The stainless steel wire shall conform to the chemical composition as specified in table I for the respective alloy.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

TABLE I. Chemical composition

	Carbon percent 1/	Manganese percent	Silicon percent 1/	Nickel percent	Chromium percent	Phosphorus percent 1/	Sulfur percent 1/	Aluminum percent	Nitrogen percent 1/
ASTM A 564 type 631	0.09	1.00 1/	1.00	6.50 to 7.75	16.00 to 18.00	0.045	0.03	0.75 to 1.50	—
AISI 302	0.15	2.00 1/	1.00	8.00 to 10.00	17.00 to 19.00	0.045	0.03	—	—
18-2 Mn	0.15	11.0 to 14.0	1.00	0.50 to 2.50	16.50 to 19.00	0.04	0.3	—	0.45

1/ Maximum

Source: https://assist.dla.mil -- Downloaded: 202640-26T11:50Z
Check the source to verify that this is the current version before use.

3.1.1.2 Tensile strength. The tensile strength of the operative ends of the files and reamers shall conform to the requirements of table II for the respective file or reamer size listed.

TABLE II. Tensile strength

Files sizes	Reamers sizes	Tensile strength (pounds per square inch)
10, 15, and 20	10, 15, and 20	310,000 minumum
25 through 100	25 through 100	270,000 to 380,000
10 through 55 1/	10 through 50 1/	260,000 to 330,000 1/

1/ For operative ends of files and reamers fabricated of alloy 631 only.

3.1.2 Handles. Handles shall be fabricated of plastic material which is rigid and of a quality suitable to withstand normal operative procedures. Handles shall be capable of being autoclaved and dry heat sterilized without losing the shape of the handle or bleaching out the color when tested as specified in 4.3.3.4.

3.2 Style, design, and dimensions. Files and reamers shall be of the standardized system conforming to the dimensions listed in 3.2.1, 3.2.2, 3.2.3, table III, and figure 1. Files and reamers shall be of two-piece construction consisting of an operative end and a handle. Type I, class I files and type II class 1 reamers shall be furnished with 25 millimeter (mm.) operative ends as specified (see 1.2 and 6.1) for the size indicated. Type I, class 2 files and type II, class 2 reamers shall be furnished with 21 mm operative ends as specified (see 1.2 and 6.1) for the size indicated.

3.2.1 Assortment. Unless otherwise specified (see 6.1), file assortment shall consist of 15 files, 1 each of sizes 10 through 100 of the files listed in table III, except that the length of the operative end shall be as specified in 3.2.2, and the overall length shall be 1-9/32 to 1-11/16 inch.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

3.2.2 Operative ends. Operative ends of instruments shall be made of stainless steel wire conforming to the requirements specified in 3.1.1. The operative ends shall be smoothly finished, uniformly twisted to the number of spirals forming the cutting edges, and shall taper to a fine point. The twisted operative lengths shall form a sharp cutting instrument. The spirals shall be right hand spirals. Operative ends of the files and reamers shall conform to the dimensions and requirements listed in table III. Operative ends of type I, class 1, and type II, class 1 instruments shall be 25 ± 1 mm in length. Operative ends of type I, class 2 and type II, class 2 instruments shall be 21 ± 1 mm in length. Operative ends of files and reamers furnished in the assortment (see 3.2.1) shall be 31 ± 1 mm. Operative ends shall have a uniform taper from D_2 to D_1 of 0.02 mm of diameter per mm of instrument length.

TABLE III. Dimensions of operative ends of files and reamers

Standardized size Numbers	Configuration 1/ Files T	Files S	Reamers T	Reamers S	D1(mm) ±0.02	D2(mm) ±0.02	Number of Spirals Files Type I Class 1 and 2	Number of Spirals Reamers Type II Class 1 and 2
10		X	X	X	.10	.42	38 ± 2	20 ± 1
15		X	X	X	.15	.47	36 ± 2	19 ± 1
20		X	X	X	.20	.52	34 ± 2	18 ± 1
25		X	X	X	.25	.57	32 ± 2	17 ± 1
30	X	X	X	X	.30	.62	24 ± 2	16 ± 1
35	X	X	X	X	.35	.67	23 ± 2	15 ± 1
40	X	X	X	X	.40	.72	22 ± 2	14-1/2 ± 1
45	X	X	X		.45	.77	21 ± 2	13-1/2 ± 1
50	X	X	X		.50	.82	20 ± 2	13 ± 1
55	X	X	X		.55	.87	19 ± 2	12 ± 1
60	X	X	X		.60	.92	18 ± 2	11 ± 1
70	X	X	X		.70	1.02	17 ± 2	9 ± 1
80	X	X	X		.80	1.12	16 ± 2	8 ± 1
90	X	X	X		.90	1.22	15 ± 2	7 ± 1
100	X	X	X		1.00	1.32	12 ± 2	6 ± 1

1/ Configuration

T - Triangular cross-sectional configuration.
S - Square cross-sectional configuration.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

3.2.3 Handles. Operative ends of reamers and files shall be securely and permanently affixed in the handles with no movement of operative ends permitted. Handle shall be in accordance with figure 1 for dimensions.

3.2.4 Identification marking. Handles shall be color-coded as listed below. The color shall be incorporated in the plastic formulation. The complete color code system is as follows:

Color	Size	Color	Size
Purple	10		
White	15, 45, 90	Blue	30, 60
Yellow	20, 50, 100	Green	35, 70
Red	25, 55	Black	40, 80

In addition to color coding, each file and reamer shall have a number corresponding to its size permanently and legibly marked on the handle.


3.3 Resistance to fracture by twisting. When tested as specified in 4.3.3.1, the torsional load at various angular deflections shall be no less than that given in table IV for files and reamers within sizes 10 through 50.


TABLE IV. Torsional load add angular deflection

Size	Minimum Torque		Minimum Deflection in degrees
	Cm. -Gm.	Inch-Oz.	
10	10.80	0.15	540
15	14.40	0.20	540
20	18.00	0.25	540
25	28.80	0.40	360
30	43.20	0.60	360
35	57.60	0.80	360
40	79.20	1.10	180
45	108.00	1.50	180
50	180.00	2.50	180

3.4 Stiffness. The stiffness (bending moment) of all files and reamers shall be no greater than that given in table V for the applicable type and size when tested as specified in 4.3.3.2.


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

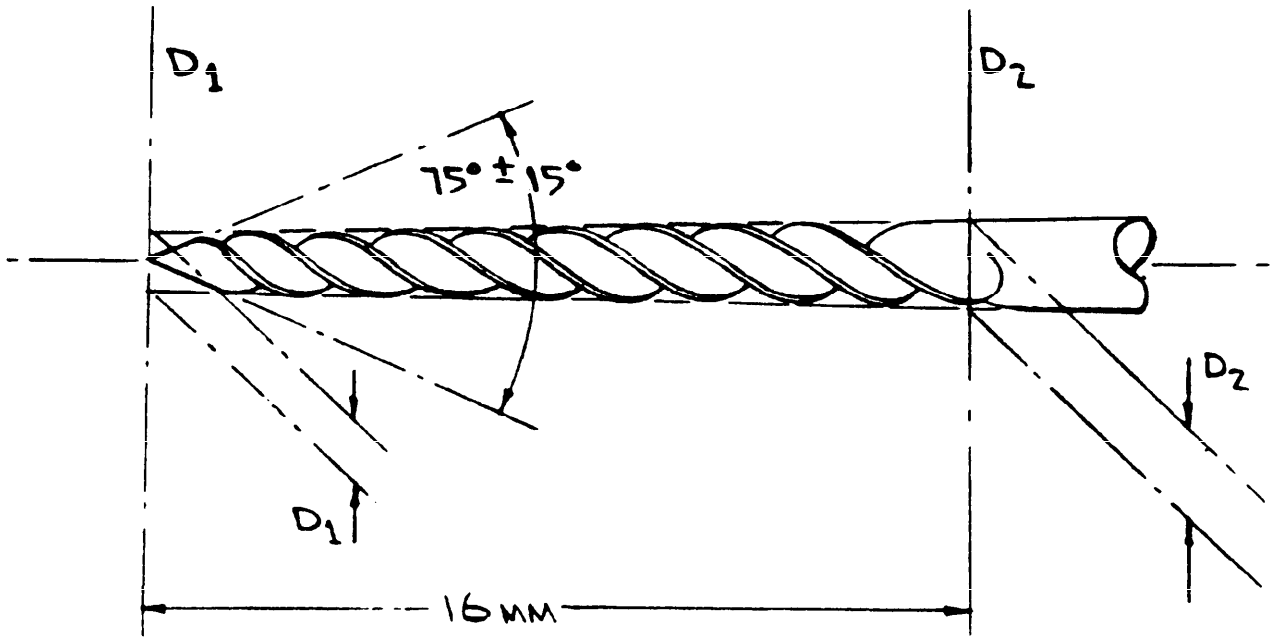

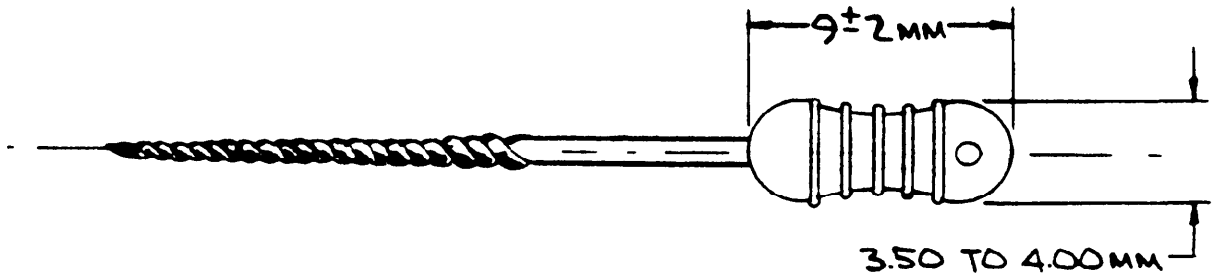

HANDLE
(PLASTIC)

NOTE:
Handles shall be in strict accordance with this figure for dimensional requirements; the styles and designs of the handles shown above are typical and are not intended to restrict or preclude the purchase of files and reamers which are otherwise in accordance with the requirements of this specification.

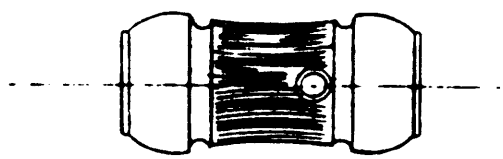

ALTERNATE HANDLE

FIGURE 1. FILE AND REAMER

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

TABLE V. Stiffness

SIZE	BENDING MOVEMENT (Maximum Values)					
	30°		45°		90°	
FILES	Cm - Gm	In - Oz	Cm - Gm	In - Oz	Cm - Gm	In - Oz
10	14.40	0.20	18.00	0.25	21.60	0.30
15	32.40	0.45	39.60	0.55	43.20	0.60
20	50.40	0.70	57.60	0.80	61.20	0.85
25	64.80	0.90	86.40	1.20	100.80	1.40
30	93.60	1.30	122.40	1.70	136.80	1.90
35	104.40	1.45	129.60	1.80	144.00	2.00
40	115.20	1.60	162.00	2.25	180.00	2.50
45	216.00	3.00	252.00	3.50	288.00	4.00
50	378.00	5.25	414.00	5.75	432.00	6.00
55	432.00	6.00	504.00	7.00	x	x
60	558.00	7.75	612.00	8.50	x	x
70	1080.00	15.00	1188.00	16.50	x	x
80	x	x	x	x	x	x
90	x	x	x	x	x	x
100	x	x	x	x	x	x
REAMERS						
10	14.40	0.20	18.00	0.25	21.60	0.30
15	28.80	0.40	32.40	0.45	36.00	0.50
20	36.00	0.50	39.60	0.55	43.20	0.60
25	61.20	0.85	64.80	0.90	68.40	0.95
30	64.80	0.90	86.40	1.20	97.20	1.35
35	79.20	1.10	115.20	1.60	126.00	1.75
40	86.40	1.20	126.00	1.75	136.80	1.90
45	126.00	1.75	136.80	1.90	162.00	2.25
50	180.00	2.50	216.00	3.00	252.00	3.50
55	252.00	3.50	288.00	4.00	x	x
60	288.00	4.00	324.00	4.50	x	x
70	468.00	6.50	540.00	7.50	x	x

3.5 Corrosion resistance. The operative ends of the files and reamers shall not show evidence of corrosion of their surface when subjected to the corrosion tests as specified in 4.3.3.3.

3.6 Finish. Spiral section of operative ends of files and reamers shall have a bright and smoothly honed finish. Handles shall be longitudinally serrated or shall have crosscut serrations. The entire handle may be serrated or only the hand-gripping portion need be serrated. Handles shall be suitable for proper hand gripping. Entire instrument shall be free from laminations, cracks, gouges, chips, or broken areas.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

3.7 Quantity.

3.7.1 Type I, classes 1 and 2 and type II, classes 1 and 2. Unless otherwise specified (see 6.1) unit of issue for type I, classes 1 and 2 files shall be six files, and unit of issue for type II, classes 1 and 2 reamers shall be six reamers.

3.7.2 File assortment. Unless otherwise specified (see 6.1), unit of issue for file assortment shall be a set, as specified in 3.2.1.

3.8 Workmanship. Workmanship shall be first class throughout. Files and reamers shall be properly constructed and finished and shall be free from defects which may detract from their appearance or impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of supplies to which such records relate.

4.1.2 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel (except for hardness requirement) or plastic may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the Item Identification, the name of the applicable raw material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

4.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item. Sampling for inspection shall be performed in accordance with MIL-STD-105, except where otherwise indicated hereinafter.

4.2.1 Examination. Files and reamers shall be examined for defects, including but not limited to those listed in table VI.

TABLE VI. Classification of defects

Categories	Defects
Major:	
101	Type, class, and size not as specified.
102	Assortment not as specified.
103	Style and design not as specified.
104	Quantity (unit of issue) not as specified.
105	Files and reamers not of two-piece construction.
106	Cutting edge not sharp.
107	Spiral section of operative end does not have a bright, smoothly honed finish.
108	Operative ends not firmly affixed in the handles.
109	Laminations or cracks, bends, deformed portions, gouges, chips, or broken areas present in any part of file or reamer.
110	Handle not rigid.
Minor:	
201	Finish of handles not as specified.
202	Color coding and size number marking not present on handle or incorrect.

The inspection levels and acceptable quality levels (AQL's) for examination shall be as listed in table VII. The unit of product for examination shall be the individual file or reamer for type I, classes 1 and 2, and type II, classes 1 and 2. Unit of product for the file assortment shall be the unit of issue (see 3.2.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

TABLE VII. Examination criteria

Type defect	Inspection level	AQL (Percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 Testing. Files and reamers shall be tested as specified in table VIII and 4.3 Inspection levels and acceptable quality levels (AQL's) shall be as listed in table VIII. Unit of product for testing shall be as specified in table VIII. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics.

TABLE VIII. Sampling for tests

Component	Characteristic	Requirement	Test procedure	Unit of product	Inspec. level	AQL
Steel stock	Composition	3.1.1.1	4.3.1	Lot of steel stock	1/	
	Tensile strength	3.1.1.2	4.3.3.5		1/	
Operative ends	Resistance to fracture by twisting	3.3	4.3.3.1	Individual type and size of file or reamer	S-2	1.0
	Stiffness	3.4	4.3.3.2		S-2	1.0
	Corrosion-resistance	3.5	4.3.3.3		S-2	1.0
	Dimensions	3.2.1 & 3.2.2	4.3.2		S-2	1.0
Handle	Sterilization tests	3.1.2	4.3.3.4		2/	4.0
	Dimensions	3.2.1 & 3.2.3	4.3.2		S-1	4.0

1/ A minimum of three specimens from each lot of steel stock shall be tested.

2/ Separate S-2 level quantities for both autoclave and dry heat tests.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

4.2.3 Examination of preparation for delivery. An examination shall be made to determine compliance with the packaging, packing and marking requirements of section 5. Defects shall be scored as specified in table IX. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with AQL of 4.0 expressed in terms of percent defective.

TABLE IX. Examination of preparation for delivery

Examine	Defect
Contents	not as specified.
Container	not as specified.
Marking	Omitted; incorrect; illegible; improper size, location, sequence or method of application.
Material	Component missing or damaged.
Workmanship	Bulging or distortion of containers.

4.2.3.1 Examination of closure, waterproofing and banding of containers. When the shipping container is required to comply with PPP-B-636, the examination for defects in closure, waterproofing or banding shall be in accordance with the appendix of the bbx specification.

4.3 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.3.1 Chemical analysis of the metals. In the absence of certificates of quality for the raw material, the samples selected in accordance with table VIII shall be analyzed in conformance with Methods 111 or 112 of Fed. Std. No. 151. In case of dispute, Method 111 shall be used for referee analysis.

4.3.2 Dimensions. All file and reamer dimensions listed in this specification shall be measured using a shadowgraph, measuring microscope, or other suitable device capable of measuring these dimensions with the accuracy specified in 3.2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

4.3.3 Physical tests. Equipment and material shall be conditioned at room temperature for at least ten (10) hours prior to testing for the following properties.

4.3.3.1 Resistance to fracture by twisting.

4.3.3.1.1 Equipment. The equipment shall consist of a torque-meter, Jacobs chuck, and clamping vise with brass jaws as shown in figure 2. The vise jaws shall be made of brass sheets (70% copper - 30% zinc) which shall not be less than 1 mm thick. The brass sheet shall have a Rockwell hardness of not less than B40 nor more than B65. The equipment shall be capable of measuring the maximum torque and the angular deflection at fracture.

4.3.3.1.2 Procedure. The off-set crank handle shall be attached to the driving end of the torque-meter which shall be mounted in a test stand as shown in figure 2. The Jacobs chuck shall be attached to the driven end of the torque-meter and the entire assembly shall be aligned vertically above the clamping vise. The torque-meter shall then be adjusted to give a "zero" reading on its angular scale. A file or reamer to be tested shall have its handle removed with a suitable wire cutter at the point at which the handle is attached to the instrument shaft. The file or reamer shaft shall then be clamped in the jaws of the Jacobs chuck. Maintaining the vertical alignment of the chuck and clamping vise the torque-meter assembly shall be lowered into position so that the apical 3 mm of the file or reamer, as measured from its tip, can be clamped in an unused portion of the brass jaws of the vise as shown in figure 2. The 3 mm level of the instrument should be flush with the top surface of the brass jaws. The off-set crank shall be used to turn the torque-meter shaft in the clockwise direction until fracture occurs. The maximum torque and angular deflection shall be recorded for each file or reamer tested.

4.3.3.2 Stiffness.

4.3.3.2.1 Equipment. The equipment shall consist of a torque-meter as specified in 4.3.3.2.2 or other suitable apparatus. The torque-meter shall be modified as shown in figure 3, so that the instrument is mounted horizontally and so that the bending moment and angular deflection can be measured simultaneously.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

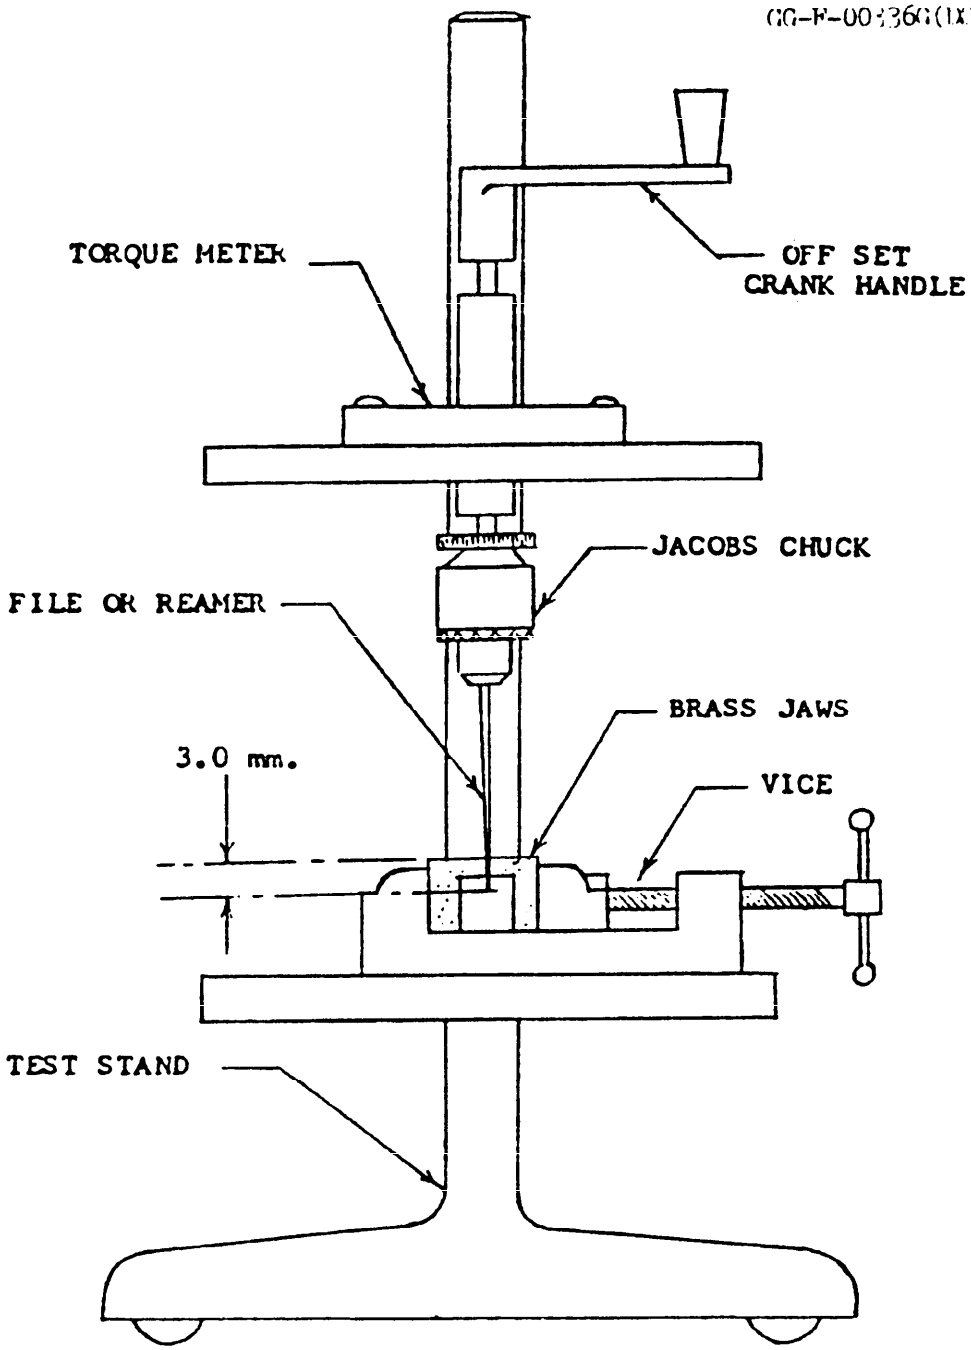


FIGURE 2 TEST EQUIPMENT

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

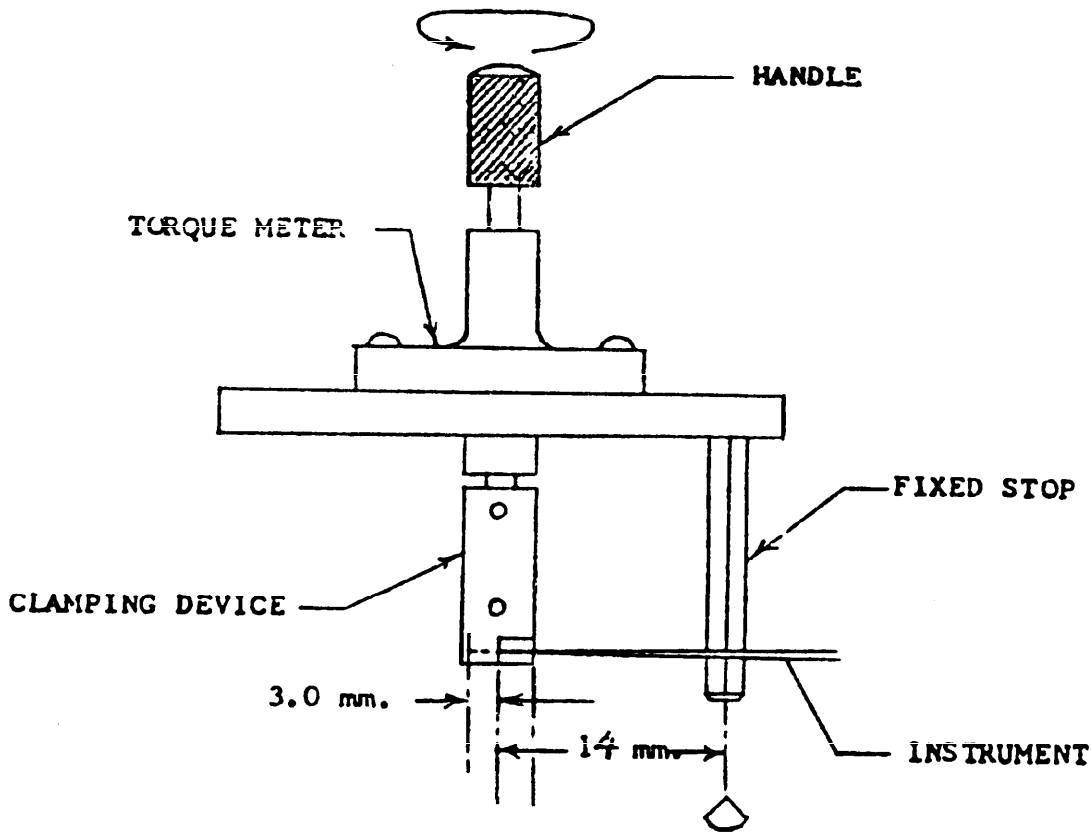


FIGURE 3 BENDING TEST

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

4.3.3.2.2 Procedure. The file or reamer to be tested shall have its handle removed with a suitable wire cutter at the point at which the handle is attached to the instrument shaft. The file or reamer shall be clamped perpendicular to the axis of the clamping device at a point 3 mm from its tip as shown in figures 3 and 4. The clamping device shall be attached to the jaws of the chuck on the torque-meter in such a way to insure that the bending will take place over a uniform span. The torque-meter shall be adjusted to a "zero" reading when the instrument is in slight contact with the edge of the fixed stop (figure 3) which shall be located 14.0 mm from the axis of the torque-meter. The off-set crank shall then be rotated against the constraint of the fixed stop and the bending moment shall be recorded. The angular deflection shall be measured as well.

4.3.3.3 Corrosion test. Files and reamers shall be tested for corrosion resistance by one of the following procedures:

4.3.3.3.1 Sample and preparation. Files or reamers of each size shall be scrubbed with soap and water, rinsed in hot water, followed by a dip in ethyl alcohol (95%), or isopropyl alcohol (isopropanol; 2-propanol) NF, and dried.

4.3.3.3.2 Copper sulfate test. A copper sulfate solution is made up as follows: Copper sulfate ($CuSO_4$, 5 H_2O) 4.0 g, Sulfuric acid (H_2SO_4, sp gr 1.84) 10.0 g, and Water (H_2O) 90.0 ml. The instruments selected and prepared shall be immersed in the copper sulfate solution at a temperature of 65° Fahrenheit (F) for six (6) minutes and then wiped off with a cloth saturated with fresh water. The instrument shall then be examined under a magnification of at least 5X for the presence of brown stains indicating corrosion.

4.3.3.3.3 Agar ion test. An agar ion gel is made up as follows: Potassium ferricyanide ($K_3Fe(CN)_6$) 0.2 g, Sodium chloride (NaCl) 1.0 g, Water (H_2O) 100 ml, Agar-agar 1.5 g. The agar sol shall be poured into a transparent container. The instruments selected and prepared are inserted into the gel (37° ± 2° Centigrade (C) at intervals of not less than 10 mm and at a distance of 10 mm from the periphery of the container. The instruments are inserted to a depth of approximately 20 mm. Visual examination of the instruments while in the gel shall be made for the presence of blue precipitates on the instrument indicating corrosion.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

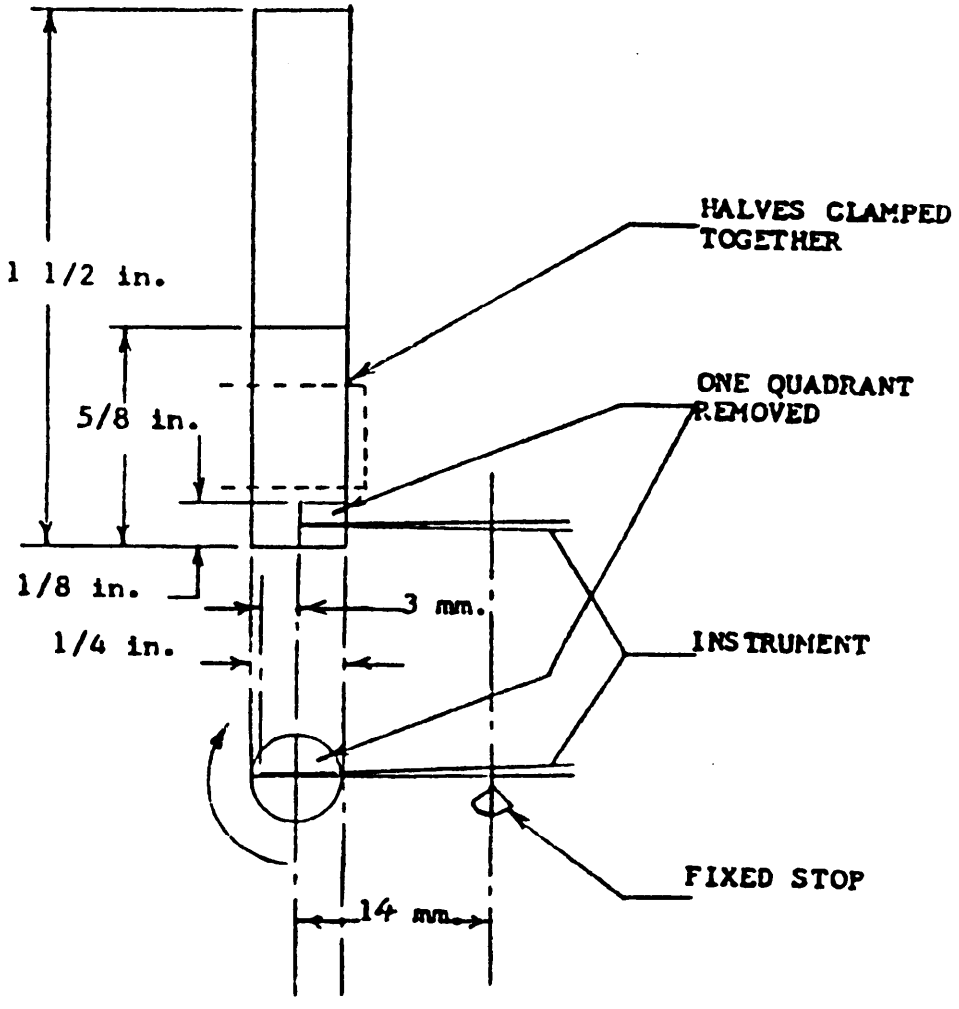


FIGURE 4 CLAMPING DEVICE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

4.3.3.4 Sterilization tests. The finished files and reamers shall be autoclaved under 27 pounds of pressure at 132°C (270°F) for 20 minutes and dry heat sterilized at 160°C (320°F) for 120 minutes. The handles of the files and reamers shall then be examined for compliance with specification requirements.

4.3.3.5 Tensile strength. Tensile strength test shall be performed in accordance with American Society for Testing and Materials (ASTM) Designation A 370.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C, as specified (see 6.1).

5.1.1 Level A.

5.1.1.1 Unit packaging. One package containing six files or six reamers of the type, class and size specified or one set containing fifteen files of one class shall be packaged in a plastic tray with a clear plastic slip-over cover or a hinged cover. The tray shall be designed with six or fifteen cavities or inserts as applicable to hold each file or reamer in such a manner so as to prevent movement and damage to the operative ends. The covers shall be secured with tape and each unit shall be further packaged in accordance with MIL-P-116, method IC-1.

5.1.1.2 Intermediate package. Twenty four unit packages, each package containing six files or reamers of one type, class and size only, or twelve sets of files, each set containing fifteen files of one class, shall be packaged in a box conforming to PPP-B-566 or PPP-B-676. Closure of the box shall be adequate to prevent accidental opening.

5.1.2 Level C. Files and reamers shall be clean, dry and packaged in a manner that will afford adequate protection against corrosion, deterioration and physical damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.1).

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

5.2.1 Level A. Twenty four intermediate packages, containing 288 unit packaged sets of files of one class or 576 unit packages of one type, class and size of the files or reamers, shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-636, class weather-resistant. Closure, banding and waterproofing shall be as specified in the appendix of the box specification.

5.2.2 Level B. Twenty four intermediate packages, containing 288 unit packaged sets of files of one class or 576 unit packages of one type, class and size of files or reamers, shall be packaged in an exterior container designed for a type 2 load and conforming to PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

5.2.3 Level C. The packaged files or reamers shall be packed in shipping containers that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier rules and regulations.

5.3 Marking.

5.3.1 Civil agencies.

5.3.1.1 Interior packages and exterior containers. In addition to any marking specified in the contract or order, interior packages and shipping containers shall be marked in accordance with Fed. Std. No. 123.

5.3.2 Military.

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2.2 Exterior containers. Exterior container shall be marked in accordance with MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Ordering data. Purchasers should select the preferred options permitted herein and include the following information in procurement documents:

(a) Title, number, and date of this specification.
(b) Type, class, and size required (see 1.2).
(c) Assortment (if required) (see 1.2.3).
(d) If assortment required different from that defined herein (see 3.2.1).
(e) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Preparing activity:
DSA-DM

Project No. 6520-1442

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS. The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE
GG-F-00336G(DSA-DM)FILE AND REAMER, PULP CANAL, DENTAL, STANDARDIZED

NAME OF ORGANIZATION AND ADDRESS	CONTRACT NUMBER
	MATERIAL PROCURED UNDER A ☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?
   A. GIVE PARAGRAPH NUMBER AND WORDING.

   B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?
   ☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*	TELEPHONE NO.
	DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.