MIL-G-8348H
15 OCTOBER 1981
SUPERSEDING
MIL-G-8348F
30 March 1972
MIL-I-008348G
15 September 1977

MILITARY SPECIFICATION

GAGE ASSEMBLIES, AIR PRESSURE, DIAL INDICATING CHUCK TYPE, SELF-CONTAINED

This specification is approved for use by all Departments and Agencies of the Department of Defense

1. SCOPE

1.1 Scope. This specification covers self-contained, chuck type high and low pressure air gaging assemblies.

1.2 Classification. Gage assemblies shall be of the following classes and sizes, as specified (see 6.2):

Class A - Screw-on chuck

Size 1 - 0 to 3,000 pounds per square inch (psi) indication
Size 2 - 0 to 1,500 psi indication
Size 3 - 2,000 to 5,000 psi indication
Size 4 - 0 to 4,000 psi indication

Class B - Push-on dual chuck

Size 1 - 0 to 400 psi indication
Size 2 - 0 to 600 psi indication
Size 3 - 0 to 200 psi indication

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: HQ AFLC CASO/LODS, Federal Center, Battle Creek MI 49016 by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6685

Source: https://assist.dla.mil -- Downloaded: 202610-17T10:21Z
Check the source to verify that this is the current version before use.

2. APPLICABLE DOCUMENTS

* 2.1 Issues of documents. The following documents, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-G-76	Gages, Pressure and Vacuum, Dial Indicating, (for Air, Steam, Oil, Water, Ammonia and Chloro-Fluoro Hydrocarbon Gases and Compressed Gases)
QQ-C-320	Chromium Plating (Electrodeposited)
QQ-N-290	Nickel Plating (Electrodeposited)
QQ-Z-325	Zinc Coating, Electrodeposited, Requirements for
PPP-B-601	Boxes, Wood, Cleated Plywood
PPP-B-636	Boxes, Shipping, Fiberboard

Military

MIL-P-116	Preservation-Packing, Methods of
MIL-T-704	Treatment and Painting of Material
MIL-A-8625	Anodic Coatings, for Aluminium and Aluminum Alloys
DOD-D-1000	Drawings, Engineering and Associated Lists

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes
MIL-STD-129	Marking for Shipment and Storage
MIL-STD-130	Identification Marking of US Military Property
MIL-STD-143	Standards and Specifications, Order of Precedence for the Selection of
MIL-STD-794	Part and Equipment, Procedures for Packaging and Packing of
MIL-STD-808	Finishes, Protective and Codes, for Finishing Schemes for Ground and Ground Support Equipment
MIL-STD-961	Outline of Forms and Instructions for the Preparation of Specifications and Associated Documents

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

MIL-STD-831	Test Reports, Preparation of
MS20813	Cap, High-Pressure Air Valve
MS28889	Valve, Air, High-Pressure Charging

Air Force-Navy Aeronautical

AN809	Core - High Pressure Air Valve

DRAWINGS

Air Force

42A3377	Washer-High Pressure Air Chuck or Valve

(Copies of specifications, standards, drawings, and publications required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

* 2.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposal shall apply.

NATIONAL BUREAU OF STANDARDS

Handbook H28 Screw-Thread Standards for Federal Services

(Application for copies should be addressed to the Superintendent of Documents, Government Printing Office, Washington DC 20404.)

UNIFORM CLASSIFICATION COMMITTEE

Uniform Freight Classification Rules

(Application for copies should be addressed to the Uniform Classification Committe, Room 202, Union Station, 516 West Jackson Boulevard, Chicago IL 60606.)

3. REQUIREMENTS

3.1 Preproduction. This specification provides for preproduction testing (see 4.4).

3.2 Selection of standards and specifications. Standards and specifications for necessary commodities and services not specified herein shall be selected in accordance with MIL-STD-143, except as provided in 3.2.1.

3.2.1 Commercial parts. Commercial parts having suitable properties may be used where, on the date of invitation for bids, there are no suitable standard parts. In any case, commercial utility parts such as screws, bolts, nuts, and cotter pins having suitable properties may be used provided:

a. They can be replaced by the MS or AN standard parts without alteration.

b. The corresponding standard part numbers are referenced in the parts list and, if practical, on the contractor's drawings.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

3.3 Materials.

3.3.1 Protective finish. All parts shall be fabricated from corrosion-resistant materials or so plated as to resist corrosion in accordance with recognized industrial recommendations covering the particular material. The use of any protective coating that will crack, chip, or scale with age or extremes of atmospheric conditions shall be avoided. All metal parts fabricated from material not corrosion resistant shall be plated or treated to withstand deterioration and corrosion as encountered in general service. Plating shall be in accordance with QQ-N-290, QQ-Z-325, or QQ-C-320. If cadmium plating is used, it shall be of good commercial practice.

3.3.2 All metal stock used in the fabrication of gage assemblies shall have a properly refined structure with uniform elemental distribution, sound and free from nonmetallic inclusions, injurious porosity, excess segregation, soft spots, hard spots, and other injurious defects. All other material not specially designated shall be entirely suitable for the intended purpose.

3.4 Design and construction. All gage assemblies shall be so designed and constructed that parts will not work loose in service. They shall be built to withstand the strains, jars, vibrations, and other conditions incident to shipping, storage, and service.

3.4.1 Maintenance. The gage shall have a minimum number of parts consistent with reliability. All parts subject to disassembly for maintenance purposes shall be readily accessible for adjustments, repairs, and cleaning without the use of special tools.

3.4.2 Heat treatment. When required, heat treatment of parts shall be accomplished in accordance with the best commercial practice and shall be such as to accent the best overall qualities of the material used. Parts requiring special characteristics such as stability, hardness, toughness, or shock resistance shall be heat treated in accordance with recognized industrial recommendations covering that particular material.

3.4.3 Threads. Threads shall conform to Handbook H28.

3.4.4 Interchangeability. All parts having the same manufacturer's part number shall be functionally and dimensionally interchangeable. The drawing number requirements of DOD-D-1000 shall govern changes in the manufacturer's part numbers.

*3.5 Performance. Classes A and B pressure gages shall be capable of accurately measuring air pressure within the range of the specified gage size when the gage chuck is engaged with the valve stems specified herein (see 4.6.2).

3.6 Pressure gages.

3.6.1 Gages. Class A and class B pressure gages shall be the Bourdon tube, indicator type, conforming to GG-G-76, class 1, style A, type 1, 2-1/2 inch dial size, with a range as specified for each size and as specified herein.

Source: https://assist.dla.mil -- Downloaded: 202610-17T10:21Z
Check the source to verify that this is the current version before use.

An overload stop shall be provided to prevent injury to the Bourdon tube or disengagement of the movement sector under severe overpressure conditions. The gage shall have an unbreakable crystal. The outlet shall have a 1/4-inch standard external pipe thread. The gage shall be provided with a safety blowout protective device, which in the event of rupture of the Bourdon tube will allow sufficient air escapement to prevent explosion of the gage. The gage shall be furnished with a bronze bushed, heavy duty movement or its equivalent which shall consist of heavy duty bronze plates and stainless steel components.

3.6.2 Case. The gage case shall be made from durable corrosion-resistant materials, or so plated or treated as to resist corrosion, with black or chrome exterior finish, and shall provide for removal of the mechanism as a unit for servicing.

3.6.3 Dial. The dial shall be direct reading, shall have a silver or white background with black scale graduations and numerals. The dial shall be marked in black as follows: Pressure LB/SQ, IN. The smallest increments of the scale graduations shall be a minimum of 1/8 inch long. Every fifth graduation shall extend a minimum of 1/16 inch beyond the smallest graduation. Every tenth graduation shall be further extended and marked with the applicable increment figure. The numerals shall be a minimum of 1/8 inch high. The pointer shall be black.

3.6.4 Mechanism. The mechanism shall be corrosion-resistant metal and shall be of rugged design to withstand rough usage encountered in service. Provisions shall be incorporated in the design to permit adjustment for correction of indications that may become necessary during the service life of the gage.

3.7 Class A gage assembly. The class A gage assembly shall consist of a pressure gage conforming to 3.6, bleeder valve, stem, hose, chuck assembly, and carrying case, and shall be in accordance with Figures 1 and 2 and of the sizes shown on Figure 2.

3.7.1 Bleeder valve. The bleeder valve shall be manually operated and shall provide a means for bleeding pressure as applied to the gage through the chuck.

3.7.2 Stem. The stem shall provide a means for applying air pressure to the gage and chuck. The stem shall be made of brass approximately 1-5/16 inches long. One end shall have a 1/8-inch standard external pipe thread; the other end shall be 0.302 inch in diameter and shall have 32 threads per inch. The stem shall have an adequate axial hole and the end with a 0.302-inch diameter shall be properly fitted with a valve core conforming to AN809 for sizes 1 and 2. The stem for size 3 and 4 shall accommodate the valve conforming to MS28889-1.

3.7.3 Chuck assembly. The chuck assembly shall incorporate a swivel nut for attachment to a valve stem conforming to MS28889. It shall be properly sealed against loss of air pressure by replaceable gaskets, washers, or packing. The chuck shall have a valve core depresser which may be turned by hand to depress the valve core after the chuck is attached to the valve by the swivel nut. A

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.


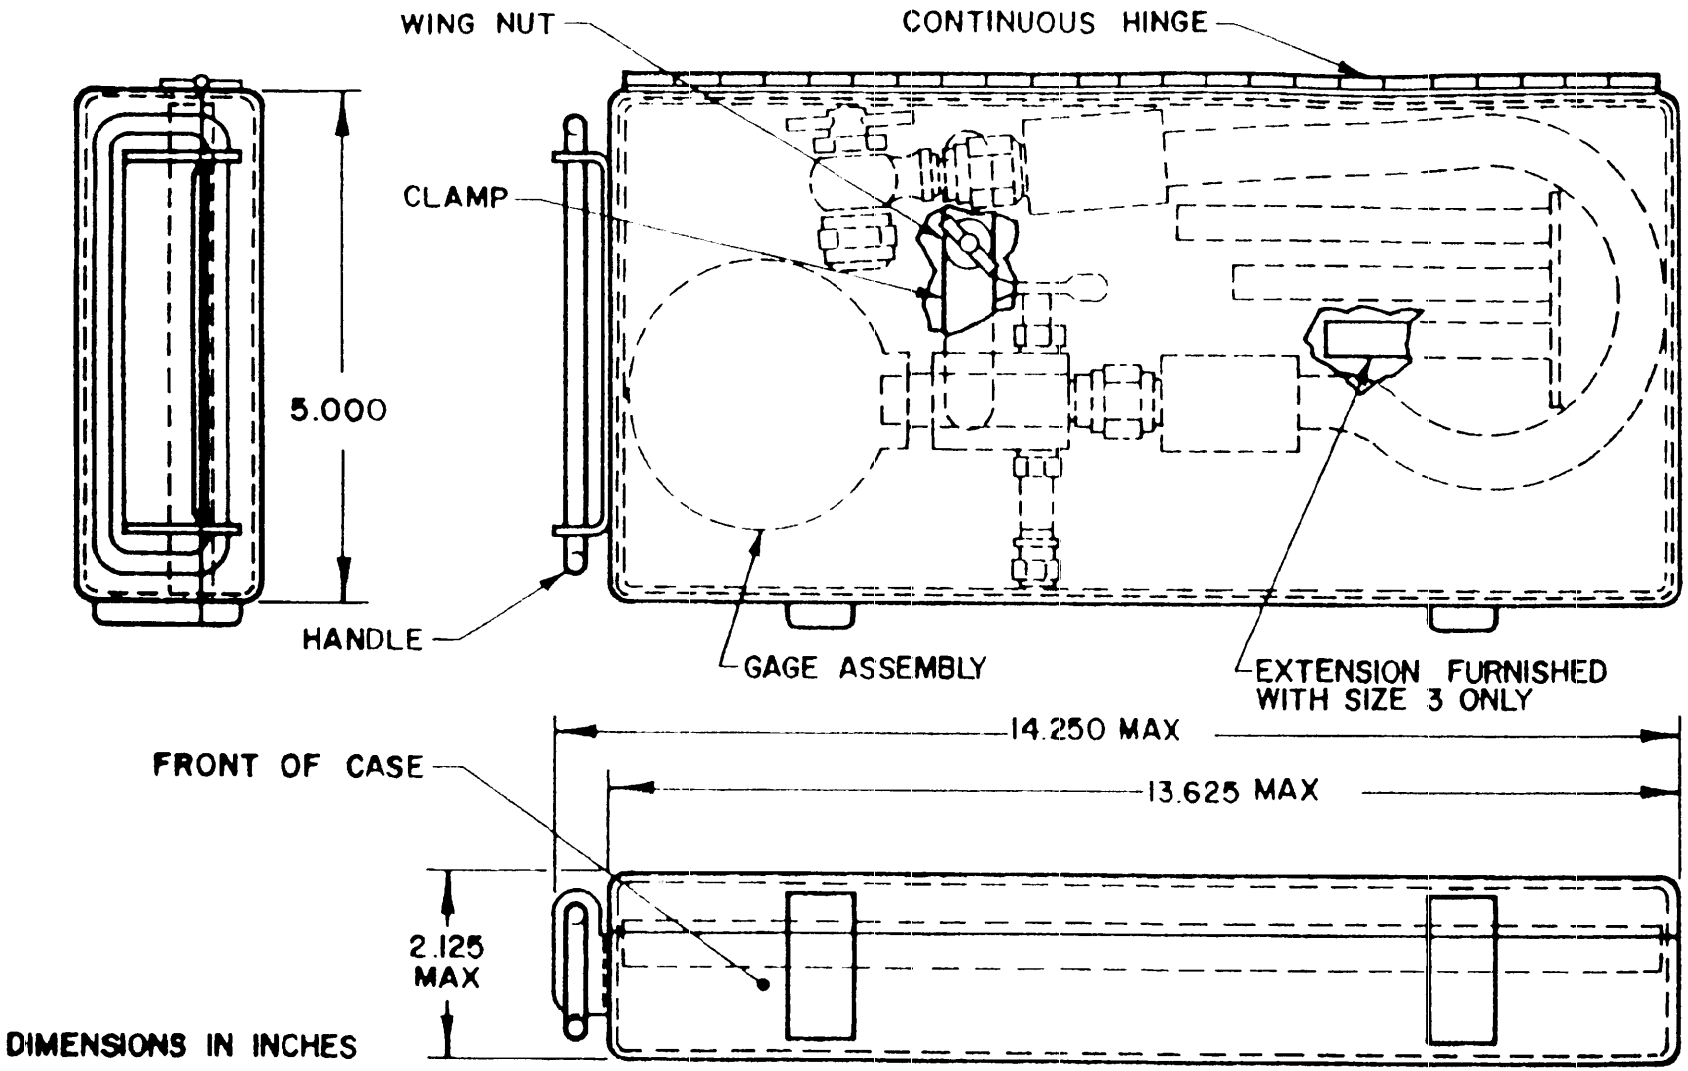


FIGURE 1. Class A, gage assembly and case

Source: https://assist.dla.mil -- Downloaded: 2026-01-17T10:21Z
Check the source to verify that this is the current version before use.

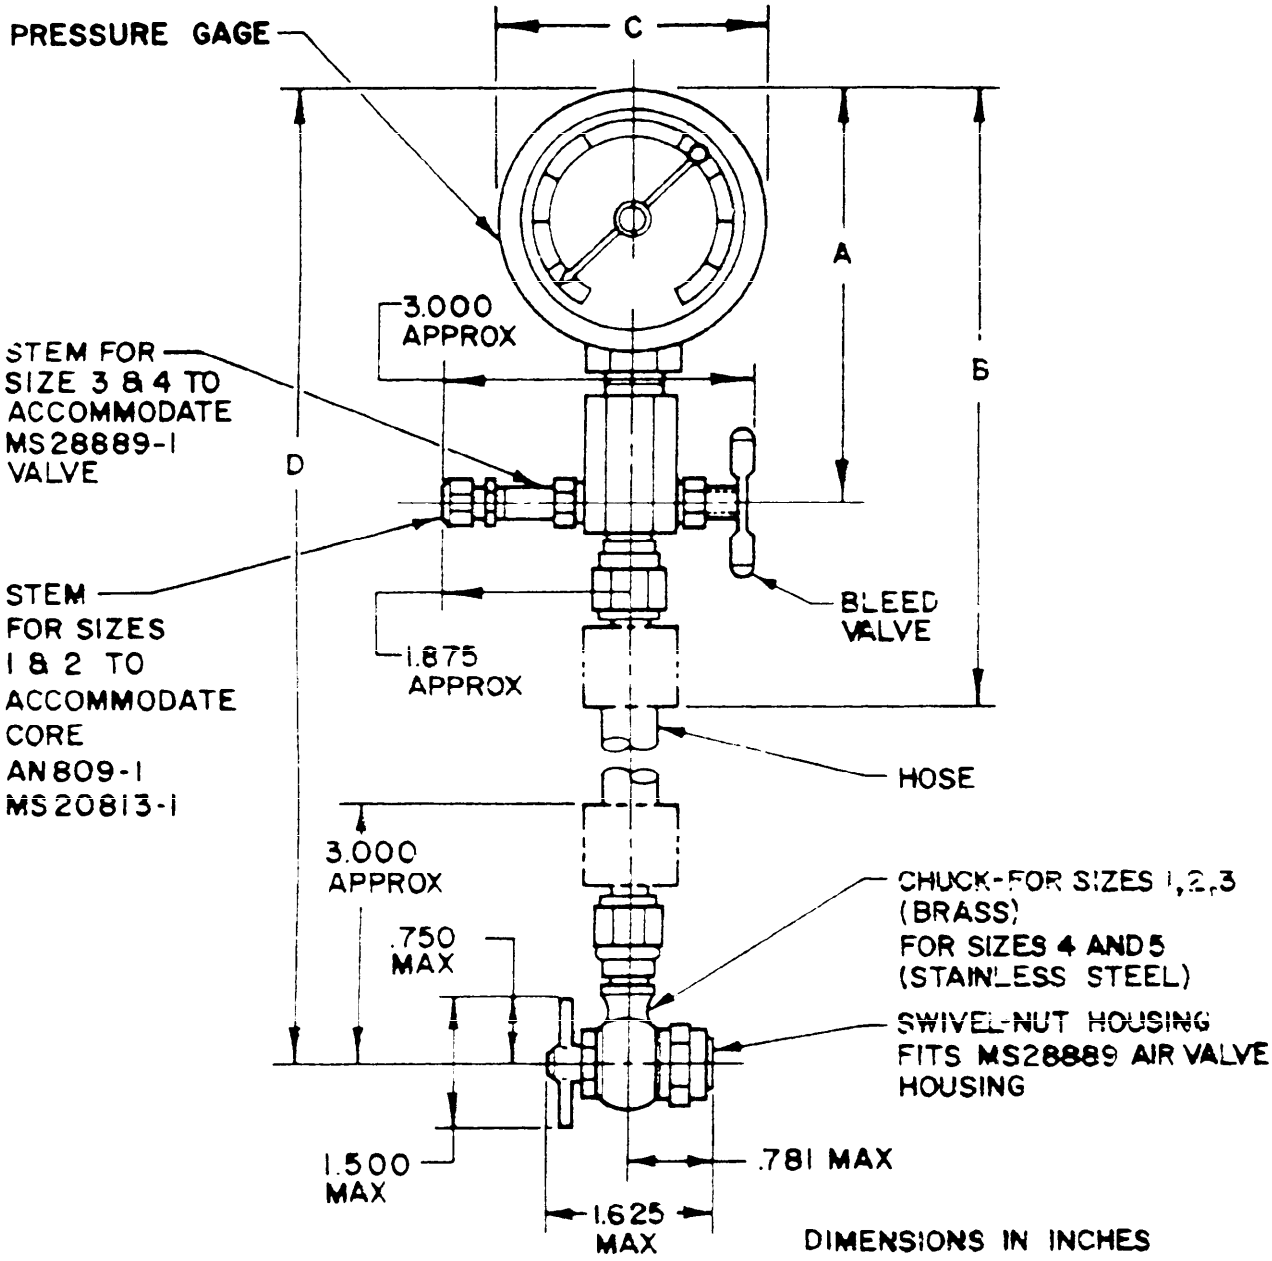

SIZE	PRESSURE GAGE	A APPROX	B MAX	C MAX	D MAX
1	0 TO 3,000 PSI	5-1/2	8	3-1/2	25-3/4
2	0 TO 1,500 PSI	5-1/2	8	3-1/2	25-3/4
3	2,000 TO 5,000 PSI	6-1/4	9	4-1/2	26-1/2
4	0 TO 4,000 PSI	5-1/2	8	3-1/2	25-3/4

FIGURE 2. **Class A gage assemblies**

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

suitable stop shall be provided to prevent the depresser from damaging the valve core. The chuck body for sizes 1 and 2 shall be brass, and for sizes 3 and 4, stainless steel.

3.7.4 Carrying case. Each class A gage shall be provided with a case so designed and constructed as to compactly enclose and protect the gage during handling and service. The case shall conform to Figure 1 and shall be fabricated from sheet steel approximately 0.030 inch thick.

3.7.4.1 Latches. The case shall incorporate two spring-type latches to securely hold the lid in a closed position. The latches shall be constructed in such manner that opening and closing of the case may be easily accomplished without the use of tools.

3.7.4.2 Clamp. The clamp shall be designed and constructed to retain the gage within the case when the open case is placed in any position. Similar provisions shall be incorporated to retain the accessories as specified herein.

3.7.4.3 Handle. The handle shall provide sufficient clearance for an easy and complete grip by a person wearing heavy gloves.

3.7.4.4 Finish. The case shall be finished yellow in accordance with MIL-STD-808, F103 Type I, color DC.

3.7.5 Accessories. The class A gage shall be furnished with the following spare parts.

* 3.7.5.1 Washers. Three space valve stem washers to fit in the swivel-nut chuck shall be furnished with each gage. The washers shall be according to Air Force Drawing 42A3377.

3.7.6 Dial marking. Class A gages shall have graduated dial markings as follows:

a. Size 1 - graduated in 30-pound increments.
b. Size 2 - graduated in 25-pound increments.
c. Size 3 - graduated in 50-pound increments. (The space allotted for 0 to 2,000 pounds shall be blanked out).
d. Size 4 - graduated in 50-pound increments.

3.7.7 Hose assembly. A reinforced hose assembly with a working pressure as specified in 1.2 for each size and a minimum burst of 4 times the working pressure shall be used. The outer cover shall be resistant to abrasion and shall withstand deteriorating effects of weather, water, oil, grease, and gasoline.

* 3.8 Class B, gage assembly. Class B, gage assemblies shall consist of a pressure gage, hose, dual chuck foot, chuck foot extension and carrying case. The gage assemblies shall conform to Figure 3. The dial markings for the different ranges, shall be 20 pound figure intervals, 2 pound smallest graduated divisions.

3.8.1 Dual-chuck foot. The chucks shall be offset approximately 30 degrees as shown on Figure 3. The chucks shall be designed and constructed to fit a valve stem conforming to MS28889. The dual chucks shall be so designed that engagement of ne of the chucks with the valve stem will render the deflator

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

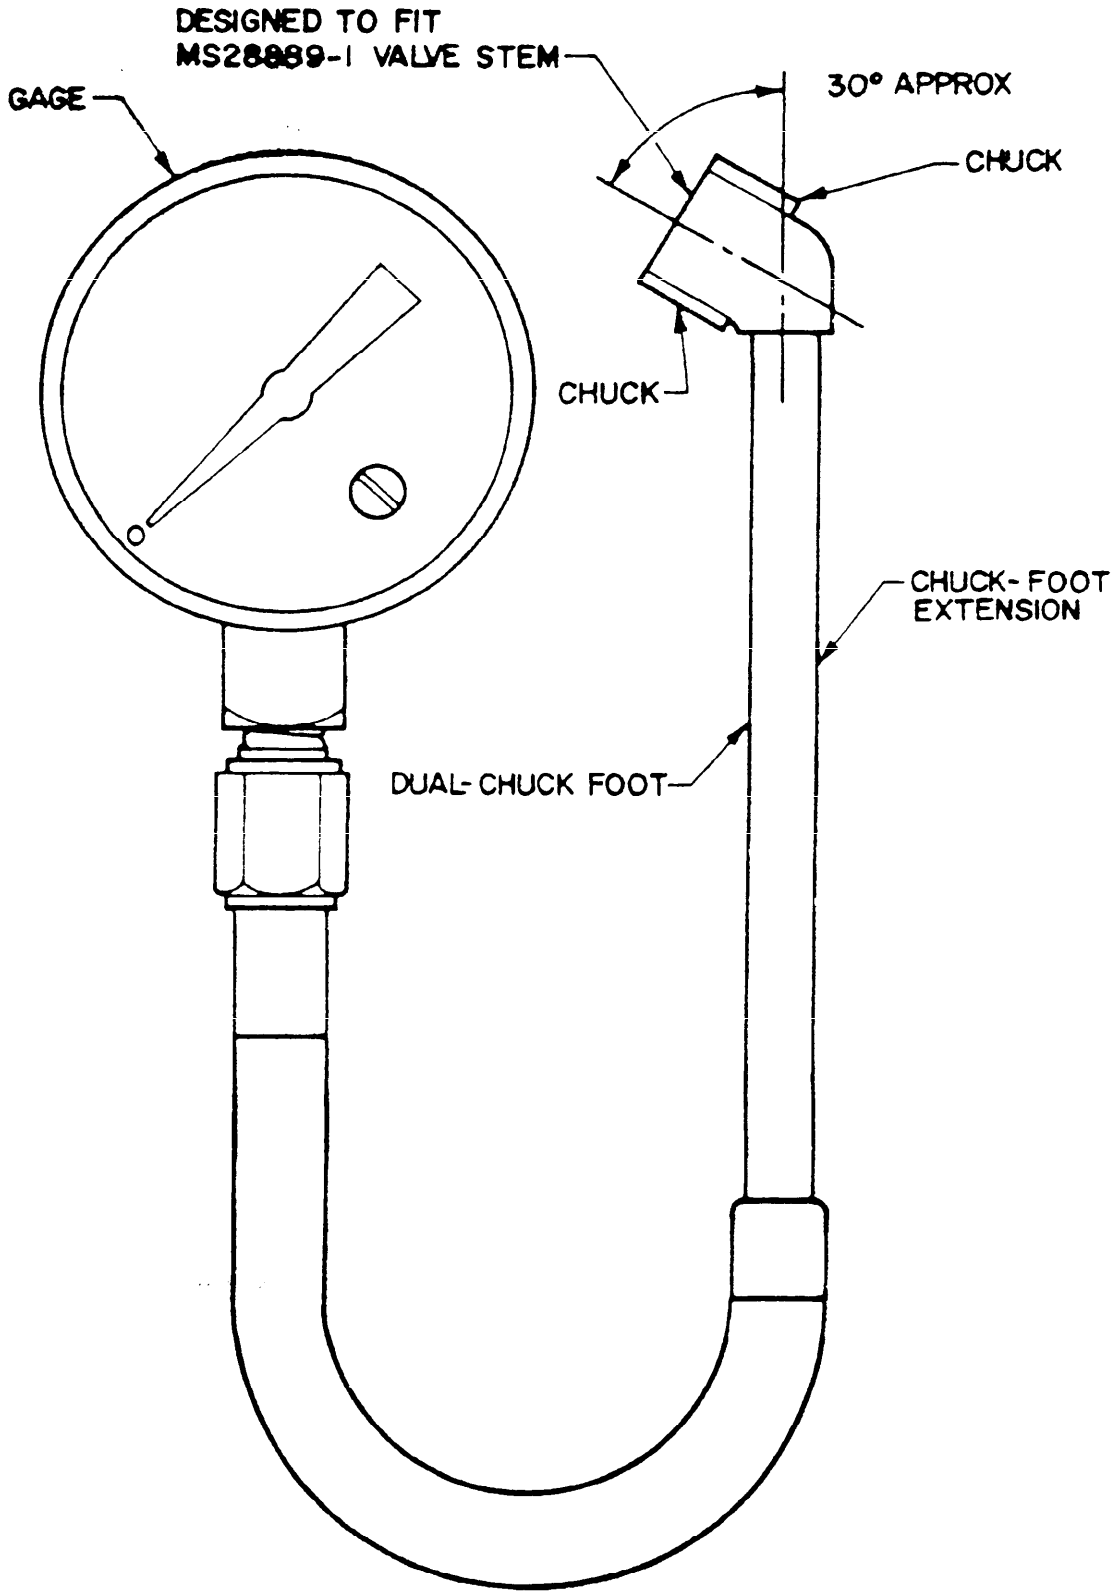


FIGURE 3. Class B gage assemblies

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

stem of the other chuck inoperative. Deflator pins shall be fabricated from hardened steel. The pins shall be designed with flats so that distortion of sealing washers will not cause any restriction of the air flow through the chuck to the gage after continued usage.

* 3.8.2 Chuck foot extension. The chuck foot shall have an extension approximately 6 inches long. The chuck foot shall either be fabricated integrally with the extension or shall be rigidly attached thereto in such manner that it will not become loose or detached under normal usage.

* 3.8.3 Hose assembly. A reinforced hose assembly with a working pressure as specified in 1.2 for each size, and a minimum burst of 4 times the working pressure shall be used. The outer cover shall be resistant to abrasion and shall withstand deteriorating effects of weather, water, oil, grease, and gasoline. The hose shall be approximately 8 inches in length.

* 3.8.4 Carrying case. The case for class P gages shall conform to the case requirements for class A gages, except that the length shall not exceed 10-5/8 inches and the width shall not exceed 5 inches.

* 3.9 Part numbering of interchangeable parts. All parts having the same manufacturer's part number shall be functionally and dimensionally interchangeable. The item identification and part number requirement of MIL-D-1000/1 shall govern the manufacturer's part numbers and changes thereto.

3.10 Identification marking. Equipment assemblies and parts shall be marked for identification in accordance with MIL-STD-130. The nomenclature and scale range of each gage assembly shall be marked on the outside of the carrying case in black letters 3/8 inch high.

3.10.1 Each separate gage assembly will be identified by a specification based part number in accordance with MIL-STD-961, 4.4 per example below:

M 8348 - A - 1 Part Number M8348-A-1

Size
Class
Specification Number
Prefix Meaning MIL Specification Item

3.11 Workmanship. Workmanship shall be of the quality necessary to produce complete units of good appearance, with safe and efficient operating characteristics as is customarily found in high grade commercial quality items of a similar nature.

3.12 Reclaimed materials. The use of reclaimed material shall be encouraged to the maximum extent possible without jeopardizing the intended end use of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

* 4.1 Responsibility for inspection. Unless otherwise specified in the contract, the contractor is responsible for the performance of all inspections requirements as specified herein. Except as otherwise specified in the contract, the contractor may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspection set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.2 Classification of inspection. The examination and testing of the gage assemblies shall be classified as:

a. Preproduction inspection (see 4.4)

b. Quality conformance inspection (see (see 4.5)

4.3 Test conditions.

4.3.1 Test equipment. Tests shall be conducted using equipment of laboratory accuracy and acceptable to the procuring activity. Tests shall be performed using air or gas pressure to simulate actual use. Tests with hydraulic pressures are not acceptable.

4.3.2 Atmospheric conditions. Unless otherwise specified, all tests required by this specification shall be made at an atmospheric pressure of approximately 30 inches of mercury and at room temperature of 70° ±5°F. When tests are made with atmospheric pressure and temperature substantially different from the above values, proper allowance shall be made for the difference from specified conditions.

4.3.3 Tapping. Unless otherwise specified, the gage assemblies incorporating Bourdon tube-type gages shall be tested in the normal operating position and shall be tapped lightly before a test reading is taken (see 6.4.1).

4.4 Preproduction inspection.

4.4.1 Sampling instructions. The contractor shall subject two gage assemblies of each class and size to the preproduction tests.

4.4.2 Tests. Preproduction tests shall consist of all the tests specified in 4.6.

4.4.3 Preproduction test report. The contractor shall prepare a report of the preproduction tests in accordance with MIL-STD-831 showing that the gaging elements conform to this specification. Three copies shall be furnished to the procuring activity.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

4.4.4 Preproduction test samples for the procuring activity. The contractor shall submit to the procuring activity, together with the preproduction test report, sample gage assemblies as specified in 4.4.1 to be used as follows (see 6.2):

a. For a review of the mechanical construction of the product.

b. To perform any tests included in the specification, after reviewing the contractor's test report.

4.5 Quality conformance inspection. Quality conformance inspection shall consist of the individual tests and sampling tests.

4.5.1 Individual tests. Each gage assembly shall be subjected to the following tests:

a. Examination of product (see 4.6.1)

b. Scale error at room temperature (see 4.6.2)

4.5.2 Sampling tests. Sampling tests and examination shall be in accordance with GG-G-76.

4.5.3 Inspection lot. A lot shall consist of all gage assemblies and carrying cases manufactured and assembled under essentially the same conditions and submitted for inspection at one time.

4.5.4 Resubmitted inspection lots. Provisions of MIL-STD-105 shall apply, with the following additions: Single sampling and tightened inspection shall be used, and the reinspection shall include all types and classes of defects.

4.6 Test methods.

4.6.1 Examination of product. The gage assembly, including carrying case, shall be inspected to determine compliance with the requirements specified herein with respect to materials, workmanship, and marking.

* 4.6.2 Scale error at room temperature. The gage assembly shall be tested for scale errors at 1/4-, 1/2-, 3/4-, and full range pressure of the gage. The test shall be made by subjecting the gage to the pressures specified herein to produce these readings, first with the pressure increasing, then with the pressures decreasing. With the pressures increasing, the pressure shall be brought up to, but shall not exceed the pressure specified to give the desired, reading; and with the pressure decreasing, the pressure shall be brought down to, but not fall below the pressure specified to give the desired reading. Accuracy of class A and B gages shall be ±(2%) during the first and last quarter of the scale and ±(1%) in the middle of the scale.

* 4.6.3 Overpressure.

4.6.3.1 Classes A and B. The gage assemblies shall be subjected to a pressure of 15 percent in excess of full-scale pressure for a period of 10 minutes. No less than 1 hour following the application of the specified pressure, the gage assemblies shall be subjected to the test specified in 4.6.2. Recalibration adjustment, if necessary, is permissible before performance of the test specified in 4.6.2. Scale errors shall not exceed the tolerance specified in 4.6.2.

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

4.6.4 Endurance.

* 4.6.4.1 Classes A and B. Classes A and B gage assemblies shall be subjected to 10,000 apllications of pressure from 0 to 80 ±5 percent of the full-scale pressure and return to zero at a rate of 20 ±10 cycles per minute. The applied pressure with respect to time shall approximate a square wave shape. Not less than 1 hour following this test the gage assemblies shall be subjected to the test of 4.6.2. Recalibration adjustment, if necessary, is permissible before performance of the test of 4.6.2. Scale errors shall not exceed the tolerance specified in 4.6.2.

4.6.5 Drop test.

* 4.6.5.1 Classes A and B. The gage assemblies shall be dropped at least five times from a height not less than 12 inches on a concrete floor. Evidence of permanent damage to the gage assembly and any change occurring to the reading mechanism which cannot be recalibrated by the provisions for adjustment for correction of indications (see 3.6.4) shall be cause for rejection.

4.6.6 Rupture.

4.6.6.1 Classes A and B. The gage shall be subjected to gradually increasing pressure until the Bourdon tube ruptures and the safety protective device is actuated. Evidence of cracks in the gage crystal or case, or failure of the crystal or case, shall be cause for rejection.

4.7 Packing, packing and marking. Preparation for delivery shall be examined for conformance to Section 5.

5. PACKAGING

5.1 Preservation and packaging. Packaging shall be level A or C in accordance with MIL-STD-794. Preservation shall be Method II in accordance with MIL-P-116 (see 6.2).

5.1.1 Unit packaging. The unit packaging shall be considered as the carrying case complete with the inflator assembly therein. The metal carrying case shall be utilized as the interior container.

5.2 Packing. Packing shall be level A, B or C in accordance with MIL-STD-794 (see 6.2).

5.3 Marking of shipments. In addition to any special marking required by the contract or order, unit packages, intermediate packages, and shipping containers shall be marked in accordance with MIL-STD-129 (see 6.2).

Source: https://assist.dla.mil -- Downloaded: 20260-17T10:21Z
Check the source to verify that this is the current version before use.

6. NOTES

6.1 Intended use. Gage assemblies are intended for use in gaging air pressure and servicing aircraft shock struts, accumulators, and tires.

6.2 Ordering data. Procurement documents should specify:

a. Title, number, and date of the specification.

b. Class and size of gage assembly (see 1.2).

c. Where the preproduction test samples should be sent and instructions concerning the submittal of the test report (see 4.4.4).

d. Applicable levels of preservation, packaging, and packing (see 5.1 and 5.2).

*6.3 Supersedure. The class A gage assembly described in this specification was formerly covered by AN6286.

6.4 Definitions.

*6.4.1 Tapped lightly. The phrase "tapped lightly" is defined as meaning the application of a light vibration sufficient to overcome that small amount of residual friction normally associated with pressure gages.

6.4.2 Gage assembly. Gage assembly is defined as meaning the entire operating unit (as described by class A and B).

6.4.3 Gage element. Gage is defined as meaning the Bourdon or indicator type gage incorporated as a component part of the complete gaging assembly.

6.5 Changes from previous issue. The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

6.5.1 Remote control inflator assemblies, formerly class C assemblies of this document, were removed by revision G. These items are replaced by inflator assemblies (piston type gage) with safety relief mechanisms covered under MIL-I-85352.

Custodian:
Air Force - 99
Navy - AS

Review activity:
DLA - GS

Preparing activity:
Air Force - 99

(Project 6685-0549)

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEPARTMENT OF THE NAVY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 12503 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEPARTMENT OF THE NAVY

Chief of Naval Material
ATTN: MAT 0434
Washington, DC 20360

Source: https://assist.dla.mil -- Downloaded: 2026-10-17T10:21Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*:

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil/ -- Downloaded: 2026-01-17 10:21Z
Check the source to verify that this is the current version before use.