A-A-54461
10 February 1992

COMMERCIAL ITEM DESCRIPTION

RESTRAINT SET, WRIST AND ANKLE

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for MIL-R-36171C which is cancelled.

This Commercial Item Description covers one type of leather wrist and ankle restraint set intended for use in restraining patients in hospitals.

Salient Characteristics:

The restraint set shall consist of two wristlets and restraining strap with lock buckle and key, and two anklets and restraining strap with lock buckle and key. The restraint set shall be provided in a suitable cotton or nylon duck carrying case. The restraint set shall be in accordance with figures 1 through 4.

The wristlets and anklets shall be fabricated of good quality 100 percent leather, lined with a good quality suede material, sewn to the inside on all sides. The leather shall be treated with a nontoxic fungicide and mildew preventative. Both the wristlet and the anklet shall have six vertical slots as shown in figure 1. They shall each have a metal loop to be used with the leather restraining straps.

The restraining straps shall be constructed of good quality 100 percent leather. The straps shall be provided with a corrosion-resisting steel sliding jaw and single tooth lock buckle and shall be capable of passing through the metal half-rings on the wristlets and anklets of the restraint set. Two keys shall be provided that are suitable to operate the lock buckles.

AMSC N/A FSC 6530

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

Each restraint set shall be provided in a cloth carrying case. The case shall be fabricated of cotton or nylon duck, color olive green or black. Each carrying case shall have a handle and some type of closure (snap, or hook and pile).

Workmanship. The restraint set shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Set (SE). One restraint set with carrying case, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 1.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one restraint set.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests, including dimensional test, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-1. The unit of product for test purposes shall be one restraint set.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics. Tests shall include, but shall not be limited to, the following:

Key and lock test. Insert key into lock assembly. The key shall enter lock without any binding and release spring plunger. Lift locking member and pin. Remove key. Relock mechanism by pushing down spring plunger and resetting locking member and pin. Repeat the above operation for four more cycles.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document.

6530-00-788-4010

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6530-2283

Location: RESTRCID.15E


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

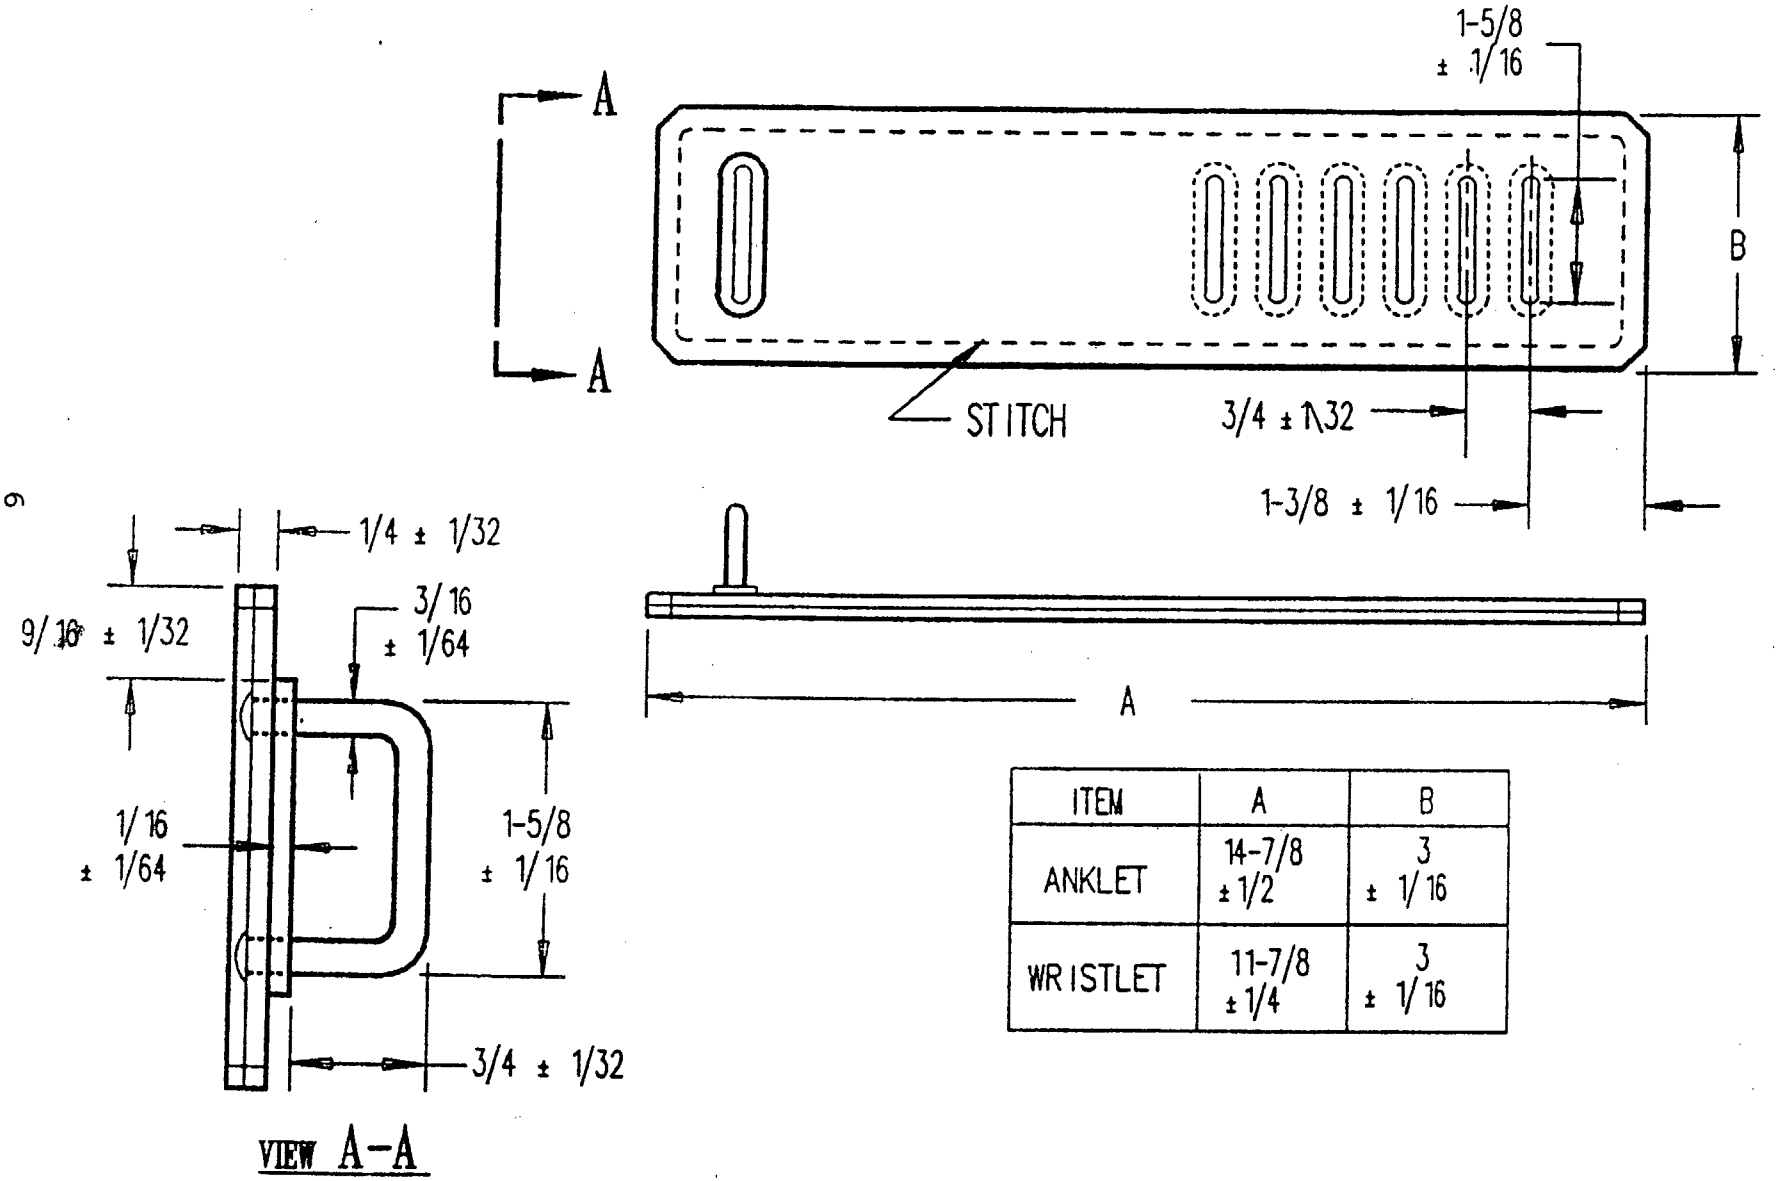

ITEM	A	B
ANKLET	14-7/8 ± 1/2	3 ± 1/16
WRISTLET	11-7/8 ± 1/4	3 ± 1/16

FIGURE 1. Wristlet and anklet.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

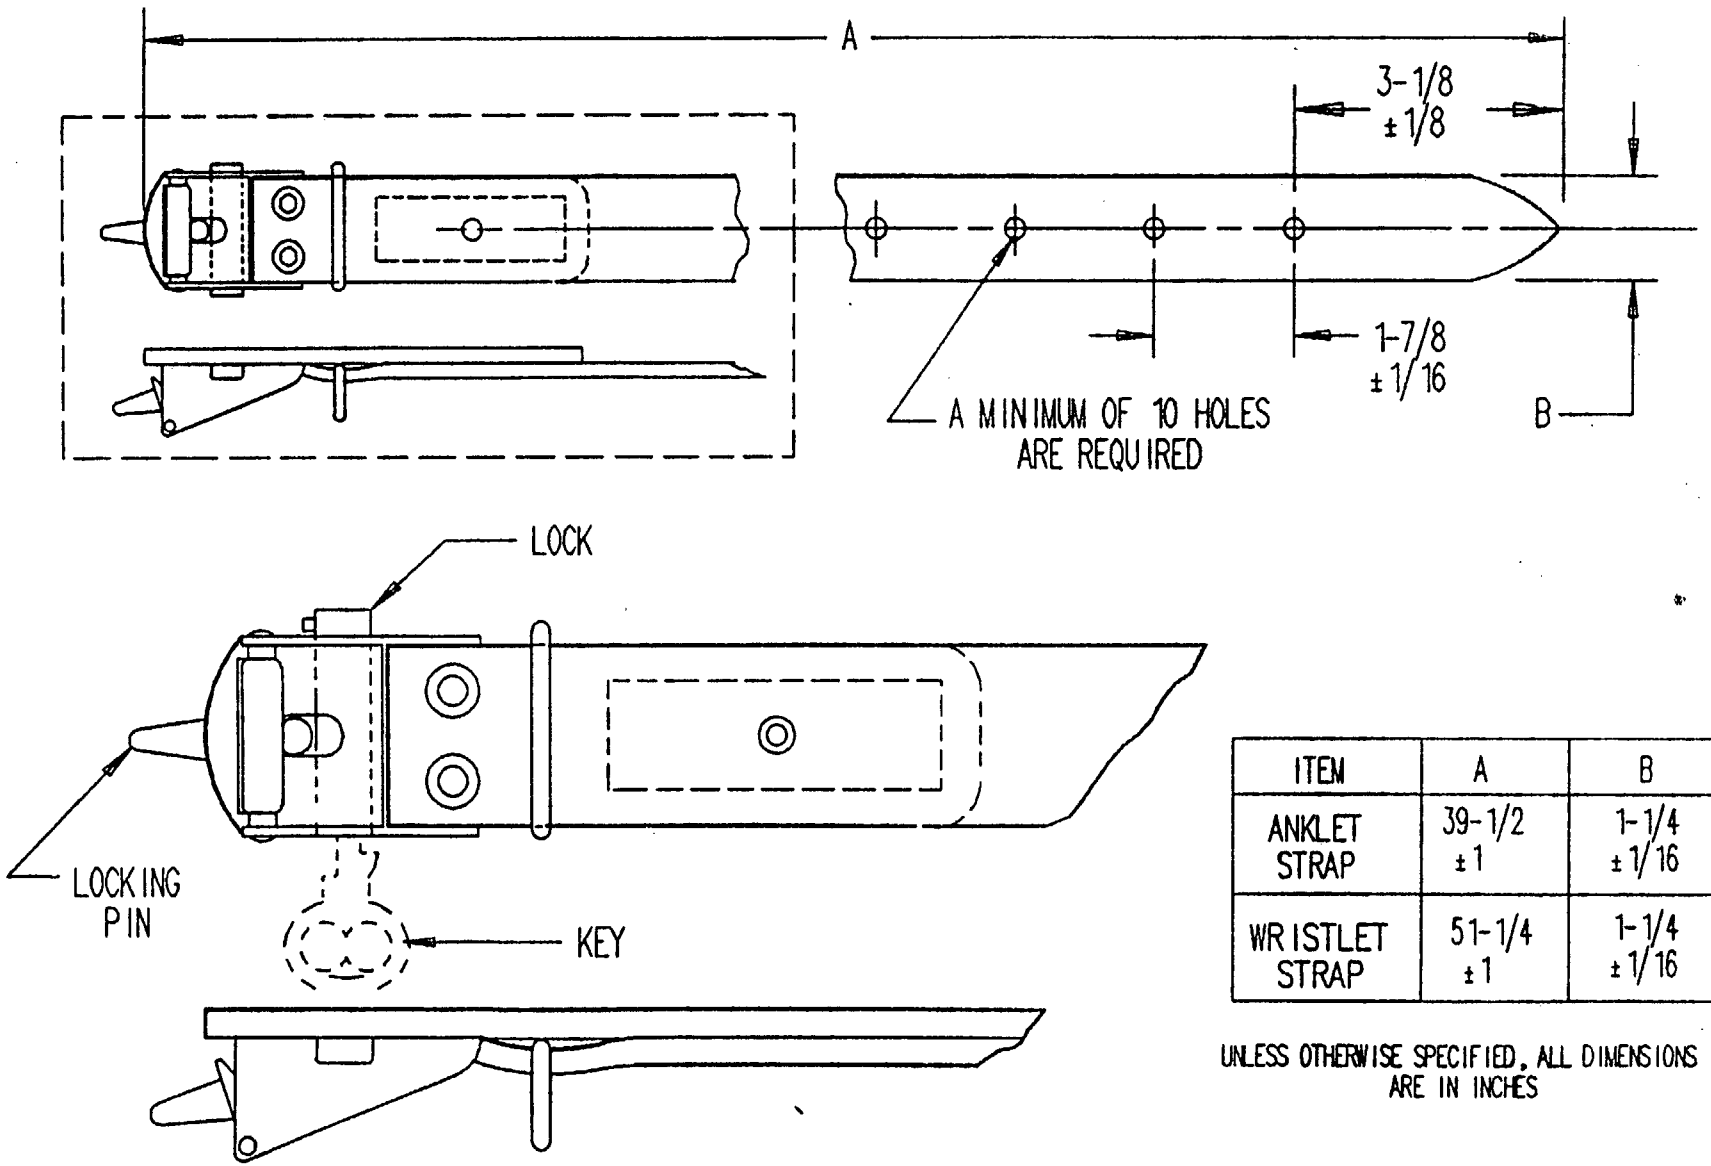


ITEM	A	B
ANKLET STRAP	39-1/2 ±1	1-1/4 ±1/16
WRISTLET STRAP	51-1/4 ±1	1-1/4 ±1/16

UNLESS OTHERWISE SPECIFIED, ALL DIMENSIONS ARE IN INCHES

A-A-54461

FIGURE 2. Buckle and restraining straps.


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

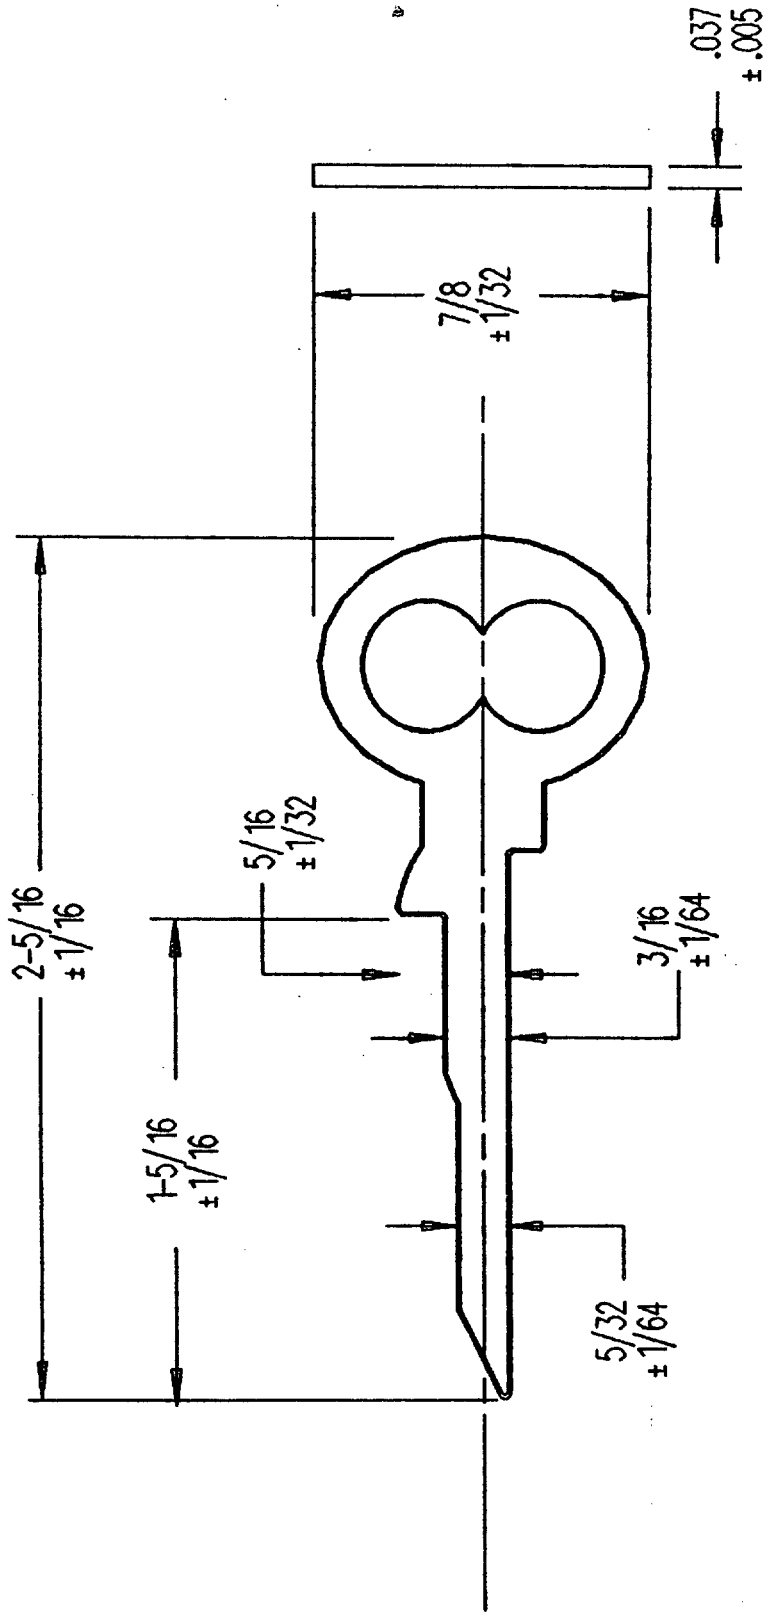

UNLESS OTHERWISE SPECIFIED, ALL DIMENSIONS ARE IN INCHES

FIGURE 3. Strap buckle unlocking key.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.

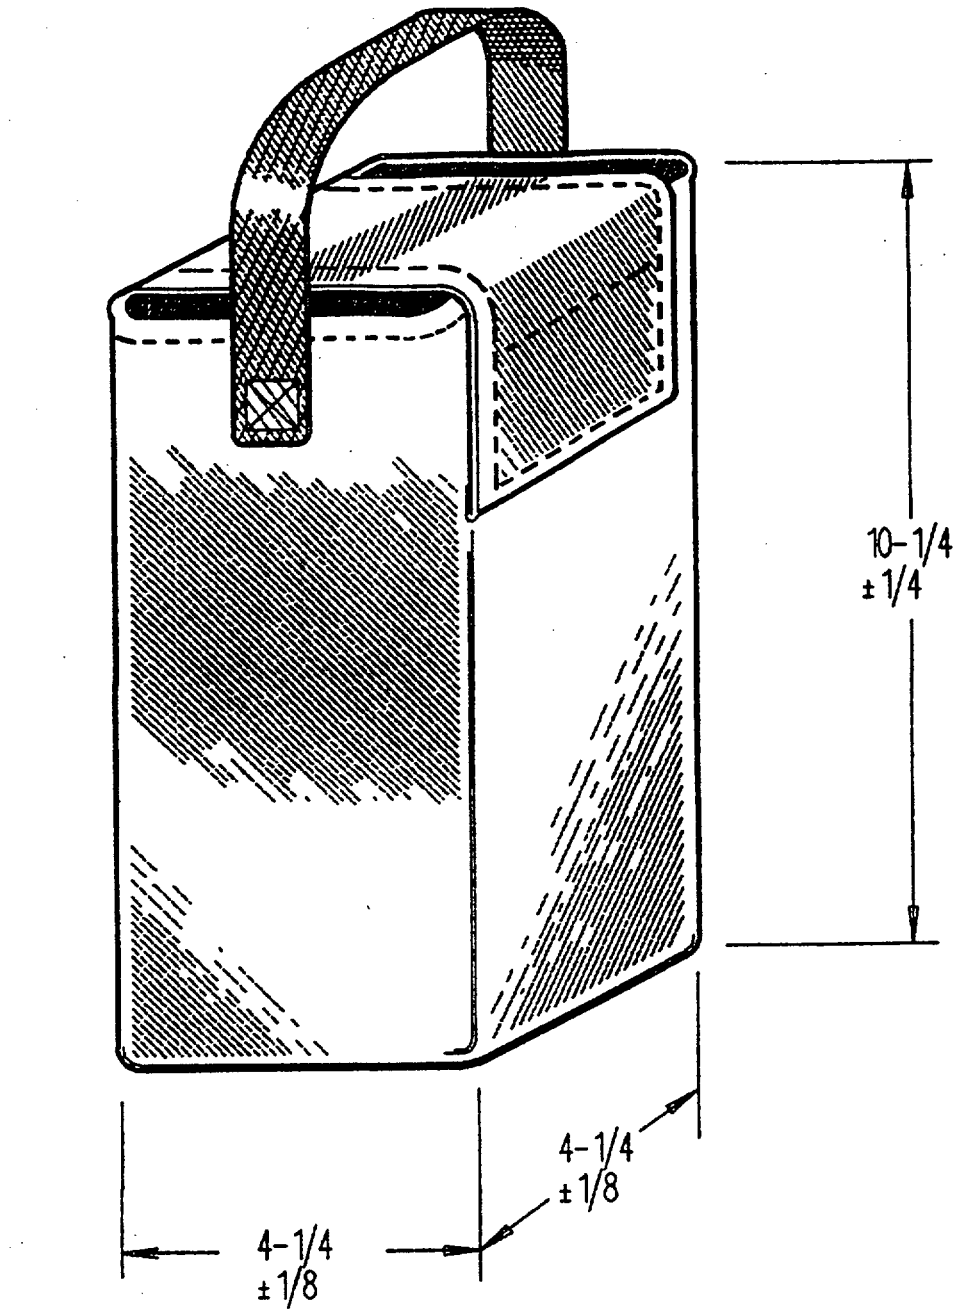

UNLESS OTHERWISE SPECIFIED, ALL DIMENSIONS ARE IN INCHES

FIGURE 4. Case.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:34Z
Check the source to verify that this is the current version before use.