A-A-54508
8 November 1991

COMMERCIAL ITEM DESCRIPTION

BURS, BONE SURGERY ("J" Notched)

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Military Specification MIL-B-42014 (DM) which is cancelled.

This Commercial Item Description covers "J" notched corrosion-resisting steel and carbide bone surgery burs.

Salient characteristics:

Classification. The bur heads shall be of the following shapes:

Shape A - Round
Shape B - Side cutting, straight, cross-cut
Shape C - Side cutting, tapered, cross-cut
Shape D - Lindeman
Shape E - Tapered, end and side cutting

Material. Shape A, B and C burs shall be fabricated from cemented tungsten carbide with cobalt binder. Titanium or tantalum carbide or both may be used in the fabrication of the bur. Shape D and E burs shall be fabricated from class 4, type 440 corrosion-resisting steel in accordance with ASTM F899.

Hardness. The burs shall be passivated. Burs fabricated from corrosion resistant steel shall have a Rockwell hardness of C50 to C56. The burs fabricated from tungsten carbide shall have a Rockwell hardness of C60 to C63. The burs shall be tested for hardness in accordance with ASTM E18 or ASTM E92 and E140.

Style and design. The burs shall be designed for use in oral and surgical procedures. The burs shall be of one piece construction and shall consist of a shank, neck and head. The blades shall be uniformly cut and sharpened. The style, design and dimensions of the burs shall be in accordance with figures 1 and 2.

Runout. The total indicated Runout of the bur shall not be greater than 0.001 inch when measured in accordance with ADA 23.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.

Autoclaving. The test bur shall be cleaned in accordance with the manufacturer's instructions. The bur shall then be autoclaved at 270°F ± 5°F and 27 psi ± 1 psi for a minimum of 20 minutes. Remove the bur from the autoclave. Any evidence of corrosion shall be cause for rejection.

Surface roughness. The surface roughness of the bur shank shall be no more than the root-mean-square (RMS) average duration of 16 micro-inches in the longitudinal direction of the shank when measured in accordance with ADA 23.

Finish. The bur head shall have a finely honed finish with sharpened blades. The neck and shank shall have a smooth finish.

Identification marking. Marking of the bur with the name or trademark shall be at the option of the supplier.

Instructions. Adequate and accurate instructions shall be furnished with each unit of issue on the use and care of the burs. The instructions shall include the type of solutions that shall not be use used for cold sterilization of the burs.

Workmanship. The burs shall have sharp, uniformly cut and formed blades, and shall be free from defects which detract from their appearance or may impair their intended use.

Unit. Each (EA). One bur of the shape specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and contractor shall be maintained by the contractor and

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:35Z
Check the source to verify that this is the current version before use.

made available to the Government upon the Government's request, at any time or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, and the lot size.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, an inspection level of II, with an AQL of 2.5 (percent defective). The unit of product for examination purposes shall be one bur of each shape.

Microscopic inspection. Examination of bur defects not readily perceptible to the naked eye shall be made using a microscope at 10 power (10x) magnification.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. The unit of product for test purposes shall be one bur of each shape. Sampling for dimensions shall be conducted at inspection level S-2, with an AQL of 1.0 (percent defective). Sampling for all other tests shall be conducted at inspection level S-1, with an AQL of 1.0 (percent defective).

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and the thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 20261O-26T09:35Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

National Stock Numbers	Item Identification
6515-01-193-5038	BUR, BONE SURGERY, Side Cutting, Tungsten Carbide, 1.85 mm Head Diameter, 5 mm Cutting Length, 55 mm Long: "J" Notched.
6515-01-193-5039	BUR, BONE SURGERY, Round, Tungsten Carbide, 2.3 mm Head Diameter, 55 mm Long. "J" Notched.
6515-01-193-5040	BUR, BONE SURGERY, Side Cutting, Tapered-End, Corrosion-Resisting Steel, 1.5 mm Head Diameter, 55 mm Long: "J" Notched.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:35Z
Check the source to verify that this is the current version before use.

National Stock Numbers	Item Identification
6515-01-193-5041	BUR, BONE SURGERY, Side Cutting, Tungsten Carbide, 1.65 mm Head Diameter, 5 mm Cutting Length, 55 mm Long: "J" Notched
6515-01-193-5042	BUR, BONE SURGERY, Side Cutting, Corrosion-Resisting Steel, Lindeman, 1.5 mm Head Diameter, 68 mm Long: "J" Notched.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4668
Location: Word/Bursbone

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.


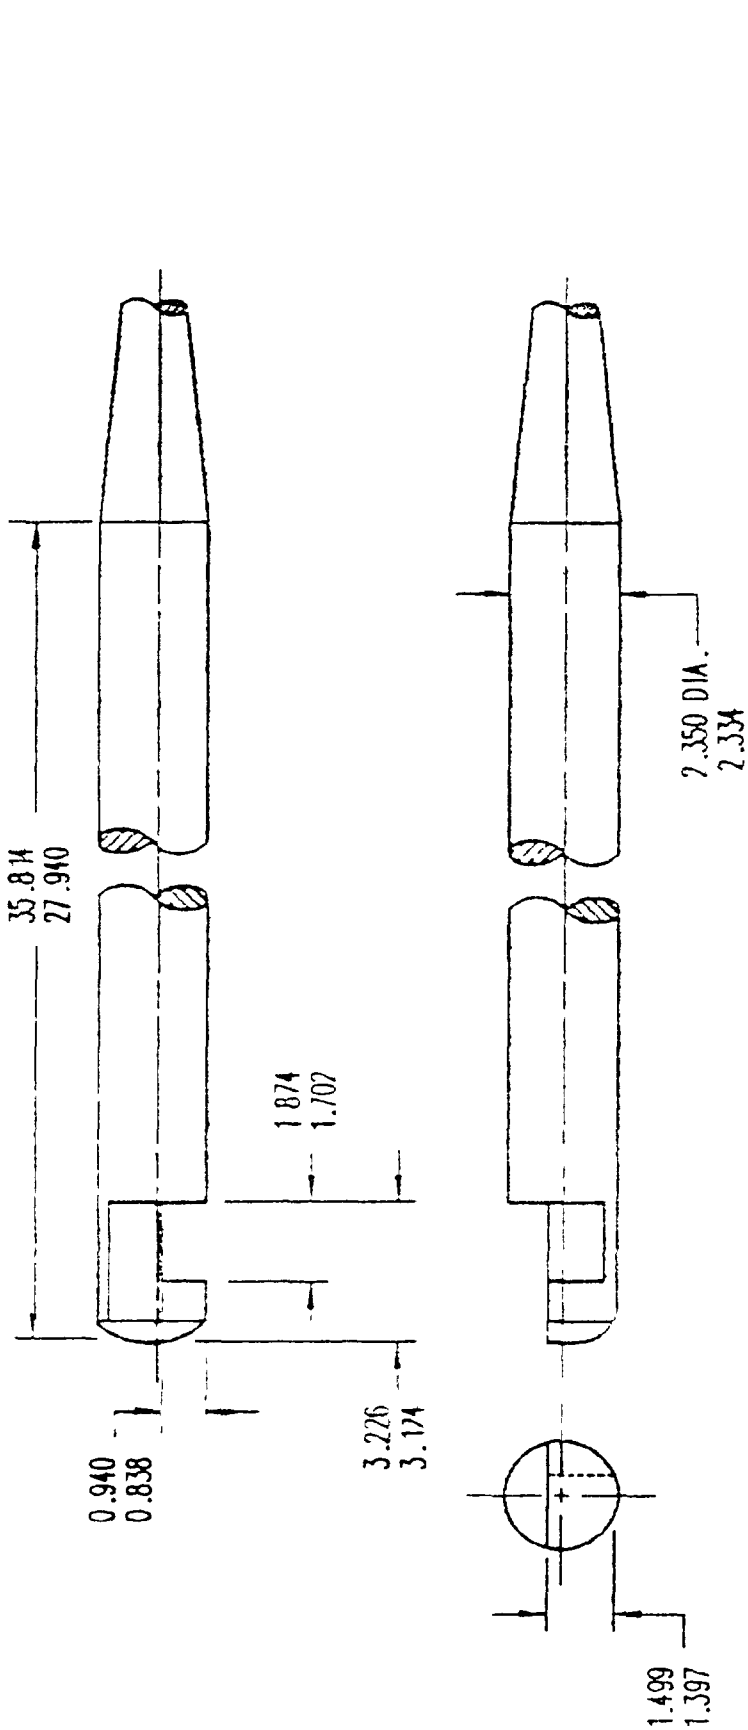



FIGURE 1 SHANK DIMENSIONS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.


SHAPE A
NO. OF FLUTES = 6
NSN65 15-01-193-5039

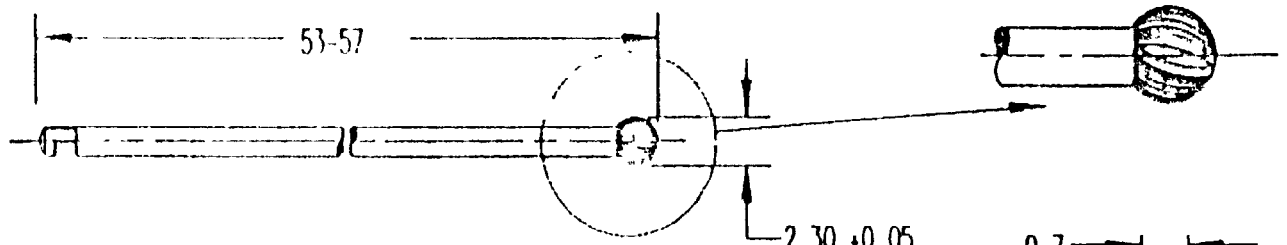


SHAPE B
NO. OF FLUTES = 6
NSN65 15-01-193-5041

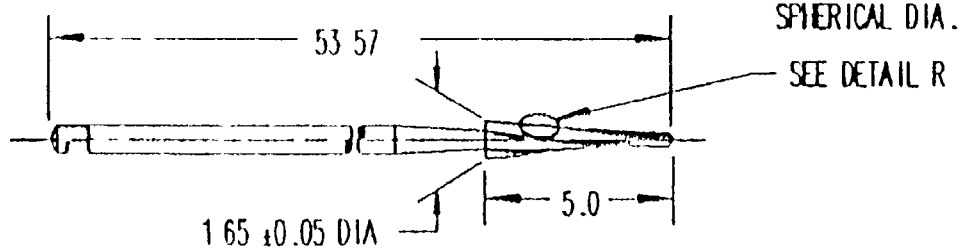


SHAPE C
NO. OF FLUTES = 6
NSN65 15-01-193-5038

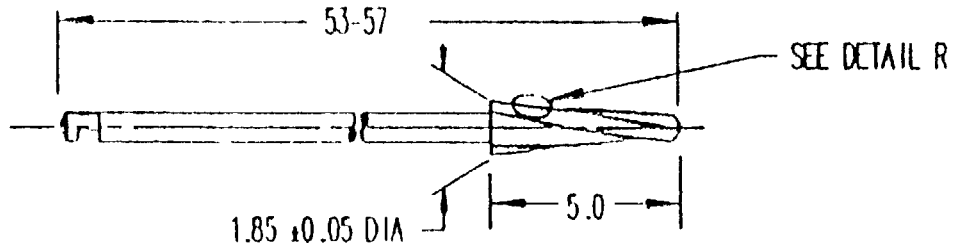


SHAPE D
NO. OF FLUTES = 4
NSN65 15-01-193-5042

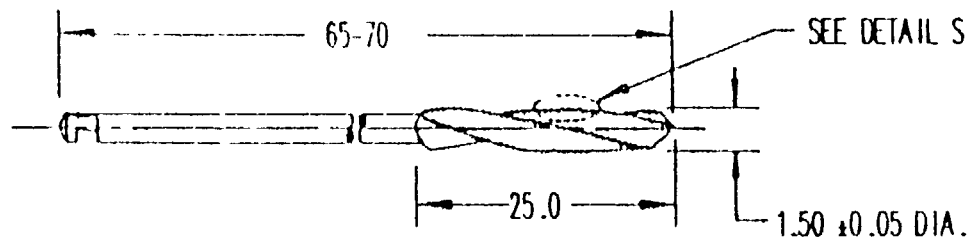


SHAPE E
NO. OF FLUTES = 3
NSN65 15-01-193-5040

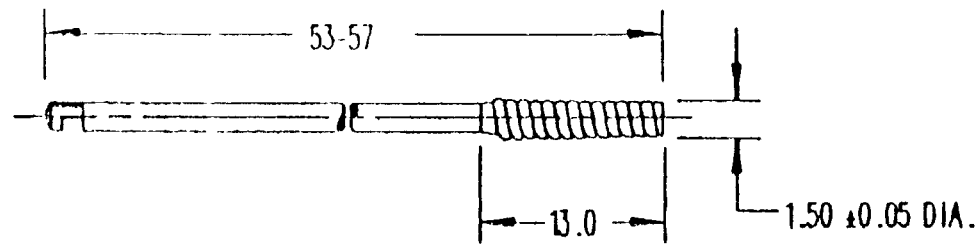

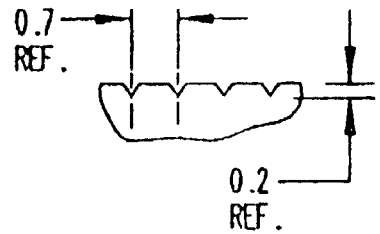

DETAIL R

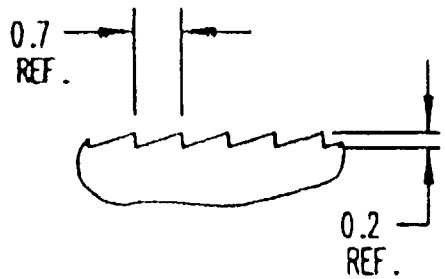

DETAIL S

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN MILLIMETERS.
TOLERANCES ON:

FRACTIONS	DECIMALS	ANGLES
	± 0.5	

FIGURE 2 BUR, BONE SURGERY

Source: https://assist.dla.mil -- Downloaded: 20260-26T09:22Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

1. RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54508	11-8-91

3. DOCUMENT TITLE
BUR, BONE SURGERY ("J" Notched)

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON	e. DATE SUBMITTED (YYMMDD)

7. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code) (1) Commercial	(2) AUTOVON
Defense Personnel Support Center	(215)737-2870	444-2870
c. ADDRESS (Include Zip Code) ATTN: DPSC-MSE 2800 S. 20th Street Philadelphia, PA 19101	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403 Falls Church VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 — Previous editions are obsolete — 90/700

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:35Z
Check the source to verify that this is the current version before use.