GG-D-00441c(DSA-DM)
April 30, 1969
Interim Revision of
Fed. Spec. GG-D-441b
May 1, 1957

INTERIM FEDERAL SPECIFICATION

DISPENSER, STRIP, DENTAL

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above.

The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification GG-D-441b.

1. SCOPE

1.1 Scope. This specification covers dispensers for holding rolls of articulating paper and dental matrix material and for dispensing this material into strip lengths.

2. APPLICABLE DOCUMENTS

2.1 The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

L-P-396	Plastic Molding, Polystyrene.
MMM-A-250	Adhesive, Water-Resistant, (For Sealing Fiberboard Boxes).
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

STANDARD

Federal

FED-STD-123 Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington, D. C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Fort Worth, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

STANDARDS

Military

MIL-STD-105 Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 Marking for Shipment and Storage.


(Copies of Military specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

* 3.1 Material. The dispensers shall be made of molded polystyrene conforming to type I, class 1 (General purpose, mechanical and electrical) polystyrene of L-P-396.

* 3.2 Style, design, and dimensions. The dispenser shall conform to figure 1 for style and design, and shall conform to the dimensions listed in table I.


Source: https://assist.dla.mil -- Downloaded: 202640-26T11:50Z
Check the source to verify that this is the current version before use.

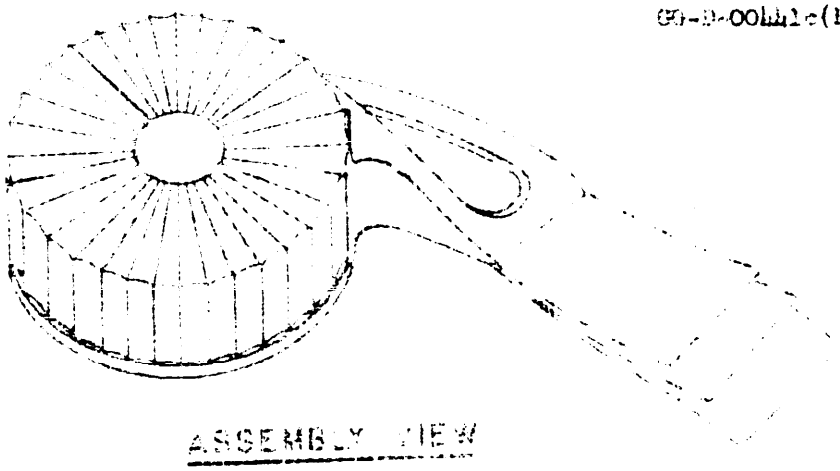


ASSEMBLY VIEW




BASE-TOP VIEW

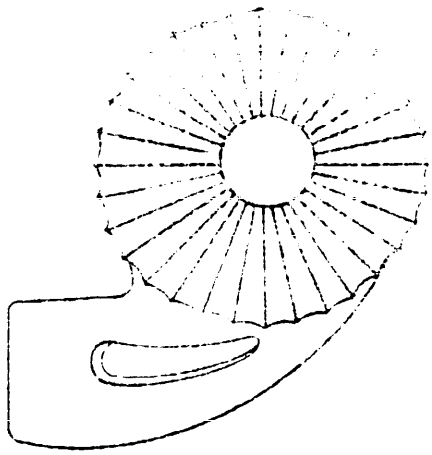

COVER-TOP VIEW

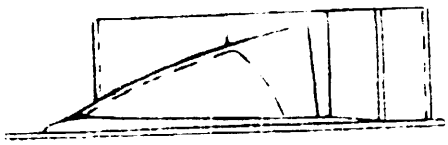

BASE-SIDE VIEW

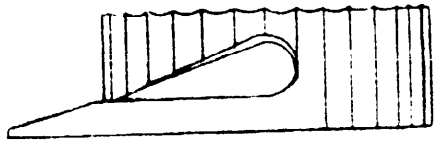

COVER-SIDE VIEW

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.

Table I. Dimensions

Characteristic	Dimension (inch)	Tolerance (inch)
Inside diameter of base	1-19/32	± 1/16
Inside diameter of cover	1-3/4	± 1/16
Wall thickness	1/16	± 1/64
Distance from center line of base to outside farthest point of channel	2-1/8	± 1/16
Distance from center line of base to inside farthest point of channel	7/8	± 1/32
Depth of base	21/32	± 1/32
Height of assembly	25/32	± 1/32
Width of channel opening at dispensing end	9/16	+ 1/8 - 1/16

* 3.3 Construction. The dispenser shall be of two-piece construction, consisting of a base and a cover. The base shall be properly molded into a roll-holding section and an outlet channel. The roll-holding section shall be capable of holding dental items such as rolls of articulating paper, celluloid and steel rolls, and rolls of dental matrix material, and shall be capable of dispensing these items (through the dispensing end) into strip lengths. Construction shall be such that the parts shall be easily taken apart and assembled, and such that material being used in the dispenser shall pass along the outlet channel and through the dispensing end in a free and easy manner, and in the lengths desired.

* 3.4 Color. Dispensers shall be either brown or black in color.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

* 3.5 Finish. Dispensers shall have a smooth finish. Cover of dispenser shall have a scalloped surface as shown in figure 1, suitable for hand gripping on outside surface of top and sides, except for portion of cover fitting over outlet channel, which shall have a smooth finish. If the name or trademark of the manufacturer appears on the top of the cover, this area shall also have a smooth finish.

* 3.6 Identification marking. Each dispenser shall be permanently and legibly marked with the name or registered trademark of the manufacturer.

* 3.7 Workmanship. Workmanship shall be first class throughout. Dispensers shall be free from defects which detract from their appearance or may impair their serviceability.

* 4. QUALITY ASSURANCE PROVISIONS

* 4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

* 4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

* 4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test methods and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

* 4.2 Quality conformance inspection. The examinations required to assure conformance of those items or lots of items to be offered for acceptance are classified as specified in tables II and III (see 4.2.2 and 4.2.3).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

* 4.2.1 Sampling for visual examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL'S) shall be indicated in table II. Unit of product for examination purposes shall be one dispenser.

* 4.2.2 Sampling for dimensional examination. Dispensers shall be examined to determine whether their dimensions fall within the tolerances listed in table I.

Table II. Inspection and Acceptable Quality Levels

Type defect	Inspection level	AQL (Percent defective)
For visual examination:		
Major	II	1.0
Minor	II	4.0
For dimensional examination	S-2	4.0

* 4.2.3 Examination. Dispensers shall be examined for defects including, but not limited to, those listed in table III.

Table III. Classification of Defects

Categories	Defects
Major:	
101	Dispenser not of two-piece construction.
102	Parts of dispenser cannot be easily taken apart or assembled.
103	Finish not as specified.
Minor:	
201	Manufacturer's name or registered trademark not present on dispenser.
202	Packaging, packing, and marking not as specified.

* 4.3 Tests. Tests shall be conducted to determine compliance with specification requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

* 5.1 Packaging. Packaging shall be level A or C, as specified (see 6.1).

5.1.1 Unit of issue. One dispenser, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table IV shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table IV. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	288 units

5.1.2.1 Variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

* 5.1.3.1 Unit package. Unit package shall be a box of appropriate size and design constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors will be acceptable, or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

* 5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2-inch wide tape conforming to PPP-T-76. Closing of bottom flaps with either adhesive (conforming to MMM-A-250) or metal stitches is permitted.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the currentversion before use.

* 5.1.4 Level C. Units shall be packaged in standard commercial containers, of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for the intended purpose.

* 5.2 Packing. Packing shall be level A, B, or C, as specified (see 6.1)

5.2.1 Level A.

* 5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table III, using type I, class 1 plywood; PPP-B-621, table III: or PPP-B-636, type CF, class weather-resistant. Closure and strapping shall be in accordance with appendix of applicable box specification.

5.2.2 Level B.

* 5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table II, using type III, class 1 plywood; or shall be designed for type 2 load and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic. Closure shall be in accordance with appendix of applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate to point of delivery called for in the contract or purchase order.

5.3 Marking.

* 5.3.1 Civil agencies. Unless otherwise specified, shipment markings shall be in accordance with FED-STD-123.

* 5.3.2 Military activities.

* 5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

* 5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the currentversion before use.

6. NOTES

* 6.1 Ordering data. Procurement documents should specify the following:

a. Title, number, and date of this specification.

b. Selection of applicable levels of packaging and packing (see 5.1 and 5.2)

* 6.2 Specification changes. The margins of this specification are marked with an asterisk to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.

6.3 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet Federal Government requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the currentversion before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION

GG-D-004416(DSA-DM) FSN

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO (If "Yes", in what way?)

4. REMARKS (Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)

SUBMITTED BY (Printed or typed name and activity - Optional)

DATE

DD FORM 1426

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:50Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
MAR 68

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:50Z
Check the source to verify that this is the current version before use.